

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN020223\
 Data File : VN076515.D
 Acq On : 02 Feb 2023 17:15
 Operator : JC\MD
 Sample : PB150614ZHE#1
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB150614ZHE#1

Quant Time: Feb 03 01:03:11 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011623W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jan 17 03:59:22 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.229	168	586532	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	985448	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.870	117	901091	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	433683	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.582	65	353273	53.793	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery = 107.580%			
35) Dibromofluoromethane	8.176	113	299614	48.604	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 97.200%			
50) Toluene-d8	10.570	98	1175748	51.645	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery = 103.300%			
62) 4-Bromofluorobenzene	12.853	95	437216	58.829	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 117.660%			
Target Compounds						Qvalue
11) Tert butyl alcohol	5.512	59	686	0.781	ug/l #	72
16) Acetone	4.453	43	37263	17.631	ug/l	100
18) Methyl Acetate	5.059	43	4395	0.616	ug/l	92
20) Methylene Chloride	5.288	84	23588	3.223	ug/l	96
25) 2-Butanone	7.500	43	5976	1.859	ug/l #	86
29) Tetrahydrofuran	7.847	42	687	0.346	ug/l #	25
31) Cyclohexane	8.229	56	11931	1.183	ug/l #	11
36) 1,1-Dichloropropene	8.229	75	44454	5.075	ug/l #	49
37) Ethyl Acetate	7.571	43	52371	7.485	ug/l	100
38) Carbon Tetrachloride	8.229	117	64083	6.560	ug/l #	17
42) 1,2-Dichloroethane	8.694	62	1997	0.223	ug/l #	73
43) Isopropyl Acetate	8.694	43	377771	33.052	ug/l #	79
45) 1,2-Dichloropropane	9.747	63	3302	0.527	ug/l #	42
48) Methyl methacrylate	9.747	41	221845	40.999	ug/l #	33
49) 1,4-Dioxane	9.747	88	380	3.328	ug/l #	1
51) 4-Methyl-2-Pentanone	10.447	43	12106	1.804	ug/l	94
53) t-1,3-Dichloropropene	10.729	75	2246	0.257	ug/l #	76
54) cis-1,3-Dichloropropene	10.359	75	116305	11.548	ug/l #	59
56) Ethyl methacrylate	10.988	69	3132	0.362	ug/l #	1
57) 1,3-Dichloropropane	11.206	76	14477	1.331	ug/l #	42
59) 2-Hexanone	11.176	43	232419	47.801	ug/l #	21
71) Bromoform	12.853	173	1949	0.381	ug/l #	1
74) N-amyl acetate	12.488	43	2841	0.294	ug/l #	41
76) 1,2,3-Trichloropropane	12.853	75	213340	26.559	ug/l #	1
77) Bromobenzene	12.982	156	58	Below Cal	#	1
81) trans-1,4-Dichloro-2-b...	12.853	75	213340	81.848	ug/l #	11
93) 1,2,4-Trichlorobenzene	15.394	180	255	1.338	ug/l #	82
95) Naphthalene	15.647	128	1519	1.904	ug/l	99
96) 1,2,3-Trichlorobenzene	15.841	180	183	1.179	ug/l #	12


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN020223\
Data File : VN076515.D
Acq On : 02 Feb 2023 17:15
Operator : JC\MD
Sample : PB150614ZHE#1
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PB150614ZHE#1

Quant Time: Feb 03 01:03:11 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011623W.M
Quant Title : SW846 8260
QLast Update : Tue Jan 17 03:59:22 2023
Response via : Initial Calibration




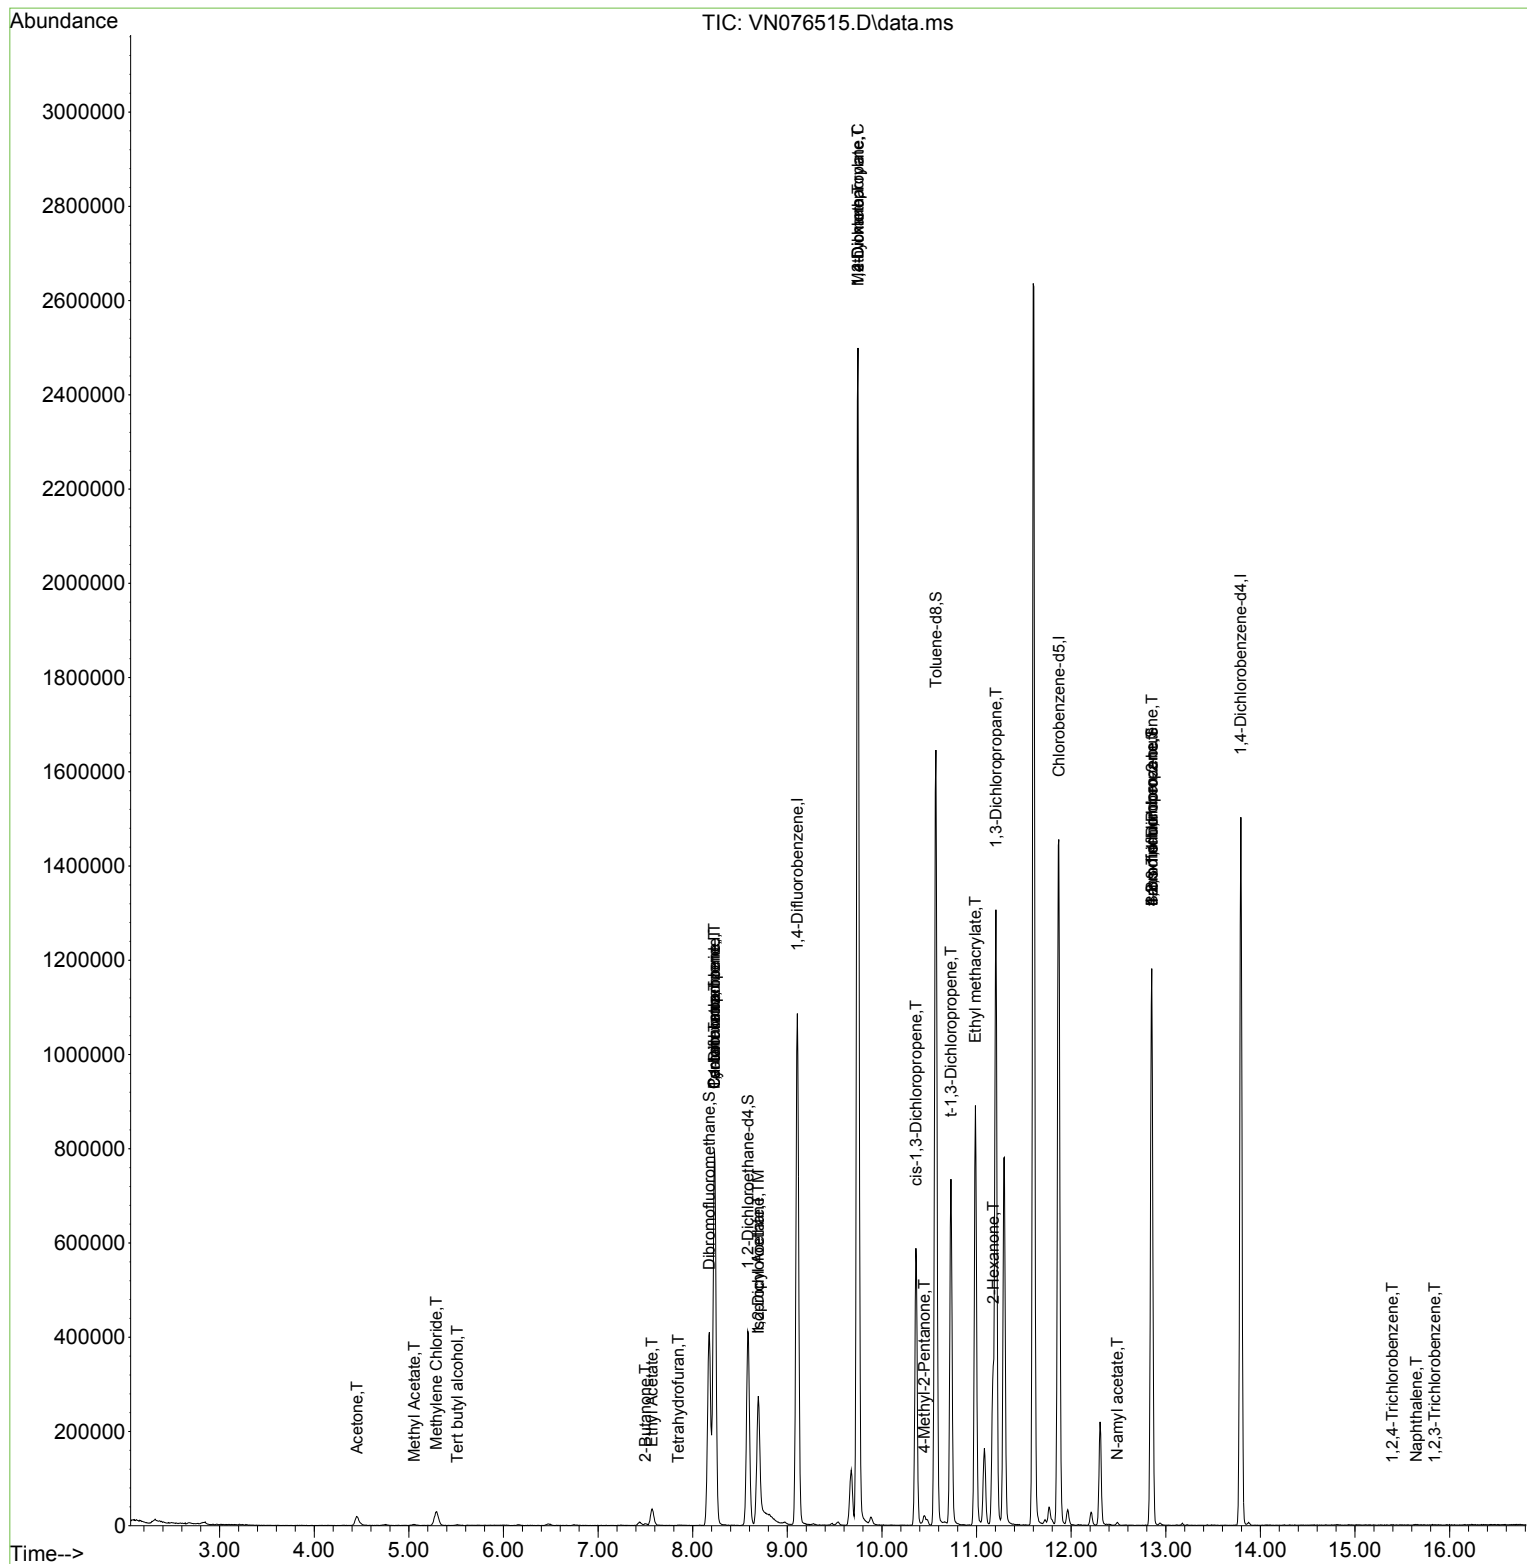




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.229 min Scan# 1050
Delta R.T. -0.001 min
Lab File: VN076515.D
Acq: 02 Feb 2023 17:15




Instrument :
MSVOA_N
ClientSampleId :
PB150614ZHE#1


Tgt Ion:168 Resp: 586532
Ion Ratio Lower Upper
168 100
99 61.0 41.6 62.4

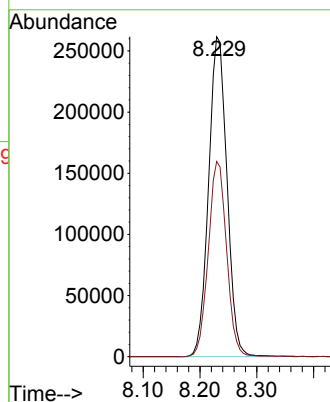

#11
Tert butyl alcohol
Concen: 0.781 ug/l
RT: 5.512 min Scan# 588
Delta R.T. -0.018 min
Lab File: VN076515.D
Acq: 02 Feb 2023 17:15

Tgt Ion: 59 Resp: 686
Ion Ratio Lower Upper
59 100
57 0.0 8.5 12.7#



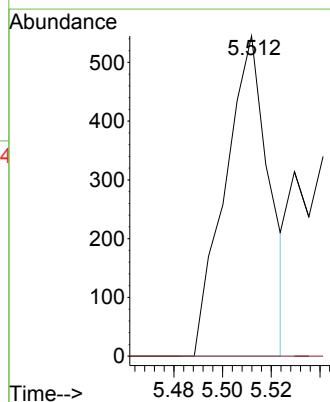
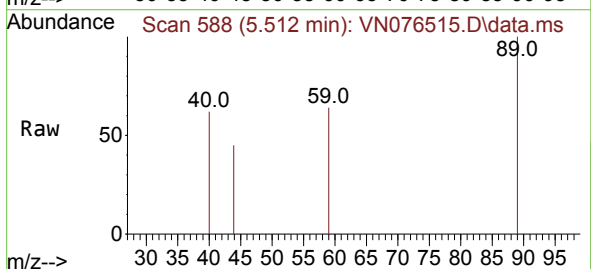




#16
Acetone
Concen: 17.631 ug/l
RT: 4.453 min Scan# 408
Delta R.T. 0.011 min
Lab File: VN076515.D
Acq: 02 Feb 2023 17:15




Instrument :
MSVOA_N
ClientSampleId :
PB150614ZHE#1

Tgt Ion: 43 Resp: 37263
Ion Ratio Lower Upper
43 100
58 33.3 26.7 40.1



#18
Methyl Acetate
Concen: 0.616 ug/l
RT: 5.059 min Scan# 511
Delta R.T. 0.023 min
Lab File: VN076515.D
Acq: 02 Feb 2023 17:15


Tgt Ion: 43 Resp: 4395
Ion Ratio Lower Upper
43 100
74 24.8 23.3 34.9

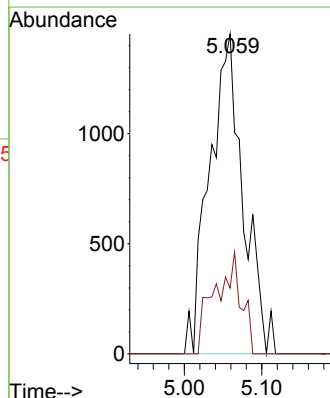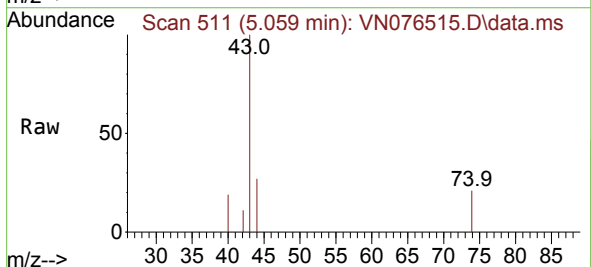






#20
Methylene Chloride
Concen: 3.223 ug/l
RT: 5.288 min Scan# 51
Delta R.T. -0.001 min
Lab File: VN076515.D
Acq: 02 Feb 2023 17:15

Instrument :
MSVOA_N
ClientSampleId :
PB150614ZHE#1







Tgt Ion: 84	Resp: 23588
Ion Ratio	Lower Upper
84 100	
49 109.4	84.5 126.7
51 37.1	26.0 39.0
86 65.8	52.0 78.0

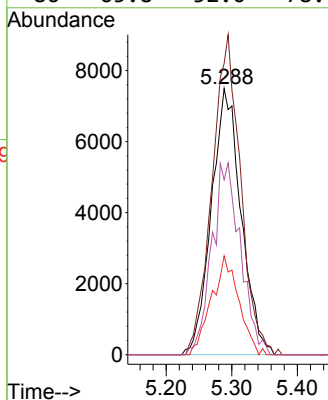

#25
2-Butanone
Concen: 1.859 ug/l
RT: 7.500 min Scan# 926
Delta R.T. 0.012 min
Lab File: VN076515.D
Acq: 02 Feb 2023 17:15

Tgt Ion: 43	Resp: 5976
Ion Ratio	Lower Upper
43 100	
72 26.5	27.4 41.2#

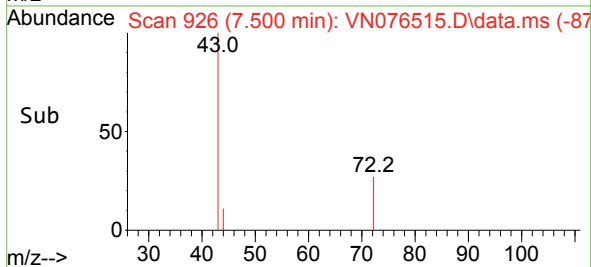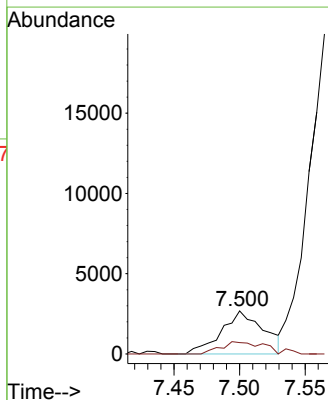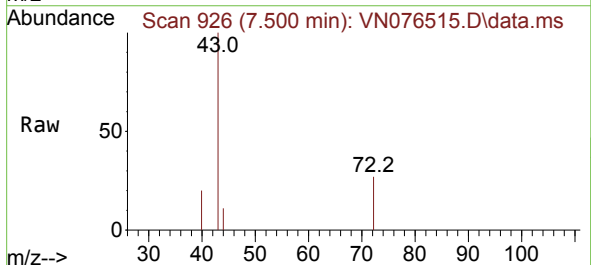



#29

Tetrahydrofuran

Concen: 0.346 ug/l

RT: 7.847 min Scan# 91

Delta R.T. 0.006 min

Lab File: VN076515.D

Acq: 02 Feb 2023 17:15

Instrument :

MSVOA_N

ClientSampleId :

PB150614ZHE#1





Tgt Ion: 42 Resp: 687

Ion Ratio Lower Upper

42 100

72 0.0 44.0 66.0#

71 0.0 41.1 61.7#

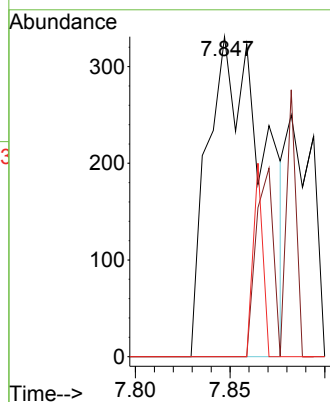

#31

Cyclohexane

Concen: 1.183 ug/l

RT: 8.229 min Scan# 1050

Delta R.T. -0.030 min

Lab File: VN076515.D

Acq: 02 Feb 2023 17:15




Tgt Ion: 56 Resp: 11931


Ion Ratio Lower Upper

56 100

69 163.4 25.8 38.8#

84 139.6 79.0 118.4#

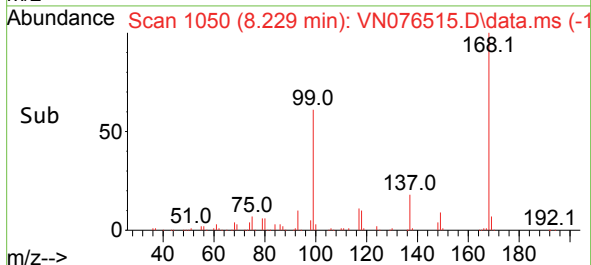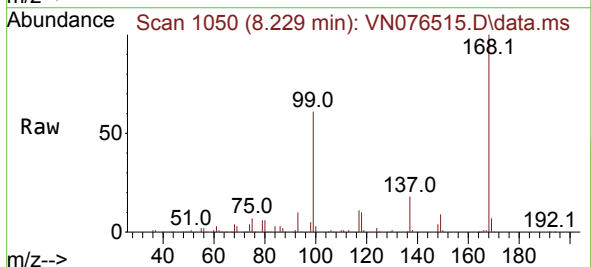



#33

1,2-Dichloroethane-d4

Concen: 53.793 ug/l

RT: 8.582 min Scan# 1110

Delta R.T. 0.000 min

Lab File: VN076515.D

Acq: 02 Feb 2023 17:15

Instrument :

MSVOA_N

ClientSampleId :





PB150614ZHE#1

Tgt Ion: 65 Resp: 353273

Ion Ratio Lower Upper

65 100

67 51.0 0.0 104.6

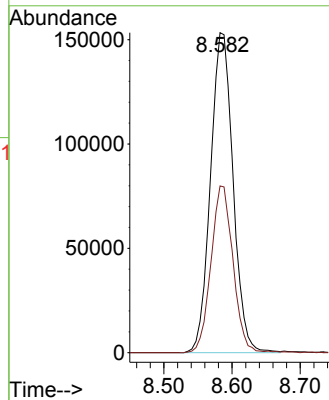

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 1199

Delta R.T. -0.000 min

Lab File: VN076515.D

Acq: 02 Feb 2023 17:15




Tgt Ion: 114 Resp: 985448


Ion Ratio Lower Upper

114 100

63 18.6 0.0 35.8

88 15.7 0.0 28.0



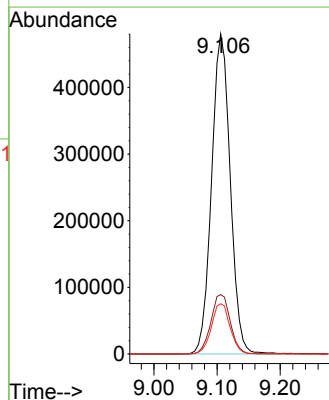
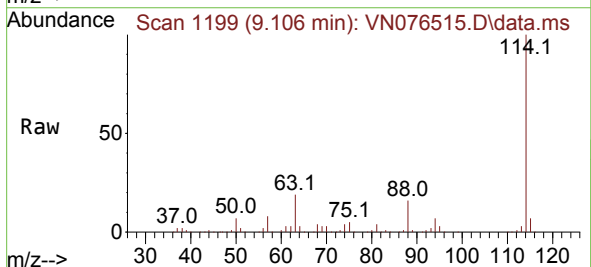




#35
Dibromofluoromethane
Concen: 48.604 ug/l
RT: 8.176 min Scan# 1040
Delta R.T. 0.005 min
Lab File: VN076515.D
Acq: 02 Feb 2023 17:15




Instrument :
MSVOA_N
ClientSampleId :
PB150614ZHE#1


Tgt Ion:113 Resp: 299614
Ion Ratio Lower Upper
113 100
111 102.5 82.7 124.1
192 18.6 15.6 23.4

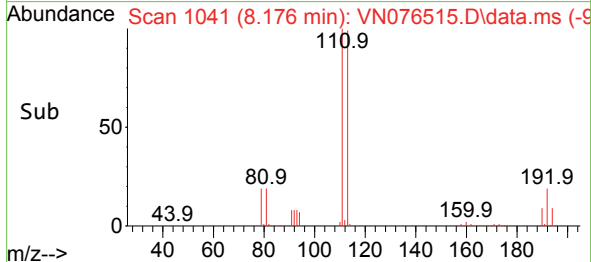

#36
1,1-Dichloropropene
Concen: 5.075 ug/l
RT: 8.229 min Scan# 1050
Delta R.T. -0.148 min
Lab File: VN076515.D
Acq: 02 Feb 2023 17:15

Tgt Ion: 75 Resp: 44454
Ion Ratio Lower Upper
75 100
110 9.8 18.8 56.3#
77 0.0 25.0 37.4#


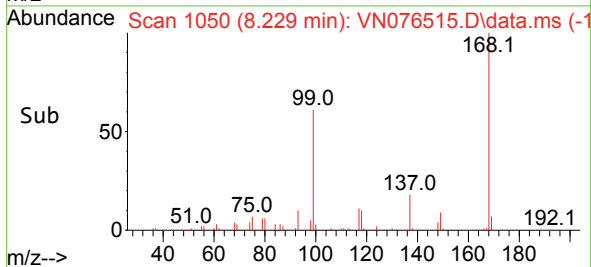

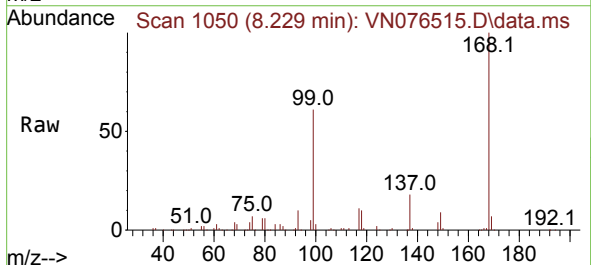




#37
Ethyl Acetate
Concen: 7.485 ug/l
RT: 7.571 min Scan# 91
Delta R.T. 0.006 min
Lab File: VN076515.D
Acq: 02 Feb 2023 17:15




Instrument :
MSVOA_N
ClientSampleId :
PB150614ZHE#1


Tgt Ion:	43	Resp:	52371
Ion	Ratio	Lower	Upper
43	100		
61	13.9	11.1	16.7
70	12.8	10.0	15.0



#38
Carbon Tetrachloride
Concen: 6.560 ug/l
RT: 8.229 min Scan# 1050
Delta R.T. -0.136 min
Lab File: VN076515.D
Acq: 02 Feb 2023 17:15

Tgt Ion:	117	Resp:	64083
Ion	Ratio	Lower	Upper
117	100		
119	5.1	75.4	113.0#
121	0.0	24.2	36.2#





#42

1,2-Dichloroethane

Concen: 0.223 ug/l

RT: 8.694 min Scan# 1129

Delta R.T. 0.017 min

Lab File: VN076515.D

Acq: 02 Feb 2023 17:15

Instrument :

MSVOA_N

ClientSampleId :





PB150614ZHE#1

Tgt Ion: 62 Resp: 1997

Ion Ratio Lower Upper

62 100

98 0.0 0.0 20.4

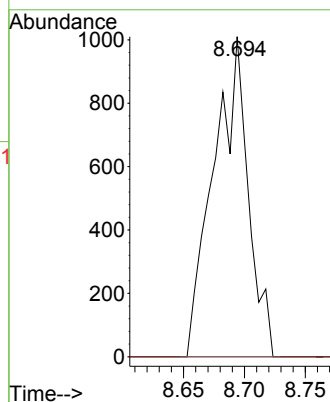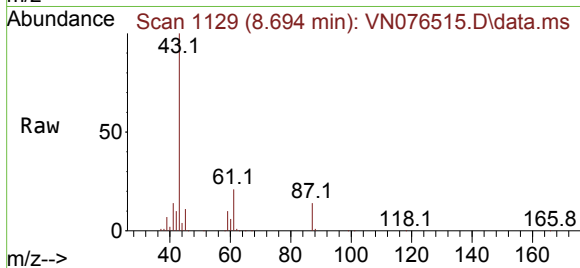

#43

Isopropyl Acetate

Concen: 33.052 ug/l

RT: 8.694 min Scan# 1129

Delta R.T. 0.000 min

Lab File: VN076515.D

Acq: 02 Feb 2023 17:15




Tgt Ion: 43 Resp: 377771


Ion Ratio Lower Upper

43 100

61 15.6 23.5 35.3#

87 11.1 13.8 20.6#

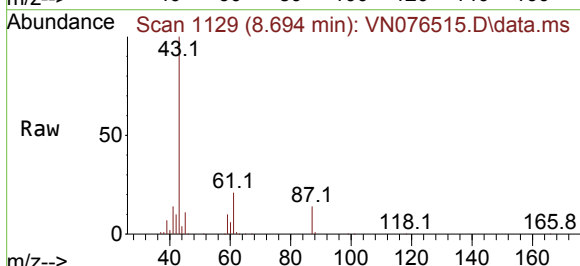



#45

1,2-Dichloropropane

Concen: 0.527 ug/l

RT: 9.747 min Scan# 1308

Delta R.T. 0.123 min

Lab File: VN076515.D

Acq: 02 Feb 2023 17:15

Instrument :

MSVOA_N

ClientSampleId :





PB150614ZHE#1

Tgt Ion: 63 Resp: 3302

Ion Ratio Lower Upper

63 100

65 0.0 26.4 39.6#

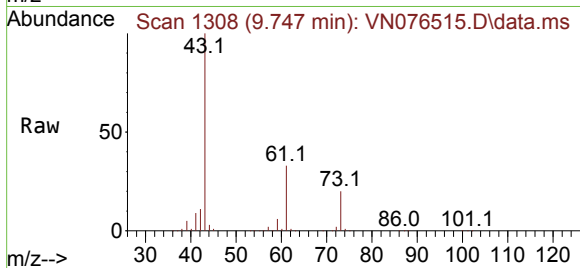

#48

Methyl methacrylate

Concen: 40.999 ug/l

RT: 9.747 min Scan# 1308

Delta R.T. 0.065 min

Lab File: VN076515.D

Acq: 02 Feb 2023 17:15




Tgt Ion: 41 Resp: 221845


Ion Ratio Lower Upper

41 100

69 0.1 80.8 121.2#

39 53.2 54.4 81.6#

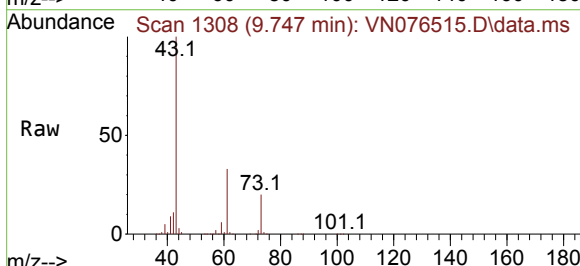



#49

1,4-Dioxane

Concen: 3.328 ug/l

RT: 9.747 min Scan# 1308

Delta R.T. 0.047 min

Lab File: VN076515.D

Acq: 02 Feb 2023 17:15

Instrument :

MSVOA_N

ClientSampleId :

PB150614ZHE#1





Tgt Ion: 88 Resp: 380

Ion Ratio Lower Upper

88 100

43 609395.8 18.1 27.1#

58 2861.3 46.5 69.7#

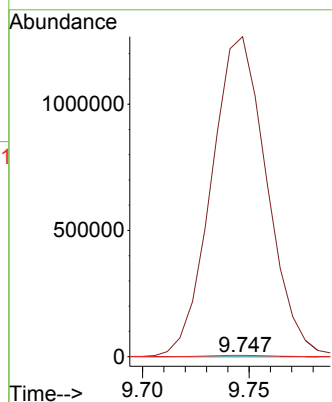

#50

Toluene-d8

Concen: 51.645 ug/l

RT: 10.570 min Scan# 1448

Delta R.T. -0.001 min

Lab File: VN076515.D




Acq: 02 Feb 2023 17:15


Tgt Ion: 98 Resp: 1175748

Ion Ratio Lower Upper

98 100

100 64.7 52.2 78.4







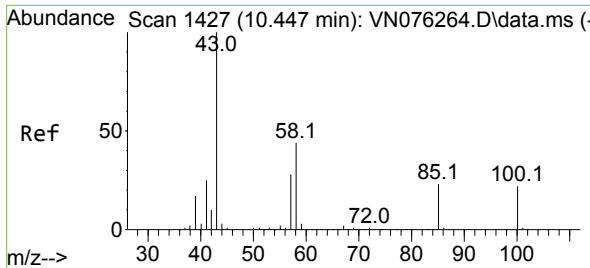

#51
4-Methyl-2-Pentanone
Concen: 1.804 ug/l
RT: 10.447 min Scan# 1427
Delta R.T. -0.000 min
Lab File: VN076515.D
Acq: 02 Feb 2023 17:15




Instrument :
MSVOA_N
ClientSampleId :
PB150614ZHE#1


Tgt Ion: 43 Resp: 12106
Ion Ratio Lower Upper
43 100
58 47.6 35.1 52.7

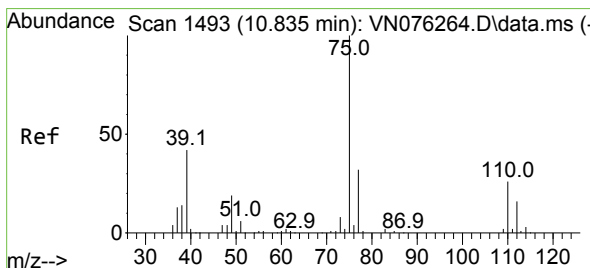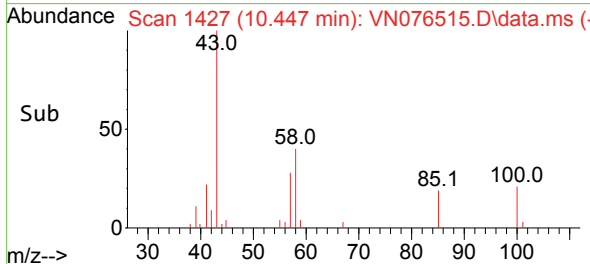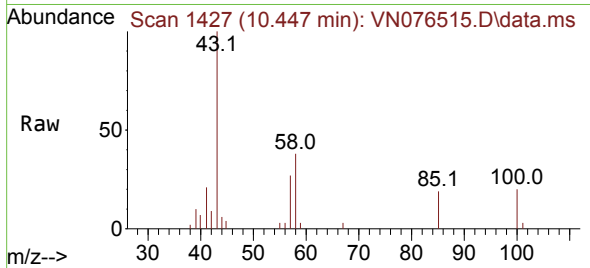

#53
t-1,3-Dichloropropene
Concen: 0.257 ug/l
RT: 10.729 min Scan# 1475
Delta R.T. -0.106 min
Lab File: VN076515.D
Acq: 02 Feb 2023 17:15

Tgt Ion: 75 Resp: 2246
Ion Ratio Lower Upper
75 100
77 18.8 25.8 38.6#


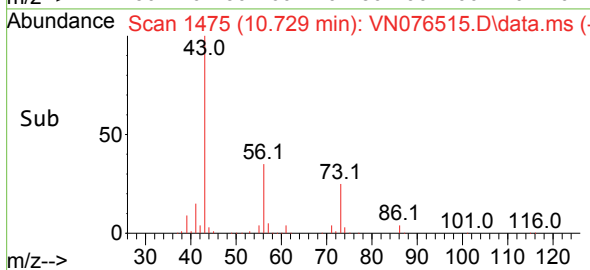

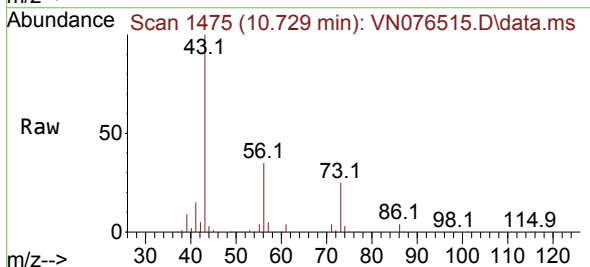


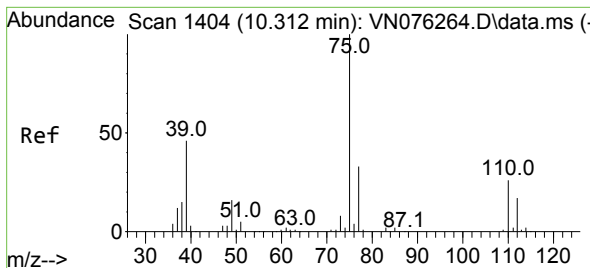

#54
cis-1,3-Dichloropropene
Concen: 11.548 ug/l
RT: 10.359 min Scan# 1412
Delta R.T. 0.047 min
Lab File: VN076515.D
Acq: 02 Feb 2023 17:15




Instrument :
MSVOA_N
ClientSampleId :
PB150614ZHE#1


Tgt Ion: 75 Resp: 116305
Ion Ratio Lower Upper
75 100
77 0.3 26.5 39.7#
39 27.4 37.1 55.7#

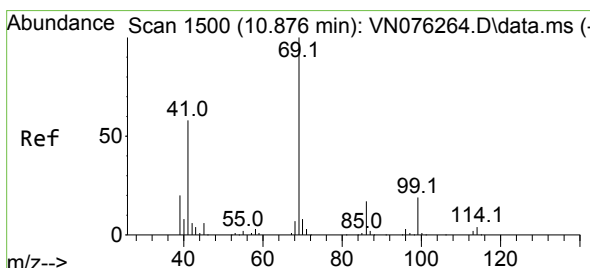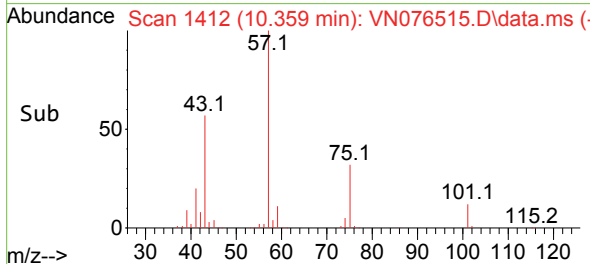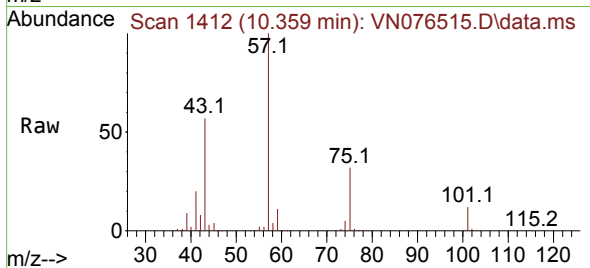

#56
Ethyl methacrylate
Concen: 0.362 ug/l
RT: 10.988 min Scan# 1519
Delta R.T. 0.112 min
Lab File: VN076515.D
Acq: 02 Feb 2023 17:15

Tgt Ion: 69 Resp: 3132
Ion Ratio Lower Upper
69 100
41 4997.8 45.3 67.9#
39 2102.7 29.3 43.9#

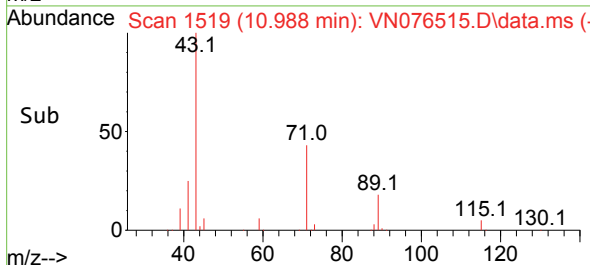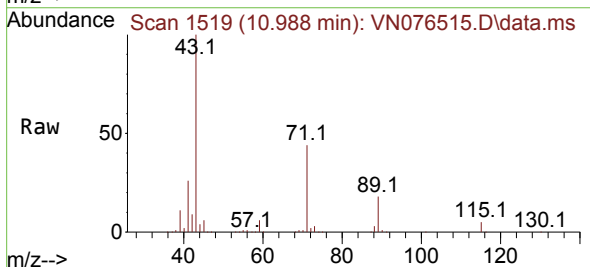



#57

1,3-Dichloropropane

Concen: 1.331 ug/l

RT: 11.206 min Scan# 1556

Delta R.T. 0.041 min

Lab File: VN076515.D

Acq: 02 Feb 2023 17:15

Instrument :

MSVOA_N

ClientSampleId :





PB150614ZHE#1

Tgt Ion: 76 Resp: 14477

Ion Ratio Lower Upper

76 100

78 0.0 26.4 39.6#

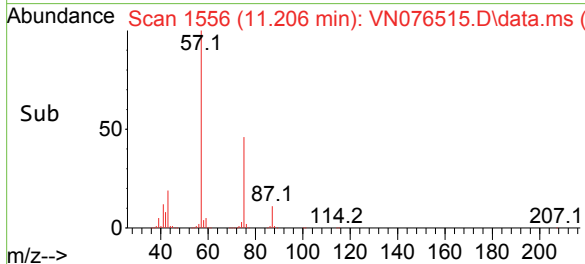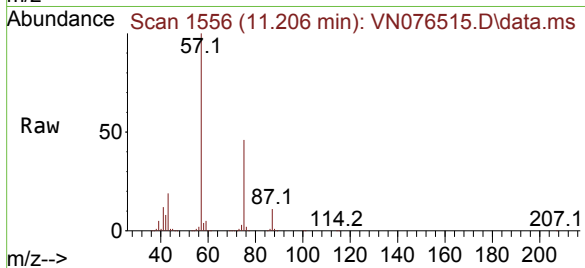

#59

2-Hexanone

Concen: 47.801 ug/l

RT: 11.176 min Scan# 1551

Delta R.T. -0.018 min

Lab File: VN076515.D




Acq: 02 Feb 2023 17:15


Tgt Ion: 43 Resp: 232419

Ion Ratio Lower Upper

43 100

58 0.0 30.1 90.3#




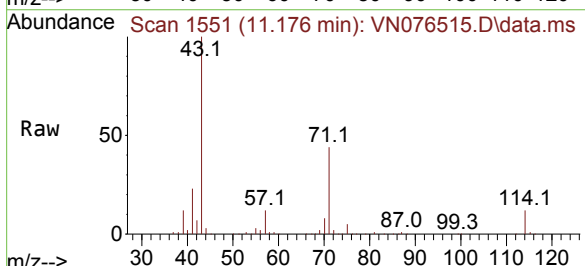




#62
4-Bromofluorobenzene
Concen: 58.829 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. 0.006 min
Lab File: VN076515.D
Acq: 02 Feb 2023 17:15




Instrument :
MSVOA_N
ClientSampleId :
PB150614ZHE#1


Tgt Ion: 95 Resp: 437216
Ion Ratio Lower Upper
95 100
174 77.3 0.0 174.6
176 73.9 0.0 167.8

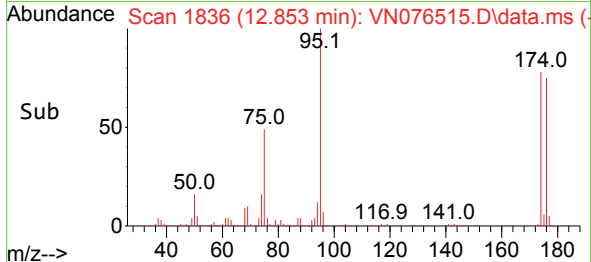

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.870 min Scan# 1669
Delta R.T. 0.005 min
Lab File: VN076515.D
Acq: 02 Feb 2023 17:15

Tgt Ion: 117 Resp: 901091
Ion Ratio Lower Upper
117 100
82 54.8 42.2 63.2
119 31.8 26.9 40.3


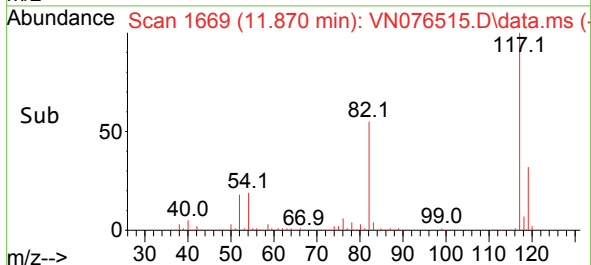
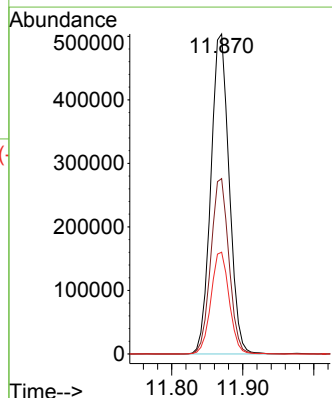
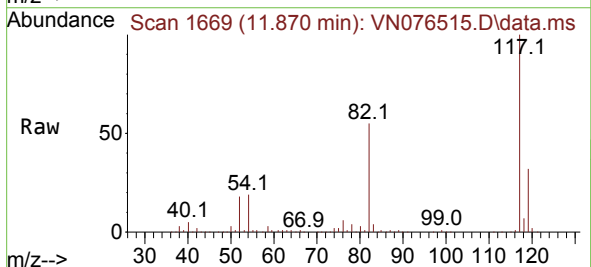




#71
Bromoform
Concen: 0.381 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. 0.271 min
Lab File: VN076515.D
Acq: 02 Feb 2023 17:15




Instrument :
MSVOA_N
ClientSampleId :
PB150614ZHE#1


Tgt Ion:173 Resp: 1949
Ion Ratio Lower Upper
173 100
175 992.3 24.1 72.4#
254 0.0 0.0 0.0



#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 1996
Delta R.T. -0.000 min
Lab File: VN076515.D
Acq: 02 Feb 2023 17:15

Tgt Ion:152 Resp: 433683
Ion Ratio Lower Upper
152 100
115 60.1 29.6 88.9
150 154.6 0.0 351.4




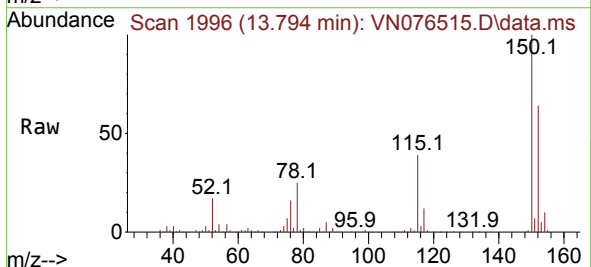




#74
N-amy1 acetate
Concen: 0.294 ug/l
RT: 12.488 min Scan# 1774
Delta R.T. -0.006 min
Lab File: VN076515.D
Acq: 02 Feb 2023 17:15




Instrument :
MSVOA_N
ClientSampleId :
PB150614ZHE#1


Tgt Ion: 43	Resp:	2841
Ion Ratio	Lower	Upper
43	100	
70	0.0	41.2
55	6.9	21.0
61	0.0	21.6



#76
1,2,3-Trichloropropane
Concen: 26.559 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. -0.141 min
Lab File: VN076515.D
Acq: 02 Feb 2023 17:15

Tgt Ion: 75	Resp:	213340
Ion Ratio	Lower	Upper
75	100	
77	1.3	75.2

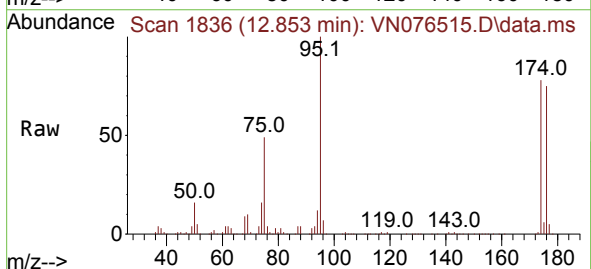



#77

Bromobenzene

Concen: Below Cal

RT: 12.982 min Scan# 1858

Delta R.T. -0.000 min

Lab File: VN076515.D

Acq: 02 Feb 2023 17:15





Instrument :

MSVOA_N

ClientSampleId :

PB150614ZHE#1

Tgt Ion:	156	Resp:	58
Ion Ratio	Lower	Upper	
156	100		
77	0.0	93.4	280.2#
158	0.0	48.4	145.2#

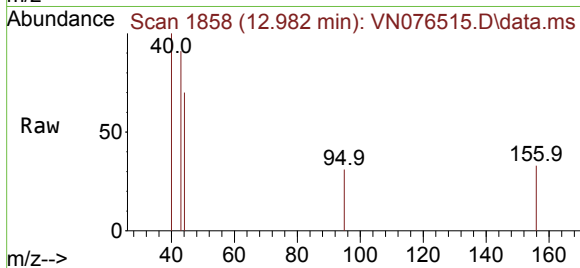

#81

trans-1,4-Dichloro-2-butene

Concen: 81.848 ug/l




RT: 12.853 min Scan# 1836


Delta R.T. 0.118 min

Lab File: VN076515.D

Acq: 02 Feb 2023 17:15

Tgt Ion:	75	Resp:	213340
Ion Ratio	Lower	Upper	
75	100		
53	0.0	75.8	113.8#
89	0.0	37.0	55.6#

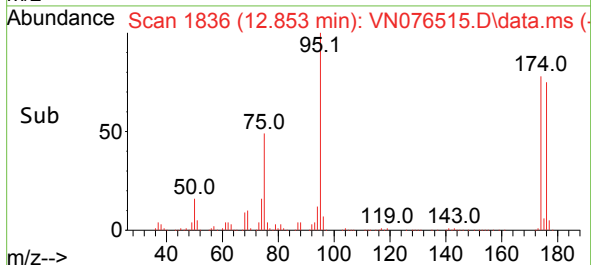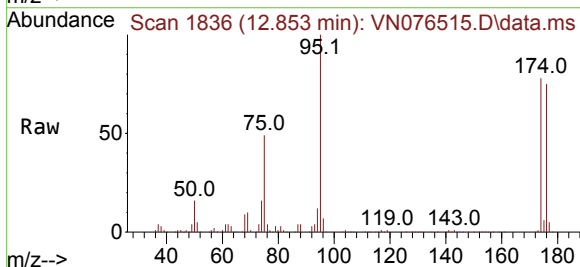



#93

1,2,4-Trichlorobenzene

Concen: 1.338 ug/l

RT: 15.394 min Scan# 21

Delta R.T. -0.000 min

Lab File: VN076515.D


Acq: 02 Feb 2023 17:15

Instrument :

MSVOA_N

ClientSampleId :

PB150614ZHE#1






Tgt Ion:180 Resp: 255

Ion Ratio Lower Upper

180 100

182 99.2 47.0 141.2

145 0.0 15.2 45.5#

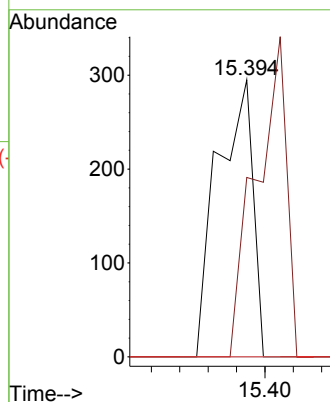

#95

Naphthalene

Concen: 1.904 ug/l

RT: 15.647 min Scan# 2311

Delta R.T. 0.006 min

Lab File: VN076515.D

Acq: 02 Feb 2023 17:15




Tgt Ion:128 Resp: 1519


Ion Ratio Lower Upper

128 100

127 12.5 10.3 15.5


129 11.1 8.6 13.0

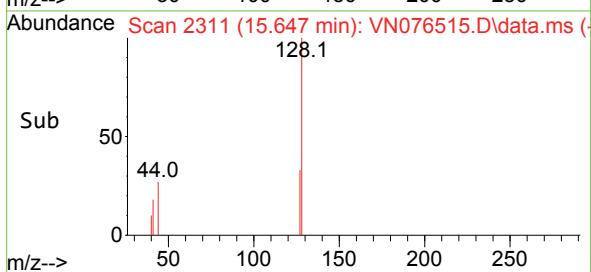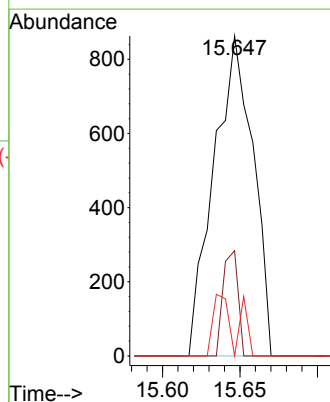



#96
 1,2,3-Trichlorobenzene
 Concen: 1.179 ug/l
 RT: 15.841 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: VN076515.D
 Acq: 02 Feb 2023 17:15

Instrument :
 MSVOA_N
 ClientSampleId :
 PB150614ZHE#1



Tgt Ion:180 Resp: 183
 Ion Ratio Lower Upper
 180 100
 182 0.0 47.5 142.5#
 145 0.0 15.9 47.6#

