


BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN020223\
Data File : VN076501.D
Acq On : 02 Feb 2023 10:05
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011623W.M
Title : SW846 8260
Last Update : Tue Jan 17 03:59:22 2023

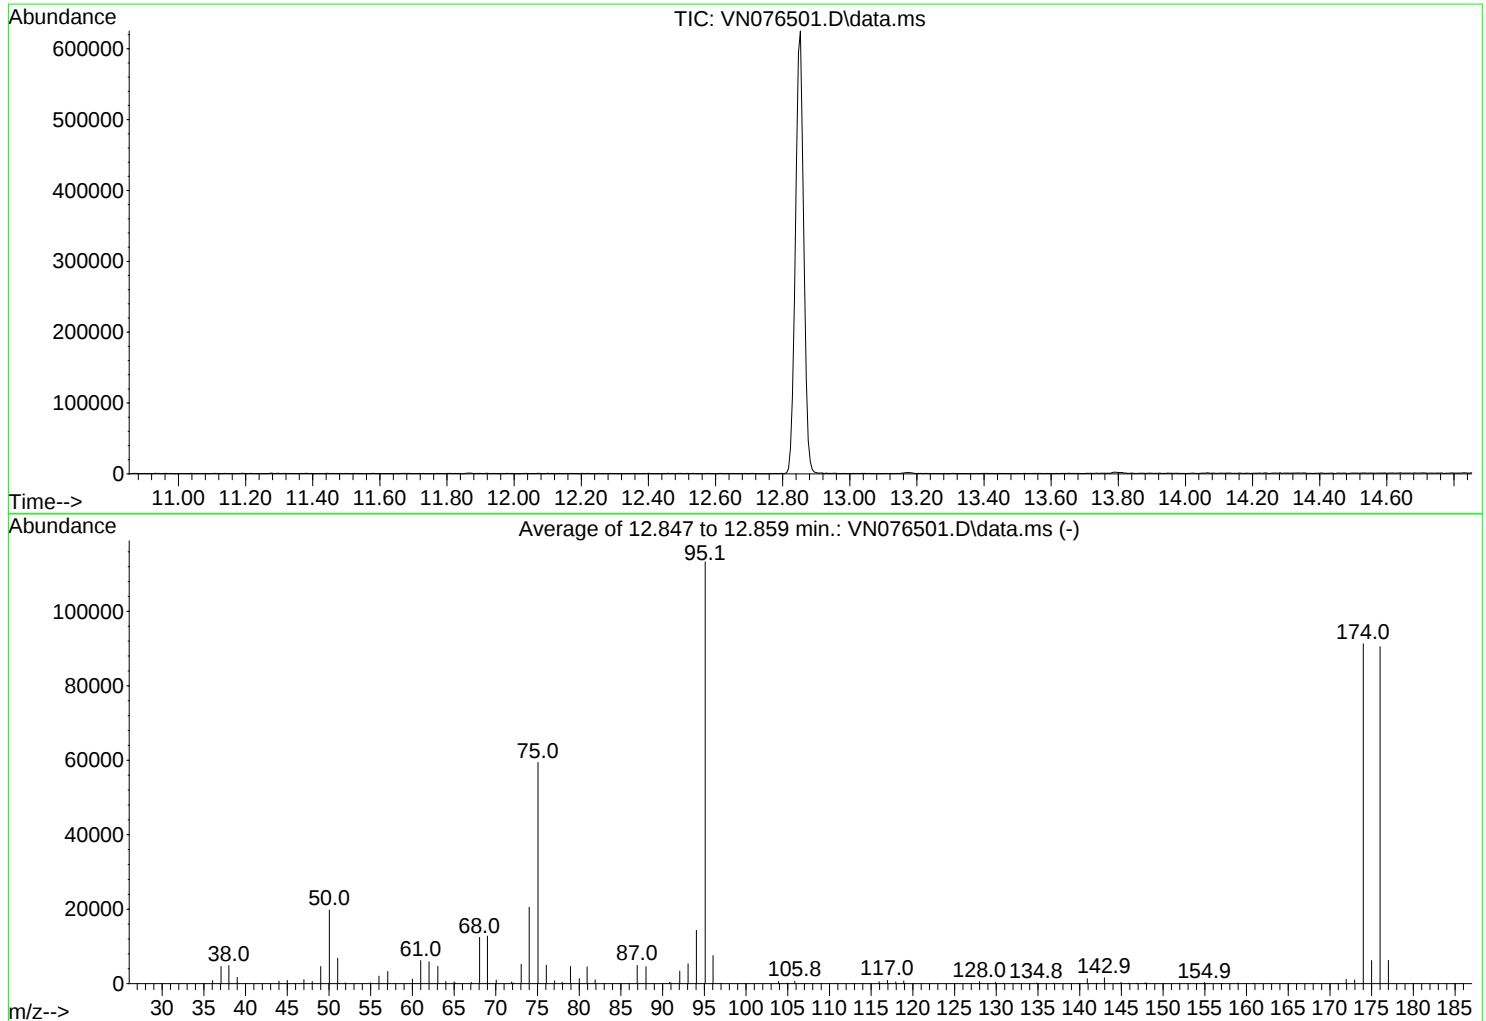

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1826

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.5	19776	PASS
75	95	30	60	52.5	59429	PASS
95	95	100	100	100.0	113301	PASS
96	95	5	9	6.6	7532	PASS
173	174	0.00	2	1.1	996	PASS
174	95	50	100	80.6	91277	PASS
175	174	5	9	6.8	6189	PASS
176	174	95	101	99.2	90528	PASS
177	176	5	9	6.9	6244	PASS

Average of 12.847 to 12.859 min.: VN076501.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	834	51.05	6826	65.00	479	76.05	496
37.05	4610	51.95	221	65.20	160	77.05	73
38.00	4846	54.95	245	67.10	289	77.95	37
39.00	1705	56.00	2041	68.05	12407	78.20	10
44.00	709	57.05	3274	69.00	12752	78.95	4583
45.00	872	57.80	58	70.05	954	80.00	1342
46.00	50	60.00	1203	71.90	453	80.95	4528
47.00	1079	61.00	6176	72.10	212	81.90	1038
48.00	560	62.00	5908	73.05	5187	82.90	92
49.00	4602	63.05	4641	74.00	20525	86.00	58
50.05	19776	64.00	602	75.05	59429	86.95	4915

Average of 12.847 to 12.859 min.: VN076501.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
88.00	4548	103.90	623	129.00	81	145.85	134
88.80	58	104.90	115	129.90	389	146.80	116
90.80	327	105.85	638	130.85	132	147.80	138
91.00	224	107.00	54	134.80	230	147.95	266
92.05	3346	110.70	73	135.00	89	154.95	339
93.05	5337	112.90	84	136.90	192	156.80	67
94.05	14318	115.95	527	140.00	53	157.10	55
95.10	113301	116.95	860	140.90	1325	158.95	190
96.05	7532	117.95	473	142.05	117	160.85	134
96.90	89	118.90	752	142.95	1591	170.70	62
97.10	105	128.00	511	144.95	327	171.00	59

Average of 12.847 to 12.859 min.: VN076501.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
171.95	1166						
172.95	996						
174.00	91277						
175.00	6189						
176.00	90528						
177.00	6244						

Instrument :

MSVOA_N

ClientSampleId :

BFB