
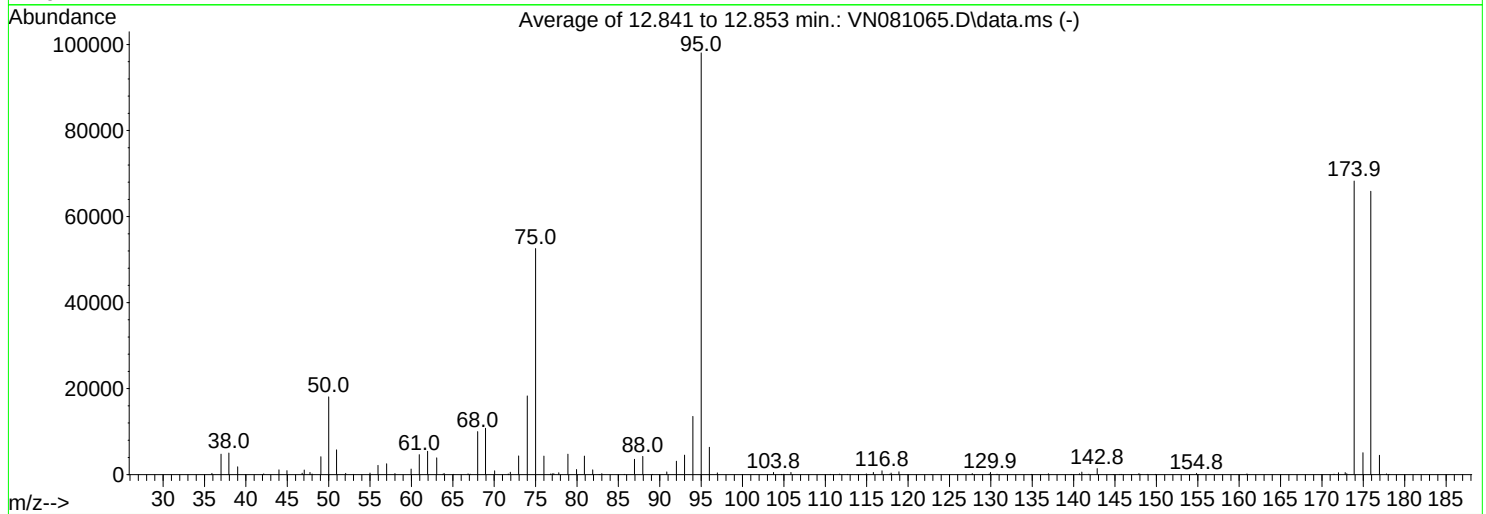


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN021924\
Data File : VN081065.D
Acq On : 19 Feb 2024 08:27
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021624W.M
Title : SW846 8260
Last Update : Fri Feb 16 23:45:20 2024

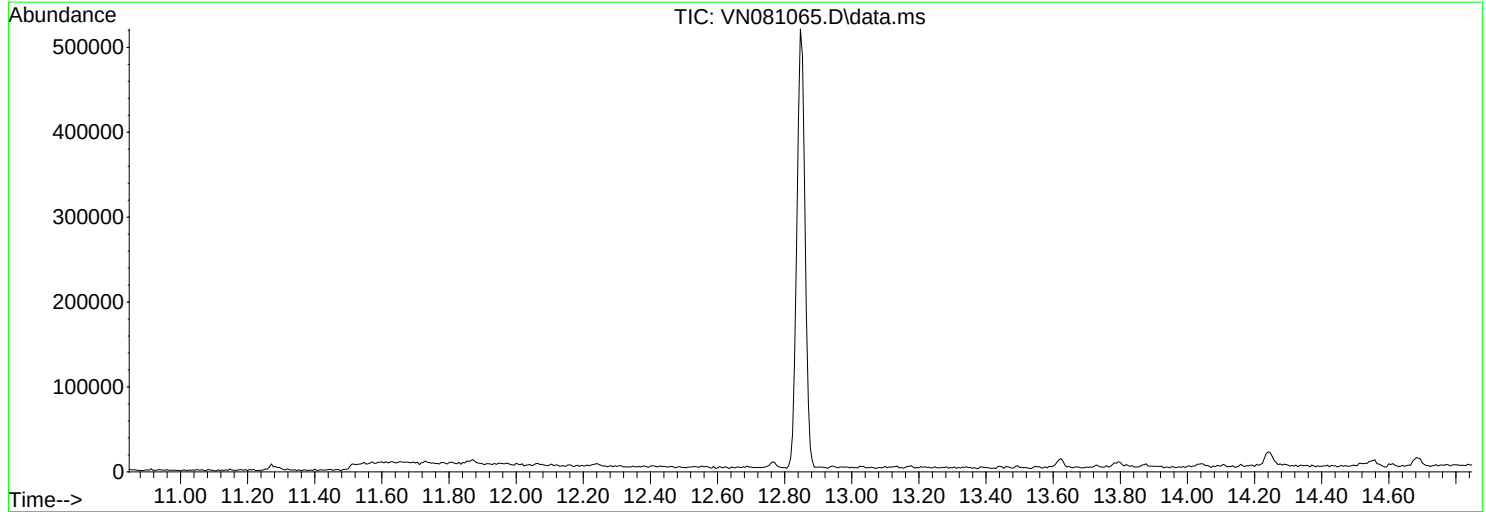

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1841

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.4	18086	PASS
75	95	30	60	53.6	52555	PASS
95	95	100	100	100.0	98067	PASS
96	95	5	9	6.5	6350	PASS
173	174	0.00	2	0.7	483	PASS
174	95	50	100	69.6	68253	PASS
175	174	5	9	7.5	5115	PASS
176	174	95	101	96.5	65891	PASS
177	176	5	9	6.9	4514	PASS

Average of 12.841 to 12.853 min.: VN081065.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	315	48.00	143	60.95	4652	71.70	15
37.00	4783	49.05	4165	61.95	5451	71.95	55
37.95	5029	50.00	18086	63.05	3912	72.95	436
39.00	1822	50.95	5761	63.80	110	74.00	1830
39.95	31	52.05	316	63.95	315	75.00	52555
42.15	191	53.00	62	65.10	86	76.00	4312
44.00	1104	55.00	367	66.85	195	76.80	155
44.95	918	55.95	2153	67.10	110	77.00	216
46.80	347	57.00	2518	68.00	10002	77.20	208
47.05	1099	58.00	245	68.95	10799	77.80	449
47.75	504	59.95	1310	70.05	915	78.90	4770

Average of 12.841 to 12.853 min.: VN081065.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
79.95	1192	93.00	4552	112.70	63	130.75	125
80.90	4307	94.00	13556	114.95	177	134.90	68
81.90	1118	95.00	98067	115.80	522	136.95	218
82.70	56	96.00	6350	116.85	911	139.70	83
83.00	211	96.95	392	117.80	125	140.70	233
85.70	65	103.75	513	117.95	368	141.00	612
86.95	3564	104.70	66	118.90	688	141.85	122
87.95	4239	105.00	115	122.80	51	142.85	1434
89.10	76	105.85	508	127.75	274	144.80	56
90.85	648	110.60	63	129.80	168	145.60	78
92.00	3146	111.75	142	129.95	508	145.80	67

Average of 12.841 to 12.853 min.: VN081065.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
147.90	256	174.95	5115				
148.10	80	175.90	65891				
148.90	64	176.95	4514				
149.90	89	177.80	174				
154.85	294	178.10	61				
160.95	201						
171.45	123						
172.00	436						
172.80	483						
173.00	243						
173.90	68253						

Instrument :

MSVOA_N

ClientSampleId :

BFB