


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032224\
Data File : VN081534.D
Acq On : 22 Mar 2024 08:39
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031824W.M
Title : SW846 8260
Last Update : Tue Mar 19 06:00:00 2024

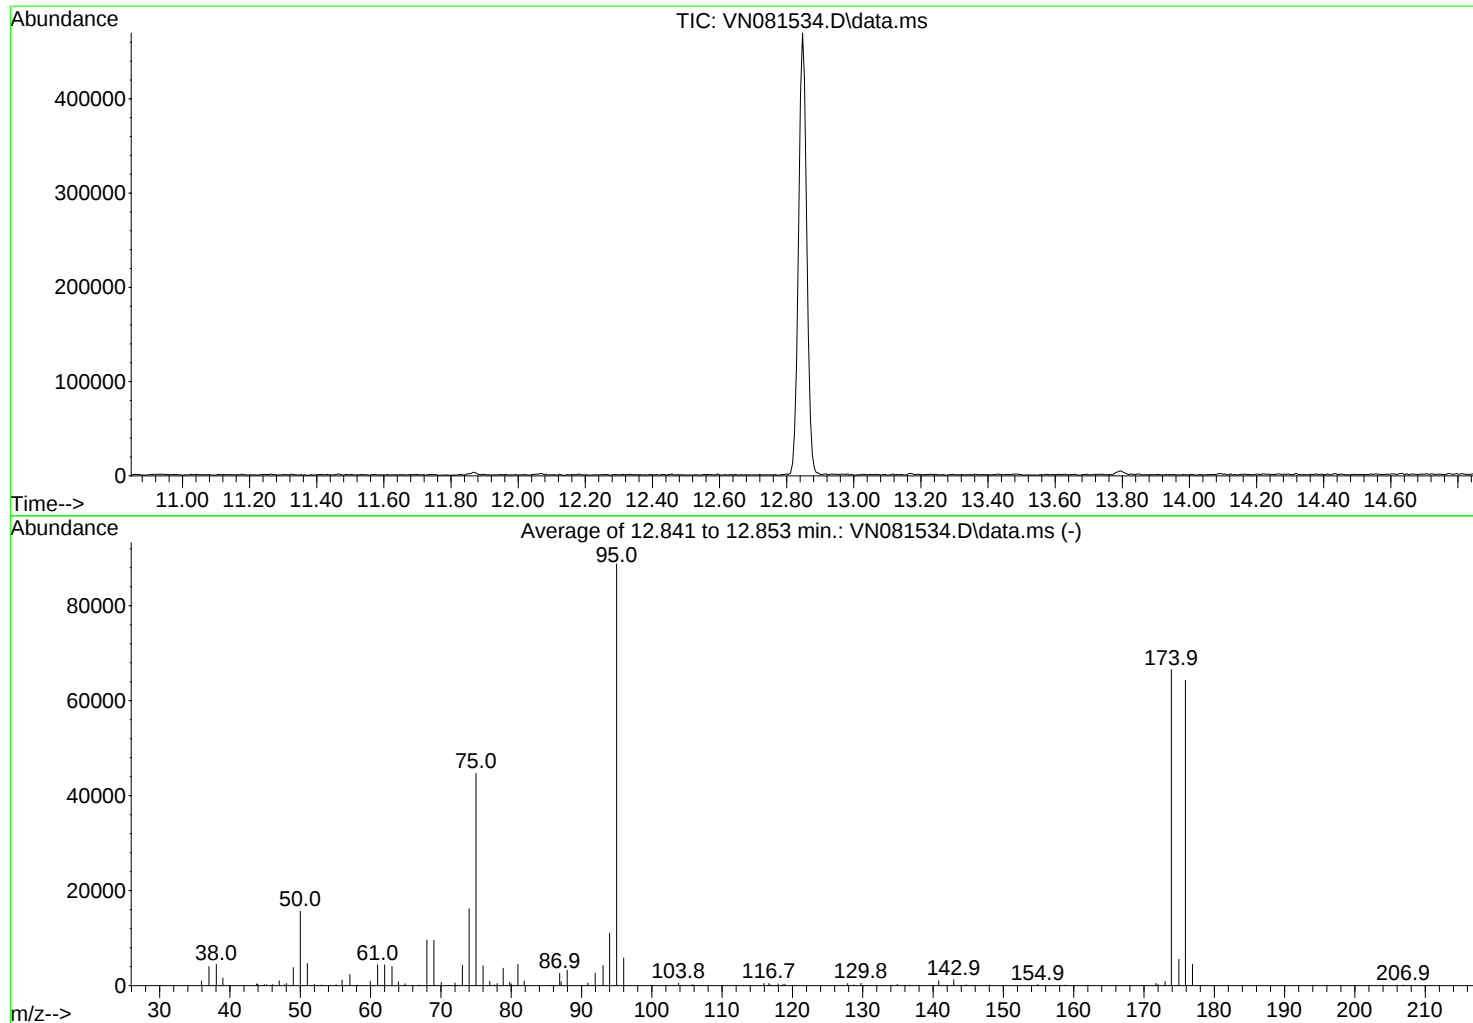

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.6	15671	PASS
75	95	30	60	50.4	44739	PASS
95	95	100	100	100.0	88827	PASS
96	95	5	9	6.6	5827	PASS
173	174	0.00	2	1.3	880	PASS
174	95	50	100	74.9	66565	PASS
175	174	5	9	8.3	5520	PASS
176	174	95	101	96.6	64288	PASS
177	176	5	9	7.0	4486	PASS

Average of 12.841 to 12.853 min.: VN081534.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	937	47.00	1027	58.10	98	71.10	71
37.00	4021	47.80	169	59.95	908	72.00	54
38.05	4466	48.05	455	61.00	4385	73.05	431
39.00	1612	49.00	3817	62.00	4347	74.00	1621
39.85	2	50.00	15671	63.05	4039	75.00	44739
43.80	366	51.00	4642	63.95	806	76.00	4223
43.95	296	52.00	291	64.90	394	76.95	925
44.70	82	53.00	144	66.90	154	77.60	148
44.90	215	55.10	199	68.00	9590	78.00	448
45.20	220	55.95	1171	69.00	9549	78.85	3685
46.10	246	57.05	2350	70.05	693	79.80	728

Average of 12.841 to 12.853 min.: VN081534.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
80.00	359	95.00	88827	116.90	123	142.95	1264
80.95	4531	96.00	5827	117.95	365	144.00	65
81.85	990	96.90	56	118.65	241	144.70	171
85.60	79	103.80	556	118.95	344	145.60	56
86.90	2609	104.80	63	127.85	447	147.60	55
87.10	801	105.60	142	128.75	160	148.05	169
87.95	3232	105.85	200	129.75	473	149.90	57
90.90	591	106.80	60	130.90	81	154.90	224
91.95	2629	113.00	62	134.90	274	158.80	134
93.05	4261	115.95	479	136.70	124	170.60	64
94.00	11059	116.65	489	140.80	1060	171.70	458

Average of 12.841 to 12.853 min.: VN081534.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
172.00	254						
173.00	880						
173.90	66565						
174.95	5520						
175.90	64288						
176.90	4486						
178.00	50						
206.90	146						

Instrument :

MSVOA_N

ClientSampleId :

BFB