

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032323\
 Data File : VN077158.D
 Acq On : 23 Mar 2023 18:43
 Operator : JC\MD
 Sample : 02048-03
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 MW-6

Quant Time: Mar 24 01:36:37 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031723W.M
 Quant Title : SW846 8260
 QLast Update : Mon Mar 20 08:50:30 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.231	168	360975	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.107	114	648146	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.871	117	559164	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.795	152	206769	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.589	65	280365	48.624	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	97.240%
35) Dibromofluoromethane	8.178	113	214469	47.250	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	94.500%
50) Toluene-d8	10.572	98	788877	48.654	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	97.300%
62) 4-Bromofluorobenzene	12.854	95	223003	38.922	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	77.840%#
Target Compounds						
19) Methyl tert-butyl Ether	5.807	73	165166	10.501	ug/l	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032323\
Data File : VN077158.D
Acq On : 23 Mar 2023 18:43
Operator : JC\MD
Sample : 02048-03
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-6

Quant Time: Mar 24 01:36:37 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031723W.M
Quant Title : SW846 8260
QLast Update : Mon Mar 20 08:50:30 2023
Response via : Initial Calibration




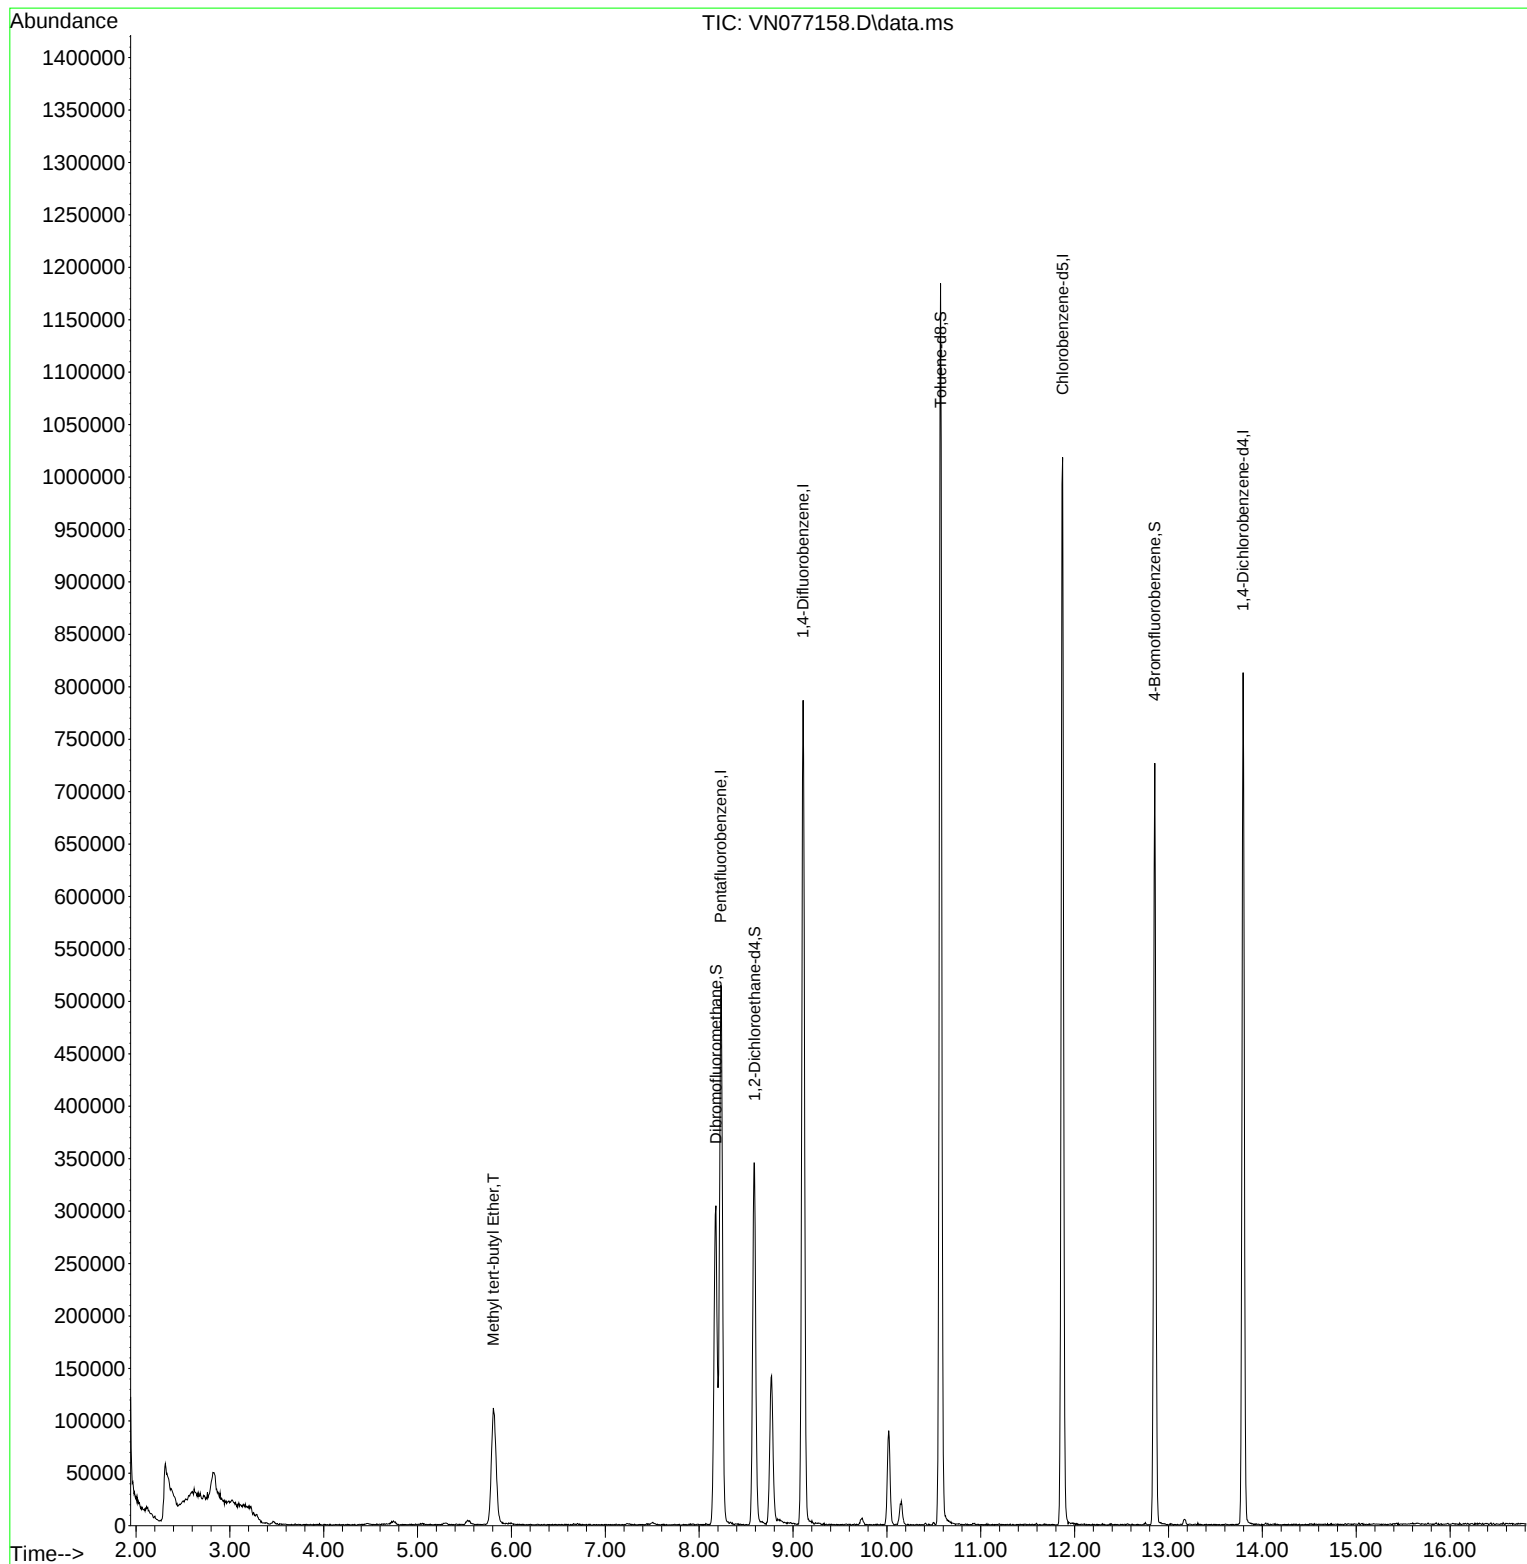


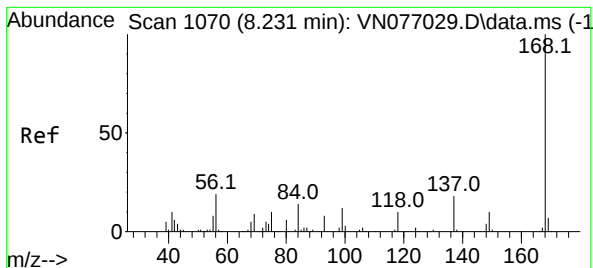

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.231 min Scan# 1070
Delta R.T. -0.000 min
Lab File: VN077158.D
Acq: 23 Mar 2023 18:43




Instrument :
MSVOA_N
ClientSampleId :
MW-6


Tgt Ion:168 Resp: 360975
Ion Ratio Lower Upper
168 100
99 62.6 53.9 80.9

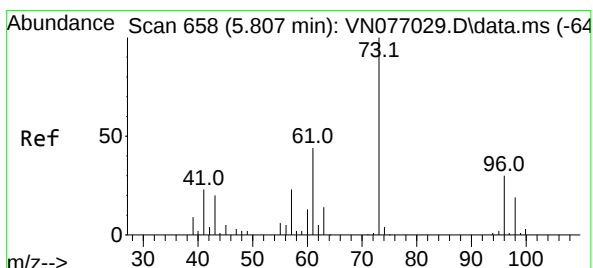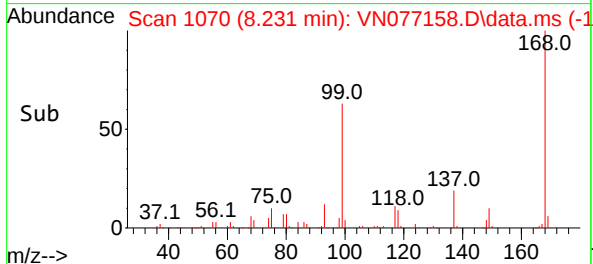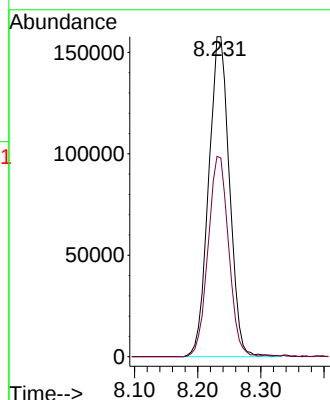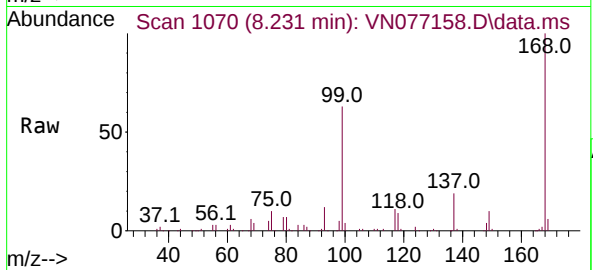

#19
Methyl tert-butyl Ether
Concen: 10.501 ug/l
RT: 5.807 min Scan# 658
Delta R.T. 0.000 min
Lab File: VN077158.D
Acq: 23 Mar 2023 18:43

Tgt Ion: 73 Resp: 165166
Ion Ratio Lower Upper
73 100
57 22.8 18.7 28.1

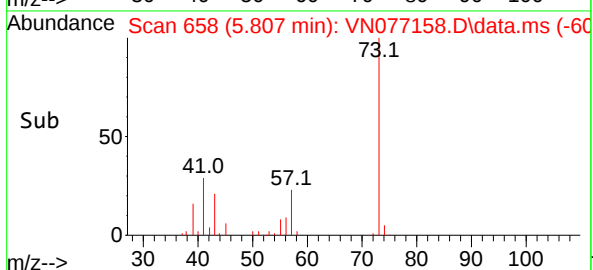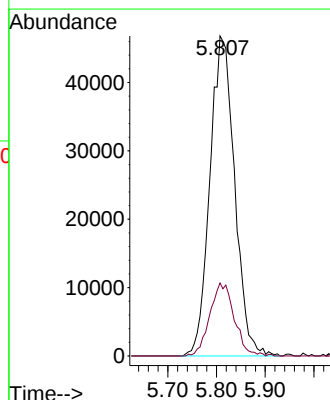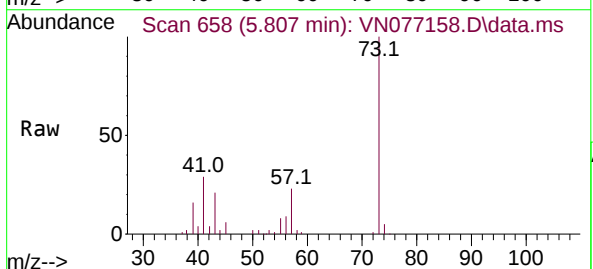

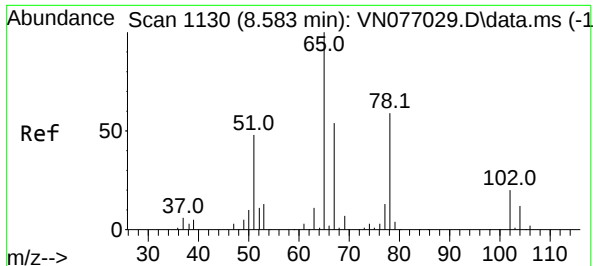

#33

1,2-Dichloroethane-d4

Concen: 48.624 ug/l

RT: 8.589 min Scan# 1130

Delta R.T. 0.006 min

Lab File: VN077158.D

Acq: 23 Mar 2023 18:43

Instrument :

MSVOA_N

ClientSampleId :





MW-6

Tgt Ion: 65 Resp: 280365

Ion Ratio Lower Upper

65 100

67 50.5 0.0 105.2

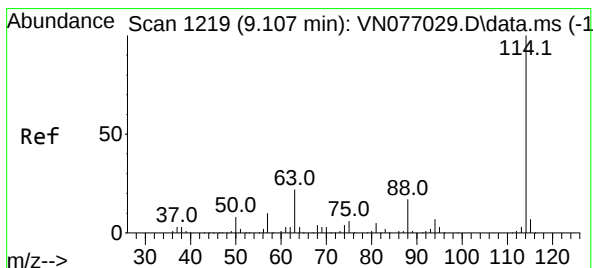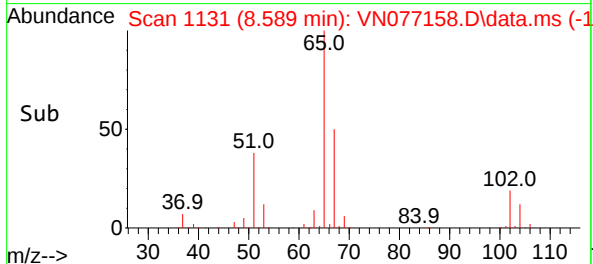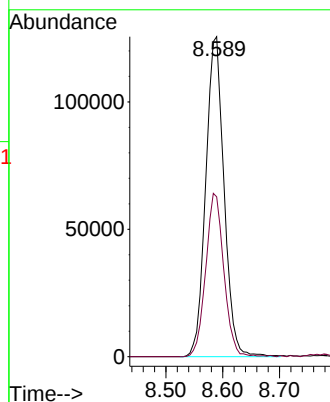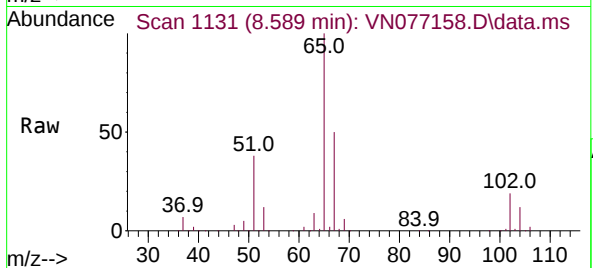

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.107 min Scan# 1219

Delta R.T. -0.000 min

Lab File: VN077158.D

Acq: 23 Mar 2023 18:43




Tgt Ion: 114 Resp: 648146


Ion Ratio Lower Upper

114 100

63 22.0 0.0 44.6

88 15.6 0.0 33.8

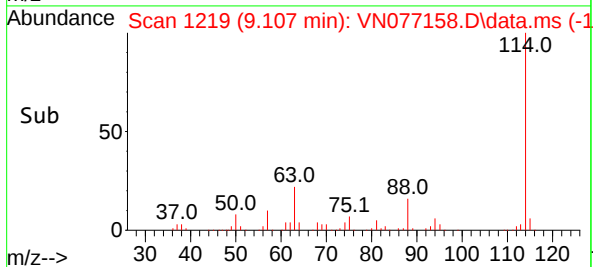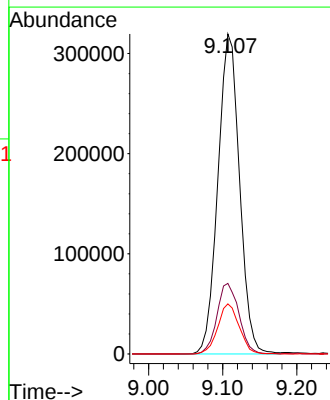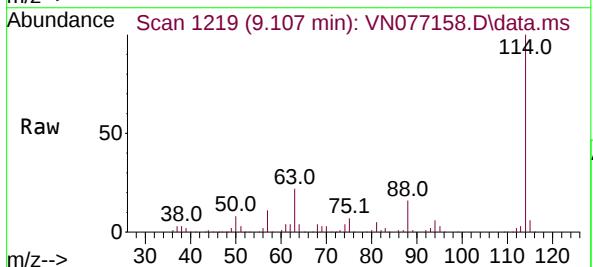

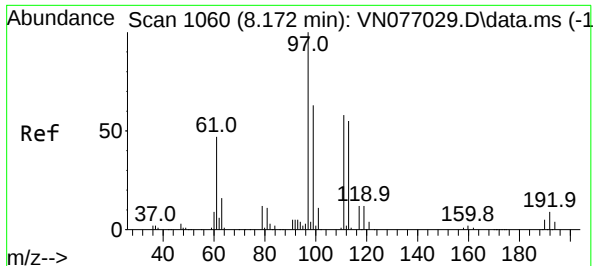

#35

Dibromofluoromethane

Concen: 47.250 ug/l

RT: 8.178 min Scan# 1060

Delta R.T. 0.006 min

Lab File: VN077158.D

Acq: 23 Mar 2023 18:43

Instrument :

MSVOA_N

ClientSampleId :

MW-6





Tgt Ion:113 Resp: 214469

Ion Ratio Lower Upper

113 100

111 102.3 82.2 123.2

192 18.1 13.0 19.6

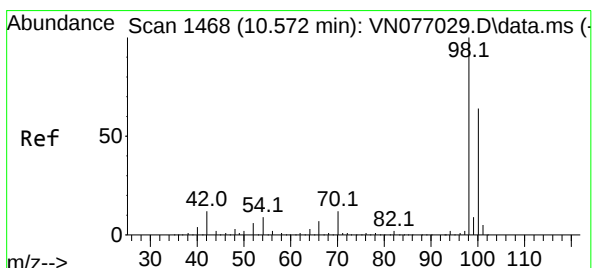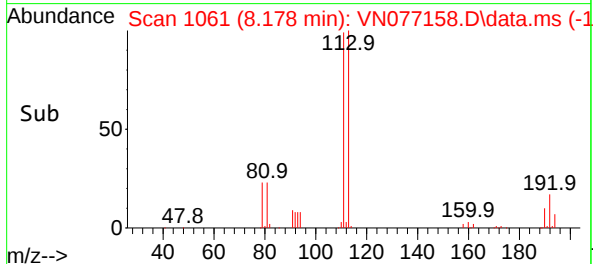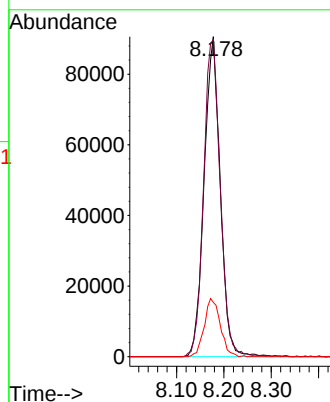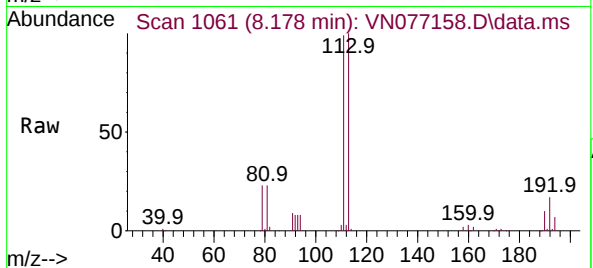

#50

Toluene-d8

Concen: 48.654 ug/l

RT: 10.572 min Scan# 1468

Delta R.T. -0.000 min

Lab File: VN077158.D




Acq: 23 Mar 2023 18:43


Tgt Ion: 98 Resp: 788877

Ion Ratio Lower Upper

98 100

100 63.7 51.6 77.4


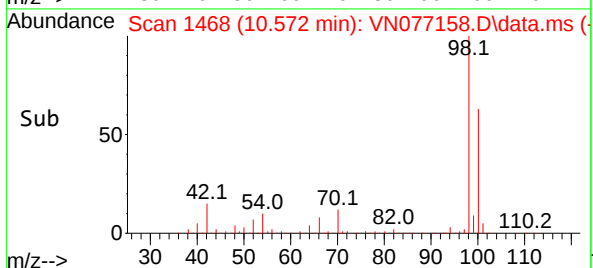
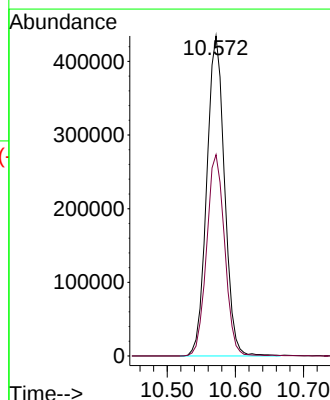
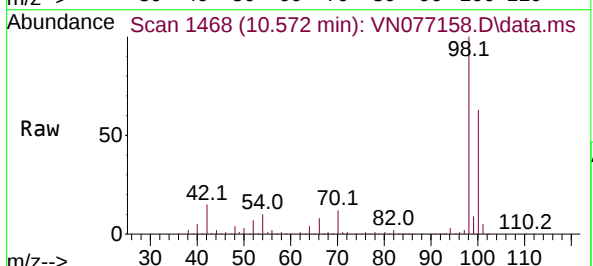


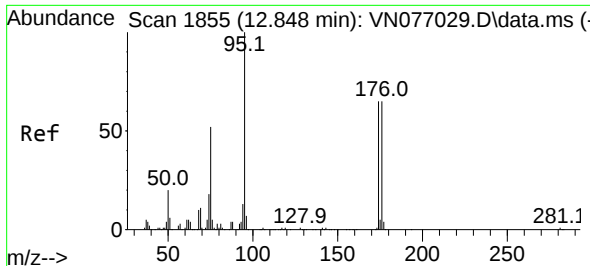

#62
4-Bromofluorobenzene
Concen: 38.922 ug/l
RT: 12.854 min Scan# 1856
Delta R.T. 0.006 min
Lab File: VN077158.D
Acq: 23 Mar 2023 18:43




Instrument :
MSVOA_N
ClientSampleId :
MW-6


Tgt Ion: 95 Resp: 223003
Ion Ratio Lower Upper
95 100
174 79.1 0.0 136.6
176 74.9 0.0 130.0

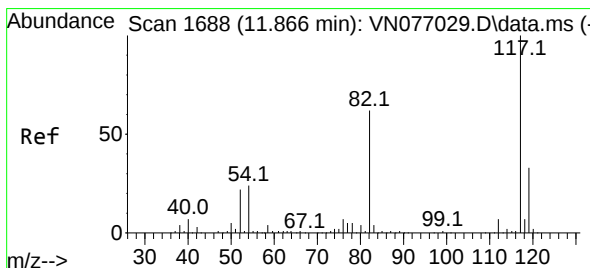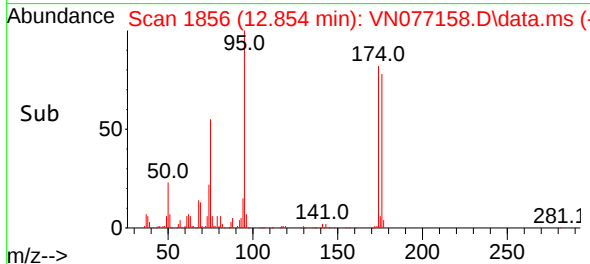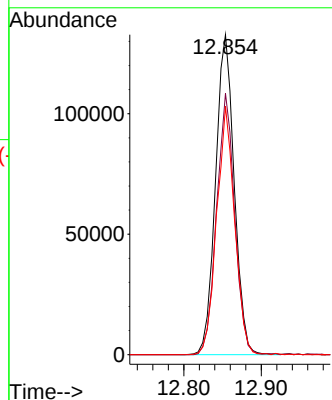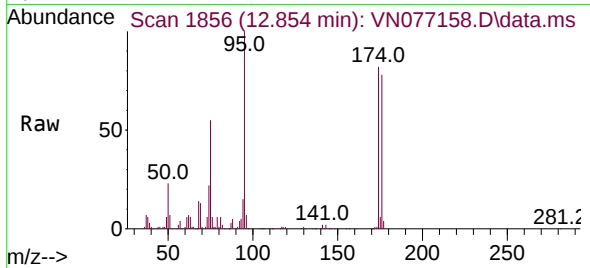

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.871 min Scan# 1689
Delta R.T. 0.005 min
Lab File: VN077158.D
Acq: 23 Mar 2023 18:43

Tgt Ion: 117 Resp: 559164
Ion Ratio Lower Upper
117 100
82 58.3 49.4 74.0
119 32.5 26.5 39.7

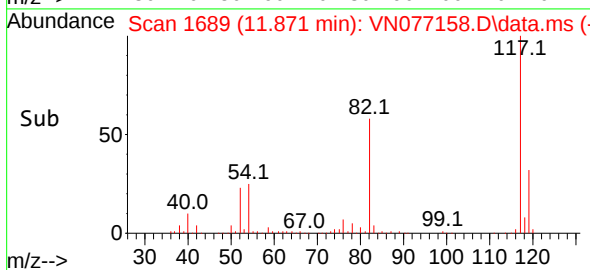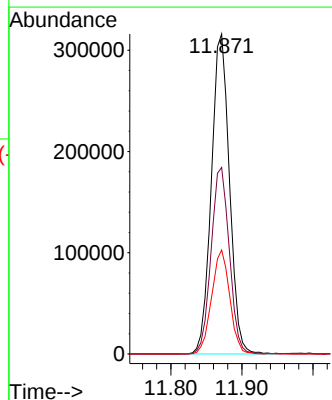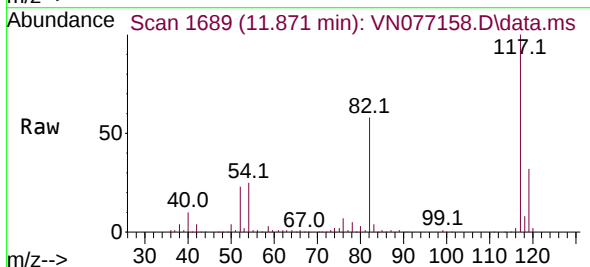

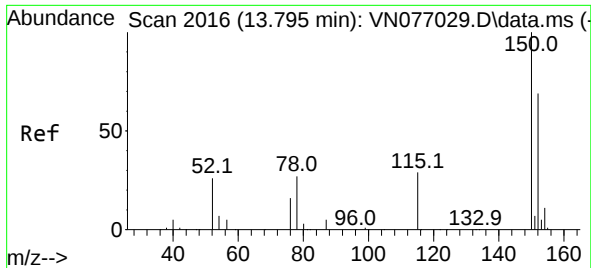

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.795 min Scan# 20

Delta R.T. -0.000 min

Lab File: VN077158.D


Acq: 23 Mar 2023 18:43

Instrument :

MSVOA_N

ClientSampleId :

MW-6

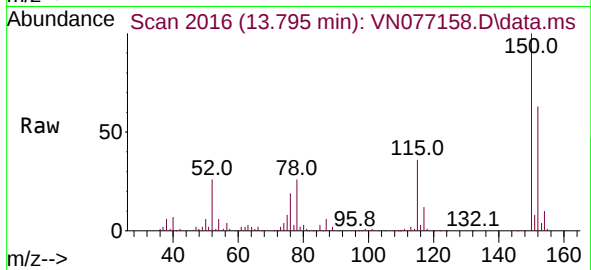

Tgt Ion:152 Resp: 206769

Ion Ratio Lower Upper

152 100

115 59.2 31.9 95.7

150 156.3 0.0 348.0

