
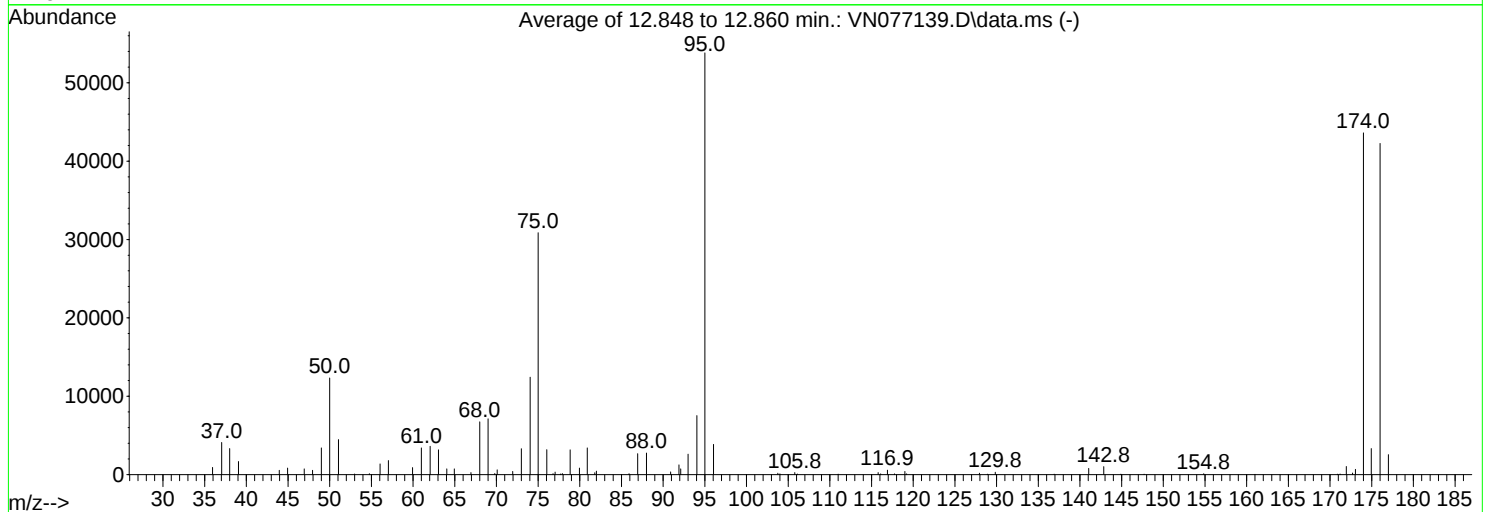


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032323\
Data File : VN077139.D
Acq On : 23 Mar 2023 09:52
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031723W.M
Title : SW846 8260
Last Update : Mon Mar 20 08:50:30 2023

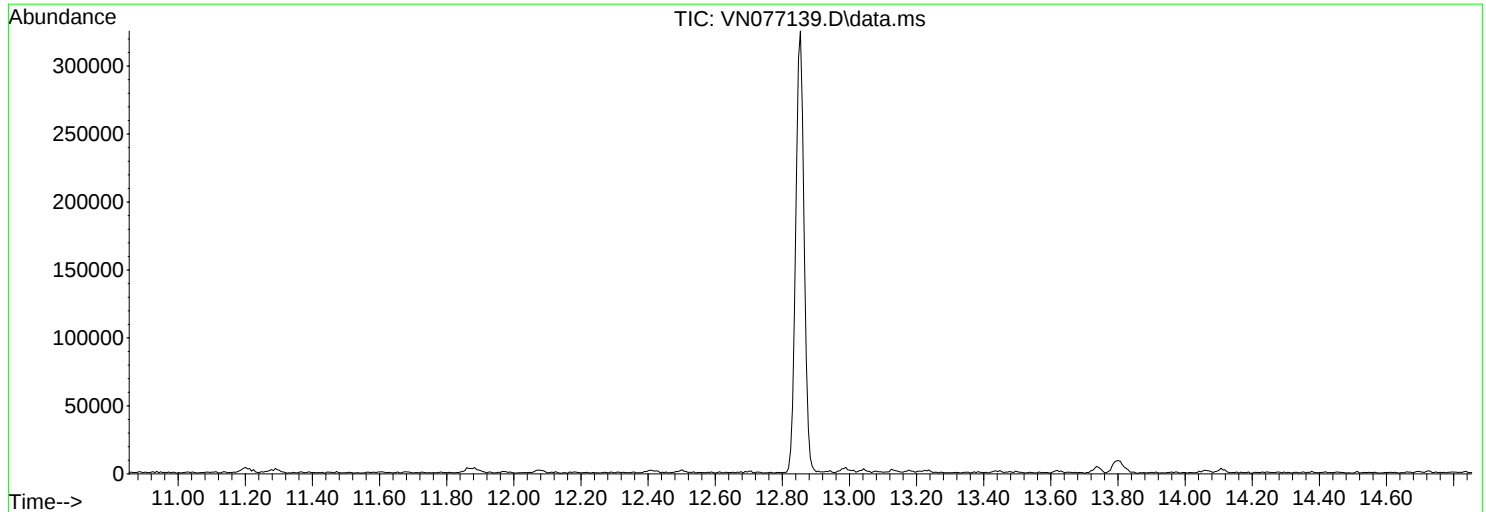

AutoFind: Scans 1855, 1856, 1857; Background Corrected with Scan 1846

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.9	12332	PASS
75	95	30	60	57.4	30875	PASS
95	95	100	100	100.0	53819	PASS
96	95	5	9	7.2	3862	PASS
173	174	0.00	2	1.5	667	PASS
174	95	50	100	81.0	43608	PASS
175	174	5	9	7.7	3338	PASS
176	174	95	101	96.9	42264	PASS
177	176	5	9	6.0	2548	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	924	53.00	82	68.00	6731	77.70	71
37.05	4108	54.75	133	69.00	7124	77.90	141
38.00	3336	56.05	1376	69.80	153	78.85	316
39.05	1678	57.05	1789	70.10	619	79.95	83
43.95	546	59.95	897	71.95	418	80.90	3403
44.95	847	61.00	3409	73.00	3304	81.80	237
46.95	729	62.05	3614	74.05	12425	82.00	454
47.95	548	63.05	3175	75.00	30875	85.90	130
49.00	3412	64.05	736	76.05	3177	86.95	2668
50.00	12332	64.95	731	76.80	128	88.00	2761
51.05	4467	66.95	264	77.05	324	90.90	343

Average of 12.848 to 12.860 min.: VN077139.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
91.90	1246	115.80	257	142.85	1017	174.95	3338
92.10	729	116.10	99	144.90	60	176.00	42264
93.00	2615	116.90	579	147.70	69	177.00	2548
94.05	7539	117.75	108	154.85	130		
95.00	53819	119.00	411	161.00	51		
96.05	3862	119.20	103	170.90	72		
103.75	180	127.95	193	171.20	82		
104.00	101	128.90	58	171.95	1043		
105.80	266	129.85	312	172.70	196		
106.10	82	136.90	64	173.05	667		
111.00	56	141.05	801	174.00	43608		

Instrument :

MSVOA_N

ClientSampleId :

BFB