

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN042020\
 Data File : VN061123.D
 Acq On : 21 Apr 2020 00:32
 Operator : JC/MD
 Sample : L2312-05
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 40693-40720-40531

Quant Time: Apr 21 04:07:28 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N041620W.M
 Quant Title : SW846 8260
 QLast Update : Fri Apr 17 03:49:39 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	0.00	168	0	0.00	ug/l	-7.64
34) 1,4-Difluorobenzene	0.00	114	0	0.00	ug/l	-8.56
63) Chlorobenzene-d5	0.00	117	0	0.00	ug/l	-11.40
72) 1,4-Dichlorobenzene-d4	0.00	152	0	0.00	ug/l	-13.34
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	7.98	65	732	0.00	ug/l	-0.02
Spiked Amount 50.000			Recovery	=	0.00%	
35) Dibromofluoromethane	0.00	113	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	
50) Toluene-d8	0.00	98	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	
62) 4-Bromofluorobenzene	0.00	95	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN042020\
Data File : VN061123.D
Acq On : 21 Apr 2020 00:32
Operator : JC/MD
Sample : L2312-05
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
40693-40720-40531

Quant Time: Apr 21 04:07:28 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N041620W.M
Quant Title : SW846 8260
QLast Update : Fri Apr 17 03:49:39 2020
Response via : Initial Calibration

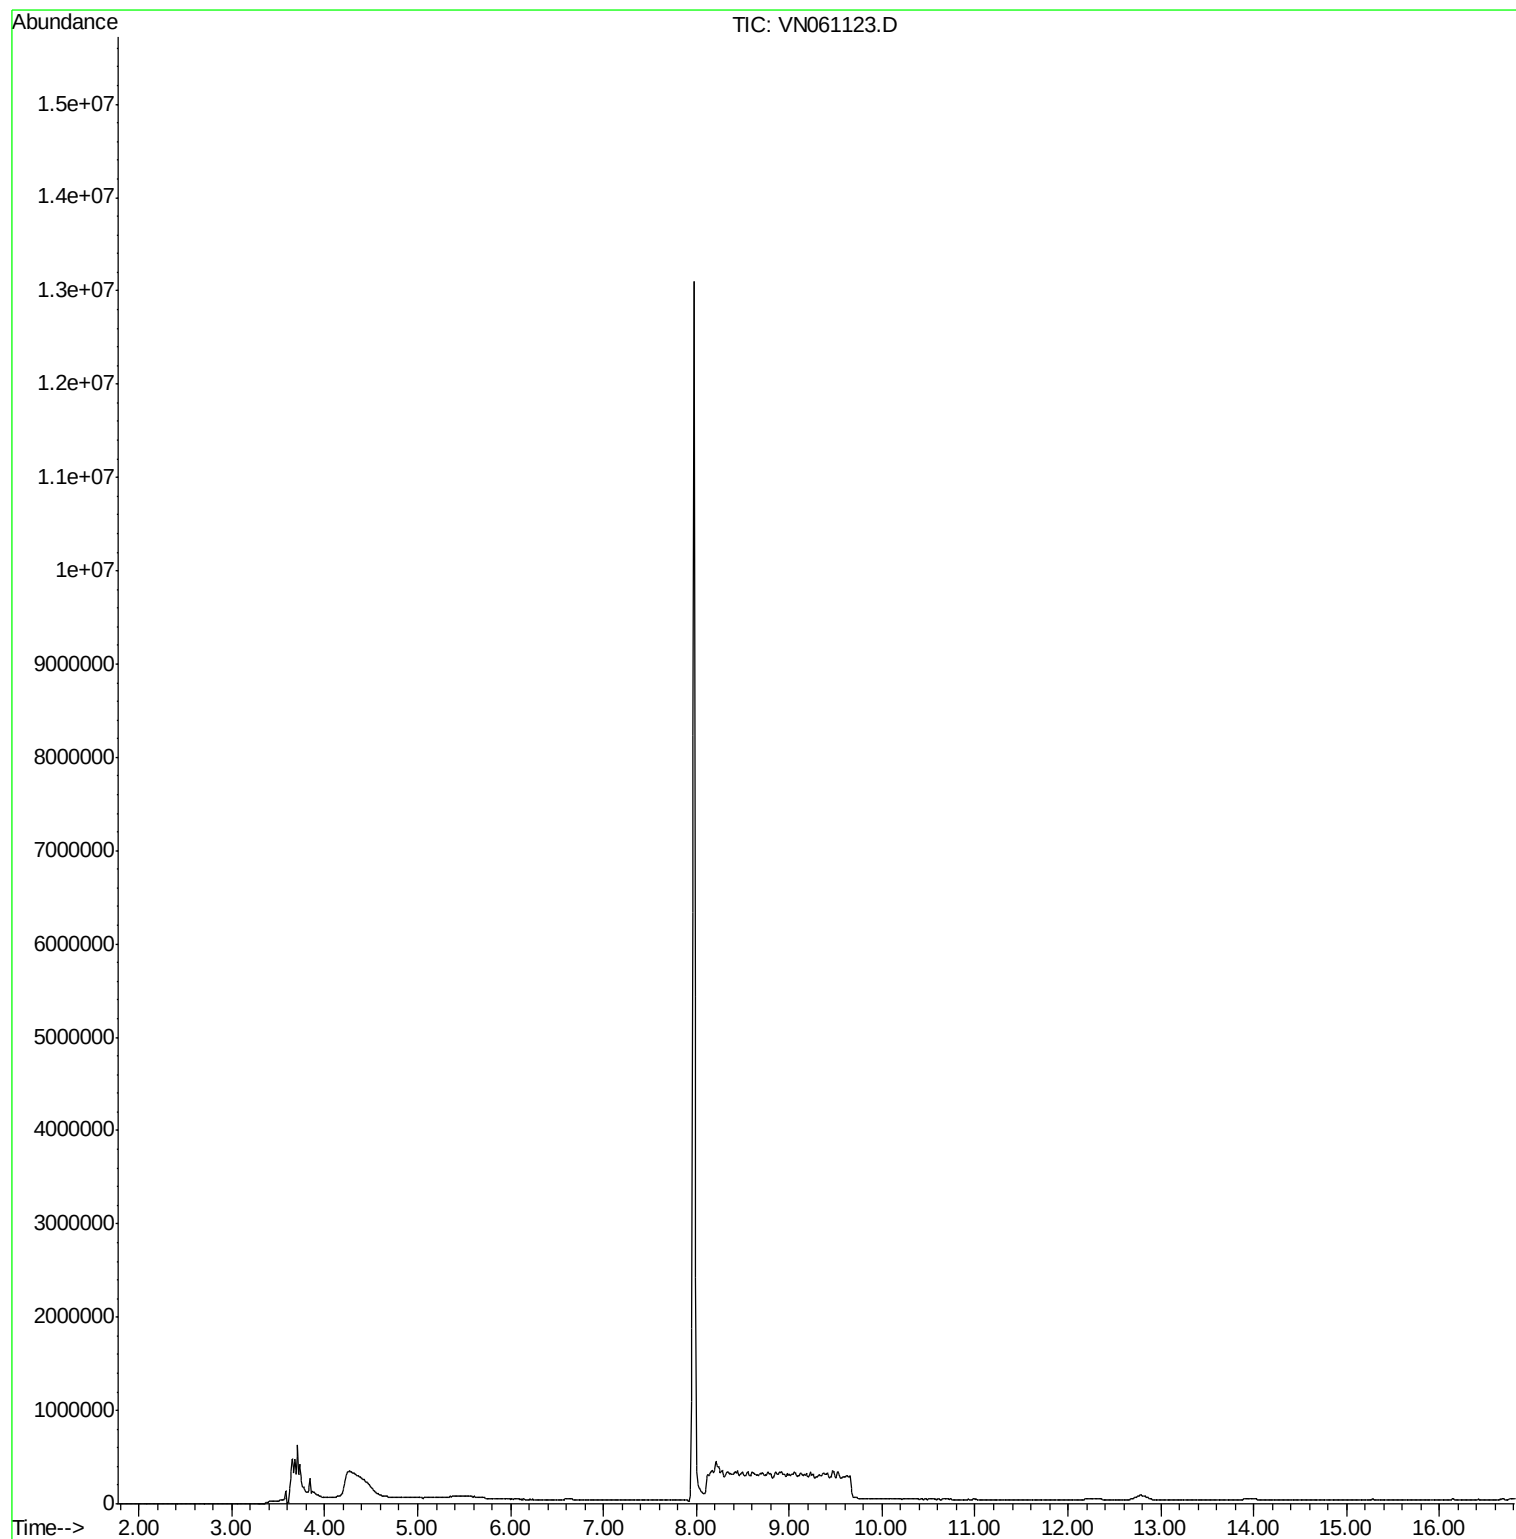

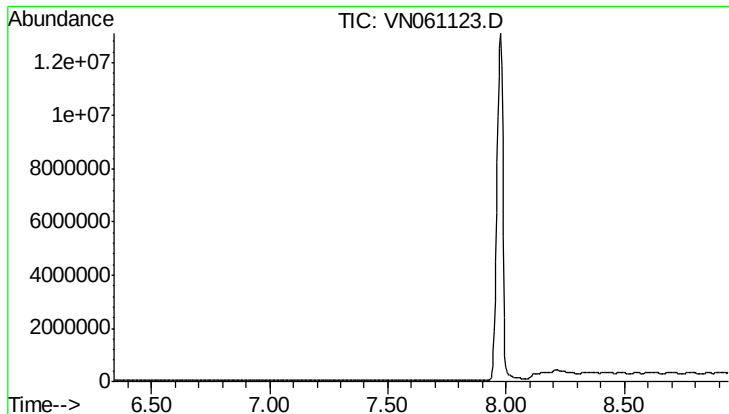

#1

Pentafluorobenzene

Concen: 0.000 ug/l

Expected RT: 7.64 min

Lab File: VN061123.D

Acq: 21 Apr 2020 00:32

Instrument :

MSVOA_N

ClientSampleId :



40693-40720-40531

Tot Ion: 168

Sig Exp Ratio

168 100

99 59.3

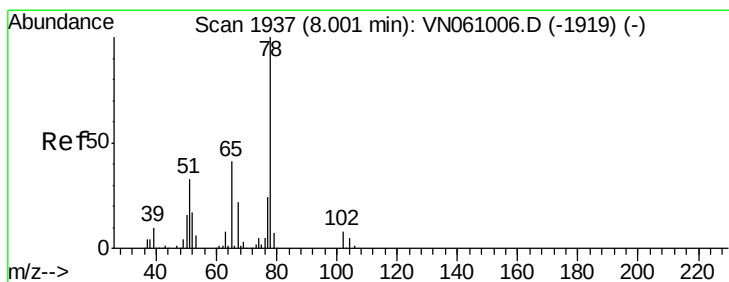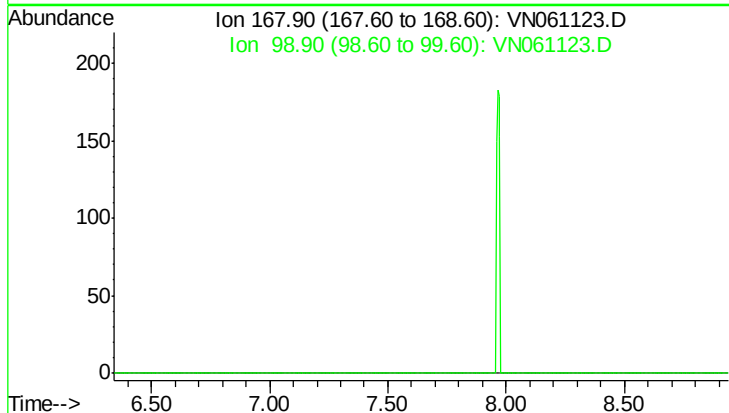

#33

1,2-Dichloroethane-d4

Concen: 0.000 ug/l

RT: 7.98 min Scan# 1930

Delta R.T. -0.02 min

Lab File: VN061123.D




Acq: 21 Apr 2020 00:32


Tgt Ion: 65 Resp: 732

Ion Ratio Lower Upper

65 100

67 120.6 0.0 107.0#

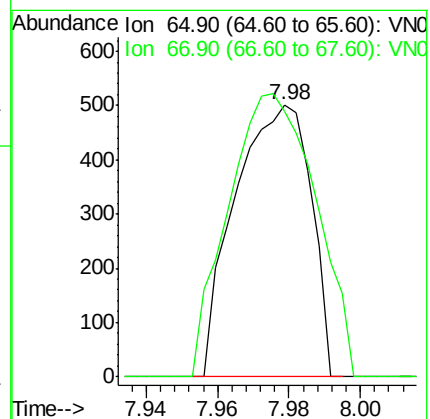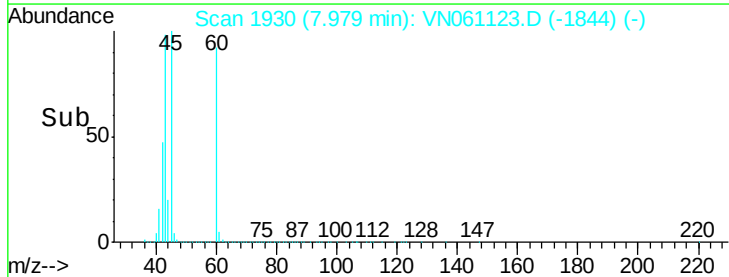
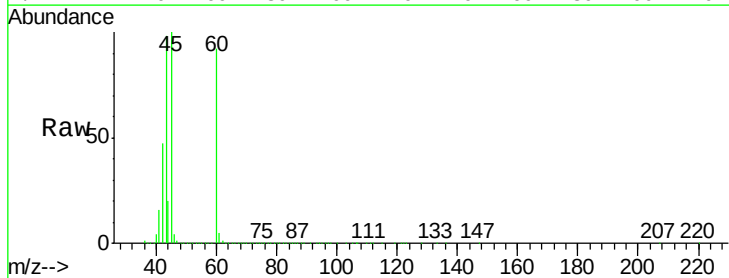


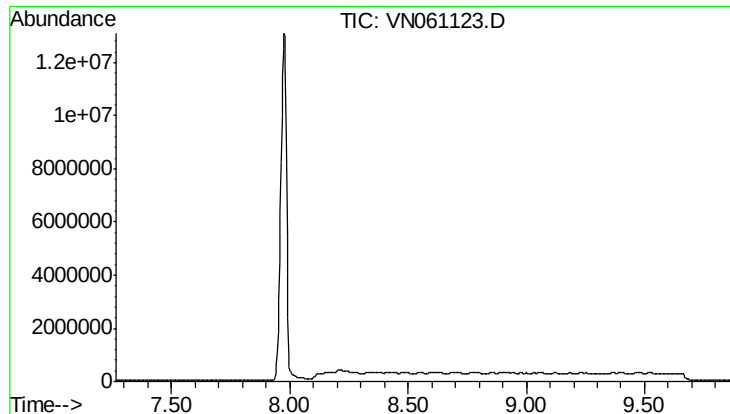

#34
 1,4-Difluorobenzene
 Concen: 0.000 ug/l
 Expected RT: 8.56 min
 Lab File: VN061123.D
 Acq: 21 Apr 2020 00:32


Instrument :
 MSVOA_N
 ClientSampleId :
 40693-40720-40531


Tot Ion: 114
 Sig Exp Ratio
 114 100
 63 23.1
 88 16.7

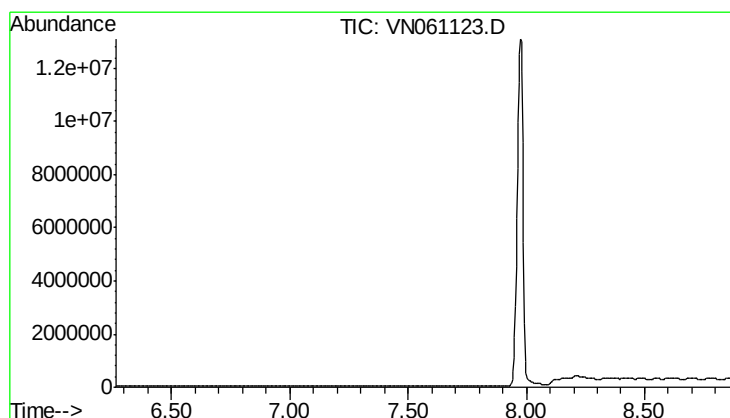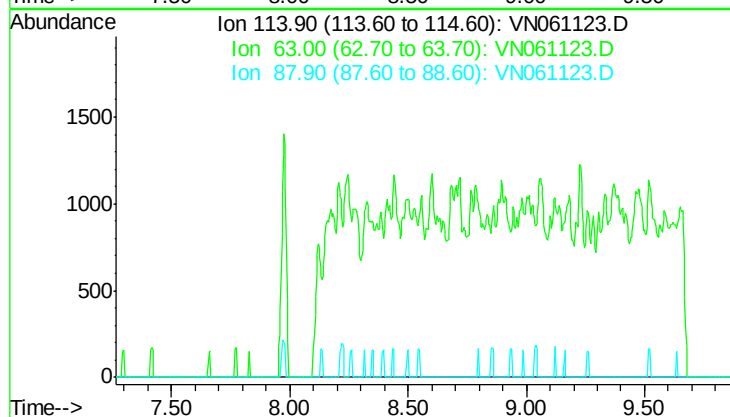

#35
 Dibromofluoromethane
 Concen: 0.000 ug/l
 Expected RT: 7.56 min
 Lab File: VN061123.D
 Acq: 21 Apr 2020 00:32

Tgt Ion: 113
 Sig Exp Ratio
 113 100
 111 104.3
 192 19.4


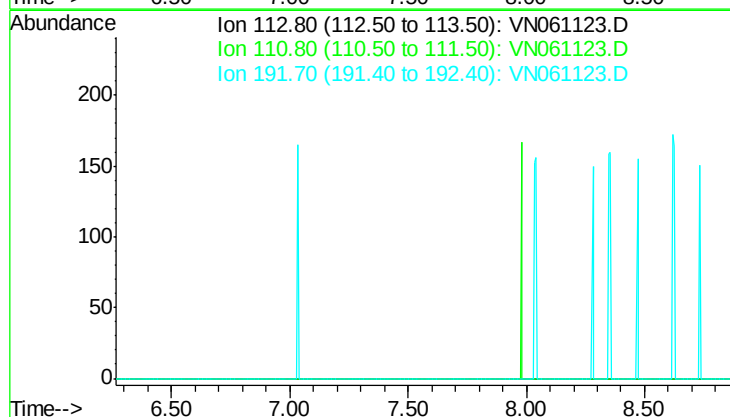


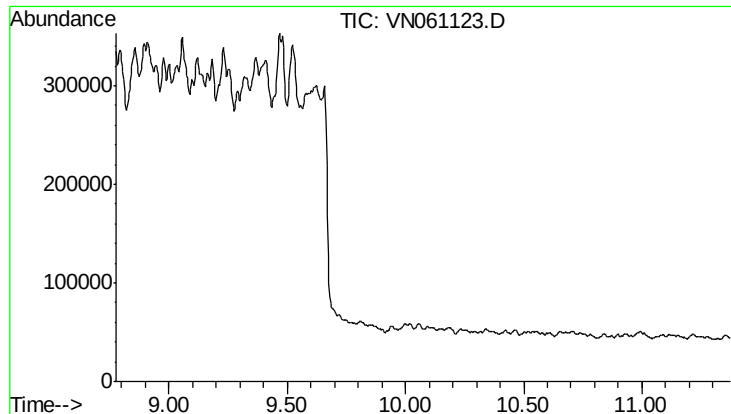

#50
 Toluene-d8
 Concen: 0.000 ug/l
 Expected RT: 10.08 min
 Lab File: VN061123.D
 Acq: 21 Apr 2020 00:32


Instrument :
 MSVOA_N
 ClientSampleId :
 40693-40720-40531


Tot Ion	98
Sig	Exp Ratio
98	100
100	64.9

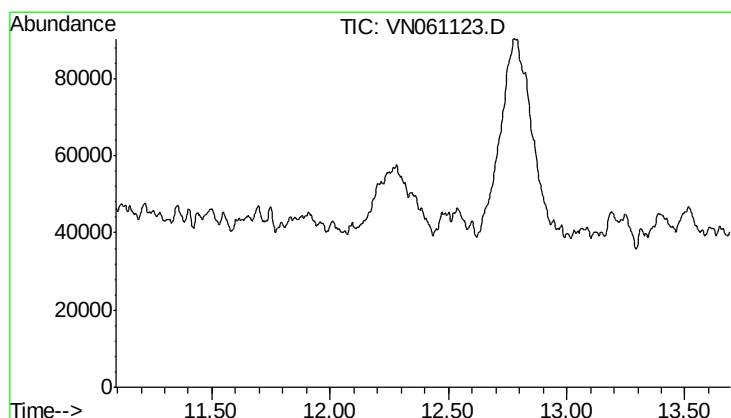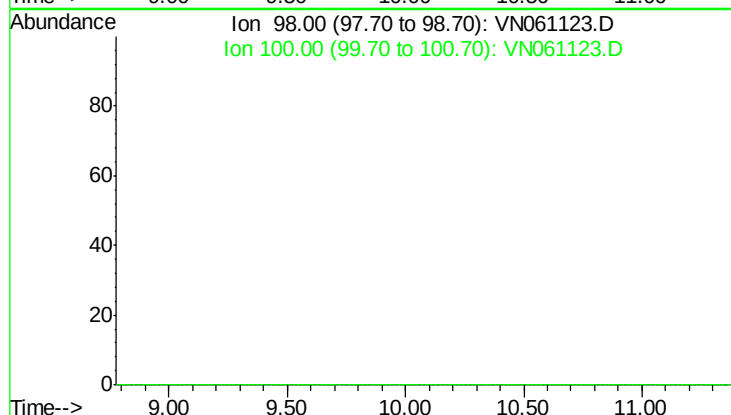

#62
 4-Bromofluorobenzene
 Concen: 0.000 ug/l
 Expected RT: 12.39 min
 Lab File: VN061123.D
 Acq: 21 Apr 2020 00:32

Tgt Ion	95
Sig	Exp Ratio
95	100
174	75.6
176	74.1

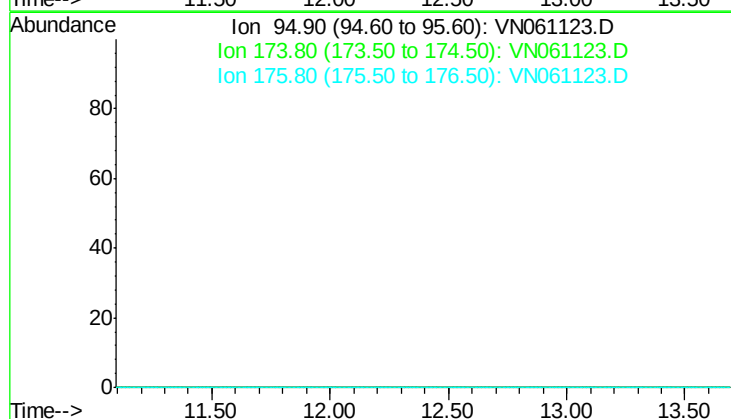


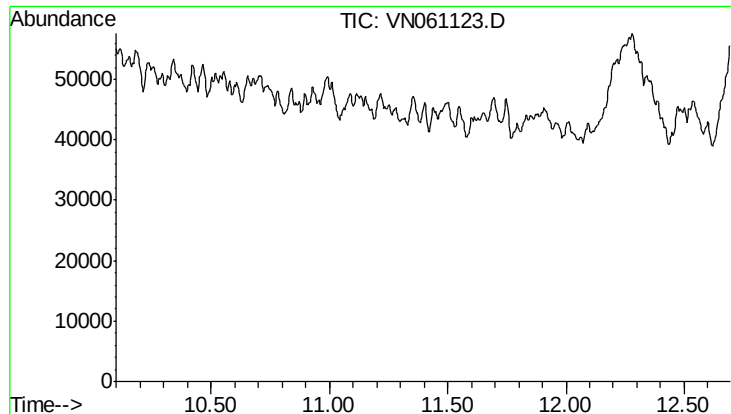


#63
 Chlorobenzene-d5
 Concen: 0.000 ug/l
 Expected RT: 11.40 min

Lab File: VN061123.D
 Acq: 21 Apr 2020 00:32

Instrument :
 MSVOA_N
 ClientSampleId :
 40693-40720-40531

Tot Ion: 117
 Sig Exp Ratio
 117 100
 82 58.9
 119 32.1

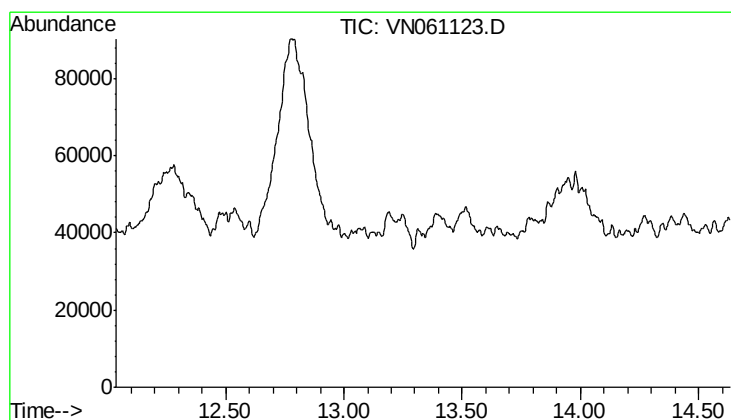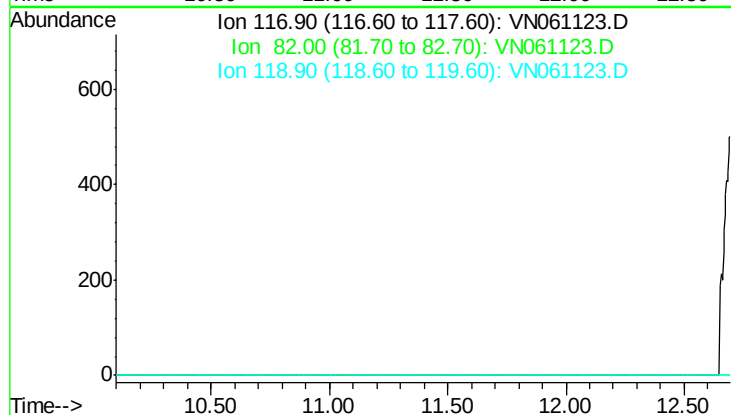

#72
 1,4-Dichlorobenzene-d4
 Concen: 0.000 ug/l
 Expected RT: 13.34 min

Lab File: VN061123.D
 Acq: 21 Apr 2020 00:32

Tgt Ion: 152
 Sig Exp Ratio
 152 100
 115 61.6
 150 174.5

