
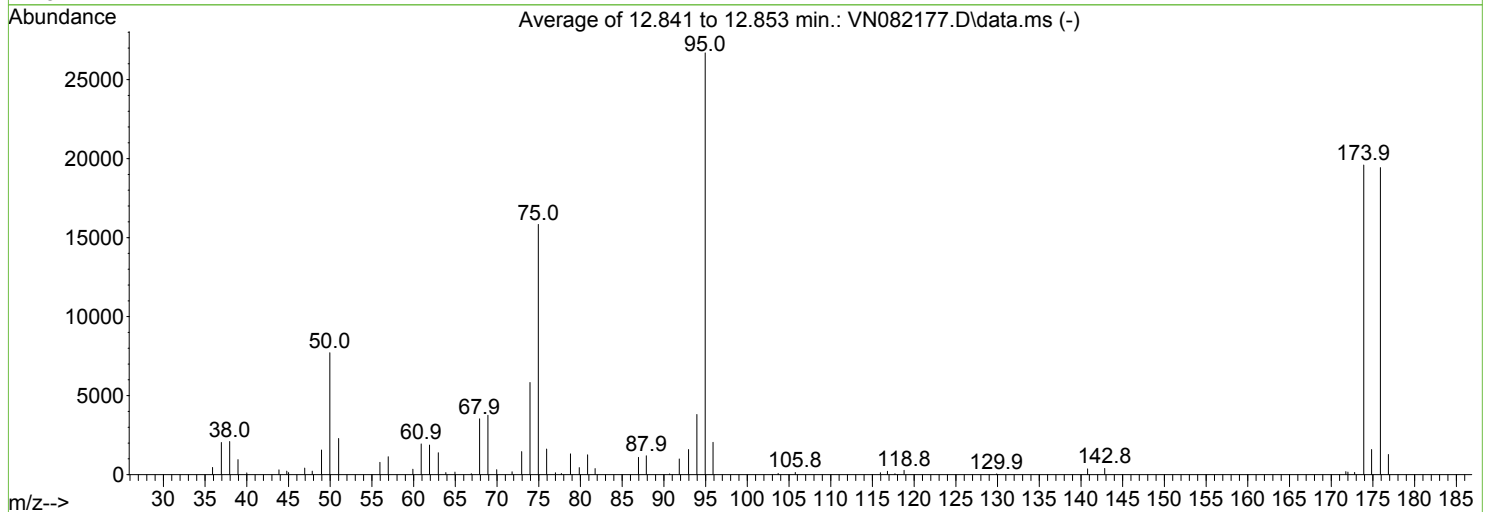


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN051724\
Data File : VN082177.D
Acq On : 17 May 2024 13:50
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051524W.M
Title : SW846 8260
Last Update : Thu May 16 05:21:06 2024

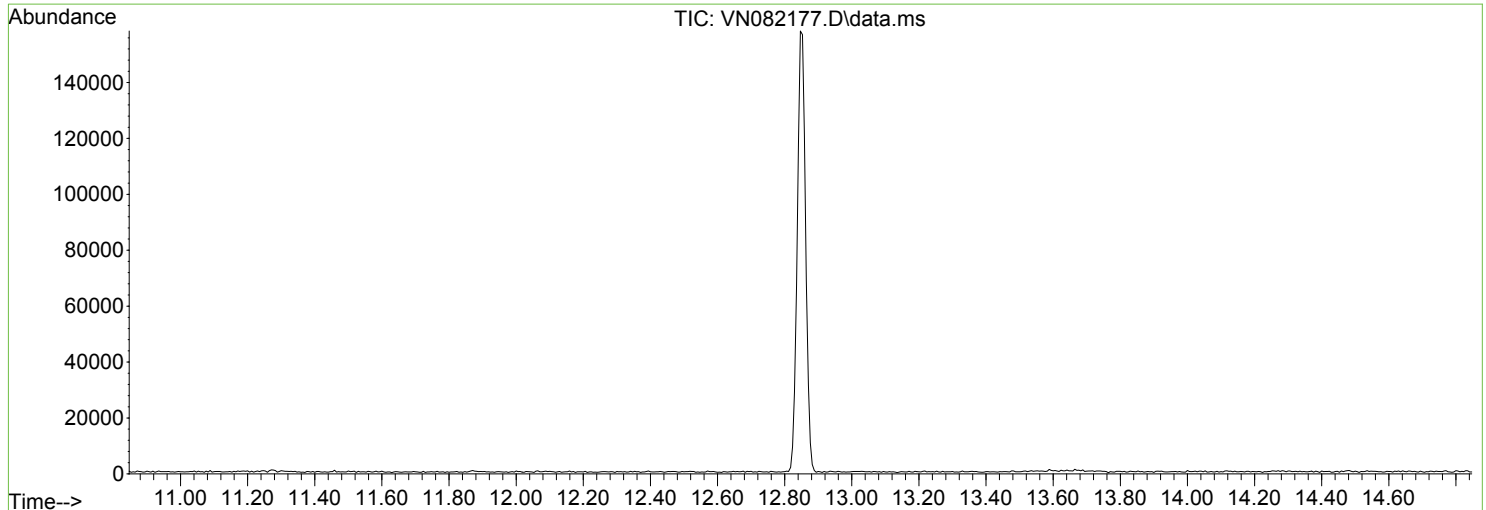

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1844

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	28.9	7719	PASS
75	95	30	60	59.3	15832	PASS
95	95	100	100	100.0	26693	PASS
96	95	5	9	7.7	2046	PASS
173	174	0.00	2	0.7	138	PASS
174	95	50	100	73.4	19598	PASS
175	174	5	9	8.1	1593	PASS
176	174	95	101	99.1	19429	PASS
177	176	5	9	6.6	1280	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	458	49.95	7719	67.90	3532	79.85	441
36.95	2037	51.00	2285	68.90	3752	80.85	125
37.95	2092	55.95	777	69.95	315	81.75	38
38.95	949	56.95	1139	71.80	187	86.95	109
40.00	116	59.90	349	72.95	1462	87.90	1192
43.85	304	60.90	1941	73.95	5833	90.70	54
44.80	226	61.90	1878	74.95	15832	91.85	996
45.00	135	62.95	1391	75.95	1621	92.95	1585
46.95	420	63.85	131	77.00	124	93.95	3810
47.85	222	64.95	167	77.70	68	94.95	26693
48.95	1556	66.90	60	78.80	1314	95.90	2046

Average of 12.841 to 12.853 min.: VN082177.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
103.70	78	172.80	138				
105.75	143	173.90	19598				
115.95	121	174.85	1593				
116.80	213	175.90	19429				
117.70	62	176.85	1280				
118.80	269						
129.90	53						
140.80	366						
142.85	400						
171.75	192						
172.00	161						

Instrument :

MSVOA_N

ClientSampleId :

BFB