


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN061418\
 Data File : VN049218.D
 Acq On : 14 Jun 2018 10:35
 Operator : MD\SY
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N061318W.M
 Title : SW846 8260
 Last Update : Thu Jun 14 05:15:23 2018

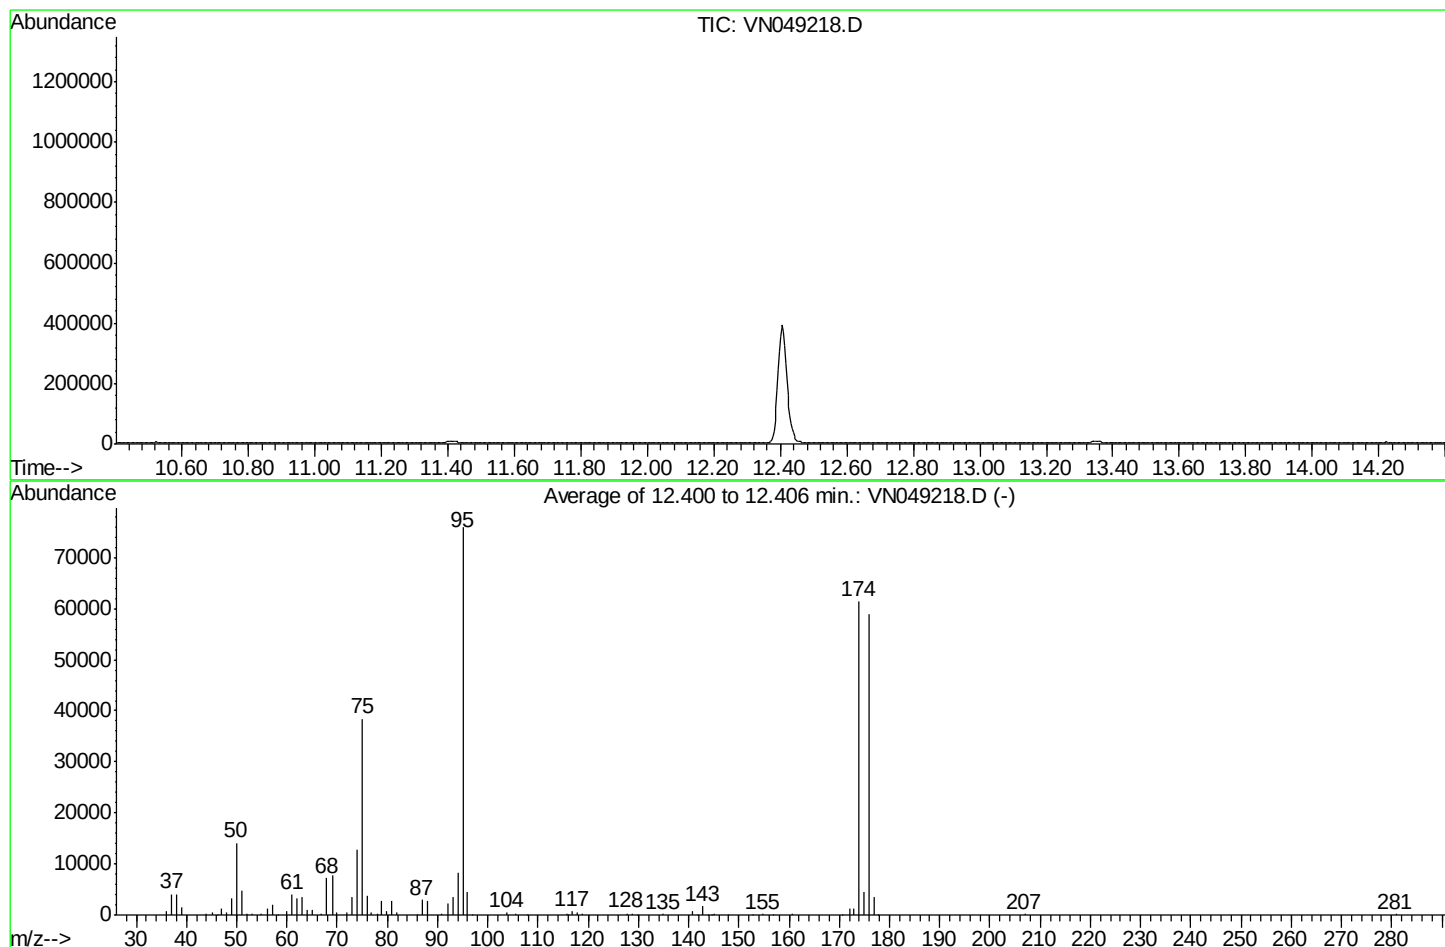

AutoFind: Scans 3362, 3363, 3364; Background Corrected with Scan 3348

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	14102	PASS
75	95	30	60	50.6	38394	PASS
95	95	100	100	100.0	75930	PASS
96	95	5	9	6.1	4597	PASS
173	174	0.00	2	2.0	1203	PASS
174	95	50	100	80.8	61362	PASS
175	174	5	9	7.4	4551	PASS
176	174	95	101	96.2	59013	PASS
177	176	5	9	5.8	3415	PASS