


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN061618\
Data File : VN049258.D
Acq On : 15 Jun 2018 12:14
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N061618W.M
Title : SW846 8260
Last Update : Sat Jun 16 01:02:01 2018

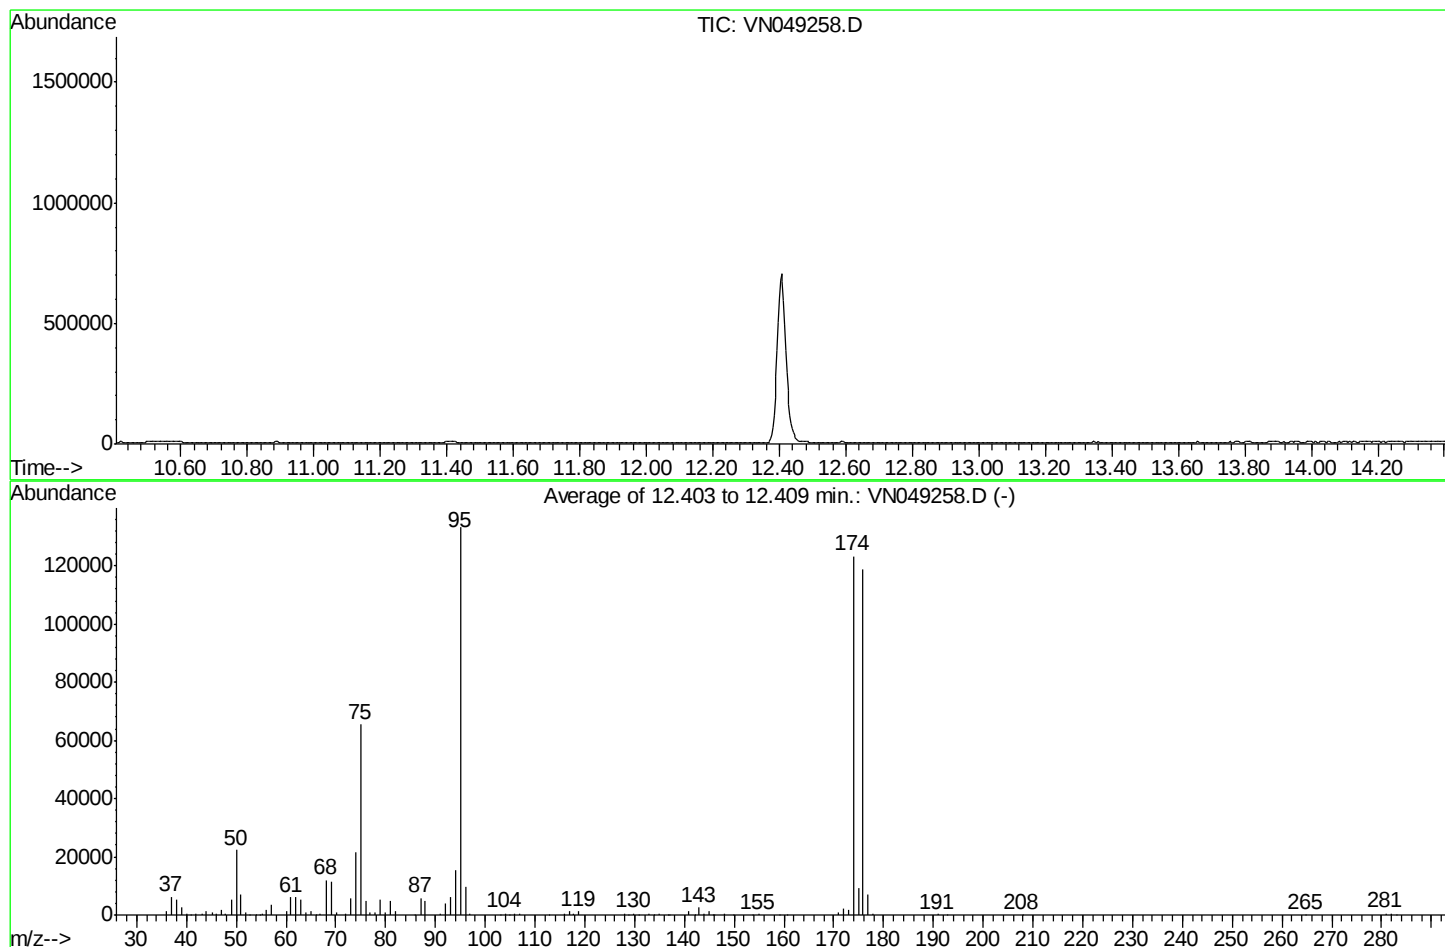

AutoFind: Scans 3363, 3364, 3365; Background Corrected with Scan 3349

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	22245	PASS
75	95	30	60	49.1	65370	PASS
95	95	100	100	100.0	133242	PASS
96	95	5	9	7.2	9629	PASS
173	174	0.00	2	1.5	1830	PASS
174	95	50	100	92.5	123240	PASS
175	174	5	9	7.7	9476	PASS
176	174	95	101	96.5	118944	PASS
177	176	5	9	6.1	7246	PASS