


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN061618\  
 Data File : VN049283.D  
 Acq On : 16 Jun 2018 2:09  
 Operator : MD\SY  
 Sample : BFB  
 Misc : 5.00mL/MSVOA N/WATER  
 ALS Vial : 26 Sample Multiplier: 1

Instrument :  
 MSVOA\_N  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_N\METHODS\82N061618W.M  
 Title : SW846 8260  
 Last Update : Sat Jun 16 01:02:01 2018

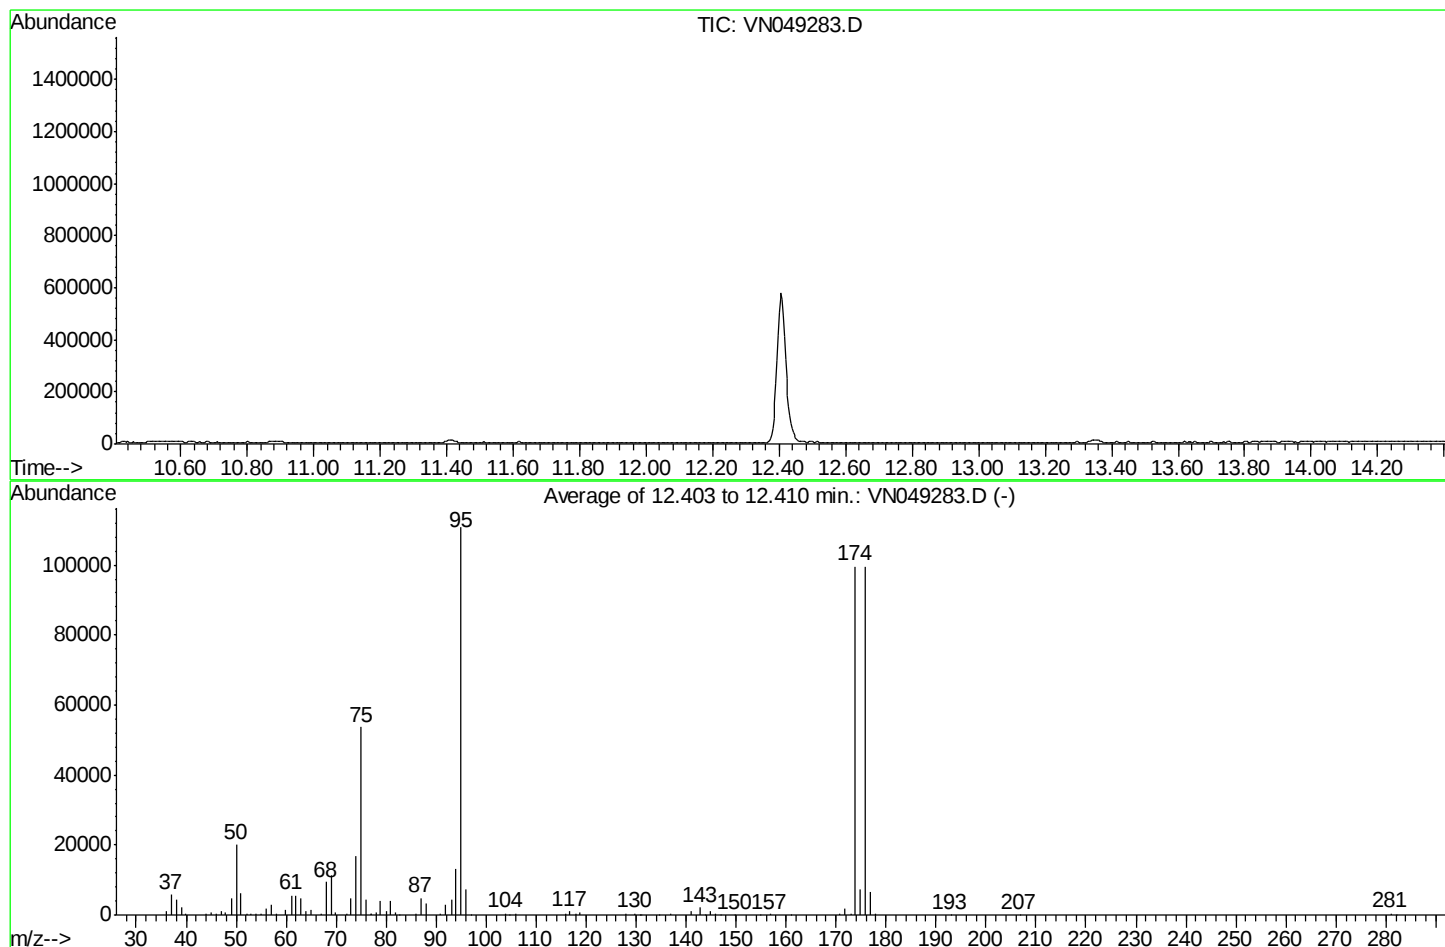

AutoFind: Scans 3363, 3364, 3365; Background Corrected with Scan 3347

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 18.1      | 20074   | PASS             |
| 75          | 95           | 30           | 60           | 48.5      | 53744   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 110749  | PASS             |
| 96          | 95           | 5            | 9            | 6.5       | 7240    | PASS             |
| 173         | 174          | 0.00         | 2            | 0.5       | 523     | PASS             |
| 174         | 95           | 50           | 100          | 90.0      | 99629   | PASS             |
| 175         | 174          | 5            | 9            | 7.5       | 7487    | PASS             |
| 176         | 174          | 95           | 101          | 99.8      | 99381   | PASS             |
| 177         | 176          | 5            | 9            | 6.5       | 6502    | PASS             |