


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN061618\
 Data File : VN049308.D
 Acq On : 16 Jun 2018 13:59
 Operator : MD\SY
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N061618W.M
 Title : SW846 8260
 Last Update : Sat Jun 16 01:02:01 2018

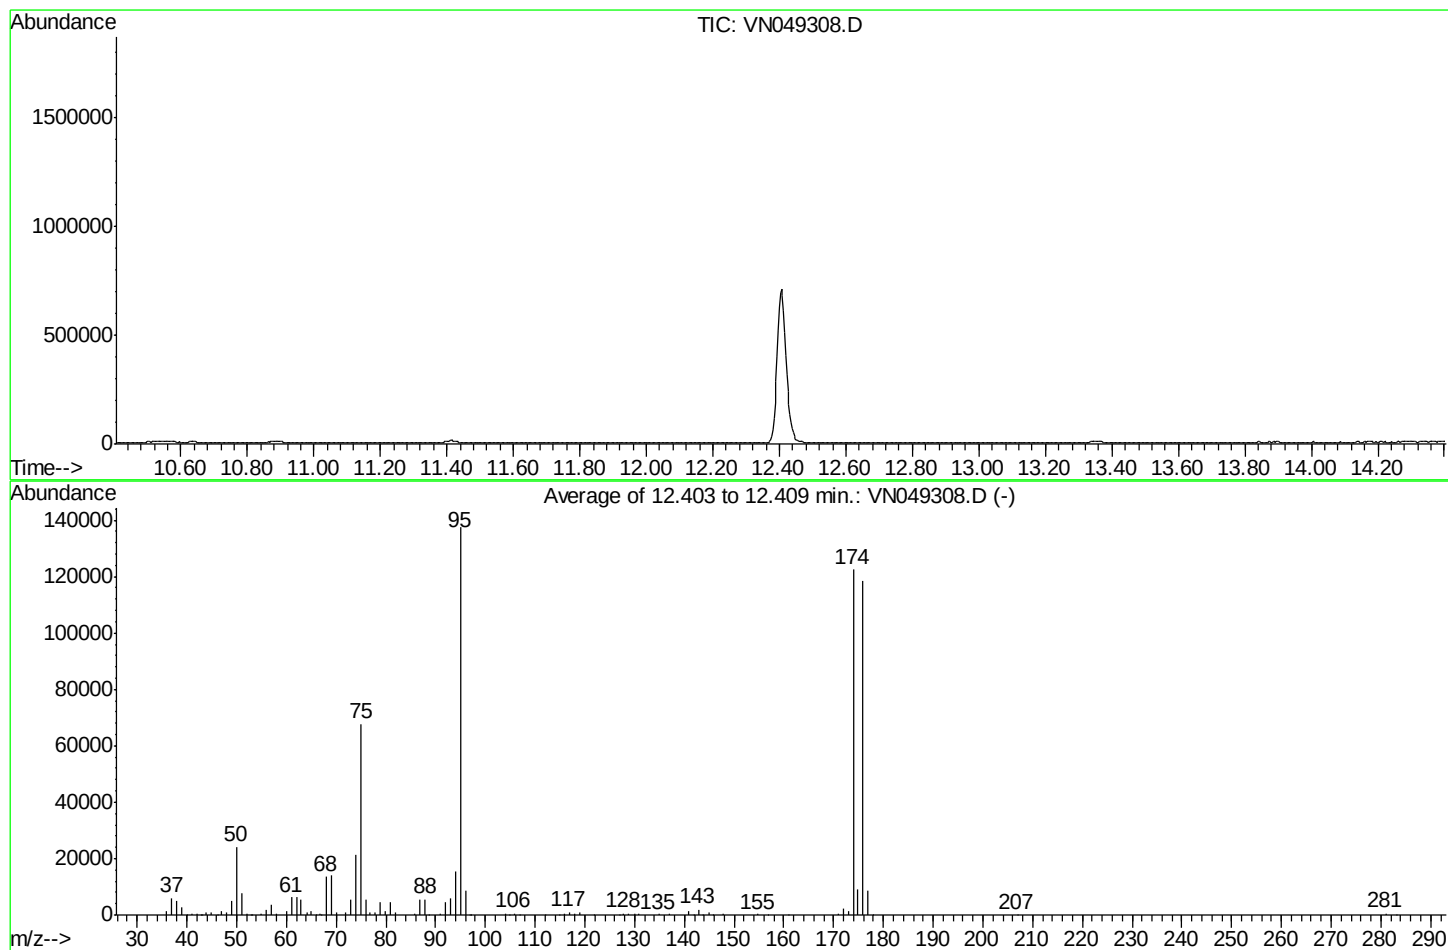

AutoFind: Scans 3363, 3364, 3365; Background Corrected with Scan 3348

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	24141	PASS
75	95	30	60	49.3	67784	PASS
95	95	100	100	100.0	137450	PASS
96	95	5	9	6.3	8612	PASS
173	174	0.00	2	1.1	1405	PASS
174	95	50	100	89.0	122357	PASS
175	174	5	9	7.5	9211	PASS
176	174	95	101	96.9	118549	PASS
177	176	5	9	7.1	8448	PASS