

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061822\
 Data File : VN072930.D
 Acq On : 18 Jun 2022 11:17
 Operator : JC\MD
 Sample : N3334-12
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 WC-14A-1A-8-GR

Quant Time: Jun 20 08:02:51 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N061722W.M
 Quant Title : SW846 8260
 QLast Update : Sat Jun 18 06:22:45 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.016	168	299169	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.898	114	527318	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.680	117	462083	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.610	152	207002	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.369	65	180599	44.651	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	89.300%
35) Dibromofluoromethane	7.951	113	144465	44.324	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	88.640%
50) Toluene-d8	10.375	98	519212	42.811	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	85.620%#
62) 4-Bromofluorobenzene	12.663	95	188344	43.188	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	86.380%

Target Compounds			Qvalue			
3) Chloromethane	2.269	50	804	0.829	ug/l #	74
5) Bromomethane	2.822	94	640	0.636	ug/l #	2
6) Chloroethane	2.940	64	473	0.296	ug/l #	42
11) Tert butyl alcohol	5.293	59	3350	3.206	ug/l #	72
13) Acrolein	3.987	56	290	0.705	ug/l #	14
16) Acetone	4.228	43	117418	52.812	ug/l	92
17) Carbon Disulfide	4.457	76	5296	0.722	ug/l #	75
18) Methyl Acetate	4.793	43	6780	1.145	ug/l #	82
20) Methylene Chloride	5.016	84	79291	22.861	ug/l	90
25) 2-Butanone	7.269	43	52137	14.778	ug/l #	87
26) 2,2-Dichloropropane	7.234	77	1755	Below Cal	#	53
29) Tetrahydrofuran	7.628	42	1896	0.814	ug/l #	51
31) Cyclohexane	8.022	56	8742	1.598	ug/l #	40
36) 1,1-Dichloropropene	8.016	75	23603	5.352	ug/l #	50
37) Ethyl Acetate	7.269	43	52137	7.391	ug/l #	67
38) Carbon Tetrachloride	8.016	117	29951	6.456	ug/l #	16
39) Methylcyclohexane	9.398	83	1927	0.363	ug/l	95
43) Isopropyl Acetate	8.492	43	40978	4.064	ug/l #	88
45) 1,2-Dichloropropane	9.557	63	2563	0.723	ug/l #	44
48) Methyl methacrylate	9.475	41	18873	4.099	ug/l #	25
49) 1,4-Dioxane	9.563	88	165	1.593	ug/l #	1
51) 4-Methyl-2-Pentanone	10.269	43	10689	1.626	ug/l	96
52) Toluene	10.439	92	2964	0.348	ug/l	90
54) cis-1,3-Dichloropropene	10.180	75	51241	9.162	ug/l #	65
57) 1,3-Dichloropropane	11.027	76	27873	4.497	ug/l #	42
59) 2-Hexanone	11.027	43	428829	84.318	ug/l #	45
68) m/p-Xylenes	11.886	106	6396	1.027	ug/l	83
69) o-Xylene	12.216	106	10080	1.619	ug/l	96
73) Isopropylbenzene	12.516	105	5297	0.331	ug/l	90
74) N-amyl acetate	12.286	43	7803	0.939	ug/l #	40
76) 1,2,3-Trichloropropane	12.669	75	95728	19.074	ug/l #	1
80) 1,3,5-Trimethylbenzene	12.998	105	5976	0.454	ug/l	98
81) trans-1,4-Dichloro-2-b...	12.669	75	95728	51.512	ug/l #	11
84) 1,2,4-Trimethylbenzene	13.304	105	26063	1.989	ug/l	92
92) 1,2-Dibromo-3-Chloropr...	14.539	75	58	Below Cal	#	1
95) Naphthalene	15.421	128	12810	0.801	ug/l #	84

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061822\
Data File : VN072930.D
Acq On : 18 Jun 2022 11:17
Operator : JC\MD
Sample : N3334-12
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
WC-14A-1A-8-GR

Quant Time: Jun 20 08:02:51 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N061722W.M
Quant Title : SW846 8260
QLast Update : Sat Jun 18 06:22:45 2022
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061822\
Data File : VN072930.D
Acq On : 18 Jun 2022 11:17
Operator : JC\MD
Sample : N3334-12
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
WC-14A-1A-8-GR

Quant Time: Jun 20 08:02:51 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N061722W.M
Quant Title : SW846 8260
QLast Update : Sat Jun 18 06:22:45 2022
Response via : Initial Calibration




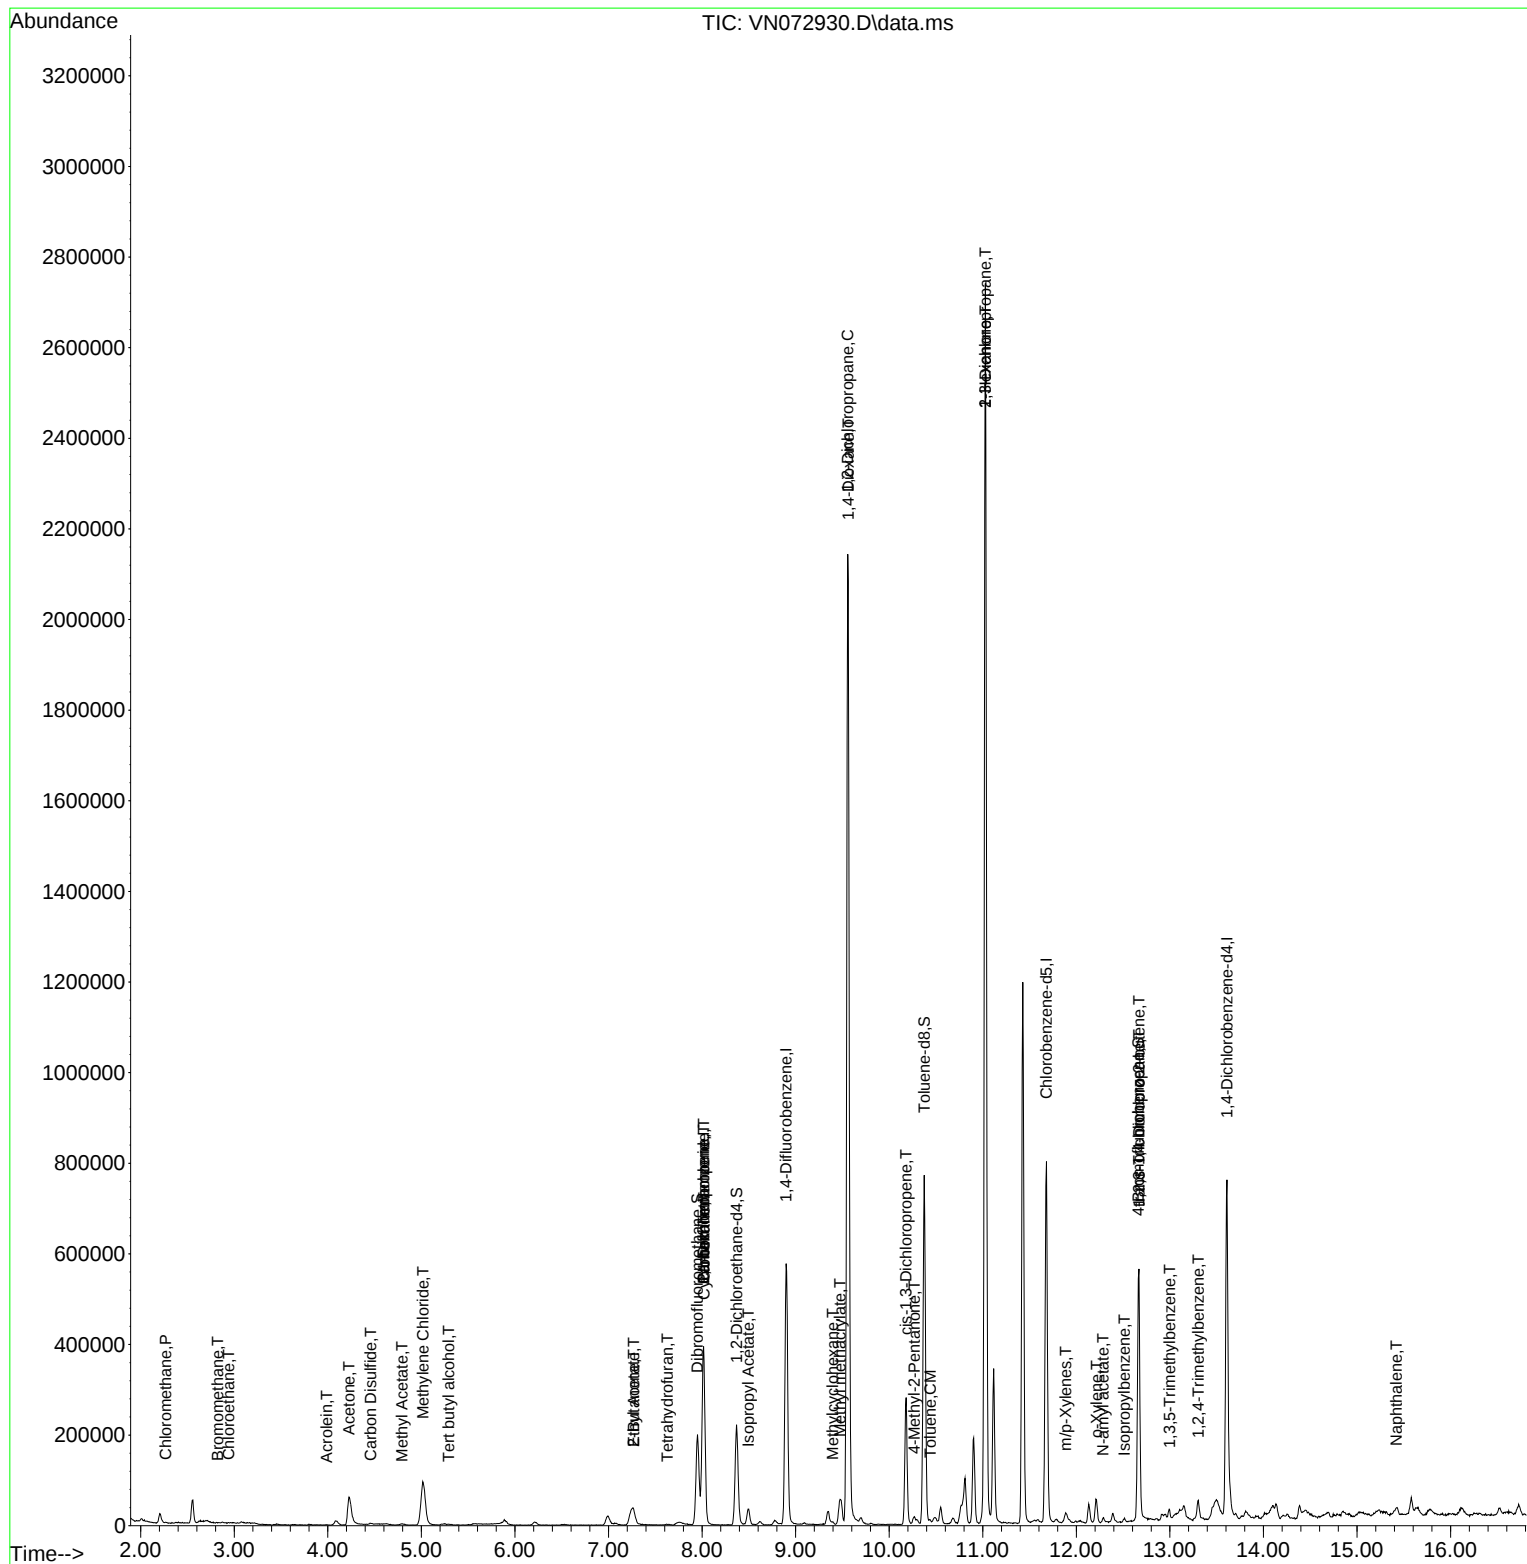




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.016 min Scan# 1042
Delta R.T. -0.000 min
Lab File: VN072930.D
Acq: 18 Jun 2022 11:17




Instrument :
MSVOA_N
ClientSampleId :
WC-14A-1A-8-GR


Tgt Ion:168 Resp: 299169
Ion Ratio Lower Upper
168 100
99 55.9 42.3 63.5

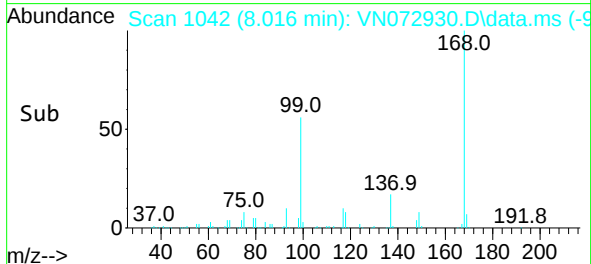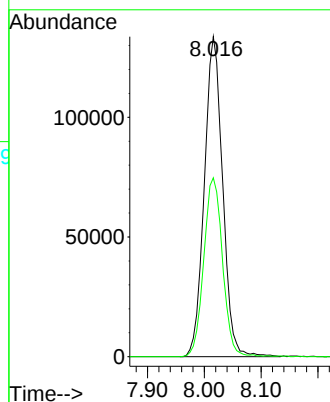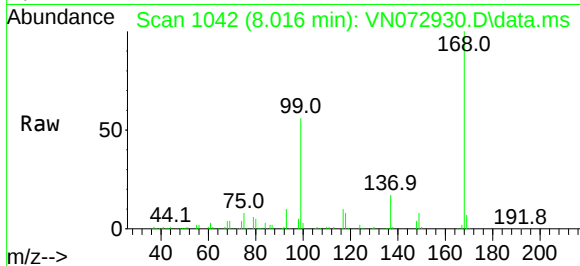

#3
Chloromethane
Concen: 0.829 ug/l
RT: 2.269 min Scan# 65
Delta R.T. 0.006 min
Lab File: VN072930.D
Acq: 18 Jun 2022 11:17

Tgt Ion: 50 Resp: 804
Ion Ratio Lower Upper
50 100
52 17.4 25.7 38.5


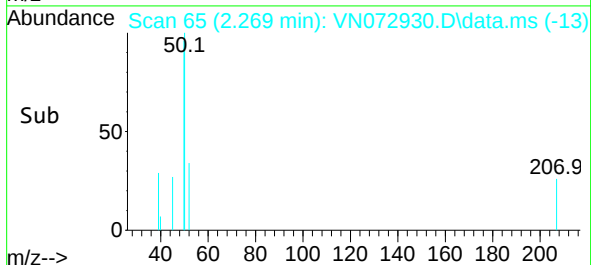
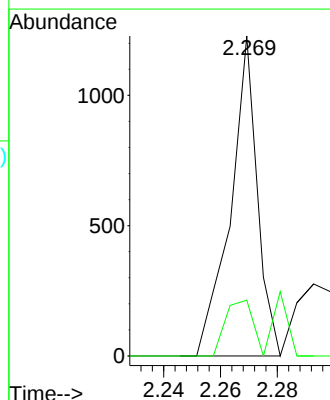
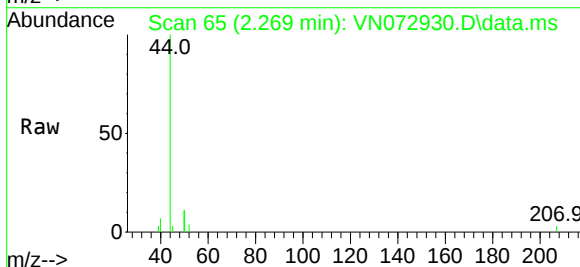




#5
Bromomethane
Concen: 0.636 ug/l
RT: 2.822 min Scan# 11
Delta R.T. 0.035 min
Lab File: VN072930.D
Acq: 18 Jun 2022 11:17




Instrument :
MSVOA_N
ClientSampleId :
WC-14A-1A-8-GR


Tgt Ion: 94 Resp: 640
Ion Ratio Lower Upper
94 100
96 0.0 76.0 114.0#

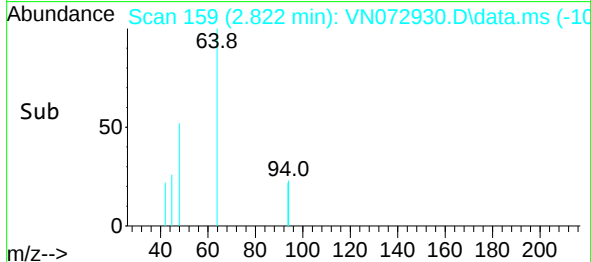

#6
Chloroethane
Concen: 0.296 ug/l
RT: 2.940 min Scan# 179
Delta R.T. -0.012 min
Lab File: VN072930.D
Acq: 18 Jun 2022 11:17

Tgt Ion: 64 Resp: 473
Ion Ratio Lower Upper
64 100
66 0.0 26.2 39.4#





#11

Tert butyl alcohol

Concen: 3.206 ug/l

RT: 5.293 min Scan# 51

Delta R.T. -0.012 min

Lab File: VN072930.D

Acq: 18 Jun 2022 11:17

Instrument :

MSVOA_N

ClientSampleId :





WC-14A-1A-8-GR

Tgt Ion: 59 Resp: 3350

Ion Ratio Lower Upper

59 100

57 0.0 8.3 12.5#

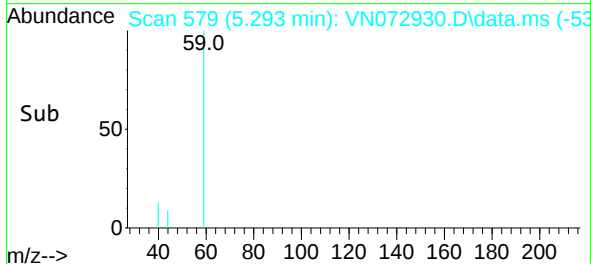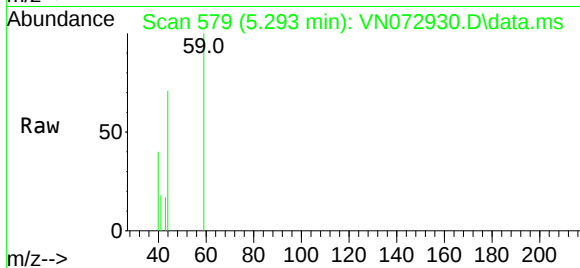

#13

Acrolein

Concen: 0.705 ug/l

RT: 3.987 min Scan# 357

Delta R.T. 0.006 min

Lab File: VN072930.D




Acq: 18 Jun 2022 11:17


Tgt Ion: 56 Resp: 290

Ion Ratio Lower Upper

56 100

55 138.3 54.8 82.2#


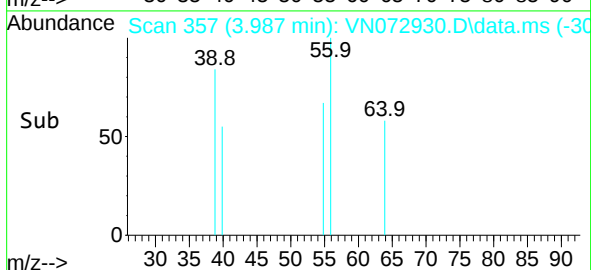

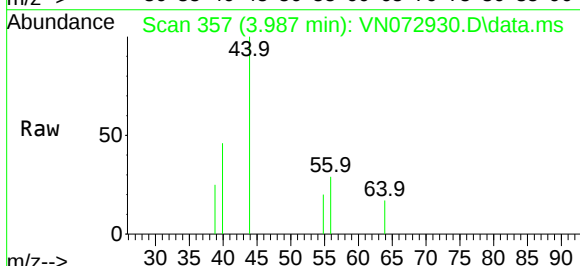




#16
Acetone
Concen: 52.812 ug/l
RT: 4.228 min Scan# 398
Delta R.T. 0.000 min
Lab File: VN072930.D
Acq: 18 Jun 2022 11:17




Instrument :
MSVOA_N
ClientSampleId :
WC-14A-1A-8-GR


Tgt Ion: 43 Resp: 117418
Ion Ratio Lower Upper
43 100
58 27.9 26.0 39.0

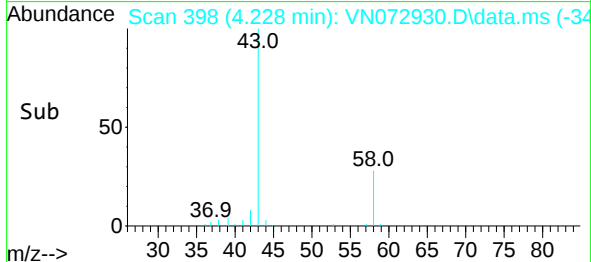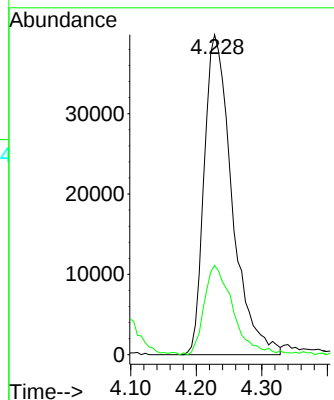

#17
Carbon Disulfide
Concen: 0.722 ug/l
RT: 4.457 min Scan# 437
Delta R.T. 0.000 min
Lab File: VN072930.D
Acq: 18 Jun 2022 11:17

Tgt Ion: 76 Resp: 5296
Ion Ratio Lower Upper
76 100
78 0.0 7.2 10.8#



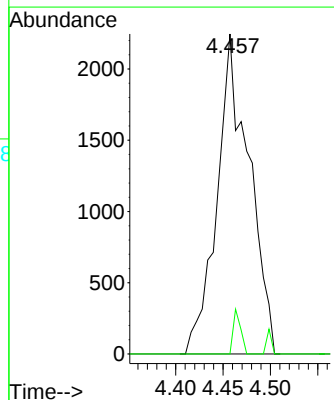
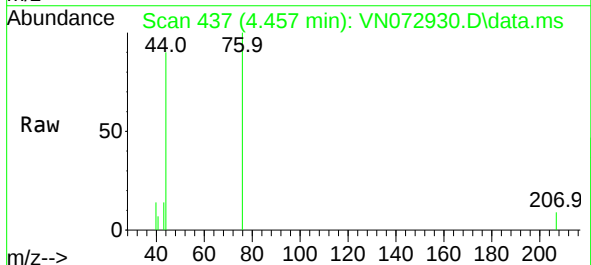




#18
Methyl Acetate
Concen: 1.145 ug/l
RT: 4.793 min Scan# 494
Delta R.T. 0.012 min
Lab File: VN072930.D
Acq: 18 Jun 2022 11:17




Instrument :
MSVOA_N
ClientSampleId :
WC-14A-1A-8-GR


Tgt Ion: 43 Resp: 6780
Ion Ratio Lower Upper
43 100
74 17.5 21.6 32.4#

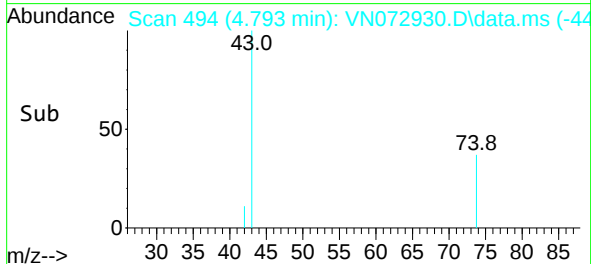

#20
Methylene Chloride
Concen: 22.861 ug/l
RT: 5.016 min Scan# 532
Delta R.T. 0.000 min
Lab File: VN072930.D
Acq: 18 Jun 2022 11:17

Tgt Ion: 84 Resp: 79291
Ion Ratio Lower Upper
84 100
49 126.7 88.3 132.5
51 33.7 28.2 42.2
86 67.5 50.6 76.0



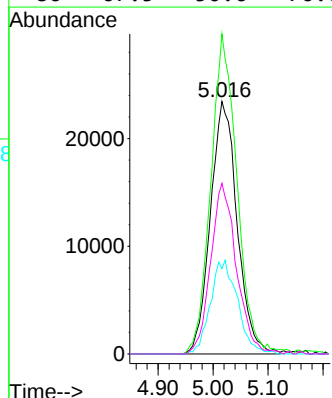





#25
2-Butanone
Concen: 14.778 ug/l
RT: 7.269 min Scan# 914
Delta R.T. 0.006 min
Lab File: VN072930.D
Acq: 18 Jun 2022 11:17




Instrument :
MSVOA_N
ClientSampleId :
WC-14A-1A-8-GR


Tgt Ion: 43 Resp: 52137
Ion Ratio Lower Upper
43 100
72 22.4 23.7 35.5#

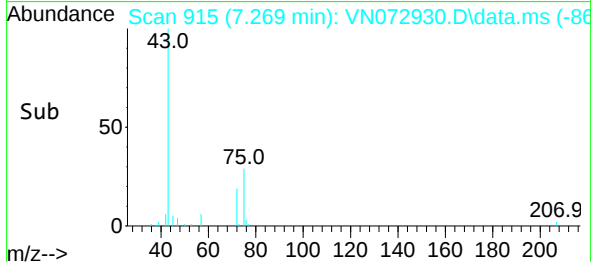

#26
2,2-Dichloropropane
Concen: Below Cal
RT: 7.234 min Scan# 909
Delta R.T. -0.017 min
Lab File: VN072930.D
Acq: 18 Jun 2022 11:17

Tgt Ion: 77 Resp: 1755
Ion Ratio Lower Upper
77 100
97 0.0 11.4 34.2#




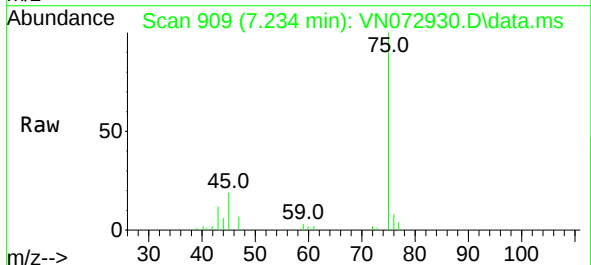




#29
Tetrahydrofuran
Concen: 0.814 ug/l
RT: 7.628 min Scan# 91
Delta R.T. 0.018 min
Lab File: VN072930.D
Acq: 18 Jun 2022 11:17




Instrument :
MSVOA_N
ClientSampleId :
WC-14A-1A-8-GR


Tgt Ion: 42 Resp: 1896
Ion Ratio Lower Upper
42 100
72 15.4 39.7 59.5#
71 14.3 36.6 55.0#

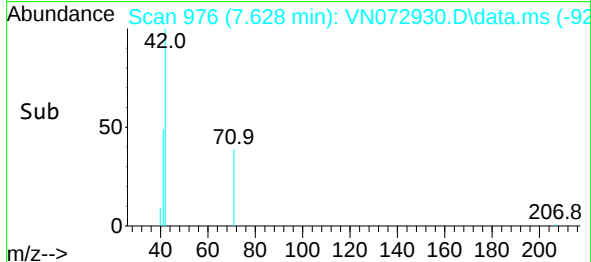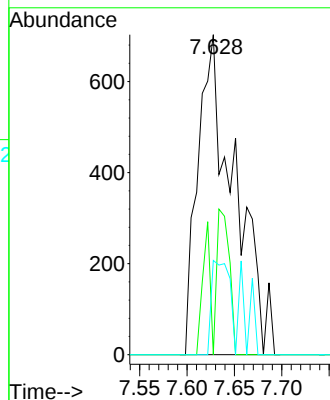

#31
Cyclohexane
Concen: 1.598 ug/l
RT: 8.022 min Scan# 1043
Delta R.T. 0.000 min
Lab File: VN072930.D
Acq: 18 Jun 2022 11:17

Tgt Ion: 56 Resp: 8742
Ion Ratio Lower Upper
56 100
69 129.9 27.8 41.8#
84 117.7 76.9 115.3#


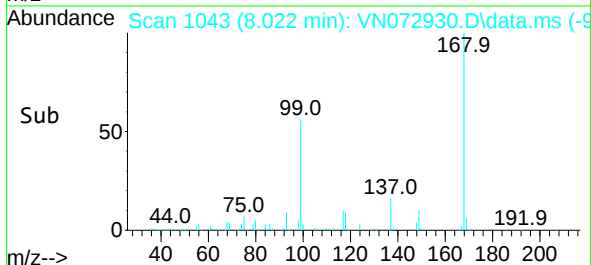
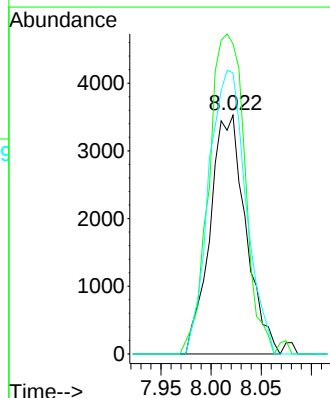
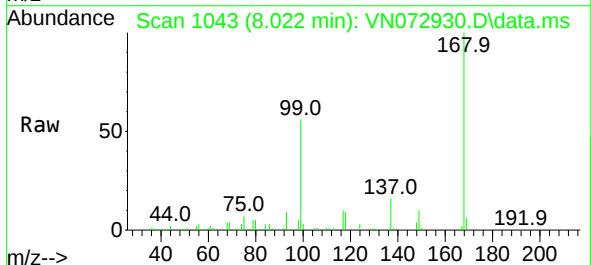




#33
 1,2-Dichloroethane-d4
 Concen: 44.651 ug/l
 RT: 8.369 min Scan# 1102
 Delta R.T. 0.000 min
 Lab File: VN072930.D
 Acq: 18 Jun 2022 11:17




Instrument :
 MSVOA_N
 ClientSampleId :
 WC-14A-1A-8-GR


Tgt Ion: 65 Resp: 180599
 Ion Ratio Lower Upper
 65 100
 67 53.1 0.0 104.8

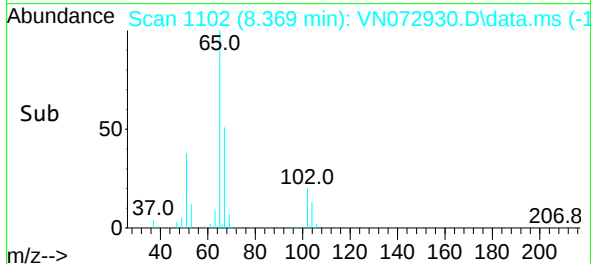

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.898 min Scan# 1192
 Delta R.T. 0.000 min
 Lab File: VN072930.D
 Acq: 18 Jun 2022 11:17

Tgt Ion: 114 Resp: 527318
 Ion Ratio Lower Upper
 114 100
 63 20.3 0.0 40.0
 88 15.6 0.0 32.6

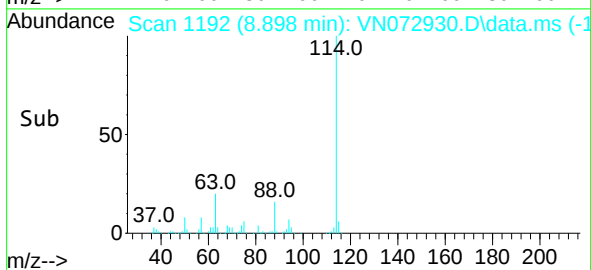

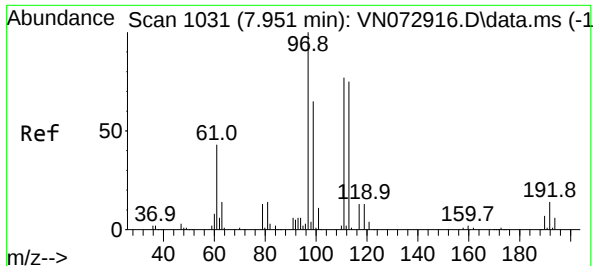

#35

Dibromofluoromethane

Concen: 44.324 ug/l

RT: 7.951 min Scan# 1042

Delta R.T. 0.000 min

Lab File: VN072930.D

Acq: 18 Jun 2022 11:17

Instrument :

MSVOA_N

ClientSampleId :

WC-14A-1A-8-GR





Tgt Ion:113 Resp: 144465

Ion Ratio Lower Upper

113 100

111 103.8 81.4 122.0

192 19.7 17.0 25.6

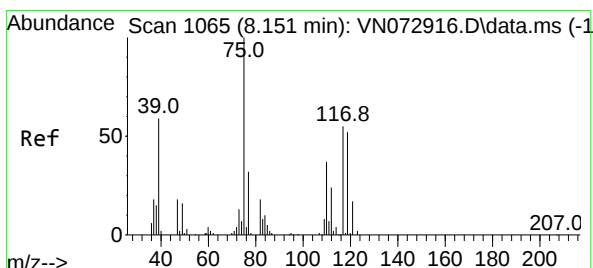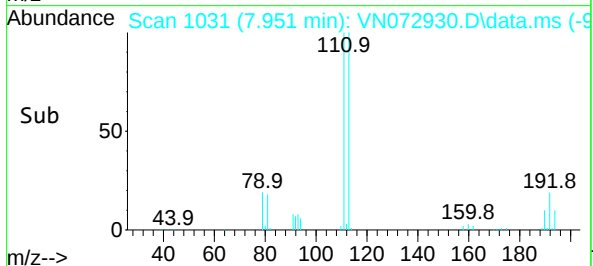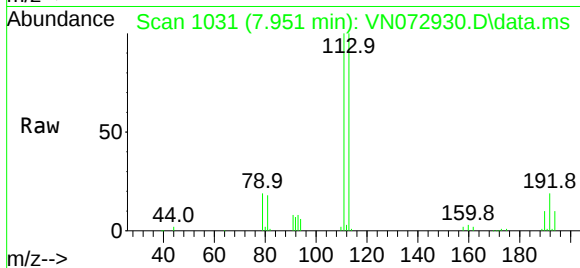

#36

1,1-Dichloropropene

Concen: 5.352 ug/l

RT: 8.016 min Scan# 1042

Delta R.T. -0.135 min

Lab File: VN072930.D

Acq: 18 Jun 2022 11:17




Tgt Ion: 75 Resp: 23603


Ion Ratio Lower Upper

75 100

110 9.9 18.3 54.8#

77 0.0 25.1 37.7#

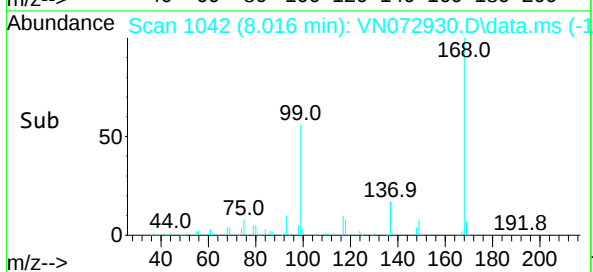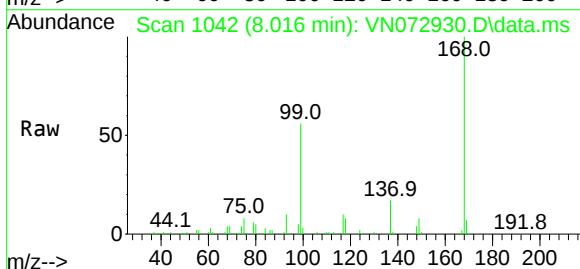



#37

Ethyl Acetate

Concen: 7.391 ug/l

RT: 7.269 min Scan# 91

Delta R.T. -0.076 min

Lab File: VN072930.D


Acq: 18 Jun 2022 11:17

Instrument :




MSVOA_N

ClientSampleId :

WC-14A-1A-8-GR

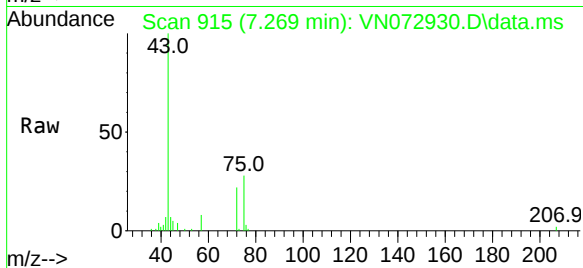

Tgt Ion:	43	Resp:	52137
Ion	Ratio	Lower	Upper
43	100		
61	0.0	11.8	17.6#
70	0.0	9.3	13.9#

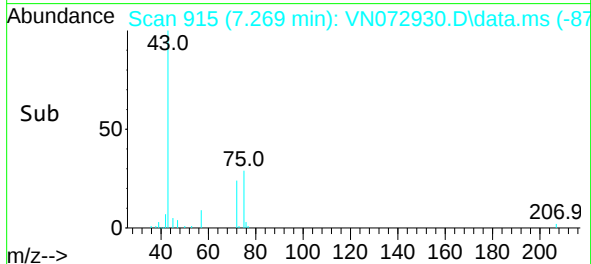

#38

Carbon Tetrachloride

Concen: 6.456 ug/l




RT: 8.016 min Scan# 1042


Delta R.T. -0.117 min

Lab File: VN072930.D

Acq: 18 Jun 2022 11:17

Tgt Ion:	117	Resp:	29951
Ion	Ratio	Lower	Upper
117	100		
119	4.3	75.8	113.8#
121	0.0	24.6	37.0#

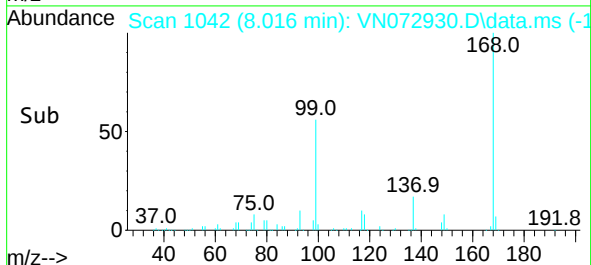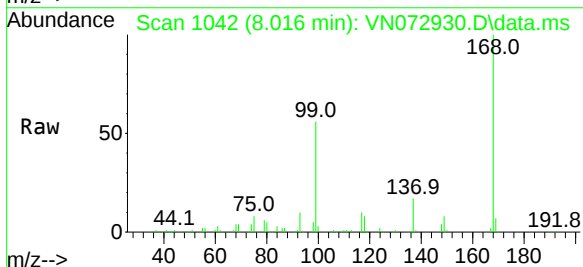

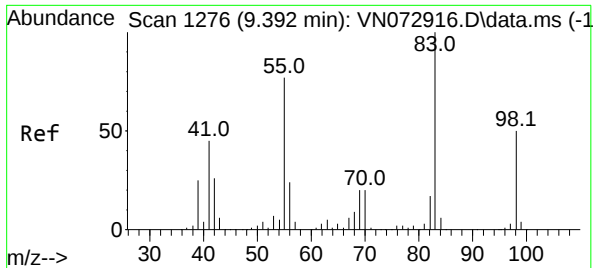

#39

Methylcyclohexane

Concen: 0.363 ug/l

RT: 9.398 min Scan# 1127

Delta R.T. 0.006 min

Lab File: VN072930.D

Acq: 18 Jun 2022 11:17

Instrument :

MSVOA_N

ClientSampleId :

WC-14A-1A-8-GR





Tgt Ion: 83 Resp: 1927

Ion Ratio Lower Upper

83 100

55 74.8 57.8 86.8

98 54.6 39.4 59.2

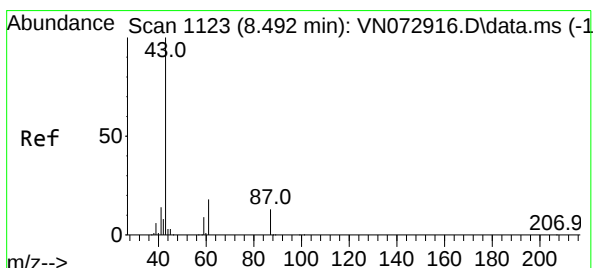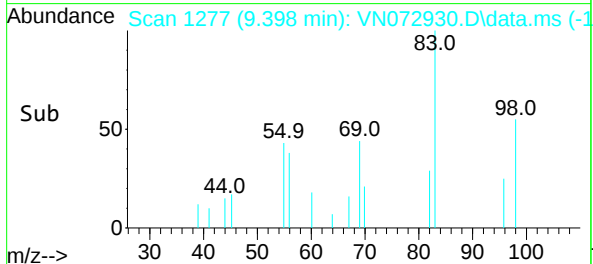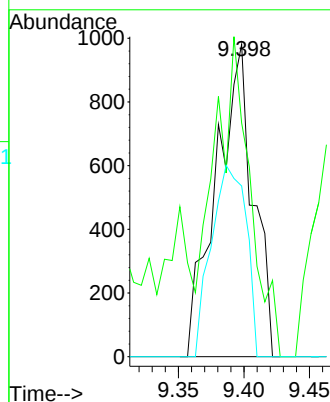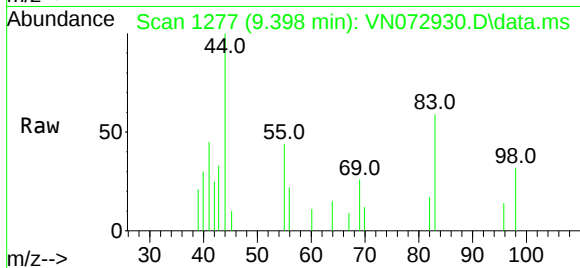

#43

Isopropyl Acetate

Concen: 4.064 ug/l

RT: 8.492 min Scan# 1123

Delta R.T. 0.000 min

Lab File: VN072930.D

Acq: 18 Jun 2022 11:17




Tgt Ion: 43 Resp: 40978


Ion Ratio Lower Upper

43 100

61 19.1 21.9 32.9#

87 12.9 12.0 18.0

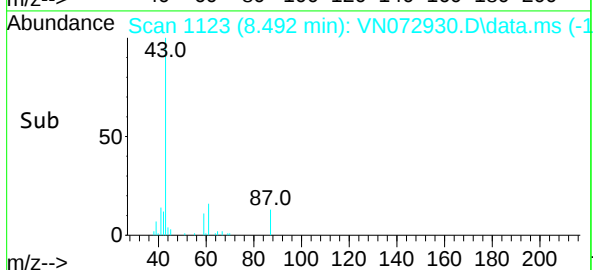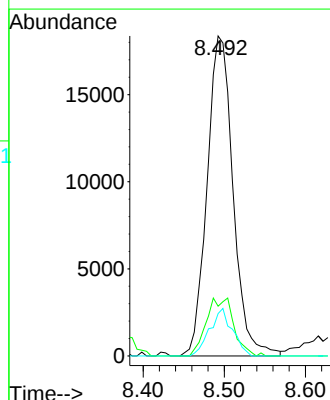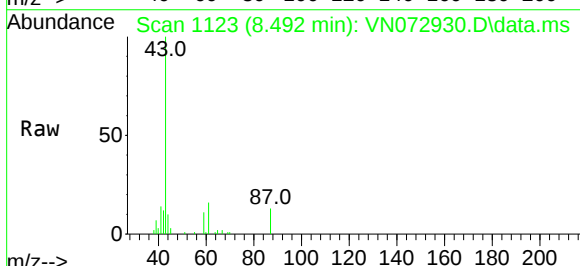

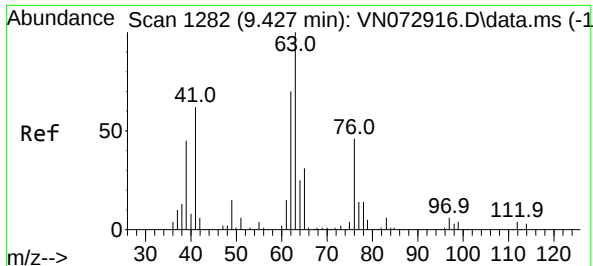

#45

1,2-Dichloropropane

Concen: 0.723 ug/l

RT: 9.557 min Scan# 11

Delta R.T. 0.130 min

Lab File: VN072930.D

Acq: 18 Jun 2022 11:17

Instrument :

MSVOA_N

ClientSampleId :





WC-14A-1A-8-GR

Tgt Ion: 63 Resp: 2563

Ion Ratio Lower Upper

63 100

65 0.0 24.9 37.3#

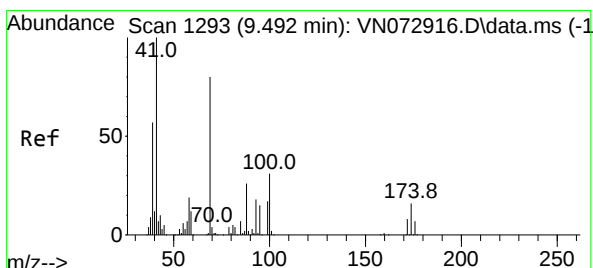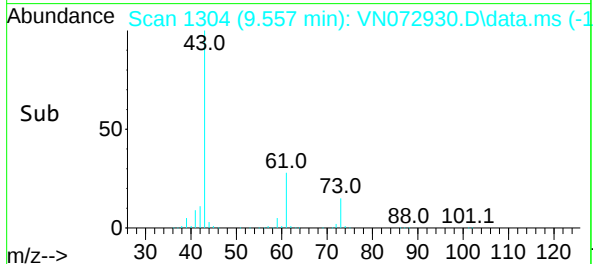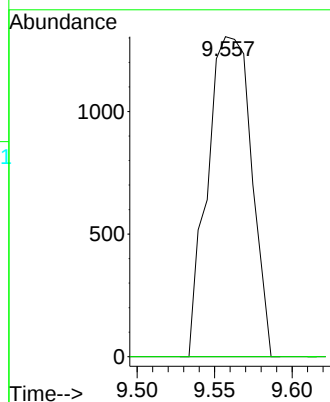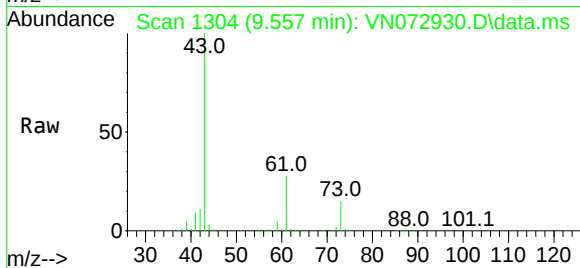

#48

Methyl methacrylate

Concen: 4.099 ug/l

RT: 9.475 min Scan# 1290

Delta R.T. -0.018 min

Lab File: VN072930.D

Acq: 18 Jun 2022 11:17




Tgt Ion: 41 Resp: 18873


Ion Ratio Lower Upper

41 100

69 0.3 74.7 112.1#

39 29.0 45.6 68.4#

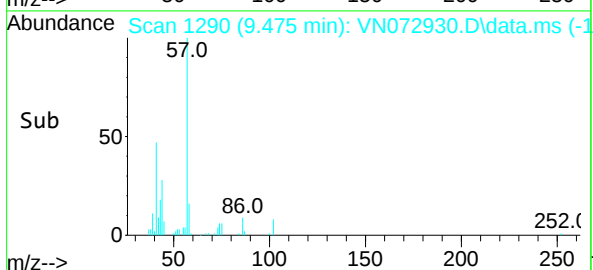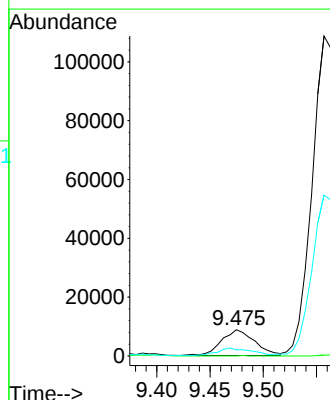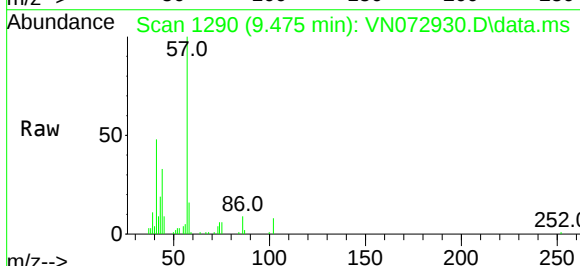

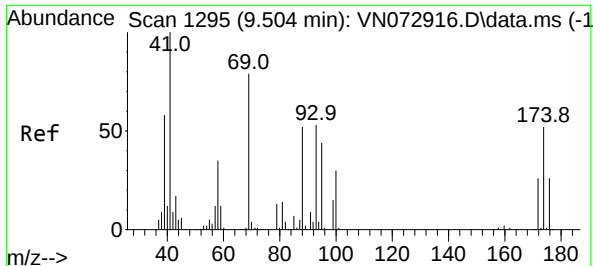

#49

1,4-Dioxane

Concen: 1.593 ug/l

RT: 9.563 min Scan# 11

Delta R.T. 0.059 min

Lab File: VN072930.D

Acq: 18 Jun 2022 11:17

Instrument :

MSVOA_N

ClientSampleId :

WC-14A-1A-8-GR





Tgt Ion: 88 Resp: 165

Ion Ratio Lower Upper

88 100

43 1309784.2 20.2 30.4#

58 5056.4 54.2 81.4#

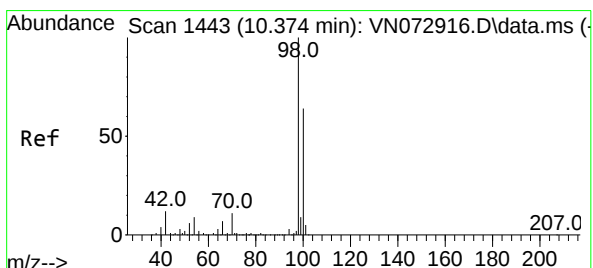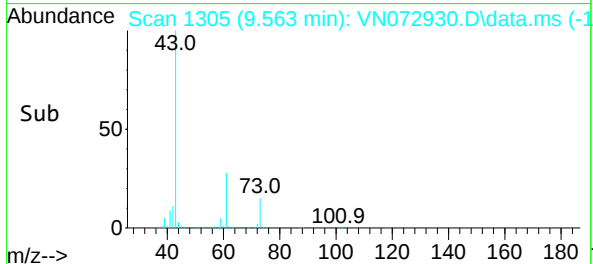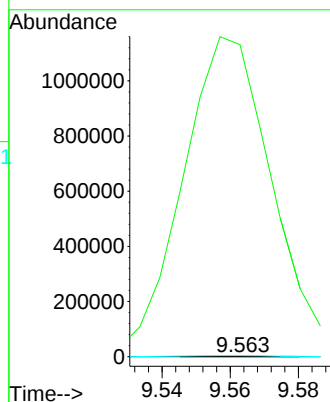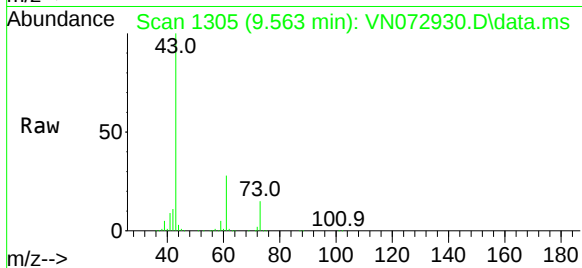

#50

Toluene-d8

Concen: 42.811 ug/l

RT: 10.375 min Scan# 1443

Delta R.T. 0.000 min

Lab File: VN072930.D




Acq: 18 Jun 2022 11:17


Tgt Ion: 98 Resp: 519212

Ion Ratio Lower Upper

98 100

100 66.0 52.6 78.8


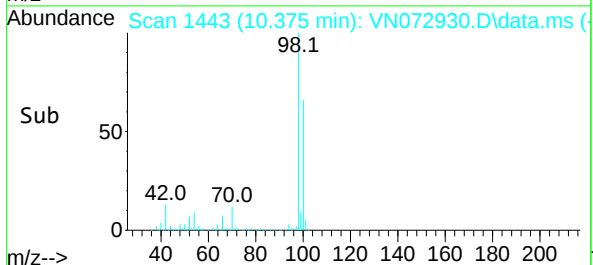
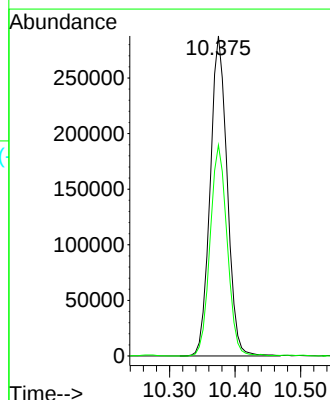
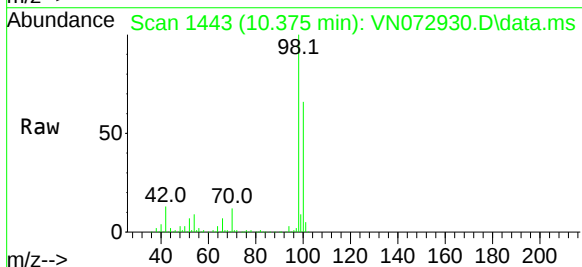


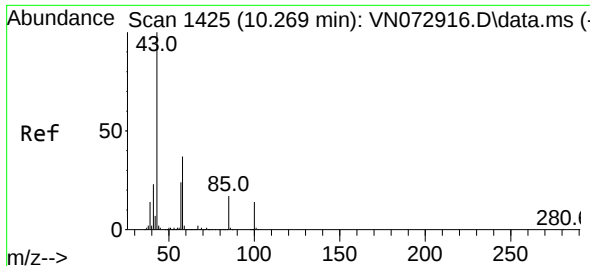

#51
4-Methyl-2-Pentanone
Concen: 1.626 ug/l
RT: 10.269 min Scan# 1425
Delta R.T. 0.000 min
Lab File: VN072930.D
Acq: 18 Jun 2022 11:17




Instrument :
MSVOA_N
ClientSampleId :
WC-14A-1A-8-GR


Tgt Ion: 43 Resp: 10689
Ion Ratio Lower Upper
43 100
58 40.4 34.1 51.1

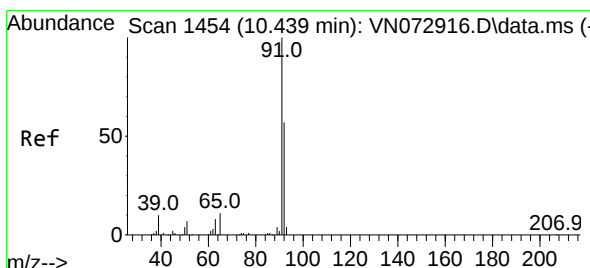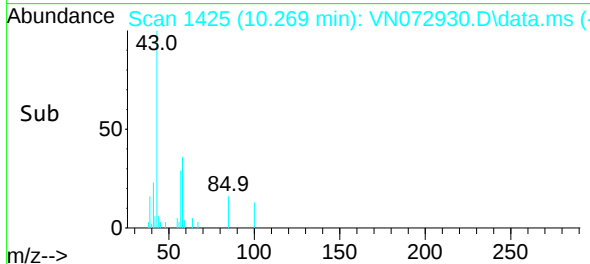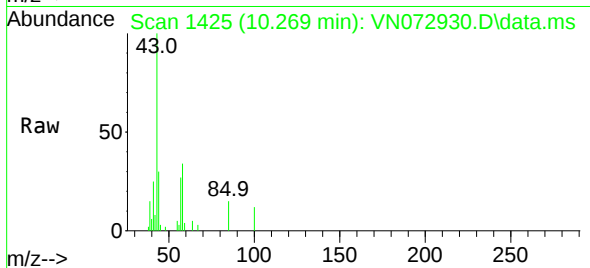

#52
Toluene
Concen: 0.348 ug/l
RT: 10.439 min Scan# 1454
Delta R.T. 0.000 min
Lab File: VN072930.D
Acq: 18 Jun 2022 11:17

Tgt Ion: 92 Resp: 2964
Ion Ratio Lower Upper
92 100
91 160.0 138.6 207.8


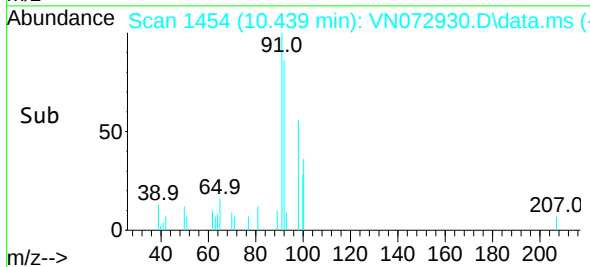

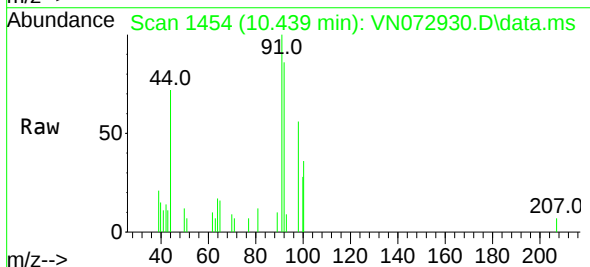


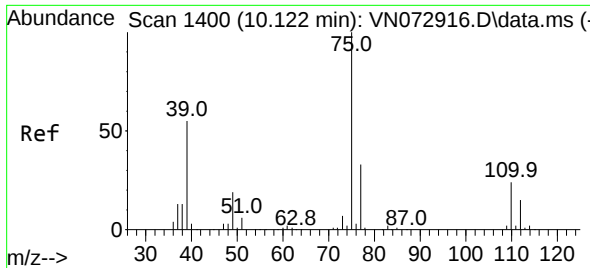

#54
cis-1,3-Dichloropropene
Concen: 9.162 ug/l
RT: 10.180 min Scan# 1400
Delta R.T. 0.059 min
Lab File: VN072930.D
Acq: 18 Jun 2022 11:17




Instrument :
MSVOA_N
ClientSampleId :
WC-14A-1A-8-GR


Tgt Ion: 75 Resp: 51241
Ion Ratio Lower Upper
75 100
77 0.6 25.2 37.8#
39 31.5 35.7 53.5#

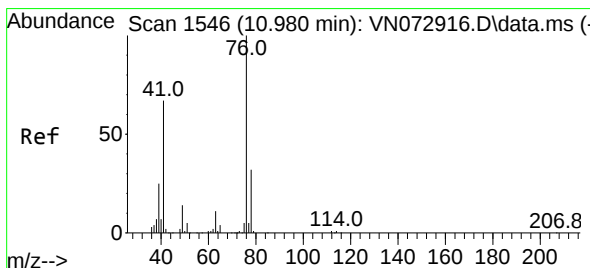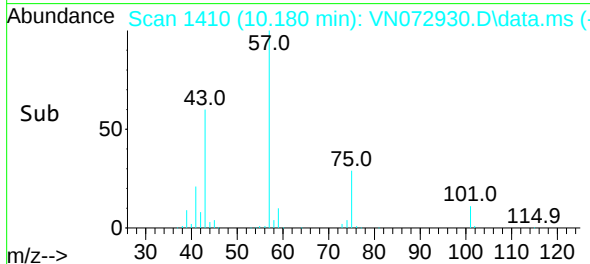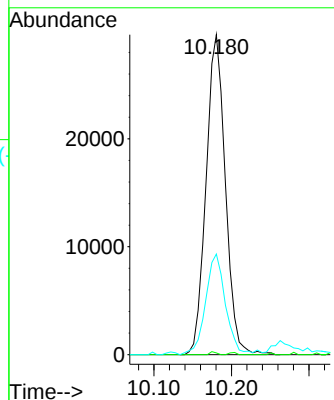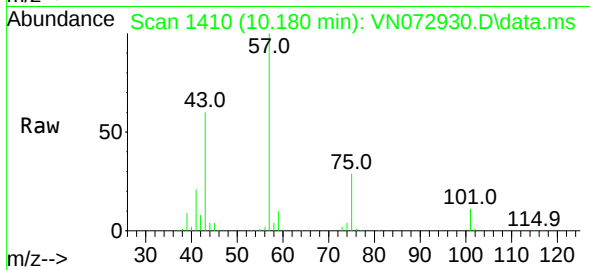

#57
1,3-Dichloropropane
Concen: 4.497 ug/l
RT: 11.027 min Scan# 1554
Delta R.T. 0.047 min
Lab File: VN072930.D
Acq: 18 Jun 2022 11:17

Tgt Ion: 76 Resp: 27873
Ion Ratio Lower Upper
76 100
78 0.2 26.2 39.2#


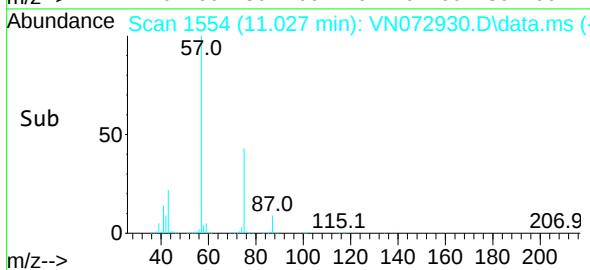
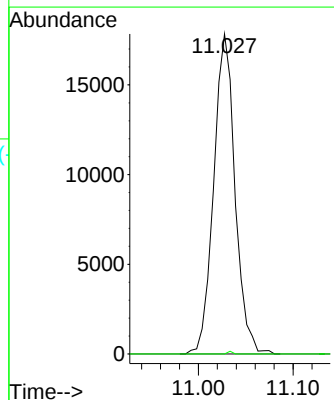
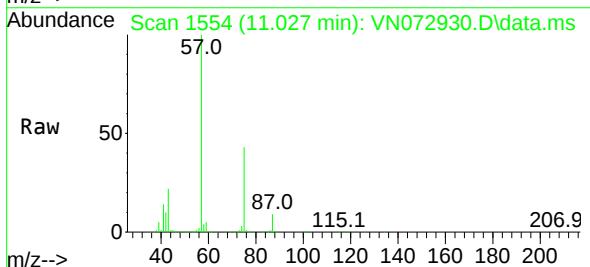




#59
2-Hexanone
Concen: 84.318 ug/l
RT: 11.027 min Scan# 11
Delta R.T. 0.006 min
Lab File: VN072930.D
Acq: 18 Jun 2022 11:17




Instrument :
MSVOA_N
ClientSampleId :
WC-14A-1A-8-GR


Tgt Ion: 43 Resp: 428829
Ion Ratio Lower Upper
43 100
58 18.0 29.7 89.1#

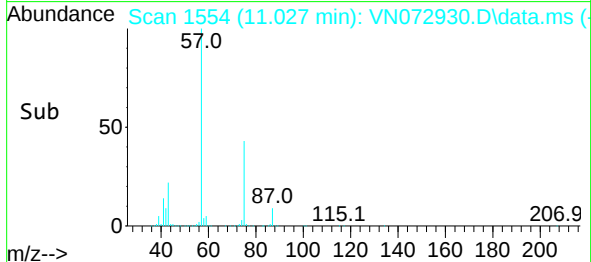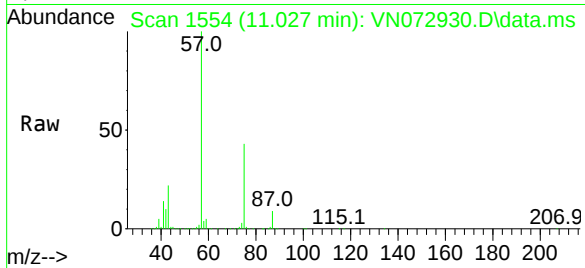

#62
4-Bromofluorobenzene
Concen: 43.188 ug/l
RT: 12.663 min Scan# 1832
Delta R.T. -0.006 min
Lab File: VN072930.D
Acq: 18 Jun 2022 11:17

Tgt Ion: 95 Resp: 188344
Ion Ratio Lower Upper
95 100
174 76.3 0.0 167.6
176 73.9 0.0 163.4




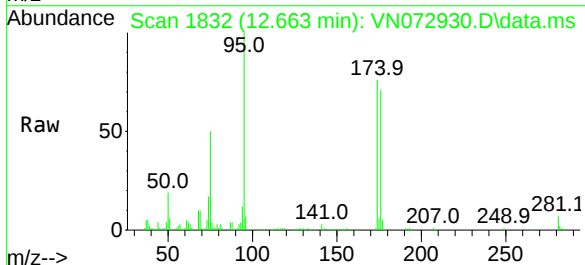




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.680 min Scan# 1170
Delta R.T. 0.000 min
Lab File: VN072930.D
Acq: 18 Jun 2022 11:17




Instrument :
MSVOA_N
ClientSampleId :
WC-14A-1A-8-GR


Tgt Ion:117 Resp: 462083
Ion Ratio Lower Upper
117 100
82 55.3 44.2 66.2
119 31.2 25.4 38.0

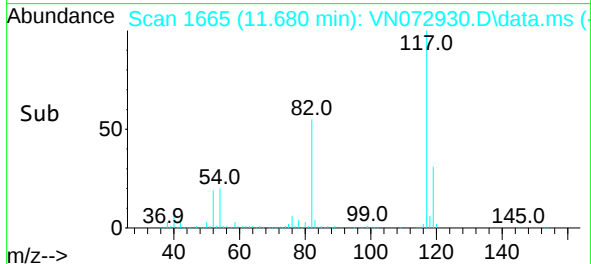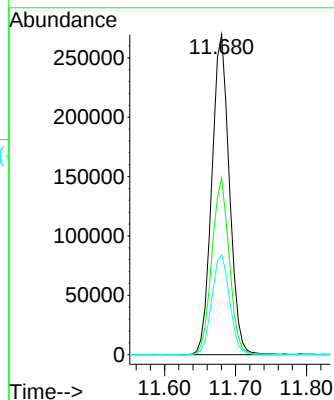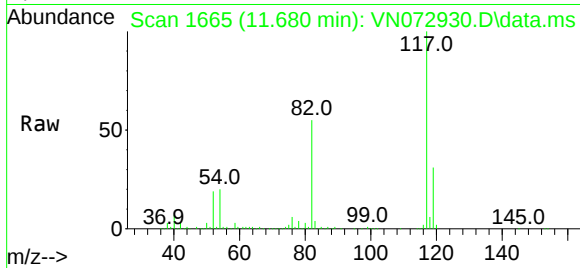

#68
m/p-Xylenes
Concen: 1.027 ug/l
RT: 11.886 min Scan# 1700
Delta R.T. 0.000 min
Lab File: VN072930.D
Acq: 18 Jun 2022 11:17

Tgt Ion:106 Resp: 6396
Ion Ratio Lower Upper
106 100
91 223.6 158.9 238.3


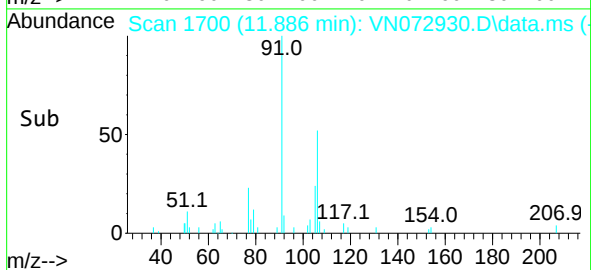
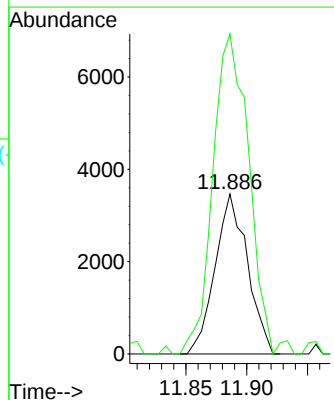
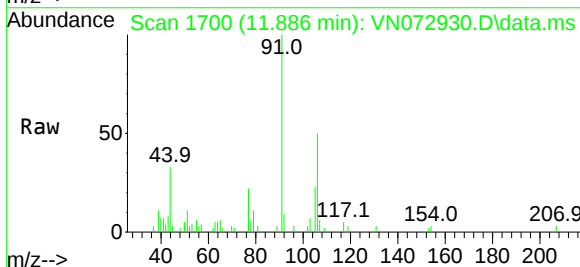


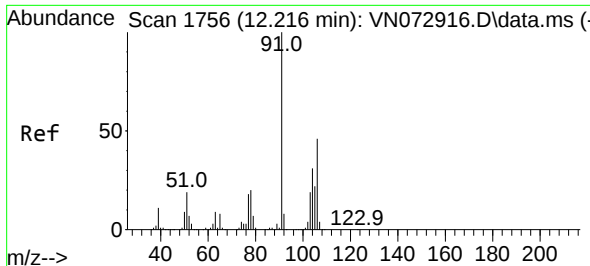

#69
o-Xylene
Concen: 1.619 ug/l
RT: 12.216 min Scan# 1756
Delta R.T. 0.000 min
Lab File: VN072930.D
Acq: 18 Jun 2022 11:17




Instrument :
MSVOA_N
ClientSampleId :
WC-14A-1A-8-GR


Tgt Ion:106 Resp: 10080
Ion Ratio Lower Upper
106 100
91 218.4 106.0 318.0

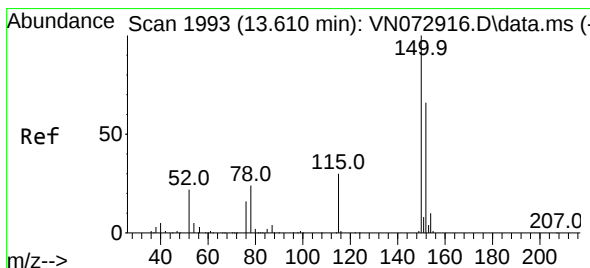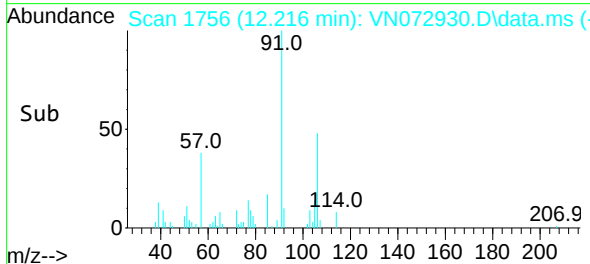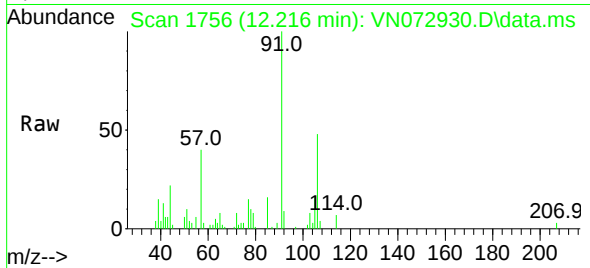

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.610 min Scan# 1993
Delta R.T. 0.000 min
Lab File: VN072930.D
Acq: 18 Jun 2022 11:17

Tgt Ion:152 Resp: 207002
Ion Ratio Lower Upper
152 100
115 62.0 28.9 86.7
150 154.3 0.0 356.2


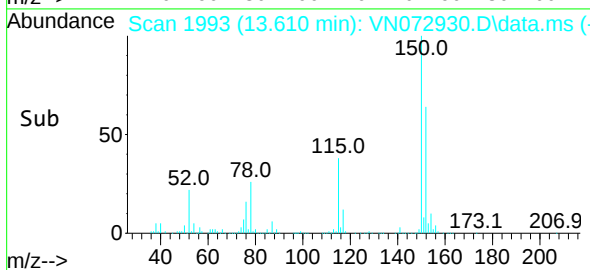

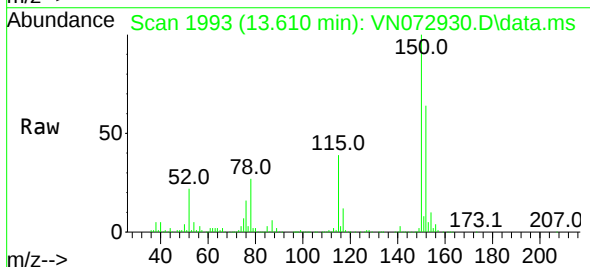




#73
Isopropylbenzene
Concen: 0.331 ug/l
RT: 12.516 min Scan# 1767
Delta R.T. 0.000 min
Lab File: VN072930.D
Acq: 18 Jun 2022 11:17




Instrument :
MSVOA_N
ClientSampleId :
WC-14A-1A-8-GR


Tgt Ion:105 Resp: 5297
Ion Ratio Lower Upper
105 100
120 21.7 13.5 40.4

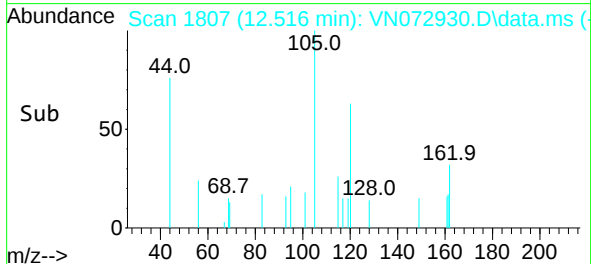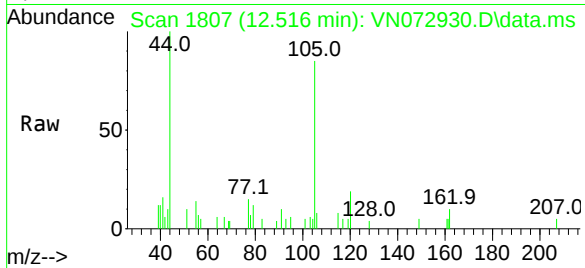

#74
N-ethyl acetate
Concen: 0.939 ug/l
RT: 12.286 min Scan# 1768
Delta R.T. -0.041 min
Lab File: VN072930.D
Acq: 18 Jun 2022 11:17

Tgt Ion: 43 Resp: 7803
Ion Ratio Lower Upper
43 100
70 0.0 39.0 58.4#
55 1.9 21.1 31.7#
61 0.0 21.1 31.7#




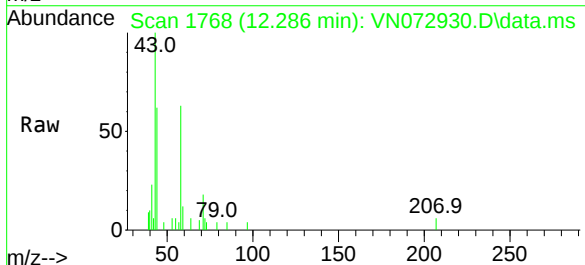




#76
1,2,3-Trichloropropane
Concen: 19.074 ug/l
RT: 12.669 min Scan# 1833
Delta R.T. -0.147 min
Lab File: VN072930.D
Acq: 18 Jun 2022 11:17




Instrument :
MSVOA_N
ClientSampleId :
WC-14A-1A-8-GR


Tgt Ion: 75 Resp: 95728
Ion Ratio Lower Upper
75 100
77 2.1 98.5 295.5#

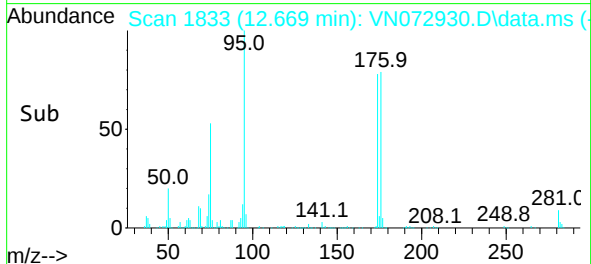

#80
1,3,5-Trimethylbenzene
Concen: 0.454 ug/l
RT: 12.998 min Scan# 1889
Delta R.T. 0.000 min
Lab File: VN072930.D
Acq: 18 Jun 2022 11:17

Tgt Ion:105 Resp: 5976
Ion Ratio Lower Upper
105 100
120 50.9 24.9 74.7









#81
trans-1,4-Dichloro-2-butene
Concen: 51.512 ug/l
RT: 12.669 min Scan# 1815
Delta R.T. 0.106 min
Lab File: VN072930.D
Acq: 18 Jun 2022 11:17




Instrument :
MSVOA_N
ClientSampleId :
WC-14A-1A-8-GR


Tgt Ion: 75 Resp: 95728
Ion Ratio Lower Upper
75 100
53 0.2 78.0 117.0#
89 0.2 37.2 55.8#

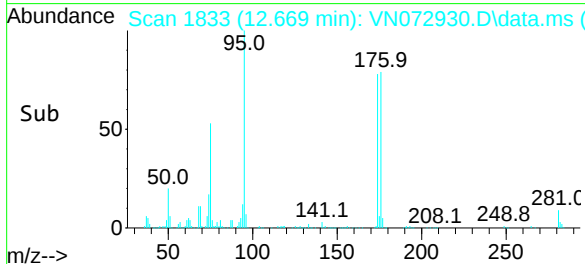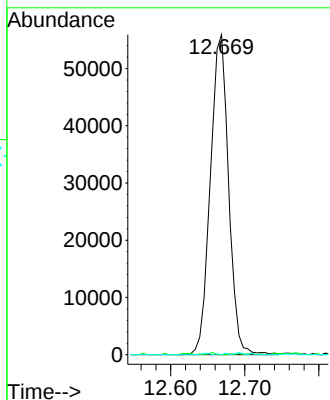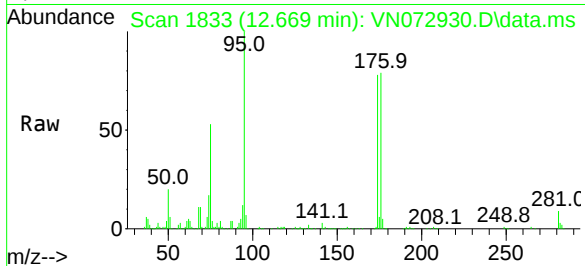

#84
1,2,4-Trimethylbenzene
Concen: 1.989 ug/l
RT: 13.304 min Scan# 1941
Delta R.T. 0.000 min
Lab File: VN072930.D
Acq: 18 Jun 2022 11:17


Tgt Ion: 105 Resp: 26063
Ion Ratio Lower Upper
105 100
120 41.0 23.3 69.8

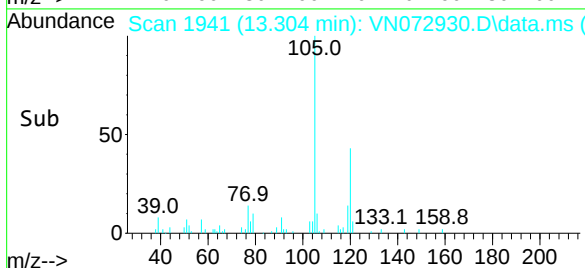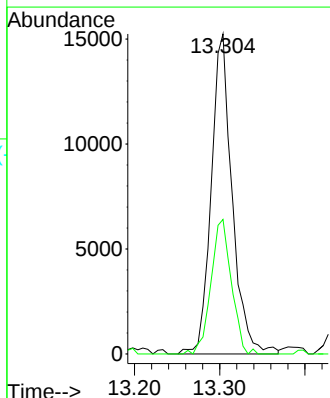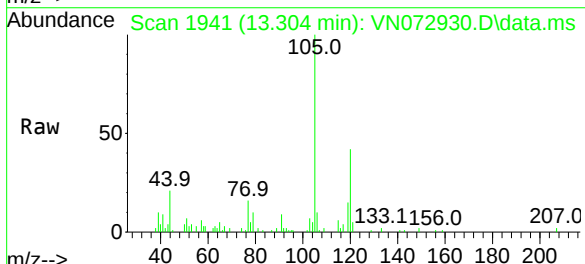

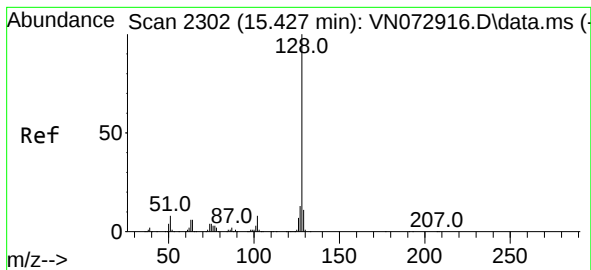

#95
Naphthalene
Concen: 0.801 ug/l
RT: 15.421 min Scan# 21
Delta R.T. -0.006 min
Lab File: VN072930.D
Acq: 18 Jun 2022 11:17

Instrument :
MSVOA_N
ClientSampleId :
WC-14A-1A-8-GR

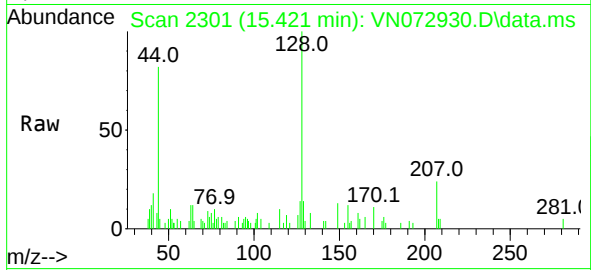

Tgt Ion:128 Resp: 12810
Ion Ratio Lower Upper
128 100
127 14.8 10.3 15.5
129 0.0 8.6 13.0#

