

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061822\
 Data File : VN072940.D
 Acq On : 18 Jun 2022 15:20
 Operator : JC\MD
 Sample : N3304-09
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 WC-14A-1A-9

Quant Time: Jun 20 08:05:04 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N061722W.M
 Quant Title : SW846 8260
 QLast Update : Sat Jun 18 06:22:45 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.016	168	326386	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.904	114	528082	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.680	117	475517	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.610	152	223819	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.369	65	243001	55.069	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery = 110.140%			
35) Dibromofluoromethane	7.951	113	202112	61.921	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 123.840%			
50) Toluene-d8	10.375	98	587733	48.391	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery = 96.780%			
62) 4-Bromofluorobenzene	12.669	95	246477	56.436	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 112.880%			
Target Compounds						Qvalue
3) Chloromethane	2.269	50	453	0.703	ug/l #	43
11) Tert butyl alcohol	5.293	59	1124	0.986	ug/l #	72
13) Acrolein	3.981	56	138	0.307	ug/l #	1
16) Acetone	4.234	43	91094	37.555	ug/l	99
18) Methyl Acetate	4.787	43	9350	1.448	ug/l #	65
20) Methylene Chloride	5.022	84	57280	15.056	ug/l	94
25) 2-Butanone	7.275	43	36746	9.547	ug/l	96
26) 2,2-Dichloropropane	7.228	77	2437	Below Cal	#	53
31) Cyclohexane	8.016	56	8323	1.394	ug/l #	18
36) 1,1-Dichloropropene	8.010	75	26557	6.013	ug/l #	48
37) Ethyl Acetate	7.275	43	36746	5.202	ug/l #	67
38) Carbon Tetrachloride	8.016	117	33421	7.194	ug/l #	15
39) Methylcyclohexane	9.398	83	1669	0.314	ug/l #	85
40) Benzene	8.387	78	5942	0.428	ug/l	99
43) Isopropyl Acetate	8.498	43	36635	3.628	ug/l #	88
45) 1,2-Dichloropropane	9.557	63	2395	0.675	ug/l #	44
48) Methyl methacrylate	9.475	41	13938	3.023	ug/l #	26
49) 1,4-Dioxane	9.557	88	80	0.771	ug/l #	1
51) 4-Methyl-2-Pentanone	10.269	43	16703	2.536	ug/l #	67
52) Toluene	10.439	92	2782	0.326	ug/l	94
54) cis-1,3-Dichloropropene	10.181	75	36378	6.495	ug/l #	62
57) 1,3-Dichloropropane	11.022	76	19654	3.166	ug/l #	42
59) 2-Hexanone	11.028	43	294495	57.821	ug/l #	45
67) Ethyl Benzene	11.780	91	5236	0.320	ug/l #	83
68) m/p-Xylenes	11.892	106	3794	0.592	ug/l	90
69) o-Xylene	12.216	106	7404	1.156	ug/l	99
73) Isopropylbenzene	12.516	105	4057	0.234	ug/l	86
74) N-amyl acetate	12.292	43	3830	0.426	ug/l #	42
76) 1,2,3-Trichloropropane	12.669	75	125145	23.062	ug/l #	1
80) 1,3,5-Trimethylbenzene	12.992	105	6017	0.423	ug/l	95
81) trans-1,4-Dichloro-2-b...	12.669	75	125145	62.282	ug/l #	11
84) 1,2,4-Trimethylbenzene	13.304	105	19578	1.382	ug/l	90
90) Hexachloroethane	14.151	117	604	0.228	ug/l #	9
92) 1,2-Dibromo-3-Chloropr...	14.516	75	71	Below Cal	#	1
95) Naphthalene	15.427	128	39545	2.287	ug/l	98

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061822\
Data File : VN072940.D
Acq On : 18 Jun 2022 15:20
Operator : JC\MD
Sample : N3304-09
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
WC-14A-1A-9

Quant Time: Jun 20 08:05:04 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N061722W.M
Quant Title : SW846 8260
QLast Update : Sat Jun 18 06:22:45 2022
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061822\
 Data File : VN072940.D
 Acq On : 18 Jun 2022 15:20
 Operator : JC\MD
 Sample : N3304-09
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 WC-14A-1A-9

Quant Time: Jun 20 08:05:04 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N061722W.M
 Quant Title : SW846 8260
 QLast Update : Sat Jun 18 06:22:45 2022
 Response via : Initial Calibration




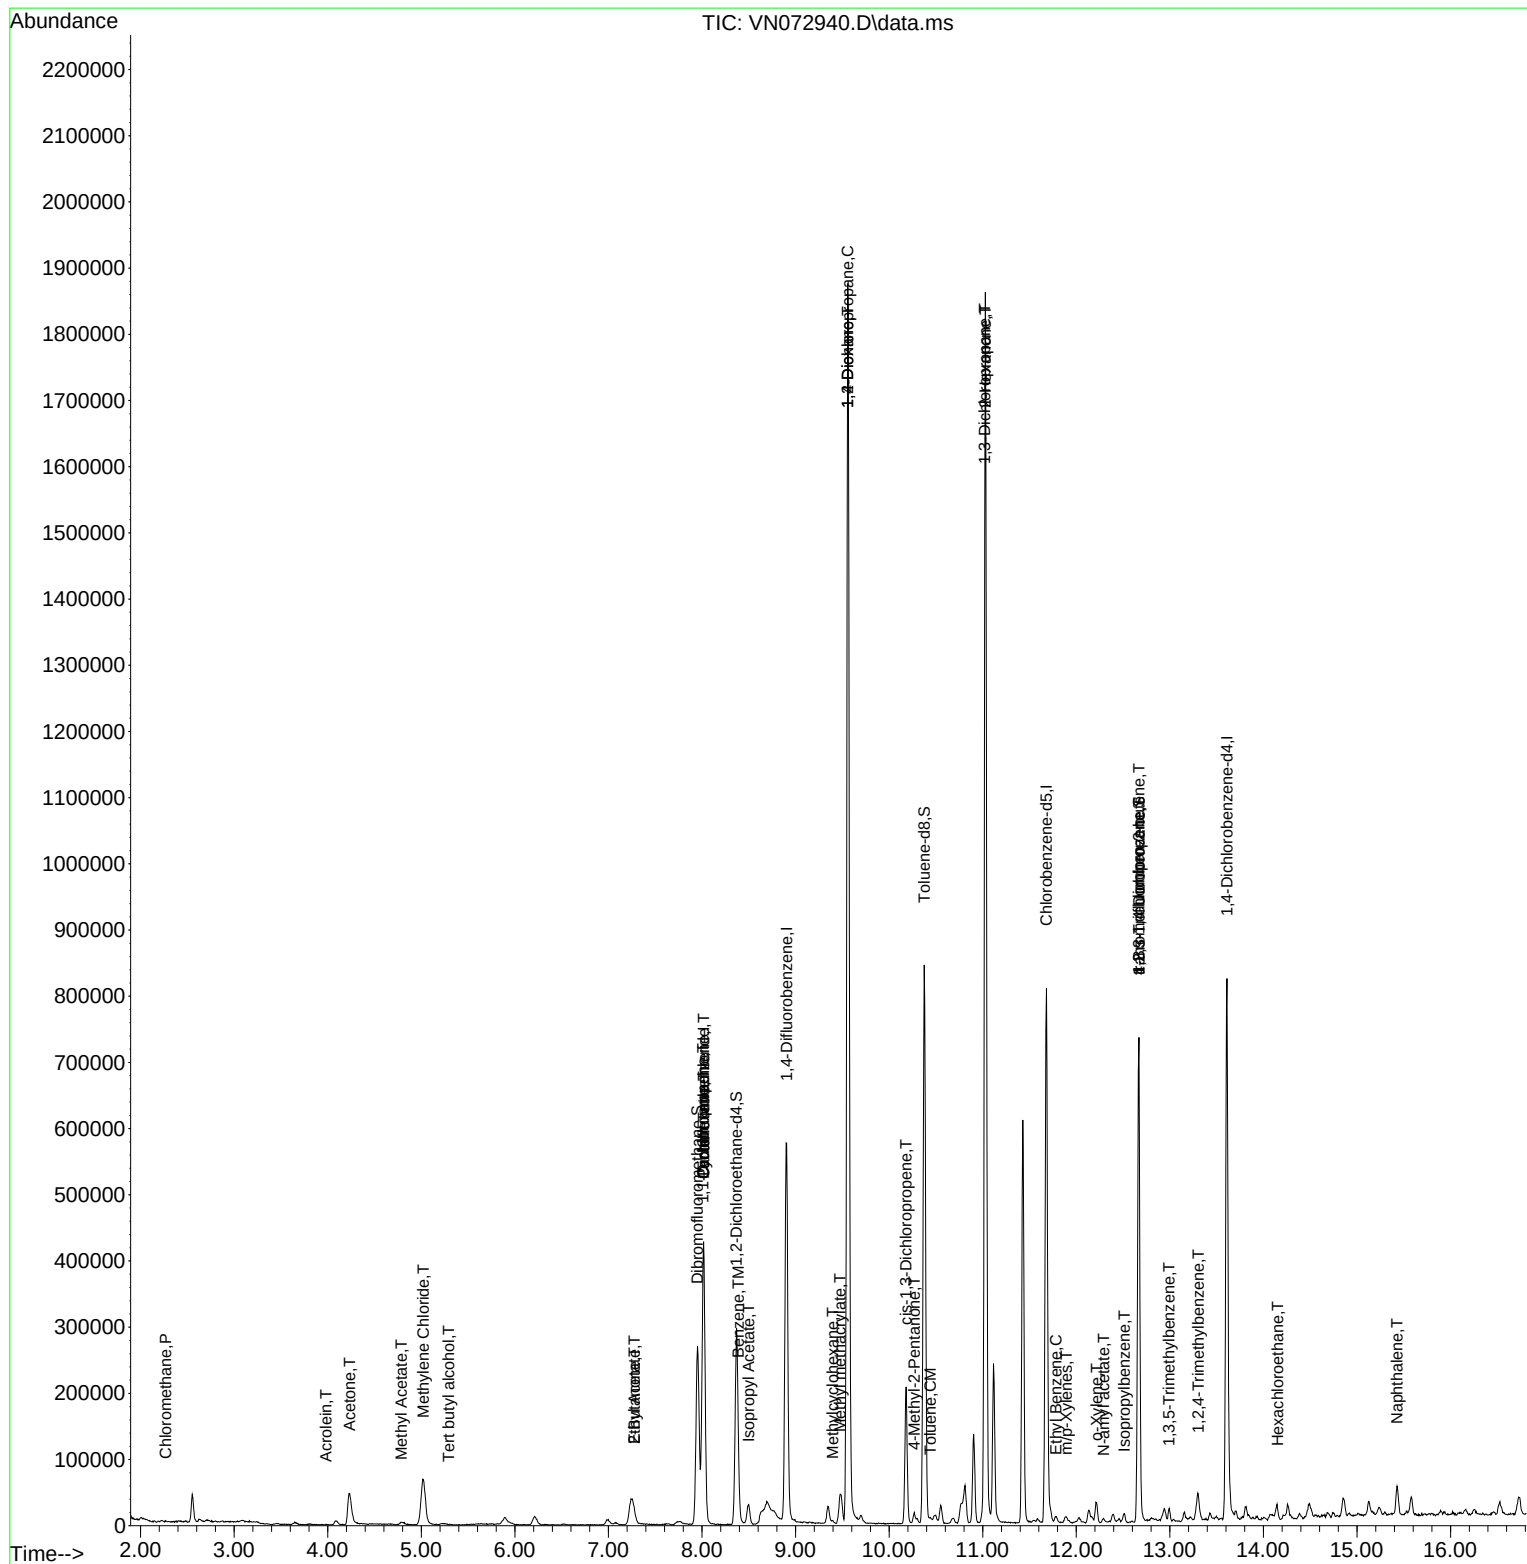




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.016 min Scan# 1042
Delta R.T. -0.000 min
Lab File: VN072940.D
Acq: 18 Jun 2022 15:20




Instrument :
MSVOA_N
ClientSampleId :
WC-14A-1A-9


Tgt Ion:168 Resp: 326386
Ion Ratio Lower Upper
168 100
99 59.1 42.3 63.5

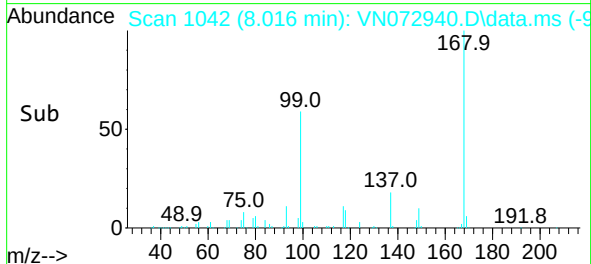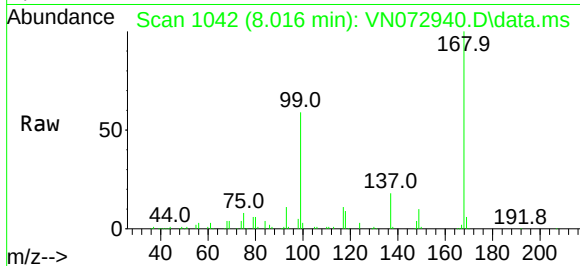

#3
Chloromethane
Concen: 0.703 ug/l
RT: 2.269 min Scan# 65
Delta R.T. 0.006 min
Lab File: VN072940.D
Acq: 18 Jun 2022 15:20

Tgt Ion: 50 Resp: 453
Ion Ratio Lower Upper
50 100
52 0.0 25.7 38.5


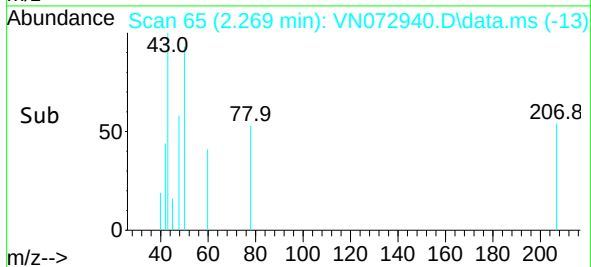

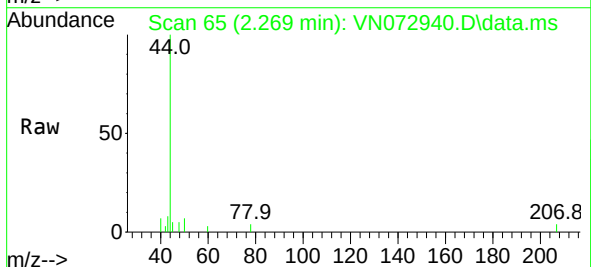




#11
Tert butyl alcohol
Concen: 0.986 ug/l
RT: 5.293 min Scan# 511
Delta R.T. -0.012 min
Lab File: VN072940.D
Acq: 18 Jun 2022 15:20




Instrument :
MSVOA_N
ClientSampleId :
WC-14A-1A-9


Tgt Ion: 59 Resp: 1124
Ion Ratio Lower Upper
59 100
57 0.0 8.3 12.5#

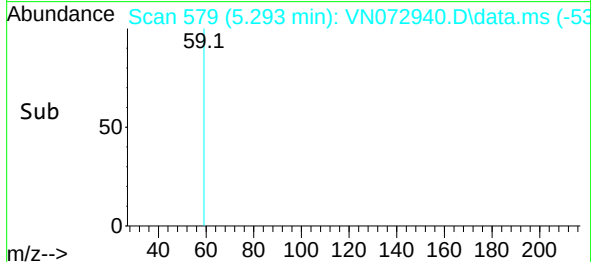

#13
Acrolein
Concen: 0.307 ug/l
RT: 3.981 min Scan# 356
Delta R.T. 0.000 min
Lab File: VN072940.D
Acq: 18 Jun 2022 15:20

Tgt Ion: 56 Resp: 138
Ion Ratio Lower Upper
56 100
55 158.7 54.8 82.2#


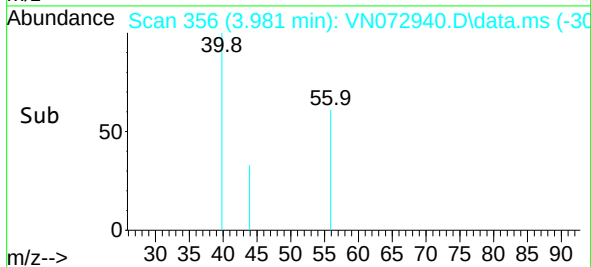

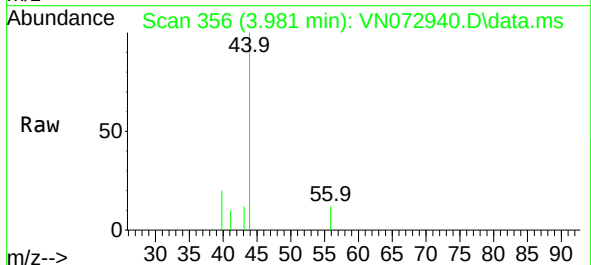




#16
Acetone
Concen: 37.555 ug/l
RT: 4.234 min Scan# 399
Delta R.T. 0.006 min
Lab File: VN072940.D
Acq: 18 Jun 2022 15:20




Instrument :
MSVOA_N
ClientSampleId :
WC-14A-1A-9


Tgt Ion: 43 Resp: 91094
Ion Ratio Lower Upper
43 100
58 32.1 26.0 39.0

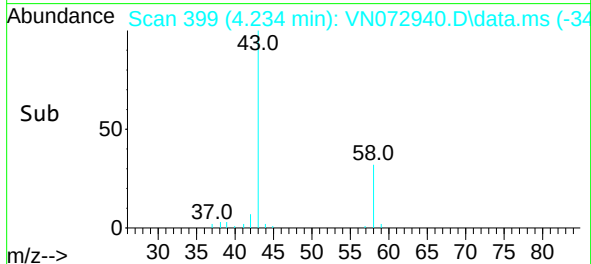

#18
Methyl Acetate
Concen: 1.448 ug/l
RT: 4.787 min Scan# 493
Delta R.T. 0.006 min
Lab File: VN072940.D
Acq: 18 Jun 2022 15:20

Tgt Ion: 43 Resp: 9350
Ion Ratio Lower Upper
43 100
74 9.1 21.6 32.4#


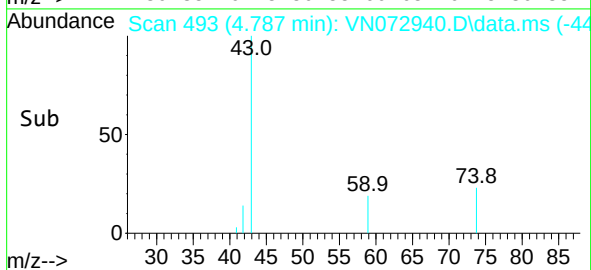

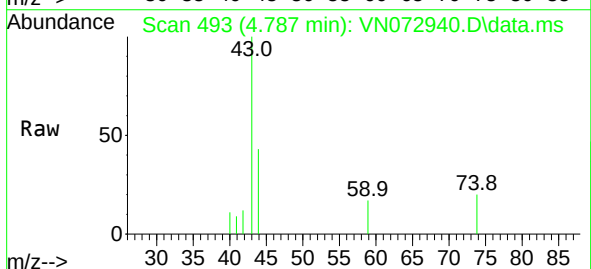


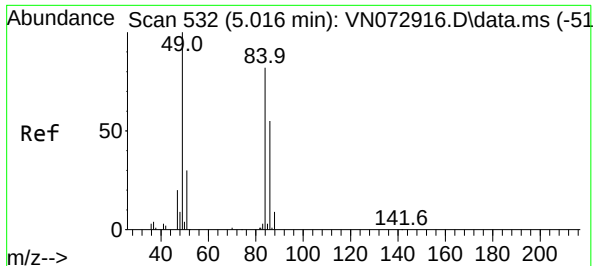

#20
Methylene Chloride
Concen: 15.056 ug/l
RT: 5.022 min Scan# 51
Delta R.T. 0.006 min
Lab File: VN072940.D
Acq: 18 Jun 2022 15:20




Instrument :
MSVOA_N
ClientSampleId :
WC-14A-1A-9


Tgt Ion:	84	Resp:	57280
Ion	Ratio	Lower	Upper
84	100		
49	122.7	88.3	132.5
51	35.2	28.2	42.2
86	63.5	50.6	76.0

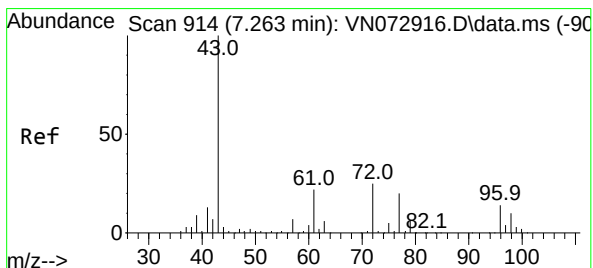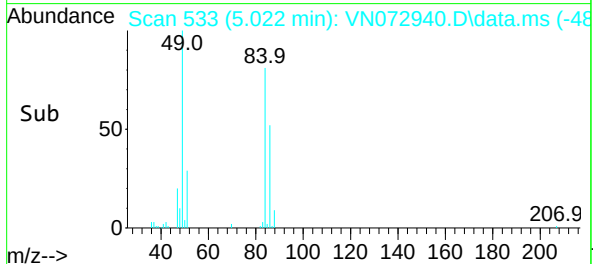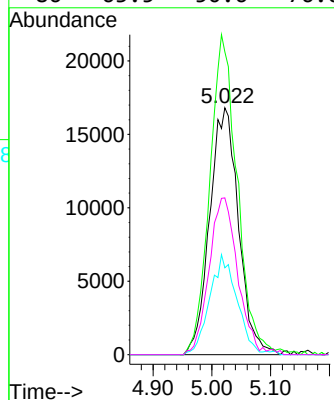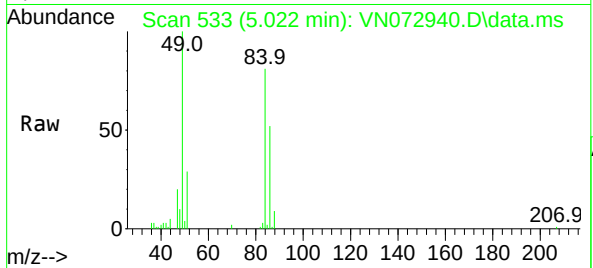

#25
2-Butanone
Concen: 9.547 ug/l
RT: 7.275 min Scan# 916
Delta R.T. 0.012 min
Lab File: VN072940.D
Acq: 18 Jun 2022 15:20

Tgt Ion:	43	Resp:	36746
Ion	Ratio	Lower	Upper
43	100		
72	27.7	23.7	35.5


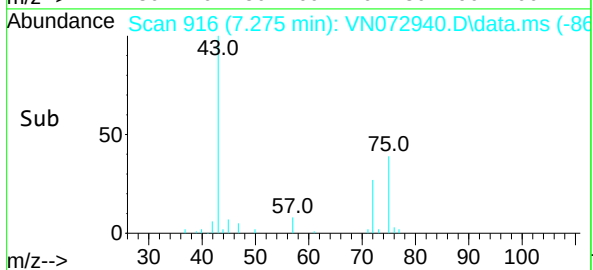
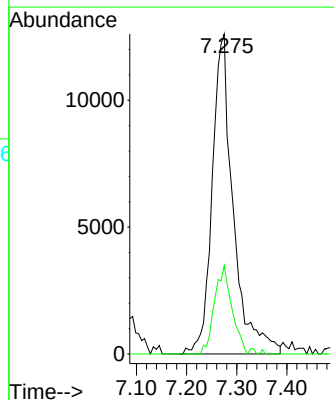
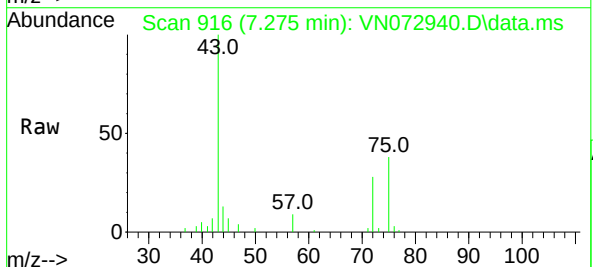


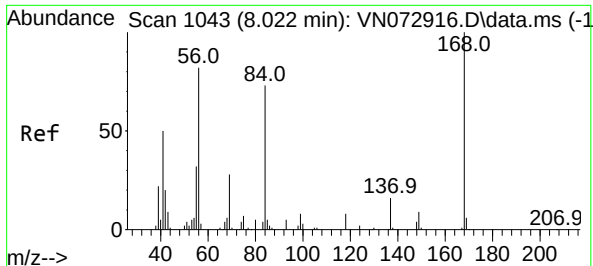

#31
Cyclohexane
Concen: 1.394 ug/l
RT: 8.016 min Scan# 1043
Delta R.T. -0.006 min
Lab File: VN072940.D
Acq: 18 Jun 2022 15:20




Instrument :
MSVOA_N
ClientSampleId :
WC-14A-1A-9


Tgt Ion: 56 Resp: 8323
Ion Ratio Lower Upper
56 100
69 152.9 27.8 41.8#
84 132.8 76.9 115.3#

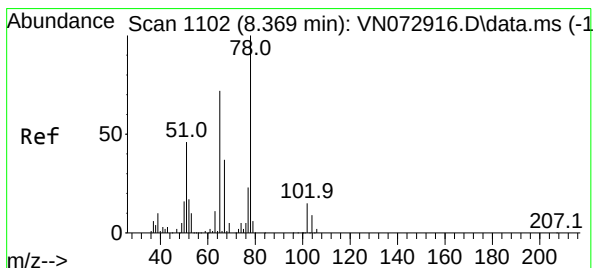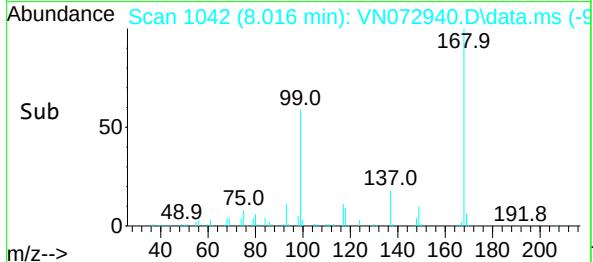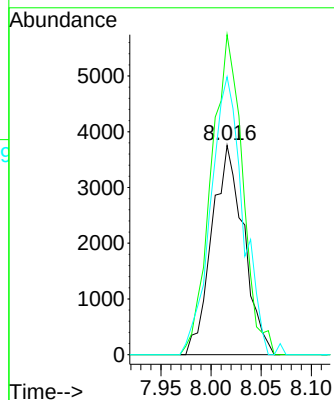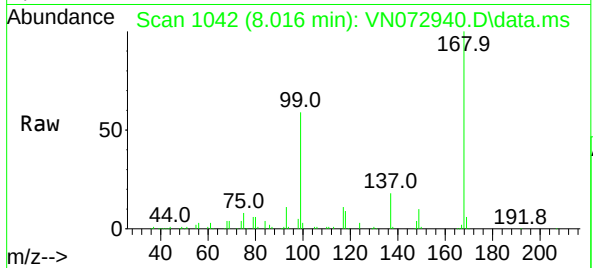

#33
1,2-Dichloroethane-d4
Concen: 55.069 ug/l
RT: 8.369 min Scan# 1102
Delta R.T. 0.000 min
Lab File: VN072940.D
Acq: 18 Jun 2022 15:20

Tgt Ion: 65 Resp: 243001
Ion Ratio Lower Upper
65 100
67 51.7 0.0 104.8

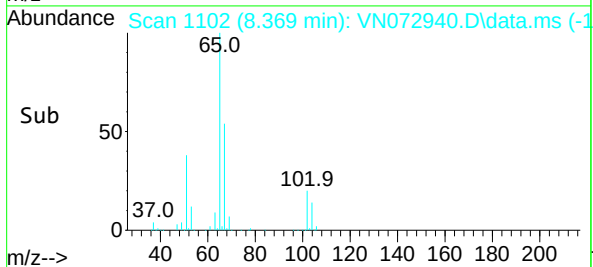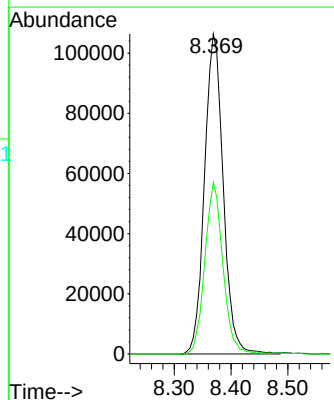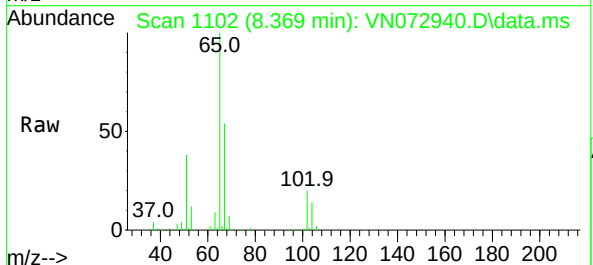



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.904 min Scan# 1192

Delta R.T. 0.006 min

Lab File: VN072940.D

Acq: 18 Jun 2022 15:20

Instrument :

MSVOA_N

ClientSampleId :

WC-14A-1A-9





Tgt Ion:114 Resp: 528082

Ion Ratio Lower Upper

114 100

63 18.5 0.0 40.0

88 15.2 0.0 32.6



#35

Dibromofluoromethane

Concen: 61.921 ug/l

RT: 7.951 min Scan# 1031

Delta R.T. 0.000 min

Lab File: VN072940.D

Acq: 18 Jun 2022 15:20




Tgt Ion:113 Resp: 202112


Ion Ratio Lower Upper

113 100

111 102.5 81.4 122.0

192 19.4 17.0 25.6

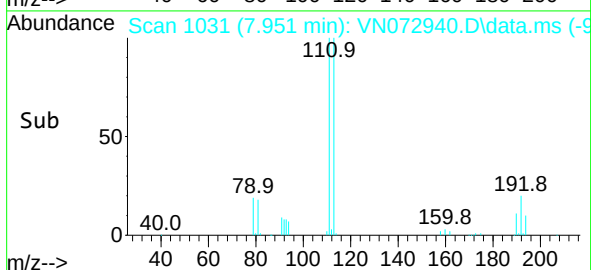



#36

1,1-Dichloropropene

Concen: 6.013 ug/l

RT: 8.010 min Scan# 1

Delta R.T. -0.141 min

Lab File: VN072940.D

Acq: 18 Jun 2022 15:20

Instrument :

MSVOA_N

ClientSampleId :

WC-14A-1A-9





Tgt Ion: 75 Resp: 26557

Ion Ratio Lower Upper

75 100

110 7.7 18.3 54.8#

77 0.0 25.1 37.7#

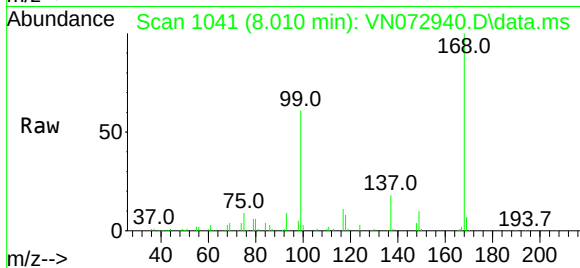

#37

Ethyl Acetate

Concen: 5.202 ug/l

RT: 7.275 min Scan# 916

Delta R.T. -0.070 min

Lab File: VN072940.D

Acq: 18 Jun 2022 15:20




Tgt Ion: 43 Resp: 36746


Ion Ratio Lower Upper

43 100

61 0.3 11.8 17.6#

70 0.0 9.3 13.9#


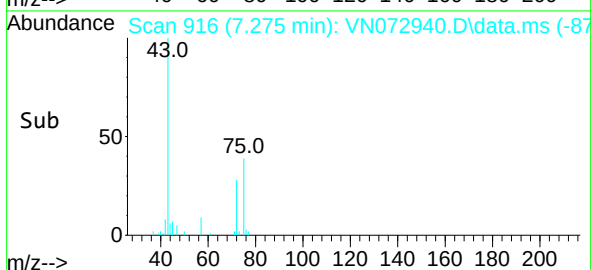

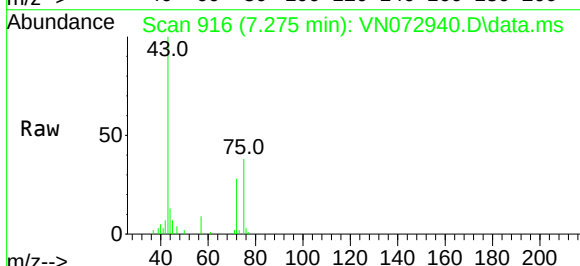


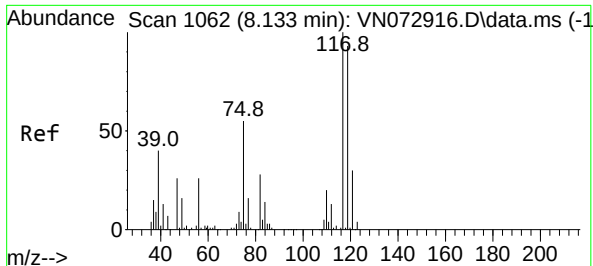

#38
Carbon Tetrachloride
Concen: 7.194 ug/l
RT: 8.016 min Scan# 1042
Delta R.T. -0.117 min
Lab File: VN072940.D
Acq: 18 Jun 2022 15:20




Instrument :
MSVOA_N
ClientSampleId :
WC-14A-1A-9


Tgt Ion:117 Resp: 33421
Ion Ratio Lower Upper
117 100
119 3.6 75.8 113.8#
121 0.0 24.6 37.0#

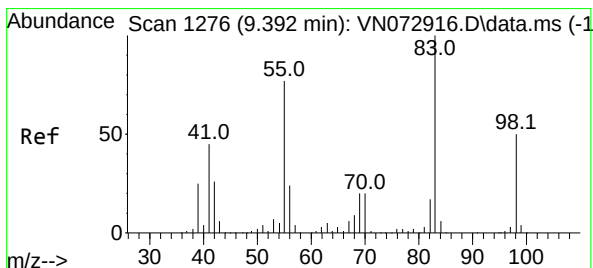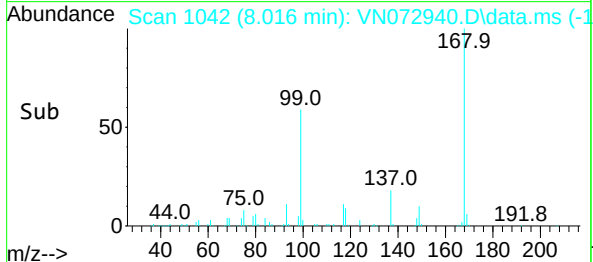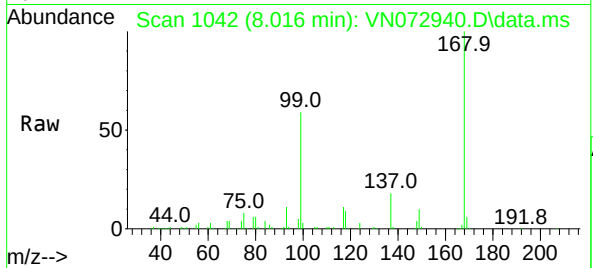

#39
Methylcyclohexane
Concen: 0.314 ug/l
RT: 9.398 min Scan# 1277
Delta R.T. 0.006 min
Lab File: VN072940.D
Acq: 18 Jun 2022 15:20

Tgt Ion: 83 Resp: 1669
Ion Ratio Lower Upper
83 100
55 74.1 57.8 86.8
98 72.4 39.4 59.2#

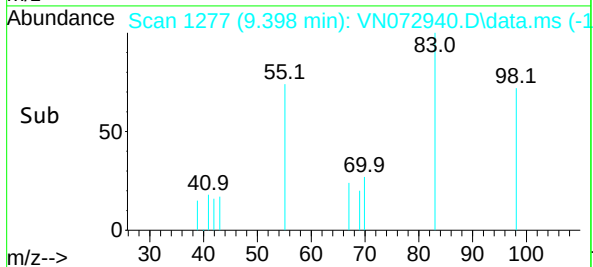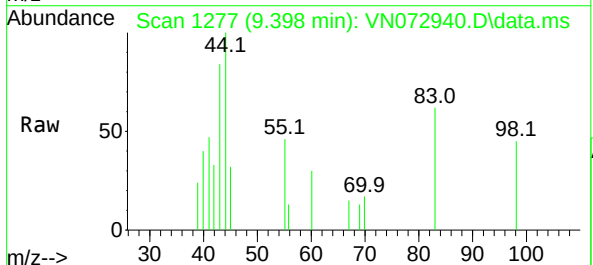

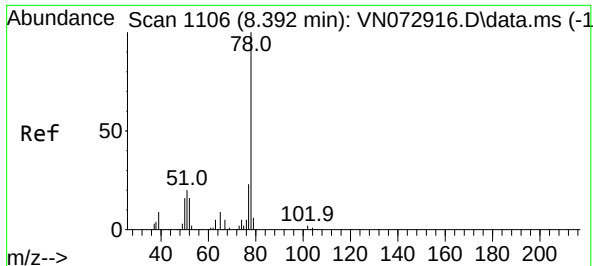

#40

Benzene

Concen: 0.428 ug/l

RT: 8.387 min Scan# 1105

Delta R.T. -0.006 min

Lab File: VN072940.D

Acq: 18 Jun 2022 15:20

Instrument :

MSVOA_N

ClientSampleId :





WC-14A-1A-9

Tgt Ion: 78 Resp: 5942

Ion Ratio Lower Upper

78 100

77 24.6 19.4 29.0

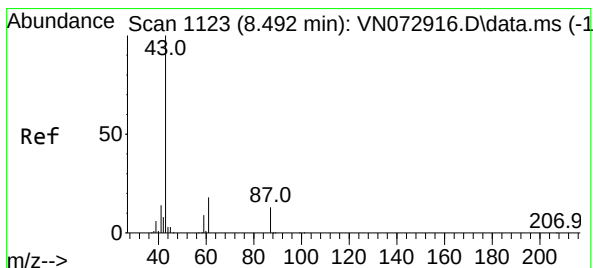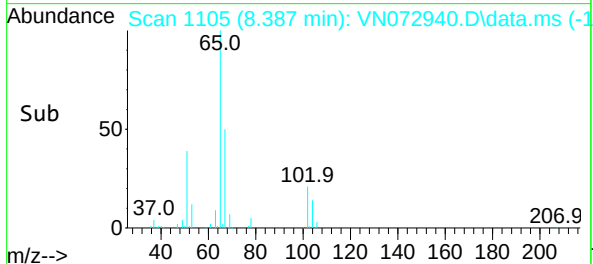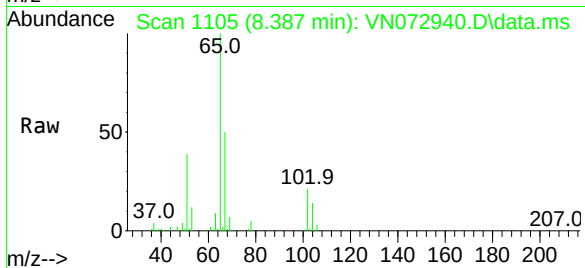

#43

Isopropyl Acetate

Concen: 3.628 ug/l

RT: 8.498 min Scan# 1124

Delta R.T. 0.006 min

Lab File: VN072940.D

Acq: 18 Jun 2022 15:20




Tgt Ion: 43 Resp: 36635


Ion Ratio Lower Upper

43 100

61 19.6 21.9 32.9#

87 12.0 12.0 18.0#

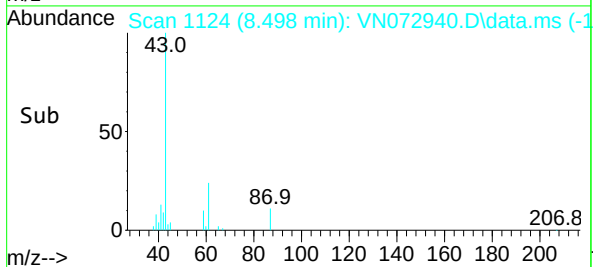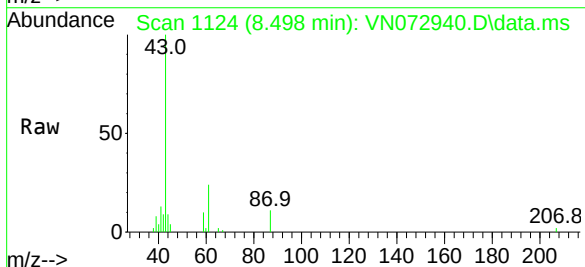

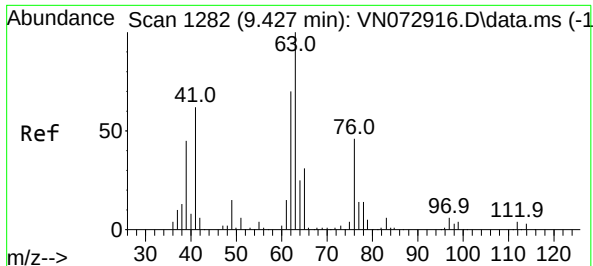

#45

1,2-Dichloropropane

Concen: 0.675 ug/l

RT: 9.557 min Scan# 11

Delta R.T. 0.130 min

Lab File: VN072940.D

Acq: 18 Jun 2022 15:20

Instrument :

MSVOA_N

ClientSampleId :





WC-14A-1A-9

Tgt Ion: 63 Resp: 2395

Ion Ratio Lower Upper

63 100

65 0.0 24.9 37.3#

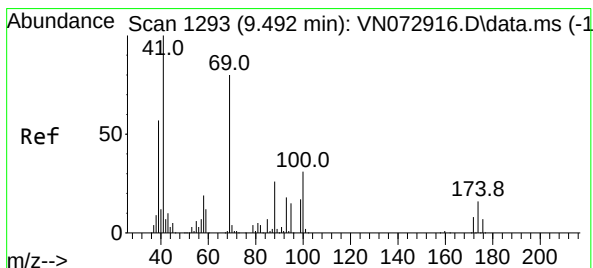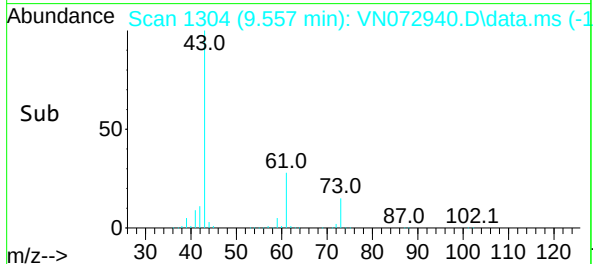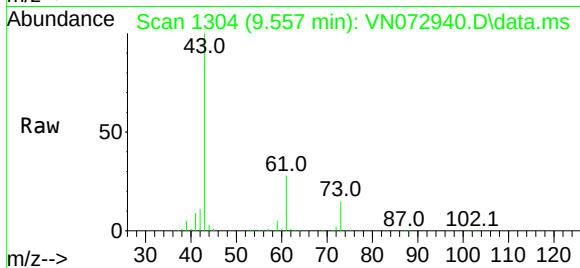

#48

Methyl methacrylate

Concen: 3.023 ug/l

RT: 9.475 min Scan# 1290

Delta R.T. -0.017 min

Lab File: VN072940.D

Acq: 18 Jun 2022 15:20




Tgt Ion: 41 Resp: 13938


Ion Ratio Lower Upper

41 100

69 0.0 74.7 112.1#

39 30.4 45.6 68.4#

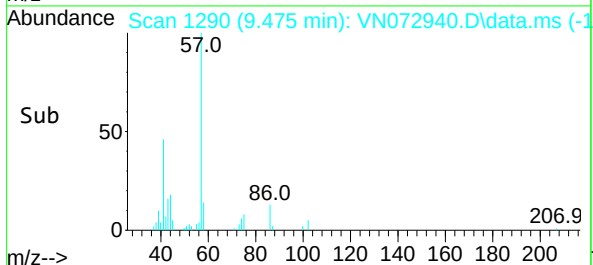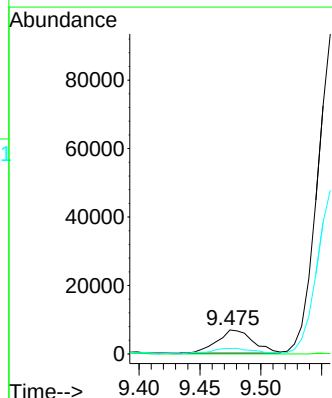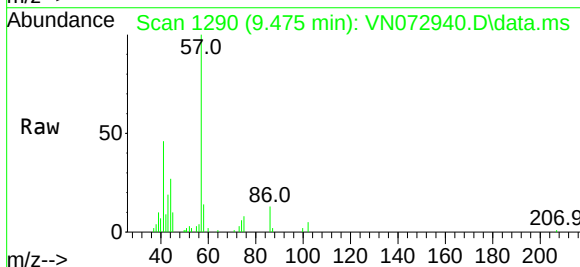

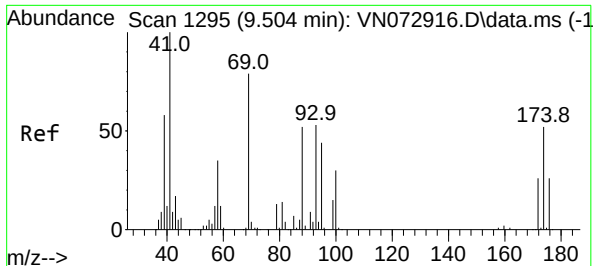

#49

1,4-Dioxane

Concen: 0.771 ug/l

RT: 9.557 min Scan# 11

Delta R.T. 0.053 min

Lab File: VN072940.D

Acq: 18 Jun 2022 15:20

Instrument :

MSVOA_N

ClientSampleId :

WC-14A-1A-9





Tgt Ion: 88 Resp: 80

Ion Ratio Lower Upper

88 100

43 2375426.3 20.2 30.4#

58 8926.3 54.2 81.4#

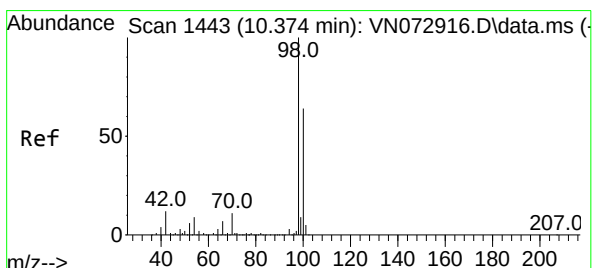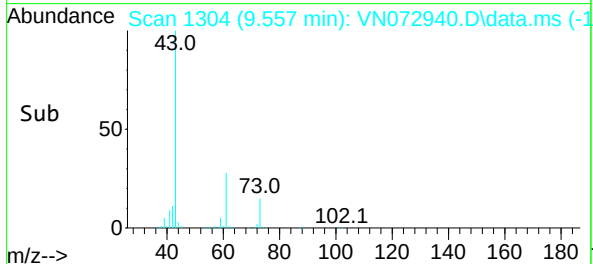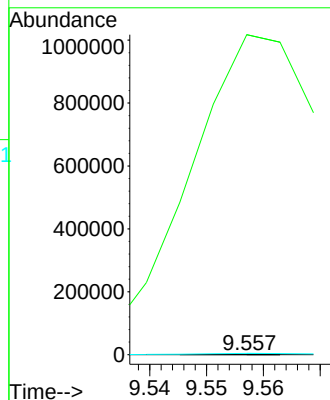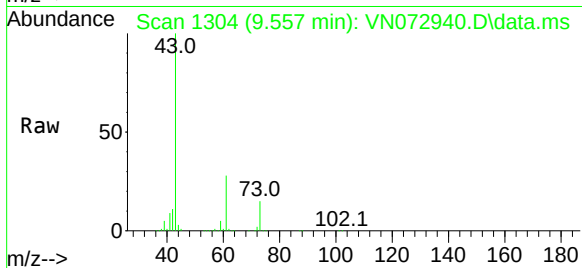

#50

Toluene-d8

Concen: 48.391 ug/l

RT: 10.375 min Scan# 1443

Delta R.T. 0.000 min

Lab File: VN072940.D




Acq: 18 Jun 2022 15:20


Tgt Ion: 98 Resp: 587733

Ion Ratio Lower Upper

98 100

100 65.7 52.6 78.8


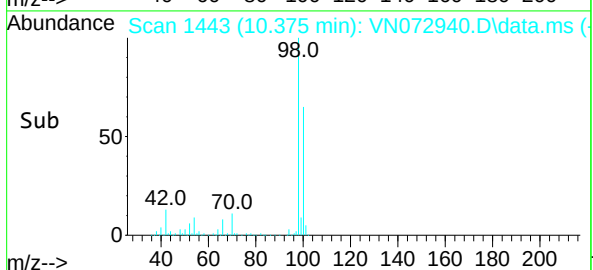
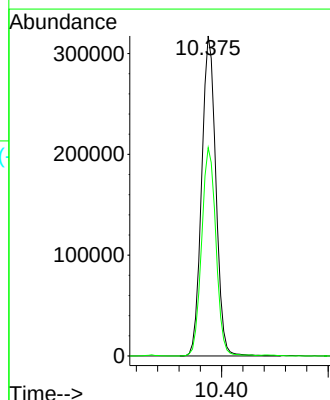
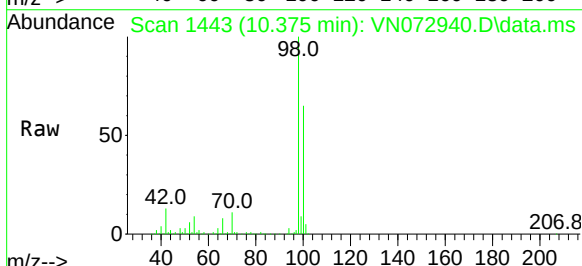




#51
4-Methyl-2-Pentanone
Concen: 2.536 ug/l
RT: 10.269 min Scan# 1425
Delta R.T. 0.000 min
Lab File: VN072940.D
Acq: 18 Jun 2022 15:20




Instrument :
MSVOA_N
ClientSampleId :
WC-14A-1A-9


Tgt Ion: 43 Resp: 16703
Ion Ratio Lower Upper
43 100
58 21.6 34.1 51.1#

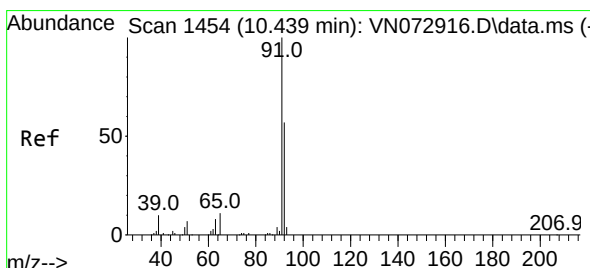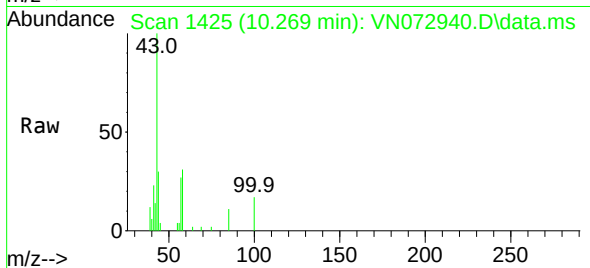

#52
Toluene
Concen: 0.326 ug/l
RT: 10.439 min Scan# 1454
Delta R.T. 0.000 min
Lab File: VN072940.D
Acq: 18 Jun 2022 15:20

Tgt Ion: 92 Resp: 2782
Ion Ratio Lower Upper
92 100
91 181.5 138.6 207.8


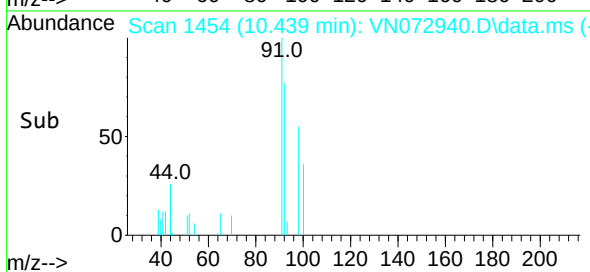

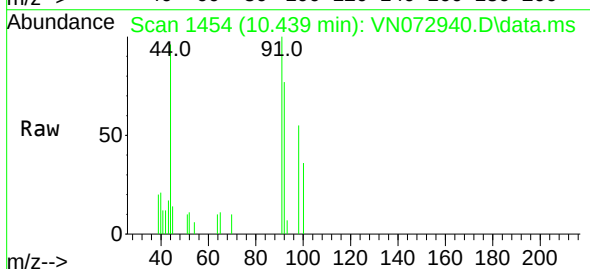




#54
 cis-1,3-Dichloropropene
 Concen: 6.495 ug/l
 RT: 10.181 min Scan# 1400
 Delta R.T. 0.059 min
 Lab File: VN072940.D
 Acq: 18 Jun 2022 15:20




Instrument :
 MSVOA_N
 ClientSampleId :
 WC-14A-1A-9


Tgt Ion: 75 Resp: 36378
 Ion Ratio Lower Upper
 75 100
 77 0.0 25.2 37.8#
 39 28.9 35.7 53.5#

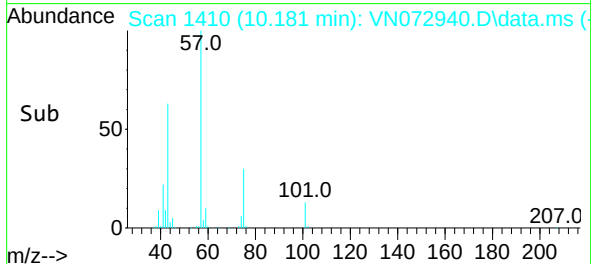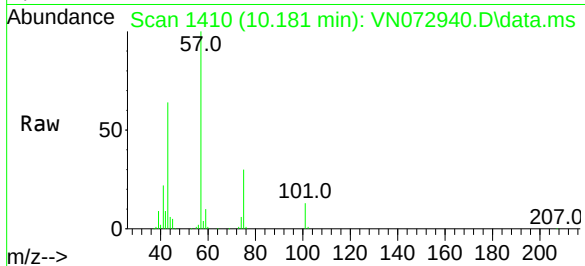

#57
 1,3-Dichloropropane
 Concen: 3.166 ug/l
 RT: 11.022 min Scan# 1553
 Delta R.T. 0.041 min
 Lab File: VN072940.D
 Acq: 18 Jun 2022 15:20

Tgt Ion: 76 Resp: 19654
 Ion Ratio Lower Upper
 76 100
 78 0.0 26.2 39.2#


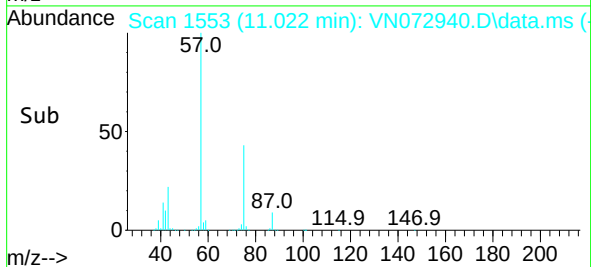

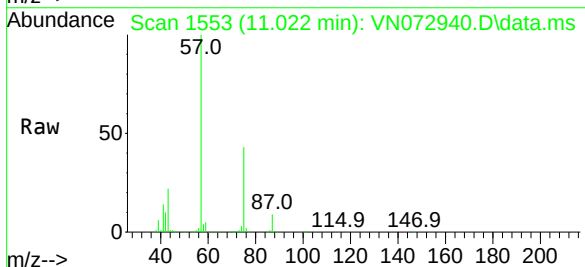




#59
2-Hexanone
Concen: 57.821 ug/l
RT: 11.028 min Scan# 1554
Delta R.T. 0.006 min
Lab File: VN072940.D
Acq: 18 Jun 2022 15:20




Instrument :
MSVOA_N
ClientSampleId :
WC-14A-1A-9


Tgt Ion: 43 Resp: 294495
Ion Ratio Lower Upper
43 100
58 17.9 29.7 89.1#

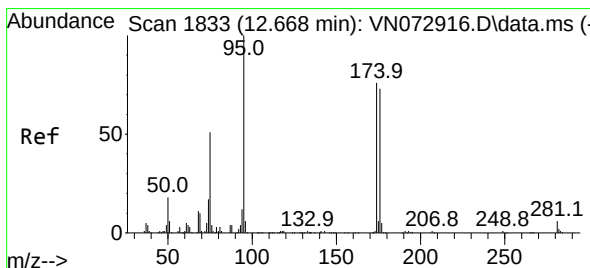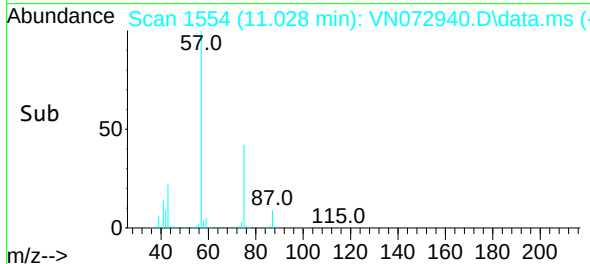

#62
4-Bromofluorobenzene
Concen: 56.436 ug/l
RT: 12.669 min Scan# 1833
Delta R.T. 0.000 min
Lab File: VN072940.D
Acq: 18 Jun 2022 15:20

Tgt Ion: 95 Resp: 246477
Ion Ratio Lower Upper
95 100
174 76.8 0.0 167.6
176 73.2 0.0 163.4


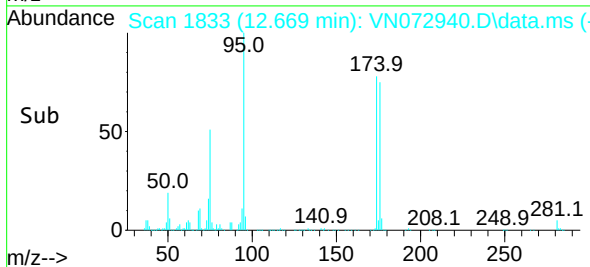

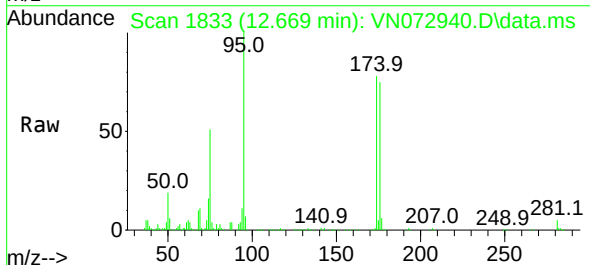




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.680 min Scan# 1
Delta R.T. 0.000 min
Lab File: VN072940.D
Acq: 18 Jun 2022 15:20




Instrument :
MSVOA_N
ClientSampleId :
WC-14A-1A-9


Tgt Ion:117 Resp: 475517
Ion Ratio Lower Upper
117 100
82 54.4 44.2 66.2
119 31.7 25.4 38.0

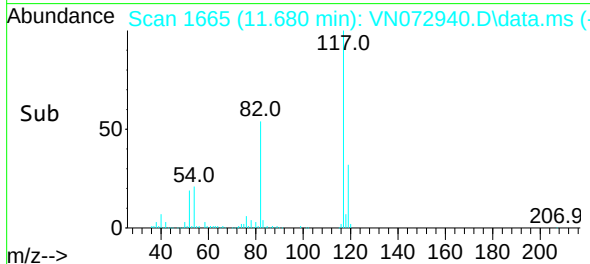

#67
Ethyl Benzene
Concen: 0.320 ug/l
RT: 11.780 min Scan# 1682
Delta R.T. 0.000 min
Lab File: VN072940.D
Acq: 18 Jun 2022 15:20

Tgt Ion: 91 Resp: 5236
Ion Ratio Lower Upper
91 100
106 40.2 24.9 37.3#


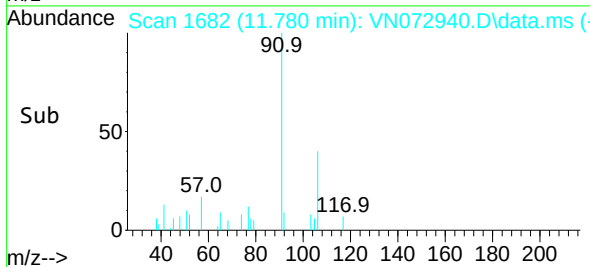

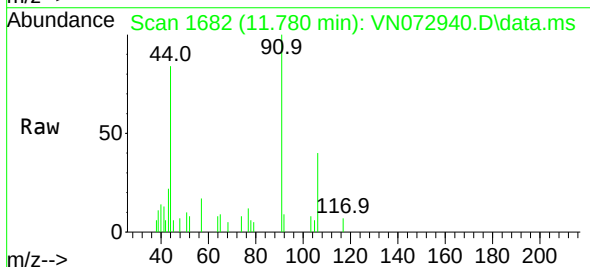




#68
m/p-Xylenes
Concen: 0.592 ug/l
RT: 11.892 min Scan# 1701
Delta R.T. 0.006 min
Lab File: VN072940.D
Acq: 18 Jun 2022 15:20




Instrument :
MSVOA_N
ClientSampleId :
WC-14A-1A-9


Tgt Ion:106 Resp: 3794
Ion Ratio Lower Upper
106 100
91 183.1 158.9 238.3

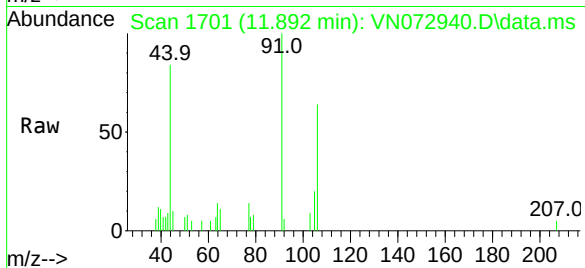

#69
o-Xylene
Concen: 1.156 ug/l
RT: 12.216 min Scan# 1756
Delta R.T. 0.000 min
Lab File: VN072940.D
Acq: 18 Jun 2022 15:20

Tgt Ion:106 Resp: 7404
Ion Ratio Lower Upper
106 100
91 214.3 106.0 318.0


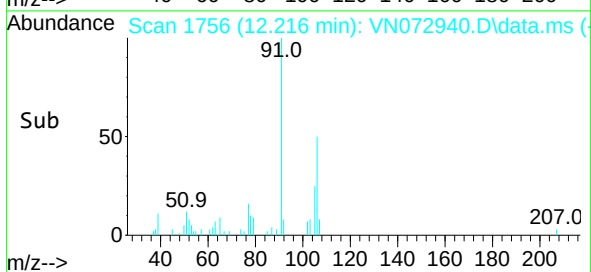

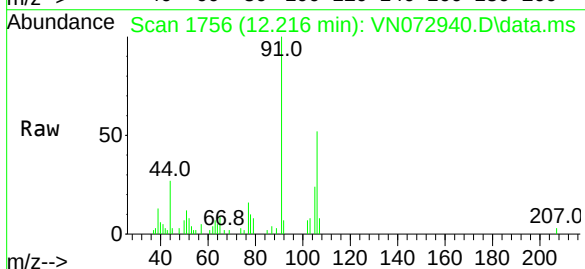




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.610 min Scan# 1993
Delta R.T. 0.000 min
Lab File: VN072940.D
Acq: 18 Jun 2022 15:20




Instrument :
MSVOA_N
ClientSampleId :
WC-14A-1A-9


Tgt Ion:152 Resp: 223819
Ion Ratio Lower Upper
152 100
115 59.6 28.9 86.7
150 161.1 0.0 356.2

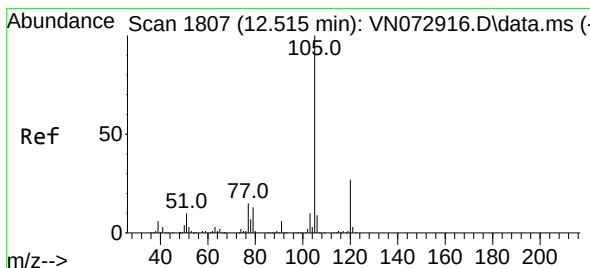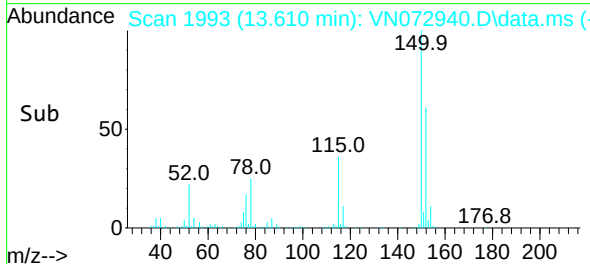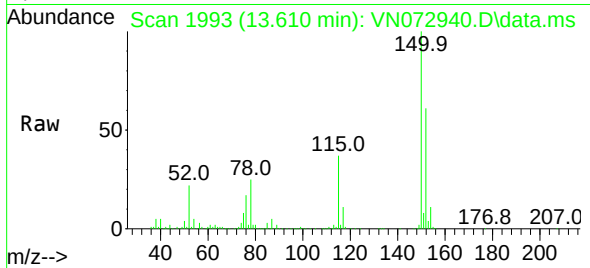

#73
Isopropylbenzene
Concen: 0.234 ug/l
RT: 12.516 min Scan# 1807
Delta R.T. 0.000 min
Lab File: VN072940.D
Acq: 18 Jun 2022 15:20

Tgt Ion:105 Resp: 4057
Ion Ratio Lower Upper
105 100
120 33.9 13.5 40.4


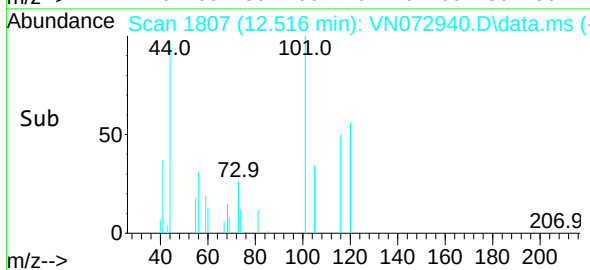

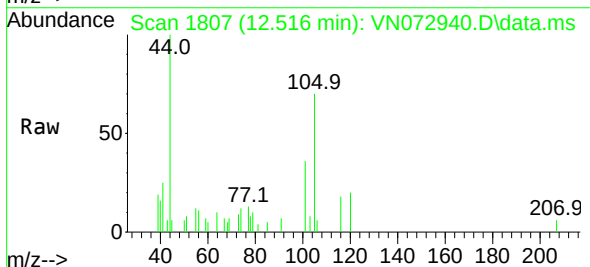




#74
N-amy1 acetate
Concen: 0.426 ug/l
RT: 12.292 min Scan# 1
Delta R.T. -0.035 min
Lab File: VN072940.D
Acq: 18 Jun 2022 15:20




Instrument :
MSVOA_N
ClientSampleId :
WC-14A-1A-9


Tgt Ion: 43 Resp: 3830
Ion Ratio Lower Upper
43 100
70 0.0 39.0 58.4#
55 5.6 21.1 31.7#
61 0.0 21.1 31.7#

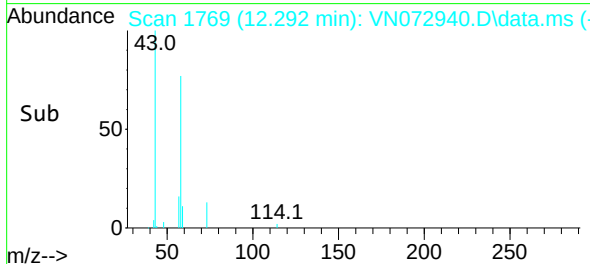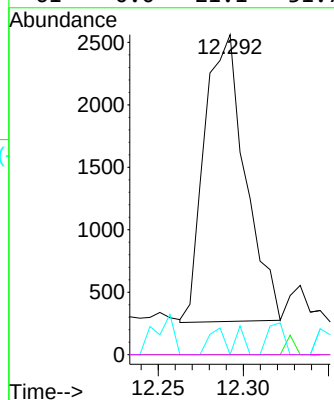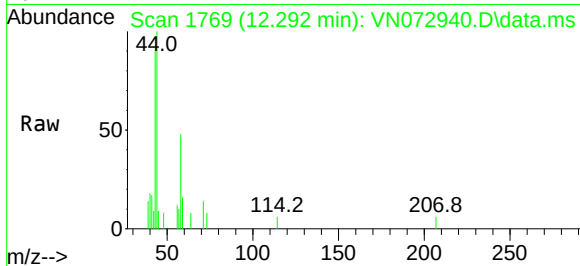

#76
1,2,3-Trichloropropane
Concen: 23.062 ug/l
RT: 12.669 min Scan# 1833
Delta R.T. -0.147 min
Lab File: VN072940.D
Acq: 18 Jun 2022 15:20

Tgt Ion: 75 Resp: 125145
Ion Ratio Lower Upper
75 100
77 1.3 98.5 295.5#


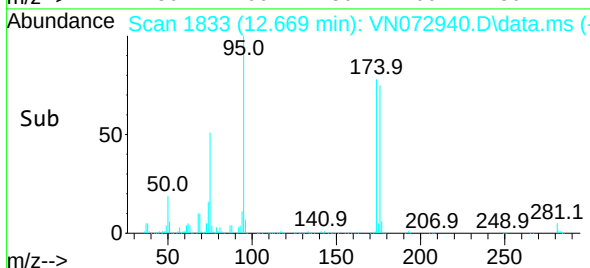
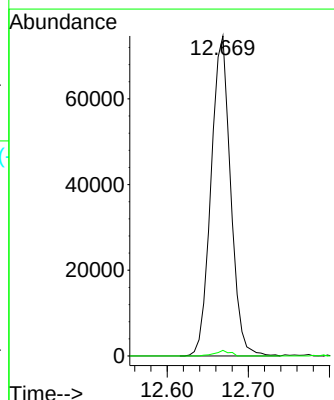
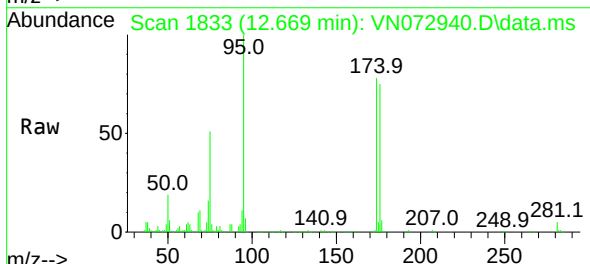




#80
 1,3,5-Trimethylbenzene
 Concen: 0.423 ug/l
 RT: 12.992 min Scan# 1888
 Delta R.T. -0.006 min
 Lab File: VN072940.D
 Acq: 18 Jun 2022 15:20




Instrument :
 MSVOA_N
 ClientSampleId :
 WC-14A-1A-9


Tgt Ion:105 Resp: 6017
 Ion Ratio Lower Upper
 105 100
 120 53.4 24.9 74.7

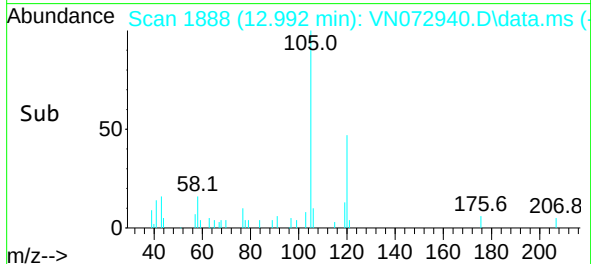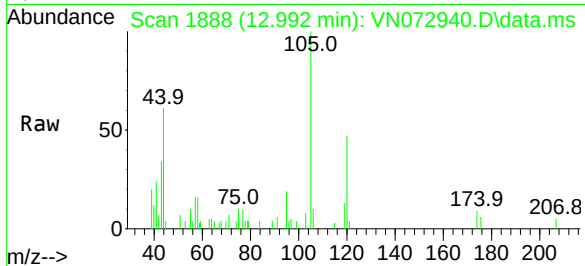

#81
 trans-1,4-Dichloro-2-butene
 Concen: 62.282 ug/l
 RT: 12.669 min Scan# 1833
 Delta R.T. 0.106 min
 Lab File: VN072940.D
 Acq: 18 Jun 2022 15:20

Tgt Ion: 75 Resp: 125145
 Ion Ratio Lower Upper
 75 100
 53 0.2 78.0 117.0#
 89 0.1 37.2 55.8#

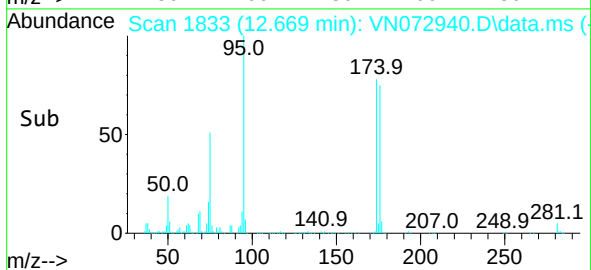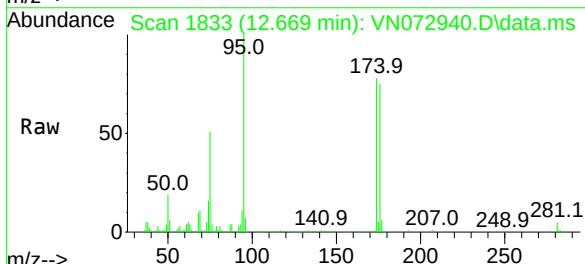



#84

1,2,4-Trimethylbenzene

Concen: 1.382 ug/l

RT: 13.304 min Scan# 1941

Delta R.T. 0.000 min

Lab File: VN072940.D

Acq: 18 Jun 2022 15:20

Instrument :

MSVOA_N

ClientSampleId :





WC-14A-1A-9

Tgt Ion:105 Resp: 19578

Ion Ratio Lower Upper

105 100

120 39.9 23.3 69.8

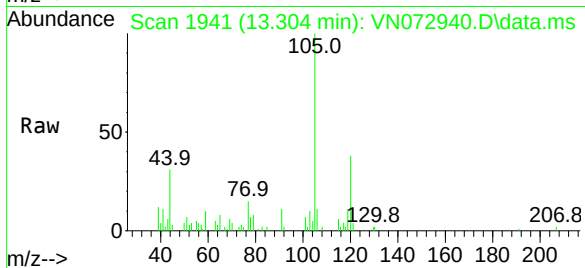

#90

Hexachloroethane

Concen: 0.228 ug/l

RT: 14.151 min Scan# 2085

Delta R.T. 0.006 min

Lab File: VN072940.D




Acq: 18 Jun 2022 15:20


Tgt Ion:117 Resp: 604

Ion Ratio Lower Upper

117 100


201 0.0 40.6 122.0#

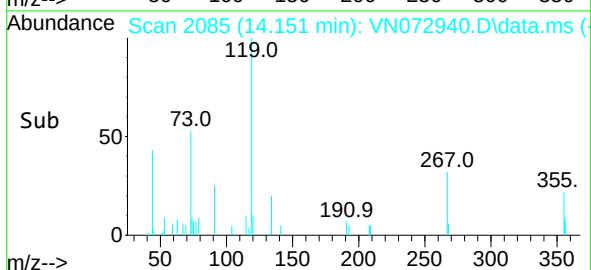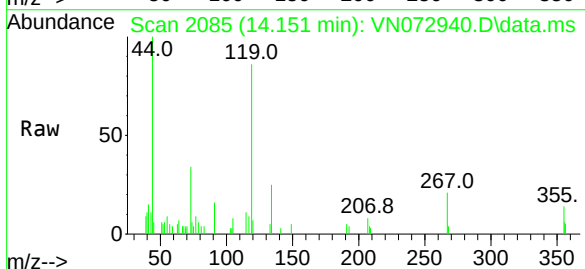

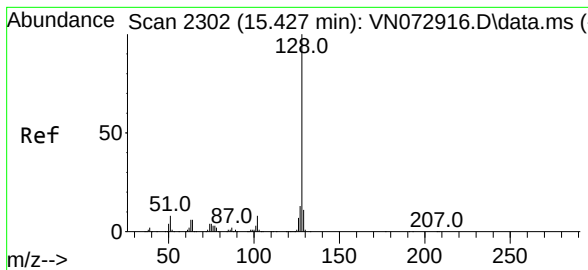

#95
Naphthalene
Concen: 2.287 ug/l
RT: 15.427 min Scan# 21
Delta R.T. 0.000 min
Lab File: VN072940.D
Acq: 18 Jun 2022 15:20

Instrument :
MSVOA_N
ClientSampleId :
WC-14A-1A-9

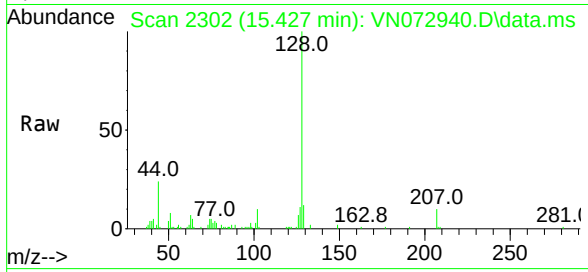

Tgt Ion:	128	Resp:	39545
Ion	Ratio	Lower	Upper
128	100		
127	11.3	10.3	15.5
129	11.0	8.6	13.0

