


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061822\
 Data File : VN072920.D
 Acq On : 18 Jun 2022 06:09
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N061722W.M
 Title : SW846 8260
 Last Update : Sat Jun 18 06:22:45 2022

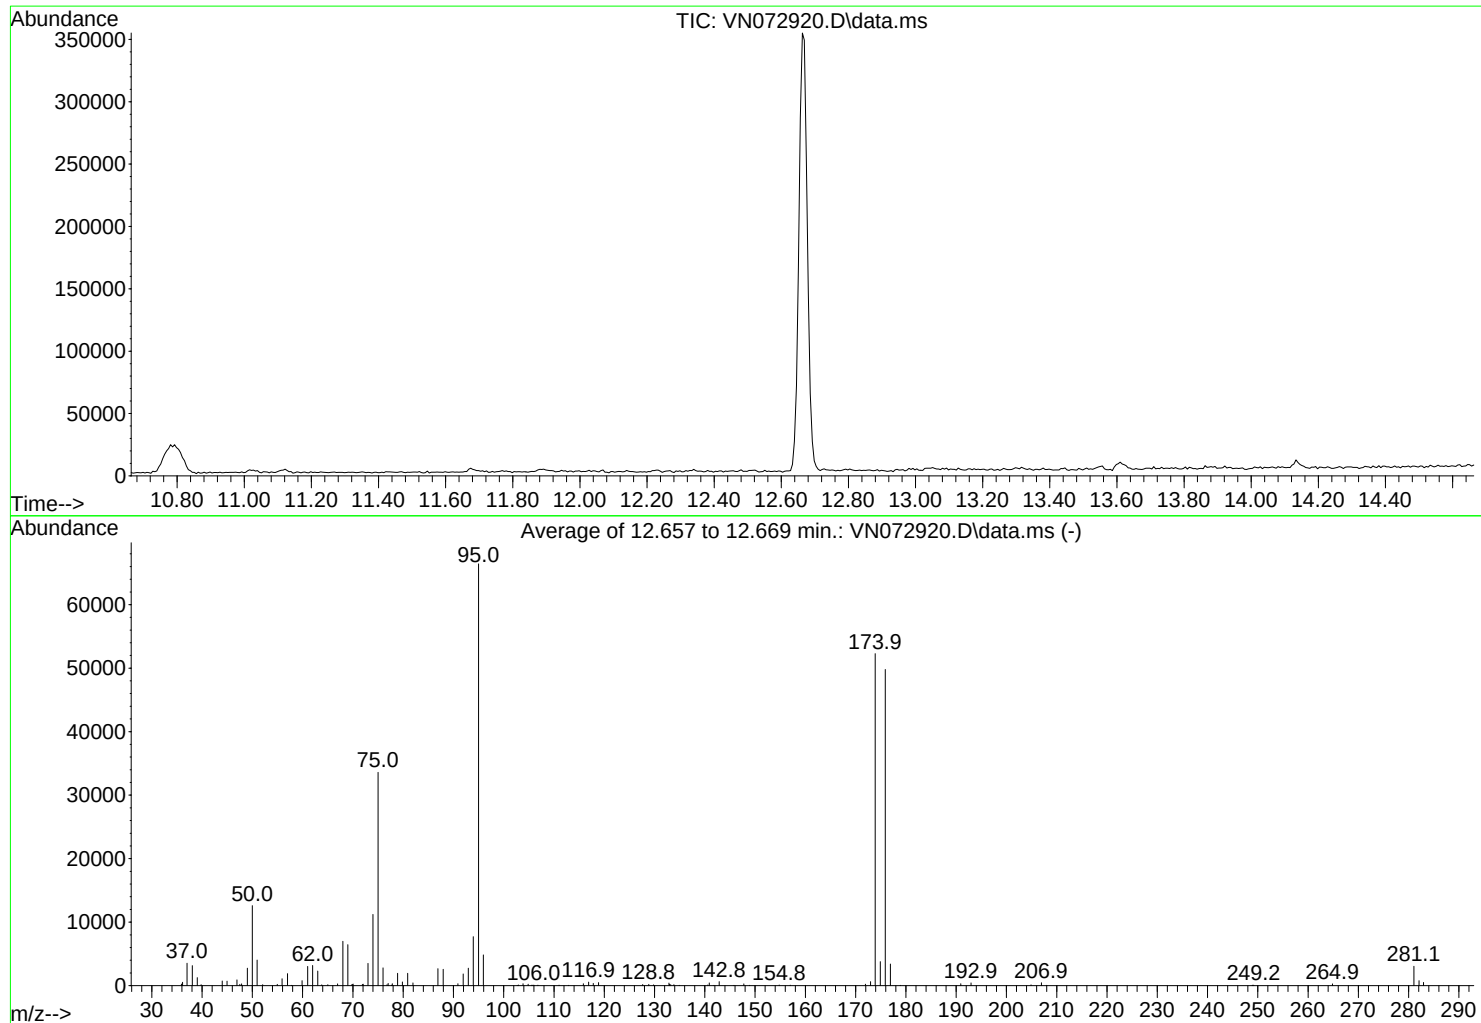

AutoFind: Scans 1831, 1832, 1833; Background Corrected with Scan 1823

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	12606	PASS
75	95	30	60	50.6	33597	PASS
95	95	100	100	100.0	66429	PASS
96	95	5	9	7.3	4846	PASS
173	174	0.00	2	1.2	641	PASS
174	95	50	100	78.7	52283	PASS
175	174	5	9	7.2	3776	PASS
176	174	95	101	95.2	49789	PASS
177	176	5	9	6.8	3406	PASS