

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN061918\
 Data File : VN049385.D
 Acq On : 19 Jun 2018 15:11
 Operator : MD\SY
 Sample : VN0619MBL01
 Misc : 5.00g/10mL/100uL/5.0mL/MSVOA_N/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0619MBL01

Quant Time: Jun 20 04:45:23 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N061618W.M
 Quant Title : SW846 8260
 QLast Update : Sat Jun 16 01:02:01 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.67	168	1592355	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.59	114	2461672	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.41	117	2099933	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.35	152	673928	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.03	65	1052984	49.86	ug/l	0.00
Spiked Amount	50.000		Recovery	=	99.72%	
35) Dibromofluoromethane	7.59	113	936877	47.04	ug/l	0.00
Spiked Amount	50.000		Recovery	=	94.08%	
50) Toluene-d8	10.09	98	3434690	45.29	ug/l	0.00
Spiked Amount	50.000		Recovery	=	90.58%	
62) 4-Bromofluorobenzene	12.40	95	932138	37.17	ug/l	0.00
Spiked Amount	50.000		Recovery	=	74.34%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN061918\
Data File : VN049385.D
Acq On : 19 Jun 2018 15:11
Operator : MD\SY
Sample : VN0619MBL01
Misc : 5.00g/10mL/100uL/5.0mL/MSVOA_N/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0619MBL01

Quant Time: Jun 20 04:45:23 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N061618W.M
Quant Title : SW846 8260
QLast Update : Sat Jun 16 01:02:01 2018
Response via : Initial Calibration

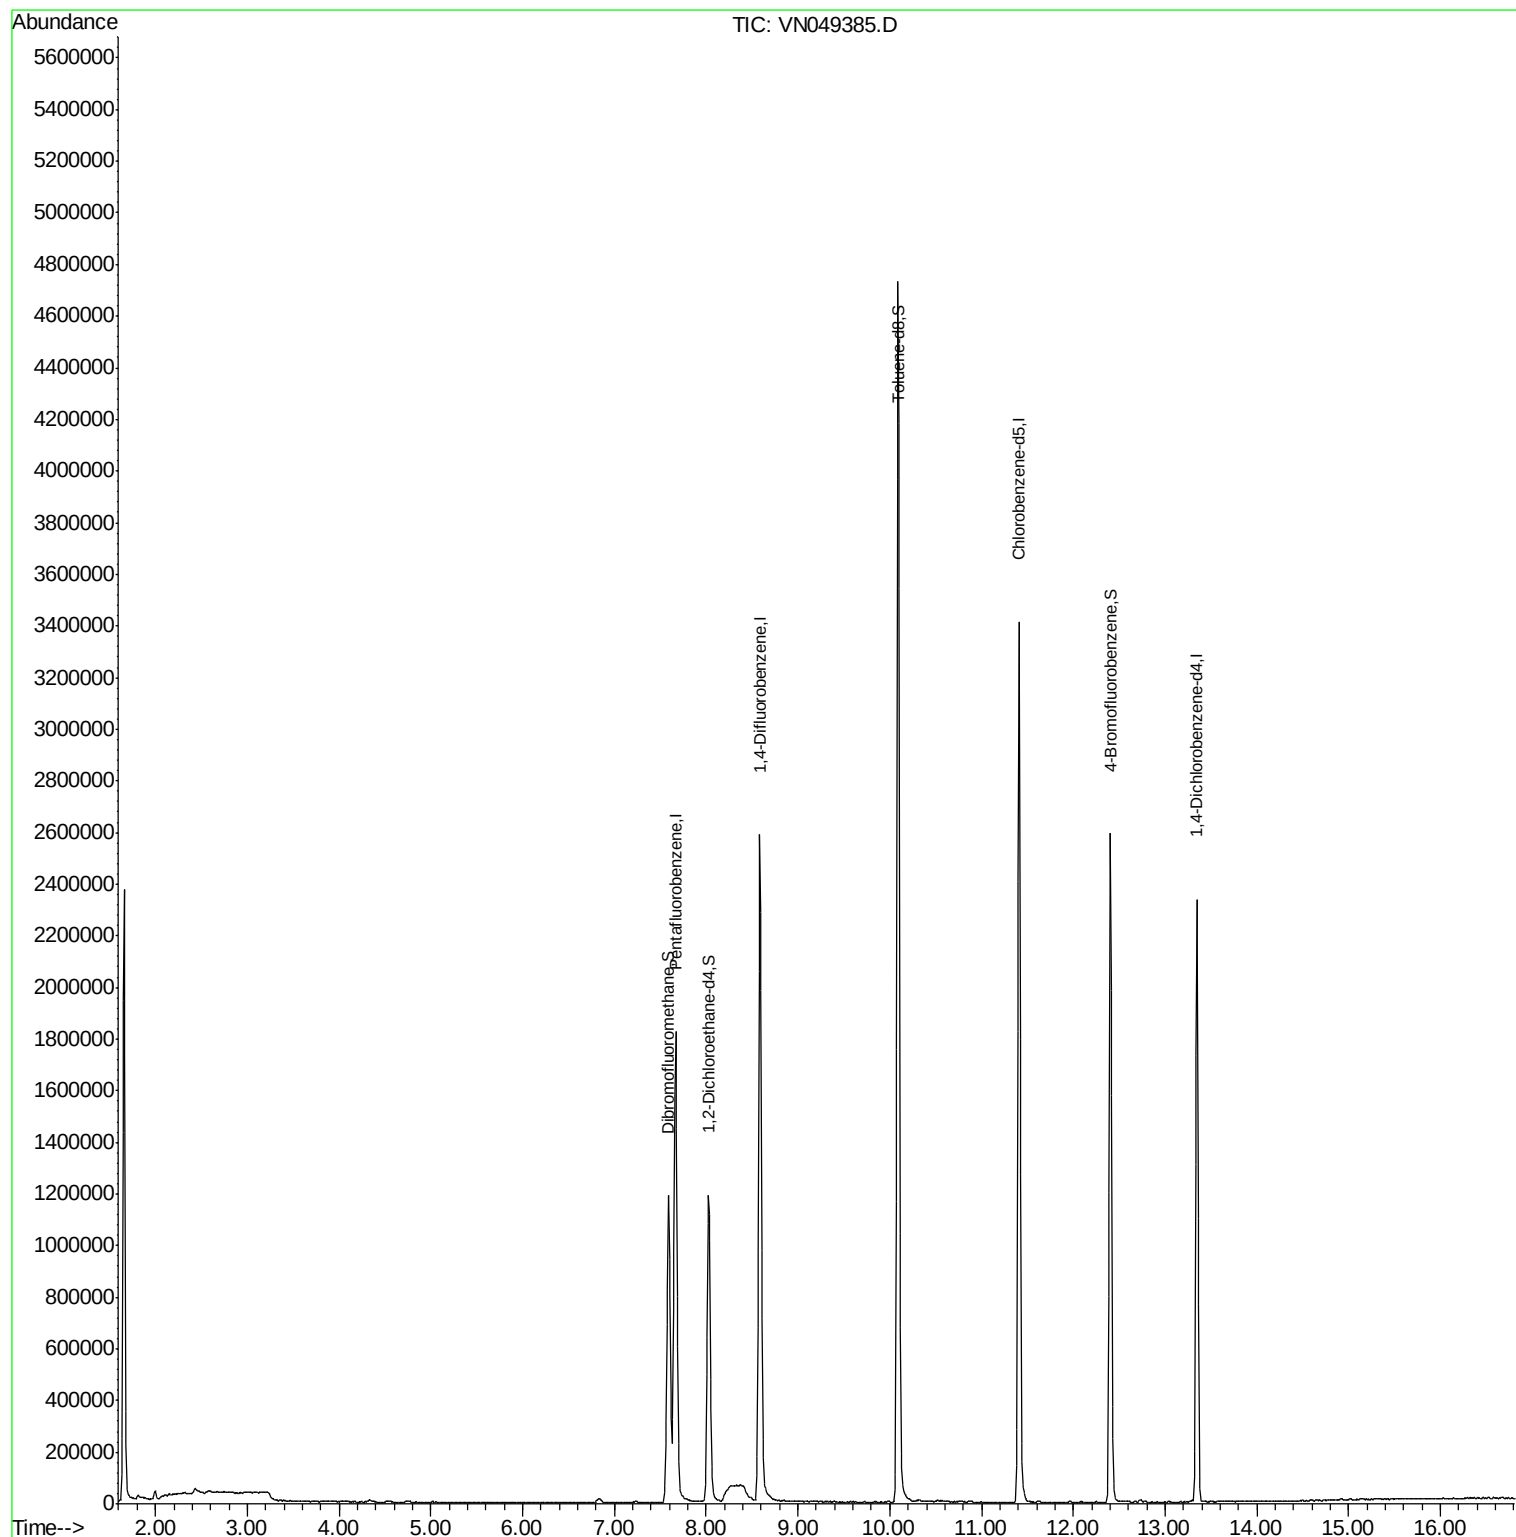

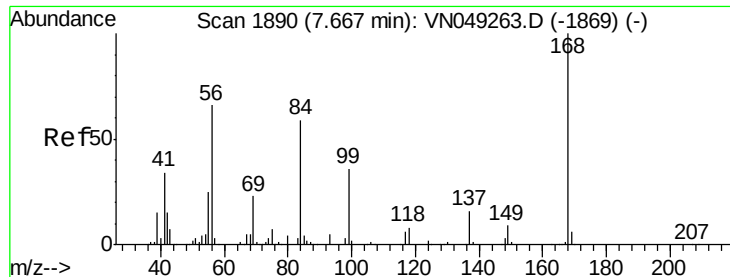

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.67 min Scan# 1890

Delta R.T. 0.00 min

Lab File: VN049385.D

Acq: 19 Jun 2018 15:11

Instrument :

MSVOA_N

ClientSampleId :


VN0619MBL01

Tot Ion:168 Resp: 1592355

Ion Ratio Lower Upper

168 100

99 50.8 45.8 68.6

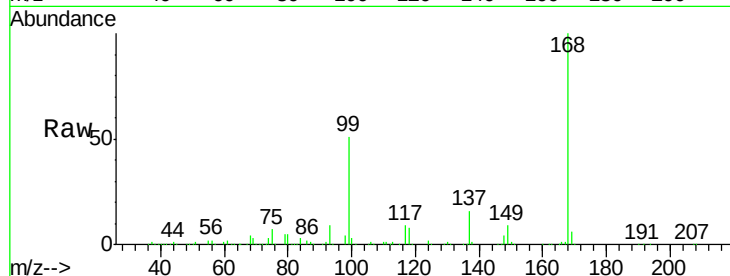

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VN0

7.67



600000

400000

200000

0

Time-->

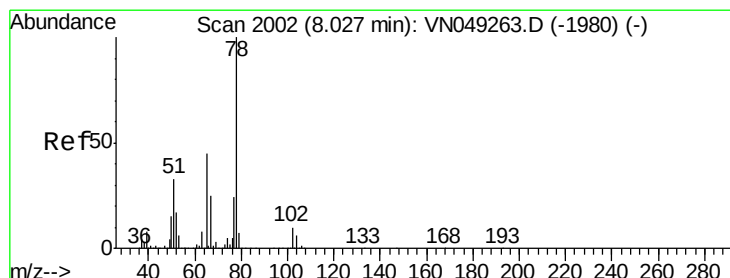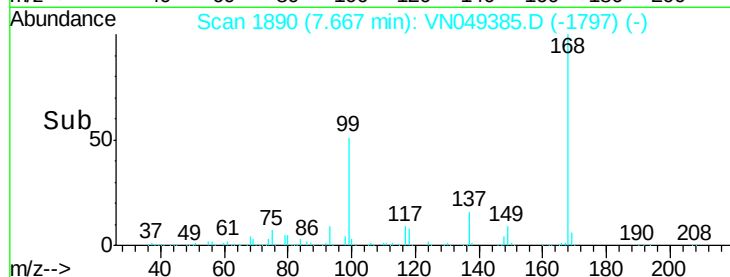

#33

1,2-Dichloroethane-d4

Concen: 49.857 ug/l

RT: 8.03 min Scan# 2002

Delta R.T. 0.00 min

Lab File: VN049385.D


Acq: 19 Jun 2018 15:11

Tgt Ion: 65 Resp: 1052984

Ion Ratio Lower Upper

65 100

67 52.8 0.0 103.8

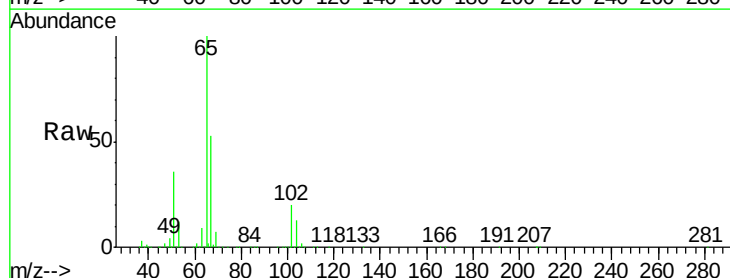

Abundance Ion 64.90 (64.60 to 65.60): VN0

Ion 66.90 (66.60 to 67.60): VN0

8.03

500000

400000


300000


200000

100000

0

Time-->

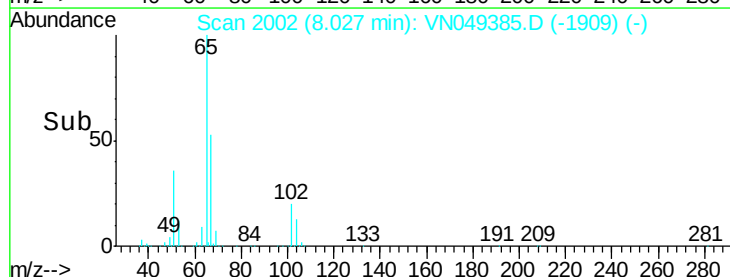

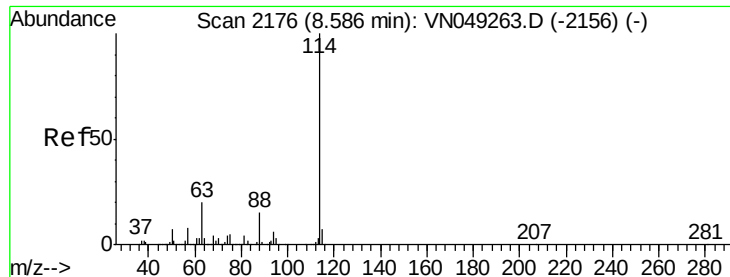

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.59 min Scan# 2176

Delta R.T. 0.00 min

Lab File: VN049385.D

Acq: 19 Jun 2018 15:11

Instrument :

MSVOA_N

ClientSampleId :

VN0619MBL01


Tot Ion:114 Resp: 2461672

Ion Ratio Lower Upper

114 100

63 19.6 0.0 44.4




88 15.7 0.0 31.4

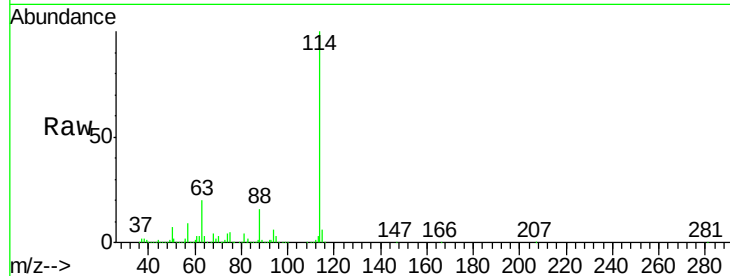

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VN

Ion 87.90 (87.60 to 88.60): VN

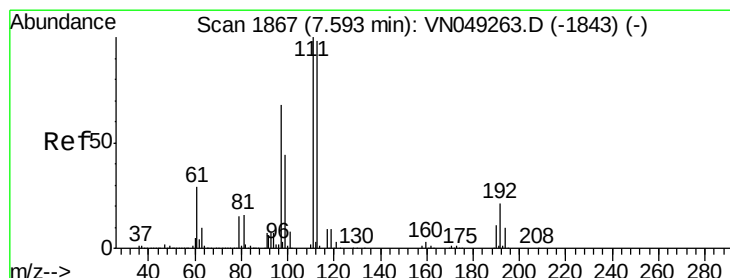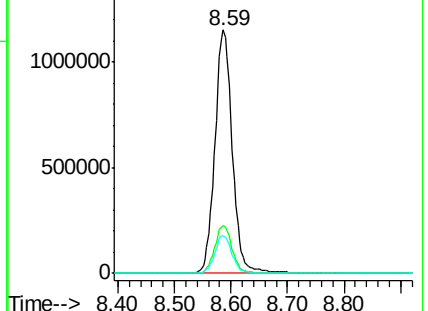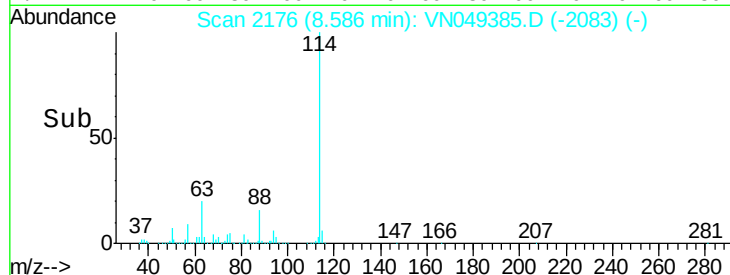

#35

Dibromofluoromethane

Concen: 47.041 ug/l

RT: 7.59 min Scan# 1866

Delta R.T. -0.00 min

Lab File: VN049385.D

Acq: 19 Jun 2018 15:11


Tgt Ion:113 Resp: 936877

Ion Ratio Lower Upper

113 100

111 101.3 82.4 123.6



192 21.7 15.0 22.6

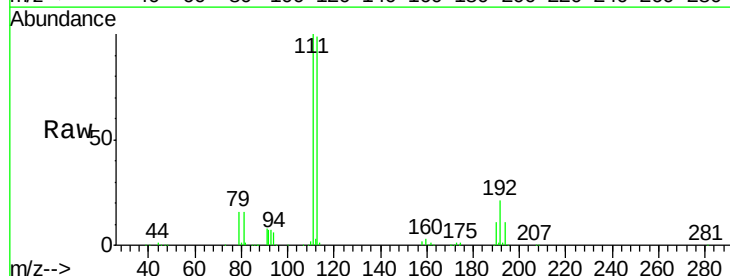


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V



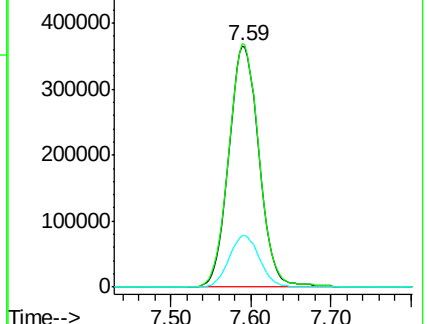
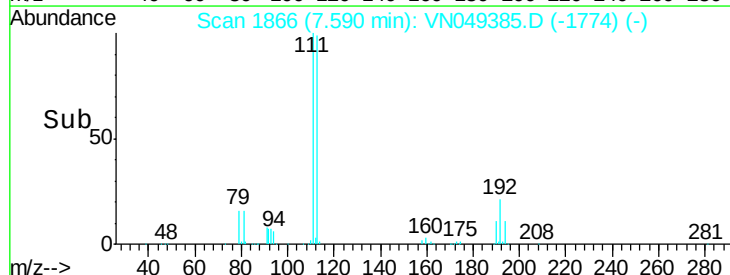


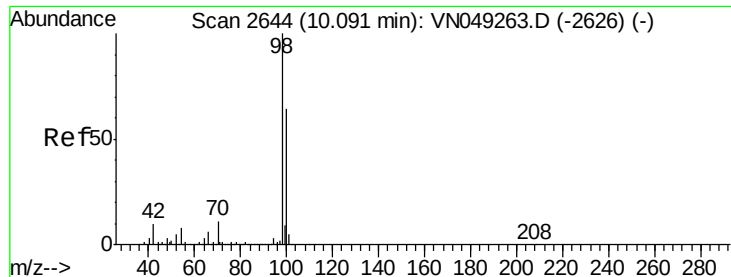

#50
Toluene-d8
Concen: 45.293 ug/l
RT: 10.09 min Scan# 2644
Delta R.T. 0.00 min
Lab File: VN049385.D
Acq: 19 Jun 2018 15:11




Instrument :
MSVOA_N
ClientSampleId :
VN0619MBL01


Tot Ion: 98 Resp: 3434690
Ion Ratio Lower Upper
98 100
100 63.8 49.8 74.8

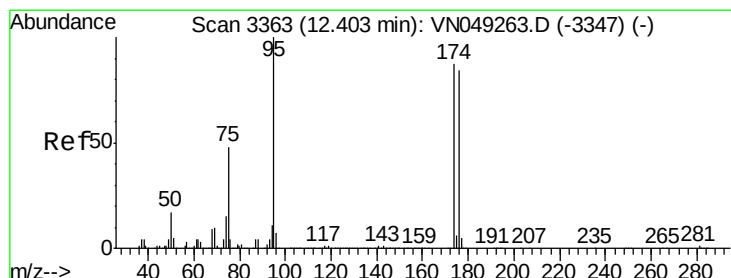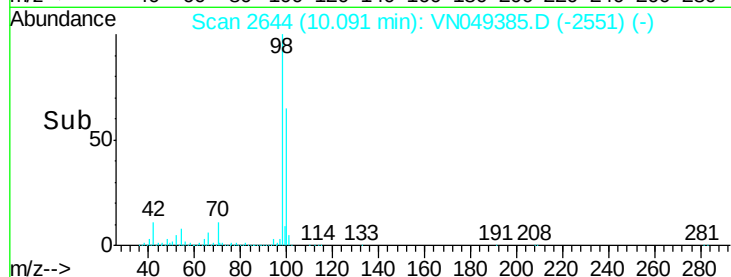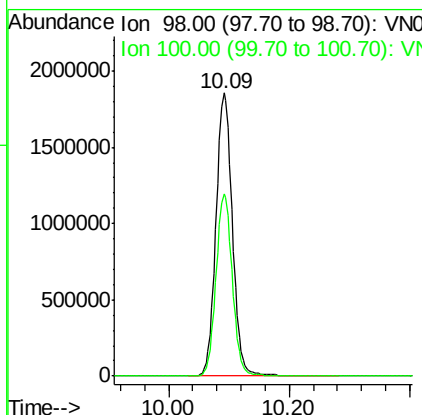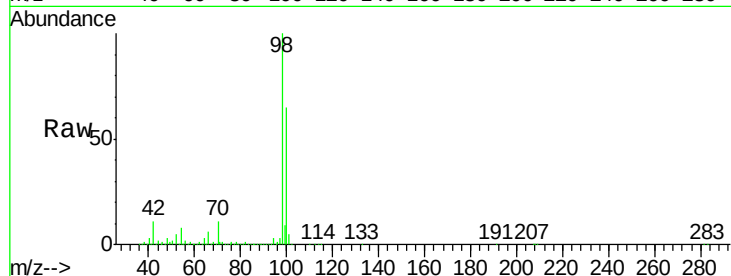

#62
4-Bromofluorobenzene
Concen: 37.175 ug/l
RT: 12.40 min Scan# 3363
Delta R.T. 0.00 min
Lab File: VN049385.D
Acq: 19 Jun 2018 15:11

Tgt Ion: 95 Resp: 932138
Ion Ratio Lower Upper
95 100
174 88.7 0.0 165.6
176 85.4 0.0 157.4

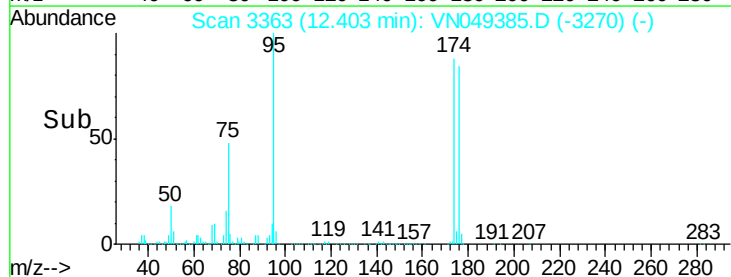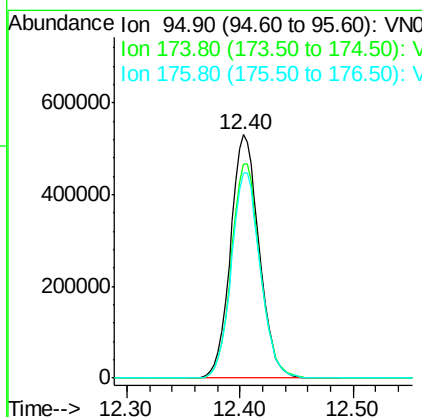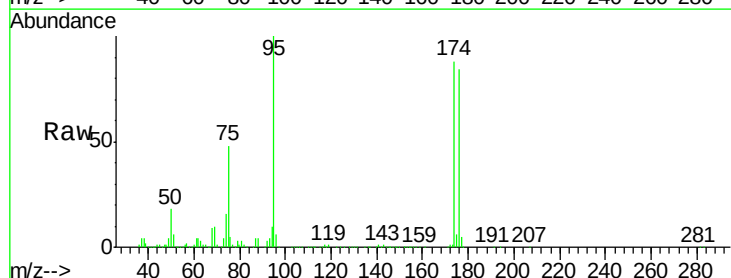


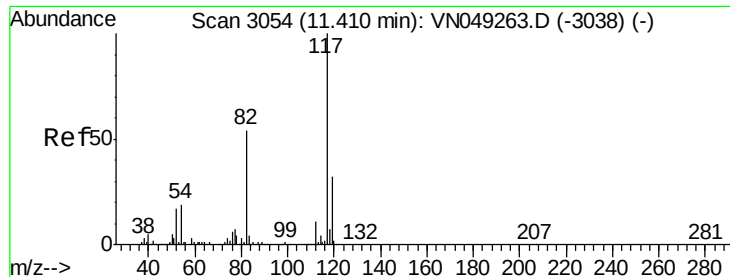




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.41 min Scan# 3054
Delta R.T. 0.00 min
Lab File: VN049385.D
Acq: 19 Jun 2018 15:11

Instrument :
MSVOA_N
ClientSampleId :
VN0619MBL01

Tot Ion:117 Resp: 2099933
Ion Ratio Lower Upper
117 100
82 53.8 45.9 68.9
119 32.4 25.5 38.3

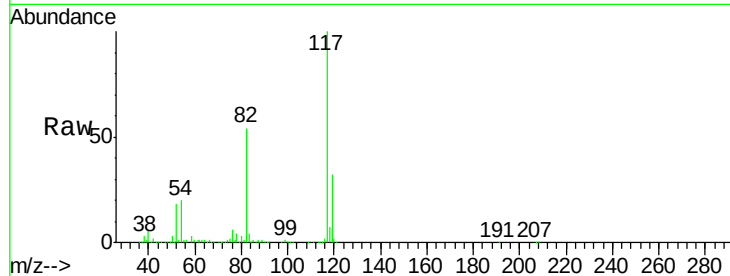


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): V
Ion 118.90 (118.60 to 119.60): V

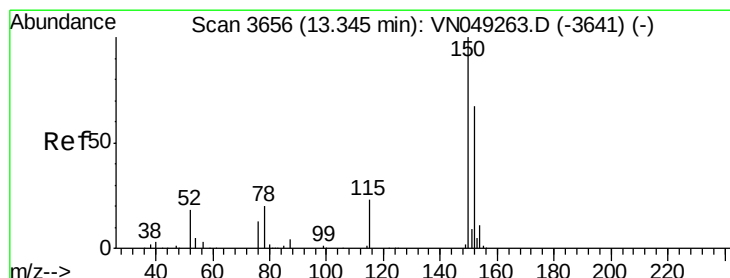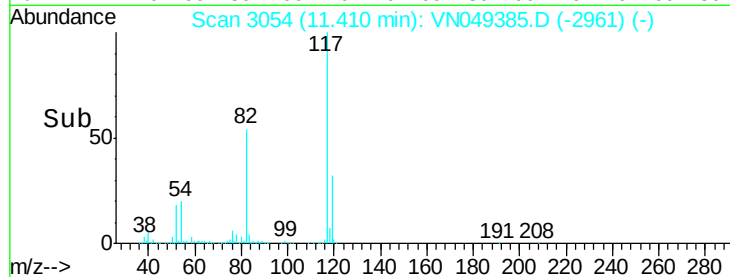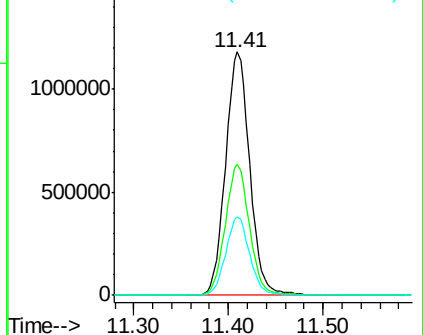

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.35 min Scan# 3657
Delta R.T. 0.00 min
Lab File: VN049385.D
Acq: 19 Jun 2018 15:11

Tgt Ion:152 Resp: 673928
Ion Ratio Lower Upper
152 100
115 57.0 28.7 86.1
150 157.9 0.0 351.0

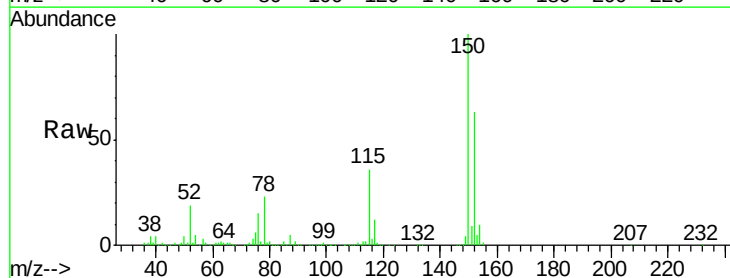

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

