

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN061918\
 Data File : VN049397.D
 Acq On : 19 Jun 2018 20:21
 Operator : MD\SY
 Sample : PB110363ZHE#09
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB110363ZHE#09

Quant Time: Jun 20 05:19:50 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N061618W.M
 Quant Title : SW846 8260
 QLast Update : Sat Jun 16 01:02:01 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.67	168	1174117	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.59	114	1904777	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.41	117	1566136	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.35	152	438898	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.03	65	813327	52.23	ug/l	0.00
Spiked Amount 50.000			Recovery	=	104.46%	
35) Dibromofluoromethane	7.59	113	707161	45.89	ug/l	0.00
Spiked Amount 50.000			Recovery	=	91.78%	
50) Toluene-d8	10.09	98	2591672	44.17	ug/l	0.00
Spiked Amount 50.000			Recovery	=	88.34%	
62) 4-Bromofluorobenzene	12.41	95	650030	33.50	ug/l	0.00
Spiked Amount 50.000			Recovery	=	67.00%	
Target Compounds						
16) Acetone	3.82	43	44879	11.869	ug/l	90
18) Methyl Acetate	4.33	43	111222	9.647	ug/l	92
20) Methylene Chloride	4.55	84	32142	2.035	ug/l	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN061918\
Data File : VN049397.D
Acq On : 19 Jun 2018 20:21
Operator : MD\SY
Sample : PB110363ZHE#09
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PB110363ZHE#09

Quant Time: Jun 20 05:19:50 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N061618W.M
Quant Title : SW846 8260
QLast Update : Sat Jun 16 01:02:01 2018
Response via : Initial Calibration

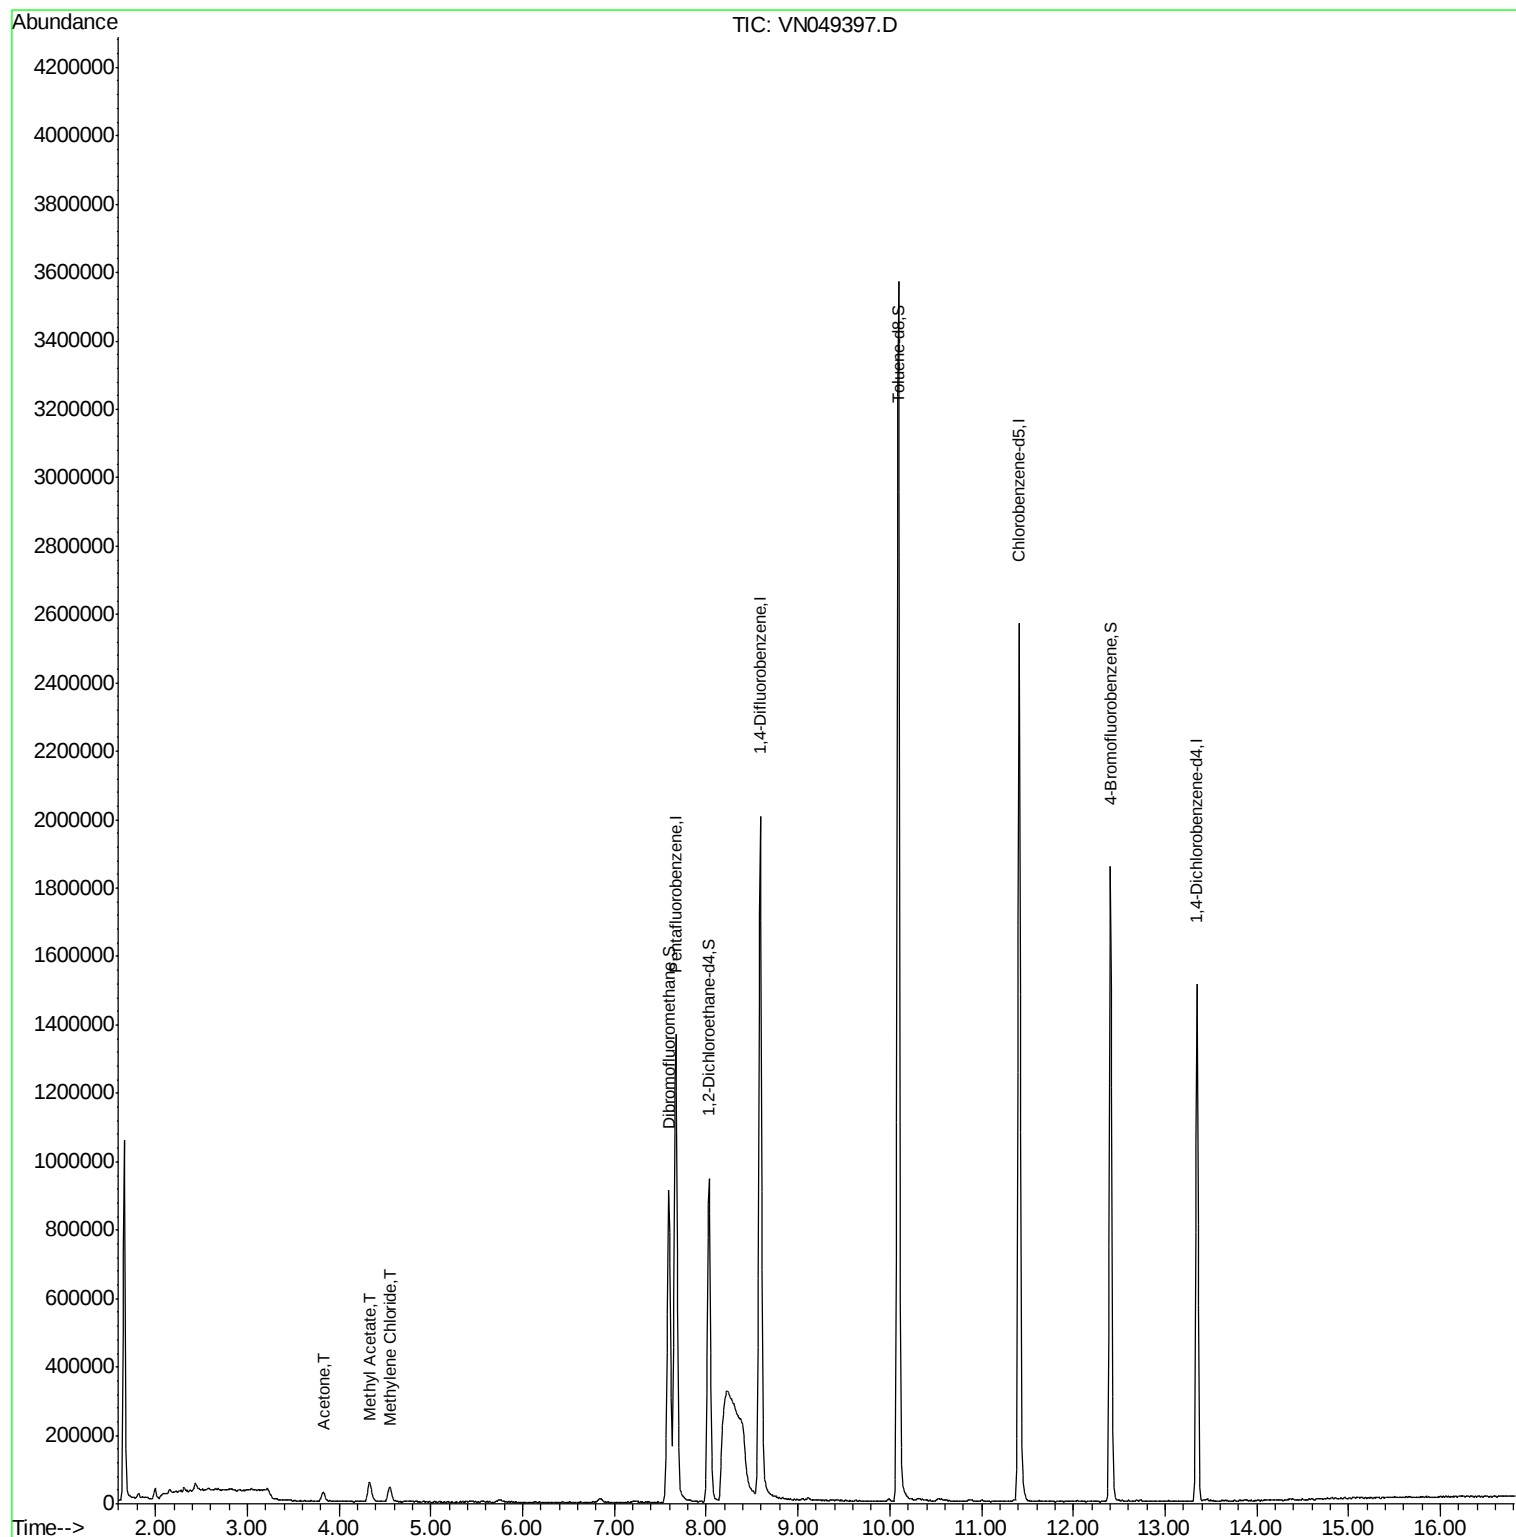



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.67 min Scan# 1891

Delta R.T. 0.00 min

Lab File: VN049397.D

Acq: 19 Jun 2018 20:21

Instrument :

MSVOA_N

ClientSampleId :


PB110363ZHE#09

Tot Ion:168 Resp: 1174117

Ion Ratio Lower Upper




168 100

99 52.4 45.8 68.6



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VN0

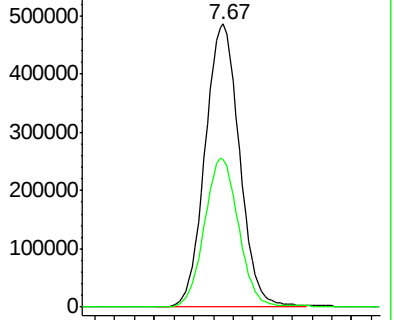

#16

Acetone

Concen: 11.869 ug/l

RT: 3.82 min Scan# 695

Delta R.T. 0.01 min

Lab File: VN049397.D


Acq: 19 Jun 2018 20:21

Tgt Ion: 43 Resp: 44879

Ion Ratio Lower Upper



43 100


58 33.4 22.4 33.6



Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 58.00 (57.70 to 58.70): VN0




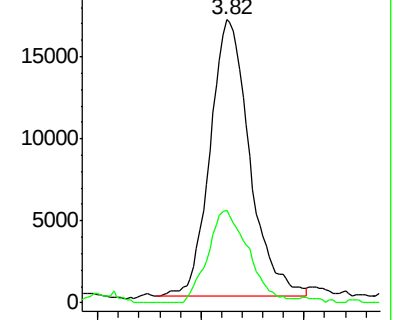




#18
Methvl Acetate
Concen: 9.647 ug/l
RT: 4.33 min Scan# 853
Delta R.T. 0.01 min
Lab File: VN049397.D
Acq: 19 Jun 2018 20:21




Instrument :
MSVOA_N
ClientSampleId :
PB110363ZHE#09


Tot Ion: 43 Resp: 111222
Ion Ratio Lower Upper
43 100
74 25.3 17.4 26.0

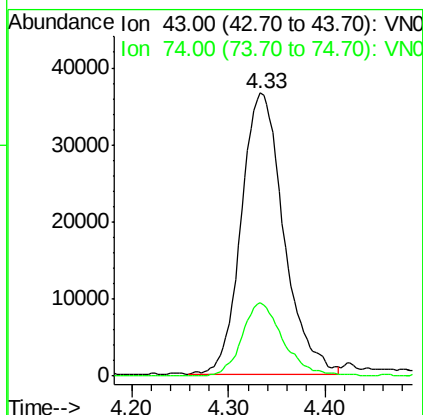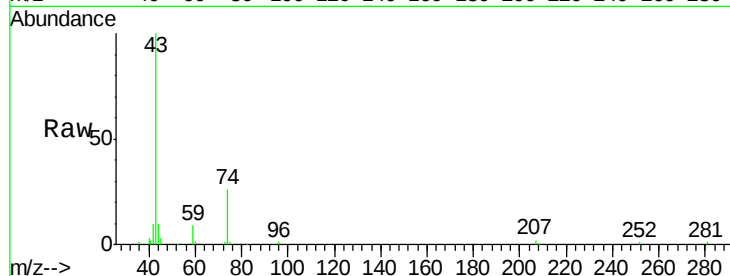

#20
Methylene Chloride
Concen: 2.035 ug/l
RT: 4.55 min Scan# 921
Delta R.T. 0.00 min
Lab File: VN049397.D
Acq: 19 Jun 2018 20:21

Tgt Ion: 84 Resp: 32142
Ion Ratio Lower Upper
84 100
49 108.4 106.9 160.3
51 38.5 32.7 49.1
86 59.0 49.8 74.8



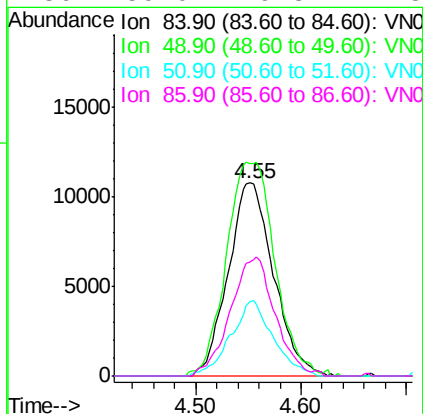



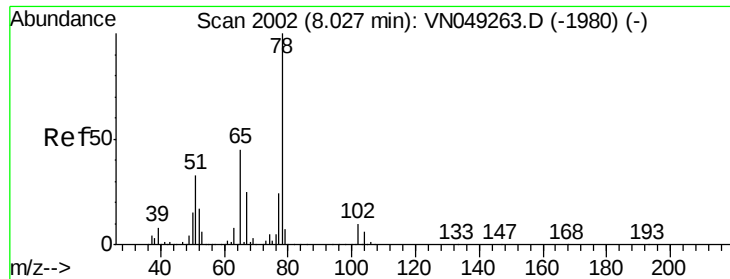

#33
 1,2-Dichloroethane-d4
 Concen: 52.228 ug/l
 RT: 8.03 min Scan# 2003
 Delta R.T. 0.00 min
 Lab File: VN049397.D
 Acq: 19 Jun 2018 20:21




Instrument :
 MSVOA_N
 ClientSampleId :
 PB110363ZHE#09


Tot Ion: 65 Resp: 813327
 Ion Ratio Lower Upper
 65 100
 67 53.2 0.0 103.8

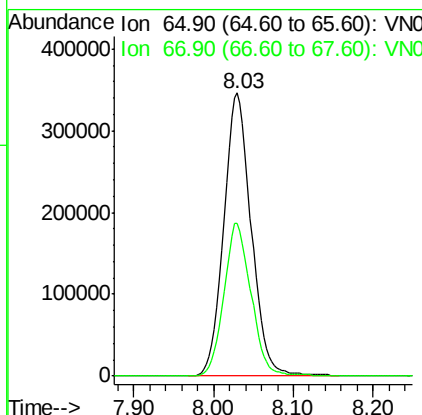

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.59 min Scan# 2177
 Delta R.T. 0.00 min
 Lab File: VN049397.D
 Acq: 19 Jun 2018 20:21

Tgt Ion: 114 Resp: 1904777
 Ion Ratio Lower Upper
 114 100
 63 19.6 0.0 44.4
 88 15.6 0.0 31.4

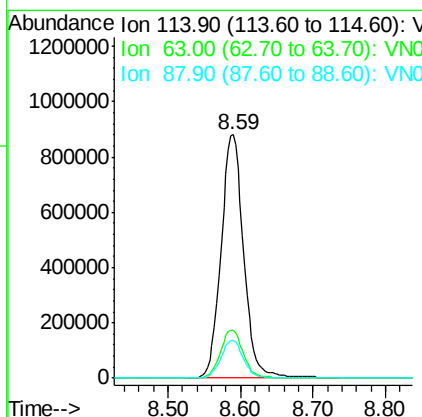


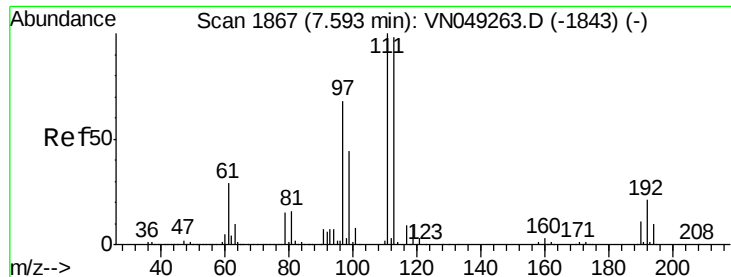


#35
Dibromofluoromethane
Concen: 45.888 ug/l
RT: 7.59 min Scan# 1867
Delta R.T. 0.00 min
Lab File: VN049397.D
Acq: 19 Jun 2018 20:21

Instrument :
MSVOA_N
ClientSampleId :
PB110363ZHE#09



Tot Ion	Ratio	Lower	Upper
113	100		
111	103.1	82.4	123.6
192	21.5	15.0	22.6

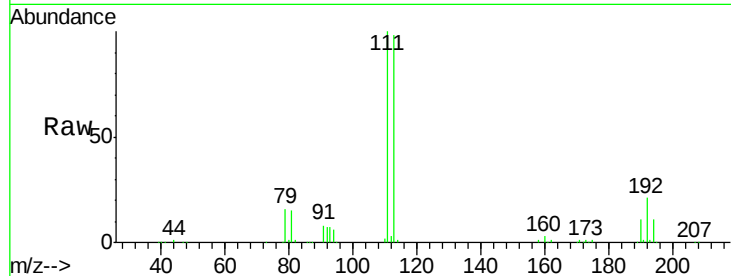

Abundance Ion 112.80 (112.50 to 113.50): V
Ion 110.80 (110.50 to 111.50): V
Ion 191.70 (191.40 to 192.40): V

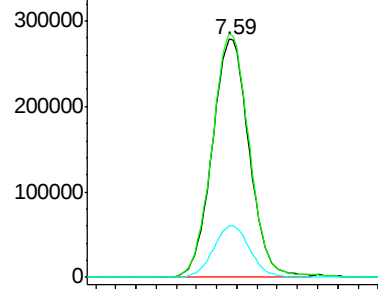


Time-->

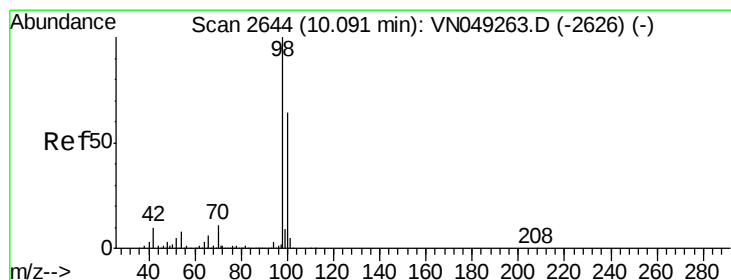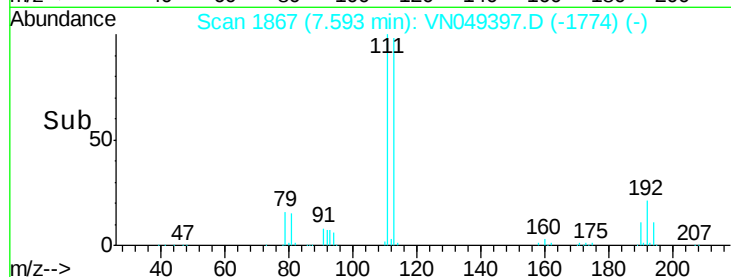


#50
Toluene-d8
Concen: 44.168 ug/l
RT: 10.09 min Scan# 2645
Delta R.T. 0.00 min
Lab File: VN049397.D
Acq: 19 Jun 2018 20:21


Tgt Ion	Ratio	Lower	Upper
98	100		
100	63.5	49.8	74.8

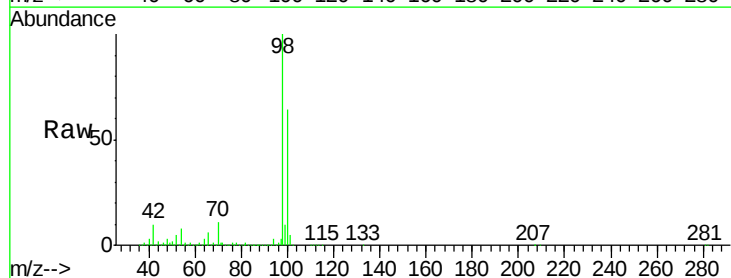

Abundance Ion 98.00 (97.70 to 98.70): VN
Ion 100.00 (99.70 to 100.70): VN

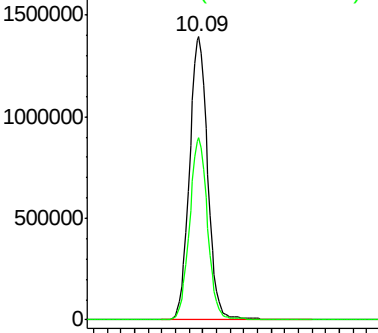

Time-->

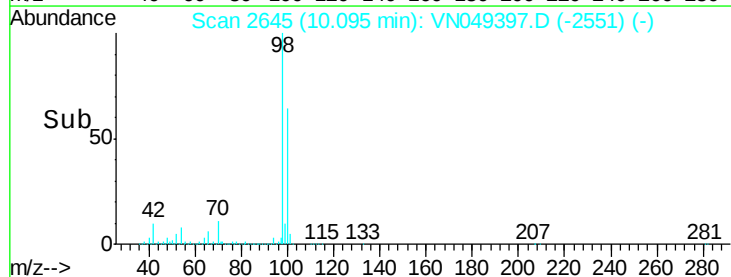



#62

4-Bromofluorobenzene

Concen: 33.503 ug/l

RT: 12.41 min Scan# 3364

Delta R.T. 0.00 min

Lab File: VN049397.D

Acq: 19 Jun 2018 20:21

Instrument :

MSVOA_N

ClientSampleId :

PB110363ZHE#09


Tot Ion: 95 Resp: 650030

Ion Ratio Lower Upper

95 100

174 90.2 0.0 165.6


176 86.5 0.0 157.4





Abundance Ion 94.90 (94.60 to 95.60): VN049263.D (-3347) (-)

Ion 173.80 (173.50 to 174.50): VN049263.D (-3347) (-)

Ion 175.80 (175.50 to 176.50): VN049263.D (-3347) (-)

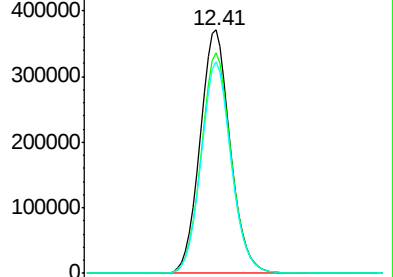

Time--> 12.30 12.40 12.50



#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.41 min Scan# 3054

Delta R.T. 0.00 min

Lab File: VN049397.D

Acq: 19 Jun 2018 20:21


Tgt Ion: 117 Resp: 1566136

Ion Ratio Lower Upper

117 100

82 54.9 45.9 68.9


119 32.6 25.5 38.3




Abundance Ion 116.90 (116.60 to 117.60): VN049263.D (-3038) (-)


Ion 82.00 (81.70 to 82.70): VN049263.D (-3038) (-)

Ion 118.90 (118.60 to 119.60): VN049263.D (-3038) (-)

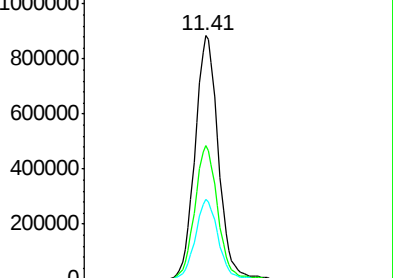

Time--> 11.30 11.40 11.50



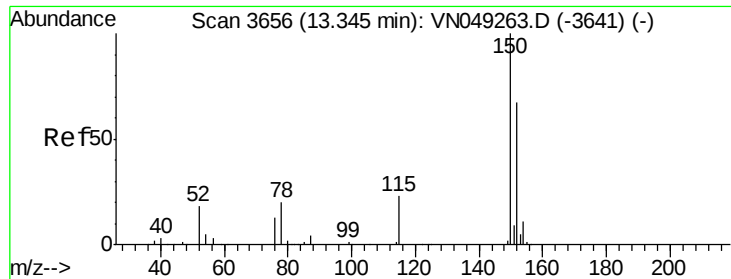

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.35 min Scan# 3657

Delta R.T. 0.00 min

Lab File: VN049397.D

Acq: 19 Jun 2018 20:21

Instrument :

MSVOA_N

ClientSampleId :

PB110363ZHE#09


Tot Ion:152 Resp: 438898

Ion Ratio Lower Upper

152 100

115 56.9 28.7 86.1

150 159.6 0.0 351.0

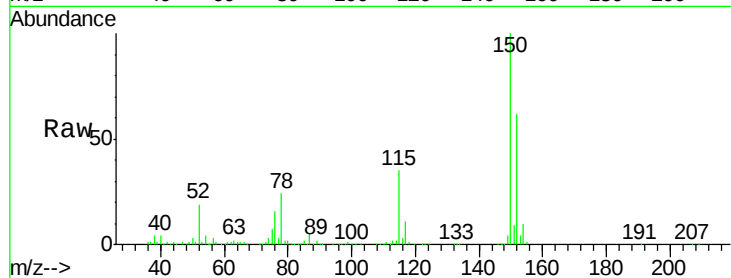

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

