


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN061918\
Data File : VN049382.D
Acq On : 19 Jun 2018 13:09
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N061618W.M
Title : SW846 8260
Last Update : Sat Jun 16 01:02:01 2018

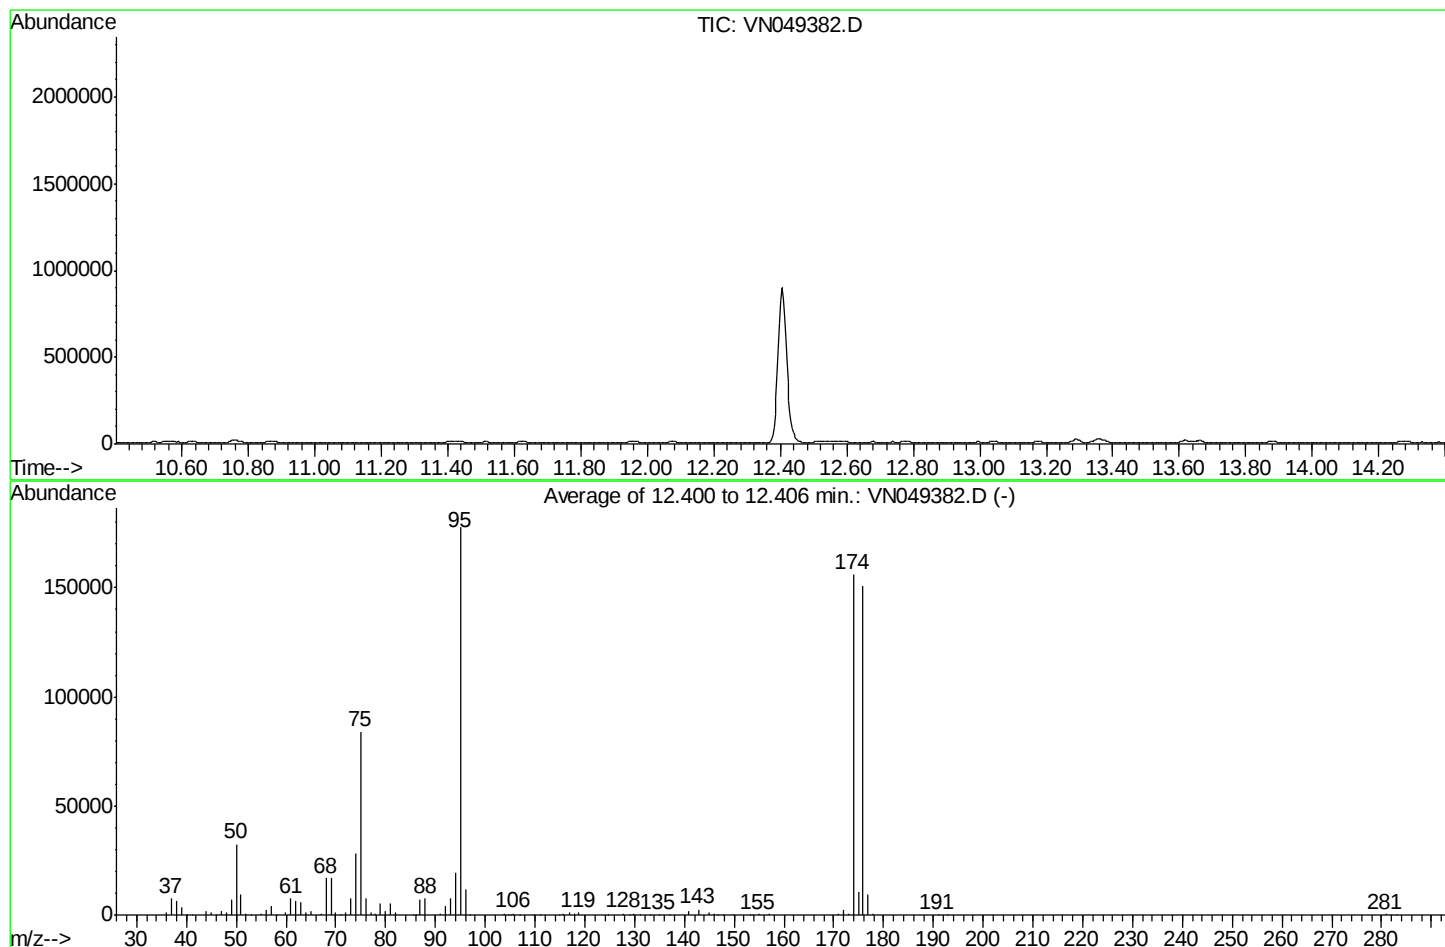

AutoFind: Scans 3362, 3363, 3364; Background Corrected with Scan 3347

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	32338	PASS
75	95	30	60	47.3	84090	PASS
95	95	100	100	100.0	177749	PASS
96	95	5	9	6.6	11715	PASS
173	174	0.00	2	0.3	541	PASS
174	95	50	100	87.8	156117	PASS
175	174	5	9	6.9	10707	PASS
176	174	95	101	96.7	150954	PASS
177	176	5	9	6.3	9488	PASS