


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN061918\
Data File : VN049408.D
Acq On : 20 Jun 2018 1:04
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N061618W.M
Title : SW846 8260
Last Update : Sat Jun 16 01:02:01 2018

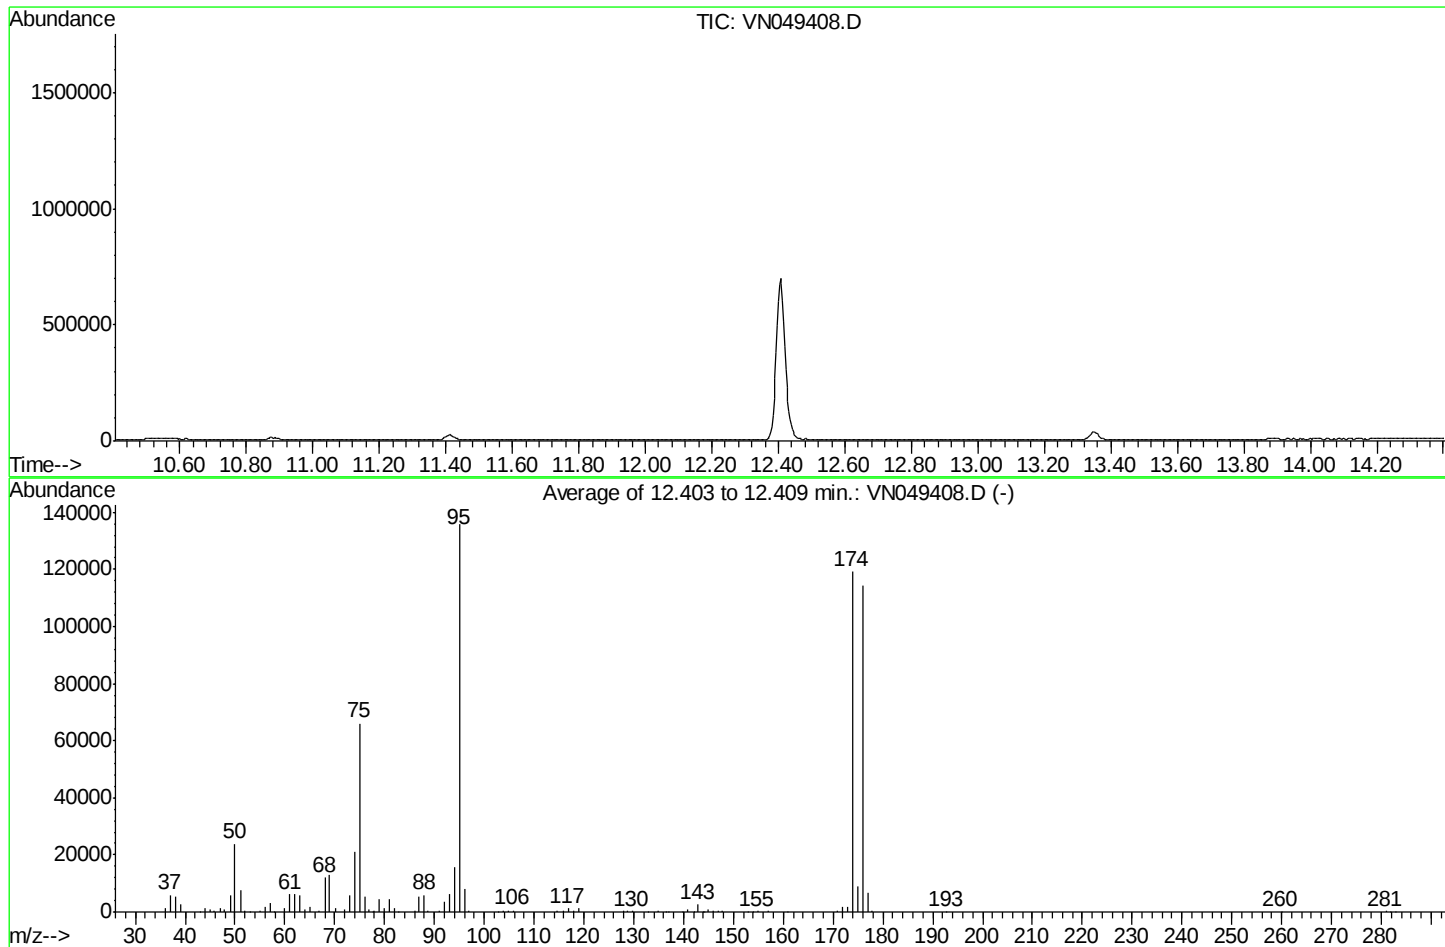

AutoFind: Scans 3363, 3364, 3365; Background Corrected with Scan 3349

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	23784	PASS
75	95	30	60	48.6	66058	PASS
95	95	100	100	100.0	135786	PASS
96	95	5	9	5.9	8061	PASS
173	174	0.00	2	1.5	1789	PASS
174	95	50	100	87.7	119152	PASS
175	174	5	9	7.5	8992	PASS
176	174	95	101	96.0	114392	PASS
177	176	5	9	6.0	6841	PASS