

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062824\
 Data File : VN082746.D
 Acq On : 28 Jun 2024 14:32
 Operator : JC\MD
 Sample : VIBLK
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VIBLK

Quant Time: Jun 28 23:04:32 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N062724W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 28 06:02:21 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.224	168	69200	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	131674	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	132008	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	53953	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.577	65	59138	55.416	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	110.840%
35) Dibromofluoromethane	8.165	113	47577	54.879	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	109.760%
50) Toluene-d8	10.565	98	175735	54.203	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	108.400%
62) 4-Bromofluorobenzene	12.853	95	55121	49.506	ug/l	0.00
Spiked Amount	50.000	Range	64 - 133	Recovery	=	99.020%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062824\
Data File : VN082746.D
Acq On : 28 Jun 2024 14:32
Operator : JC\MD
Sample : VIBLK
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VIBLK

Quant Time: Jun 28 23:04:32 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N062724W.M
Quant Title : SW846 8260
QLast Update : Fri Jun 28 06:02:21 2024
Response via : Initial Calibration




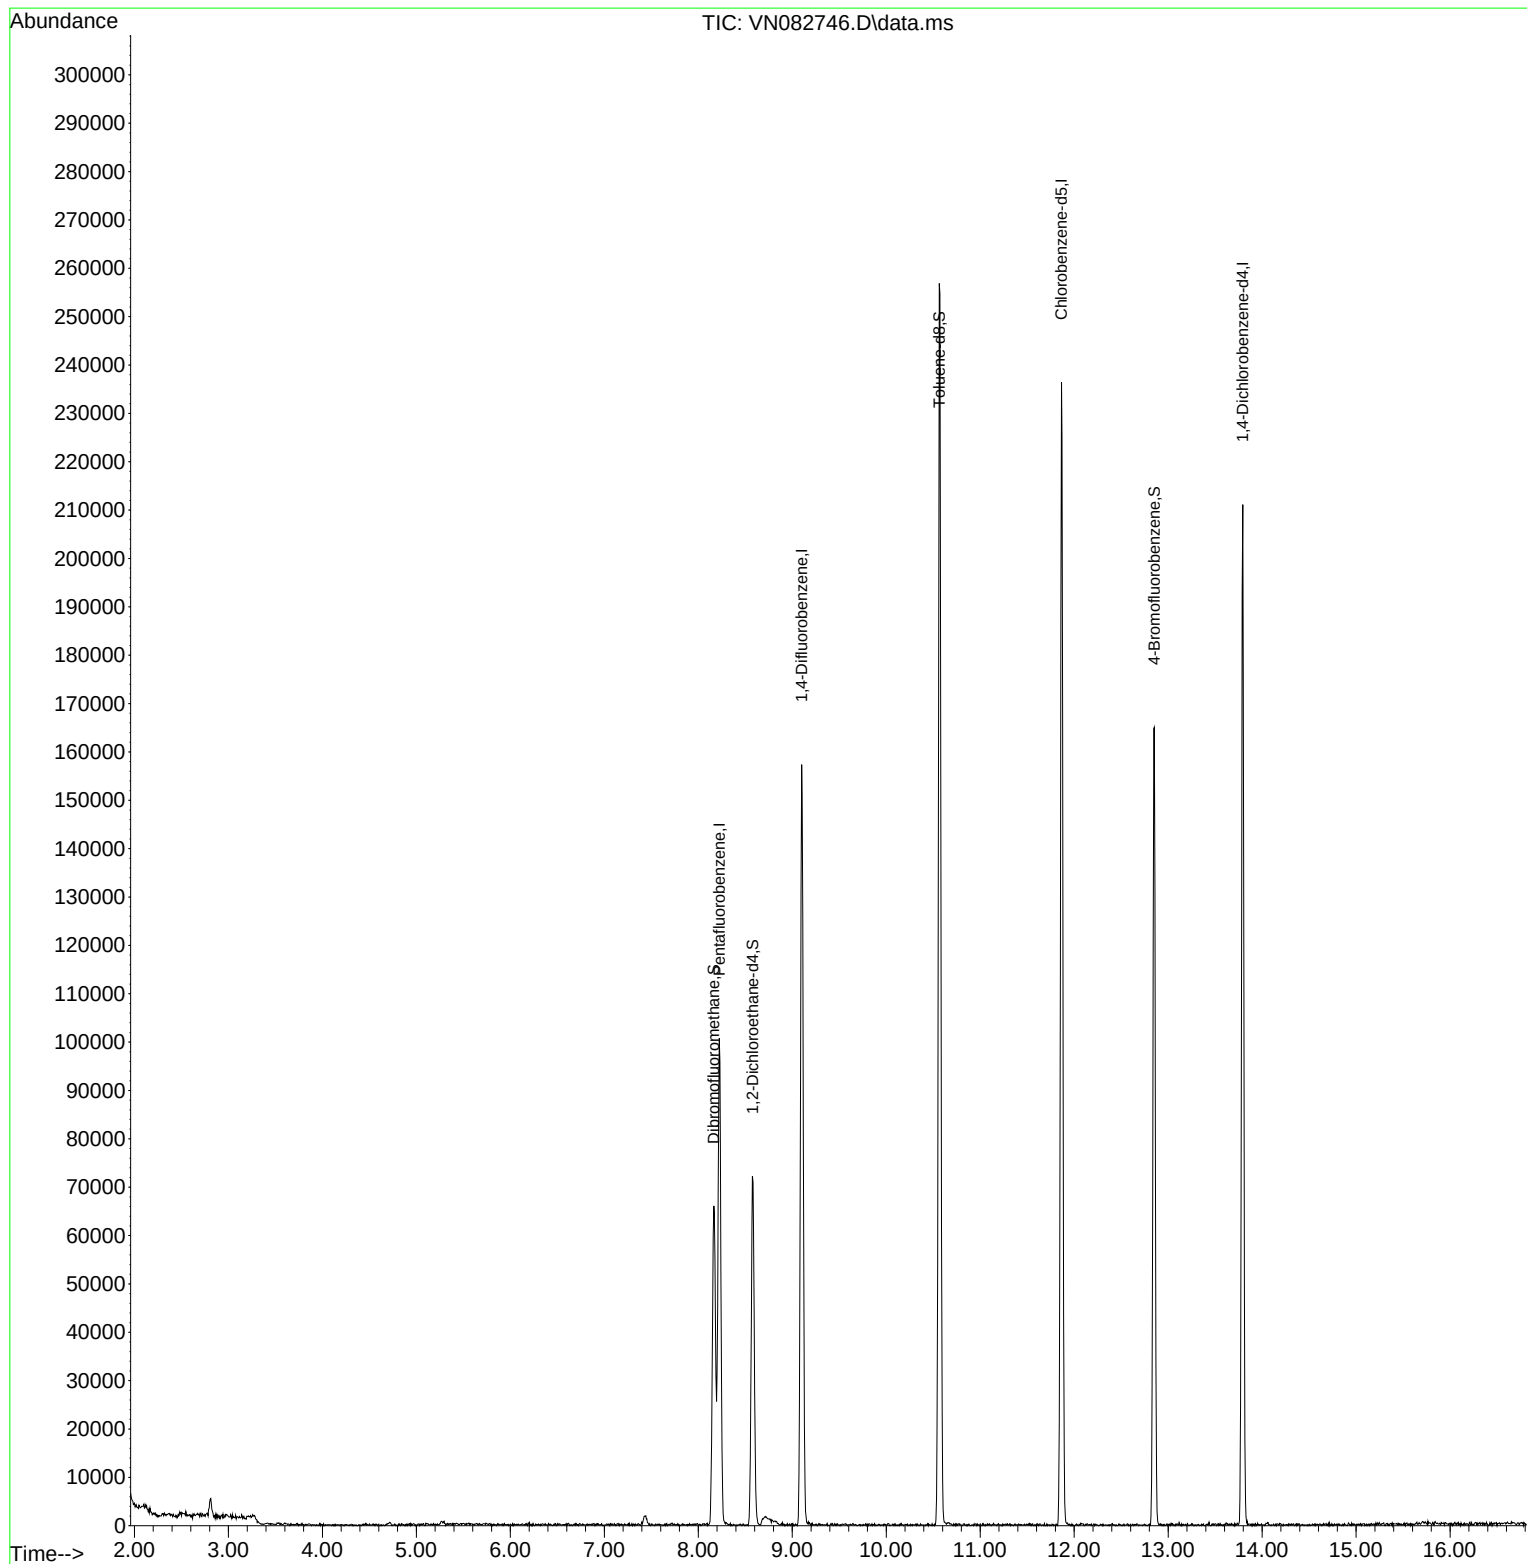


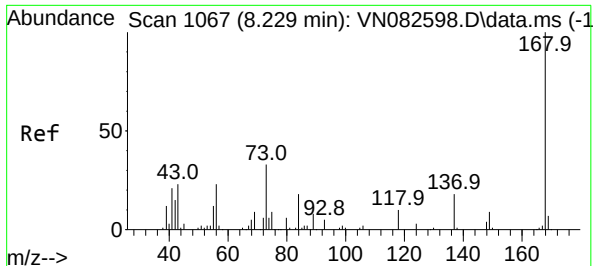

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.005 min
Lab File: VN082746.D
Acq: 28 Jun 2024 14:32




Instrument :
MSVOA_N
ClientSampleId :
VIBLK


Tgt Ion:168 Resp: 69200
Ion Ratio Lower Upper
168 100
99 65.9 48.2 72.4

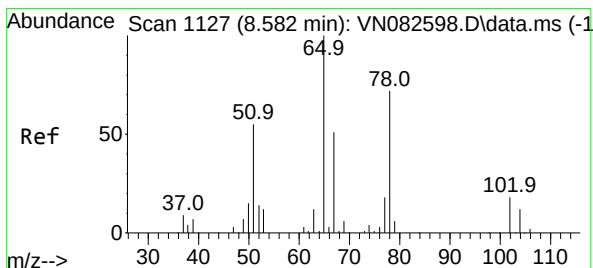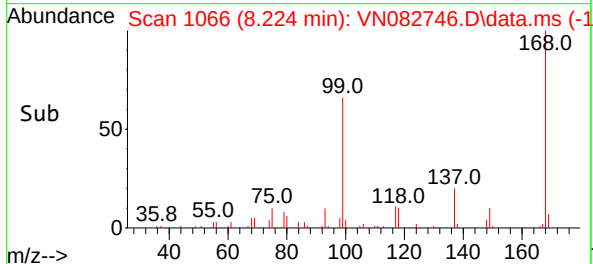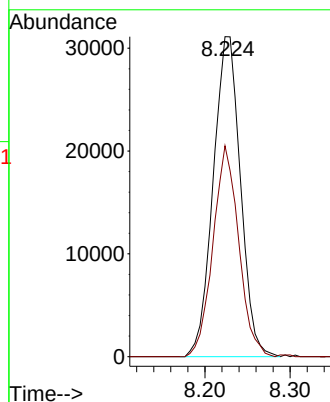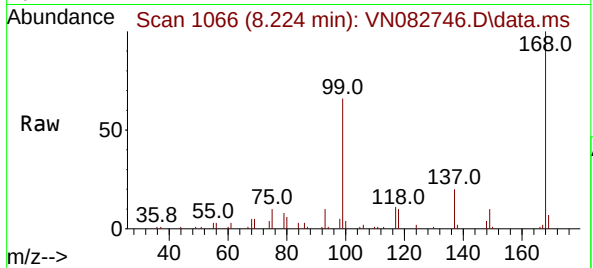

#33
1,2-Dichloroethane-d4
Concen: 55.416 ug/l
RT: 8.577 min Scan# 1126
Delta R.T. -0.005 min
Lab File: VN082746.D
Acq: 28 Jun 2024 14:32

Tgt Ion: 65 Resp: 59138
Ion Ratio Lower Upper
65 100
67 51.1 0.0 104.4


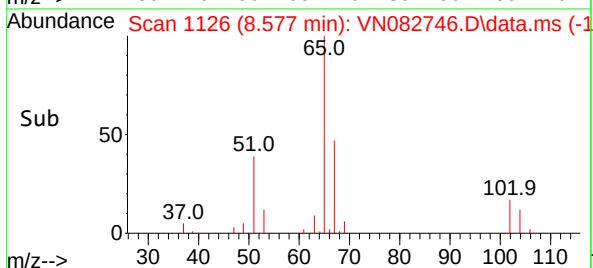
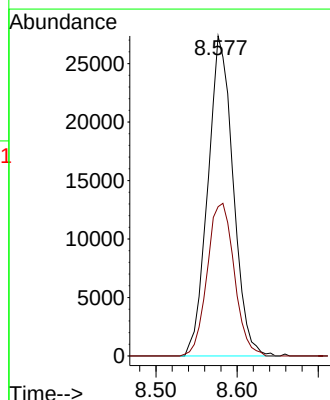
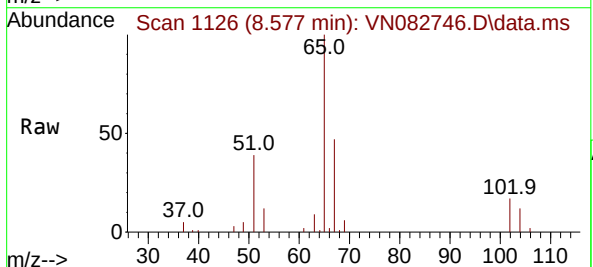


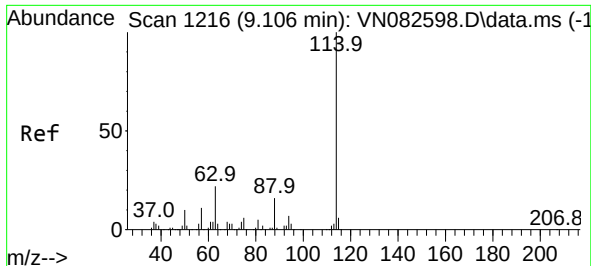

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 9.100 min Scan# 11
Delta R.T. -0.006 min
Lab File: VN082746.D
Acq: 28 Jun 2024 14:32




Instrument :
MSVOA_N
ClientSampleId :
VIBLK


Tgt Ion:114 Resp: 131674
Ion Ratio Lower Upper
114 100
63 20.6 0.0 44.6
88 15.3 0.0 31.4

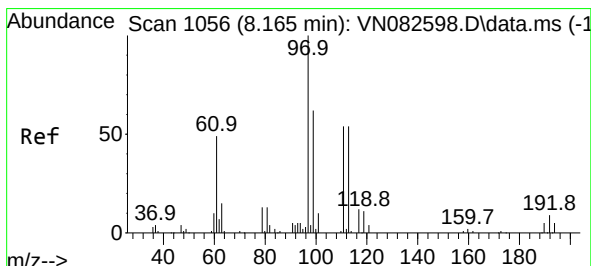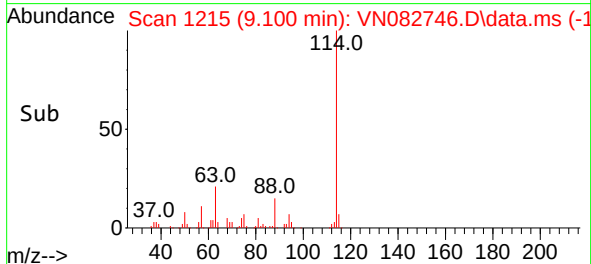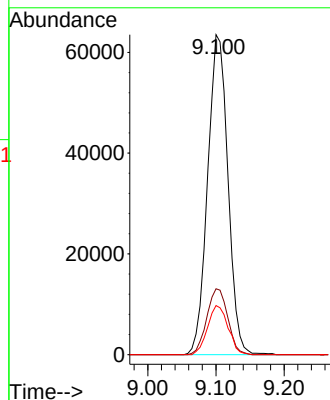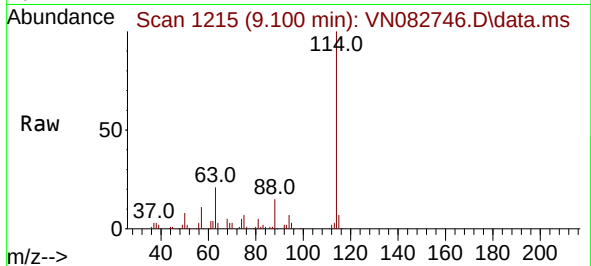

#35
Dibromofluoromethane
Concen: 54.879 ug/l
RT: 8.165 min Scan# 1056
Delta R.T. -0.000 min
Lab File: VN082746.D
Acq: 28 Jun 2024 14:32

Tgt Ion:113 Resp: 47577
Ion Ratio Lower Upper
113 100
111 104.6 82.4 123.6
192 17.3 14.9 22.3


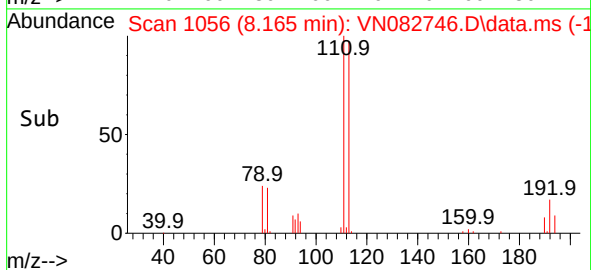
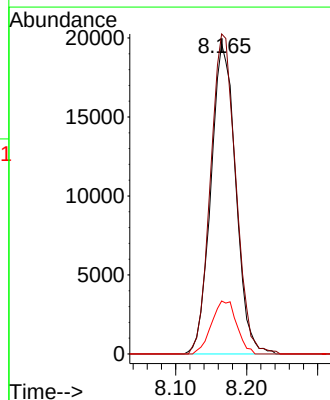
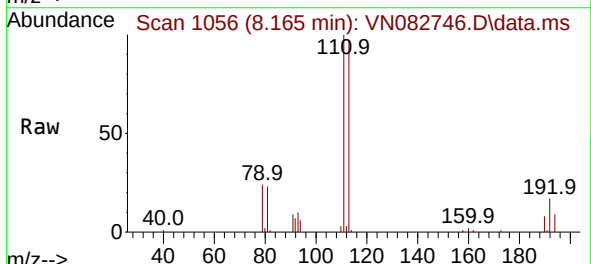


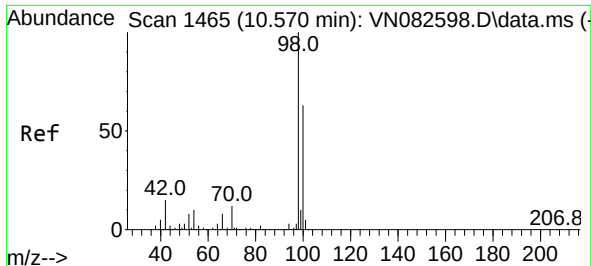

#50
Toluene-d8
Concen: 54.203 ug/l
RT: 10.565 min Scan# 1464
Delta R.T. -0.005 min
Lab File: VN082746.D
Acq: 28 Jun 2024 14:32




Instrument :
MSVOA_N
ClientSampleId :
VIBLK


Tgt Ion: 98 Resp: 175735
Ion Ratio Lower Upper
98 100
100 63.3 51.5 77.3

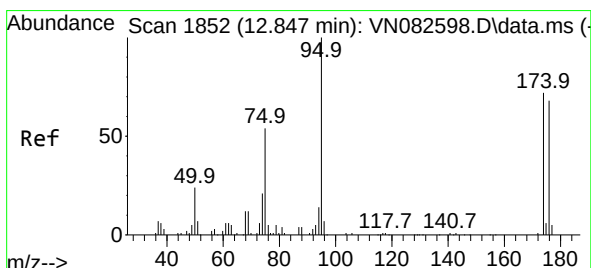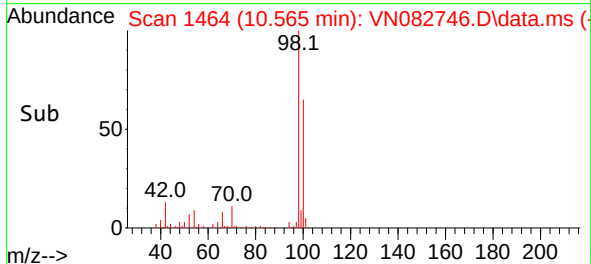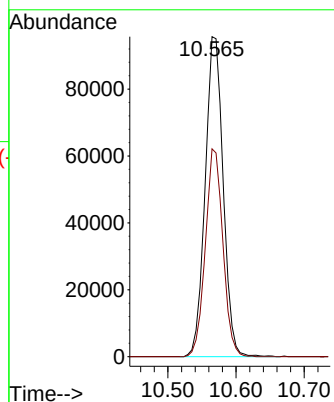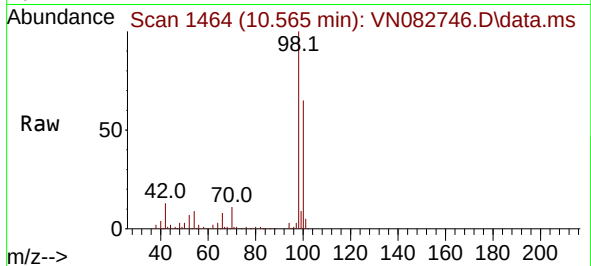

#62
4-Bromofluorobenzene
Concen: 49.506 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. 0.006 min
Lab File: VN082746.D
Acq: 28 Jun 2024 14:32

Tgt Ion: 95 Resp: 55121
Ion Ratio Lower Upper
95 100
174 77.4 0.0 159.2
176 74.7 0.0 147.6


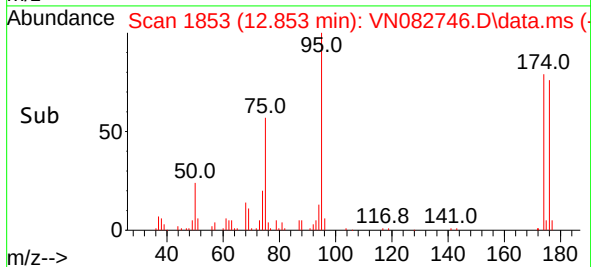
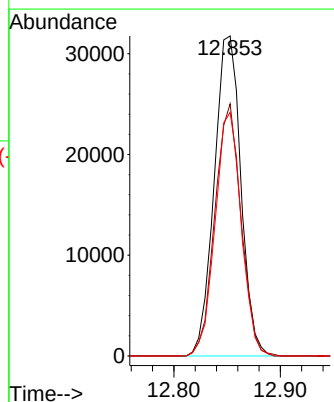
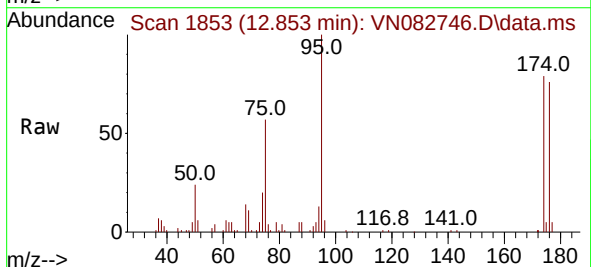


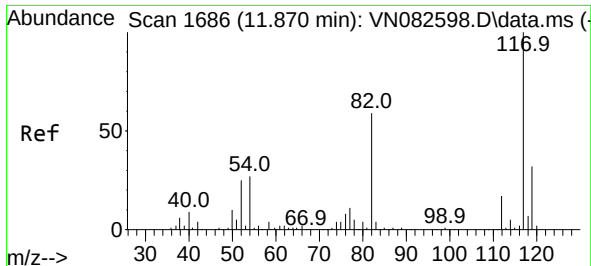

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 11
Delta R.T. -0.005 min
Lab File: VN082746.D
Acq: 28 Jun 2024 14:32

Instrument :
MSVOA_N
ClientSampleId :
VIBLK

Tgt Ion:117 Resp: 132008
Ion Ratio Lower Upper
117 100
82 56.1 47.5 71.3
119 32.3 25.6 38.4

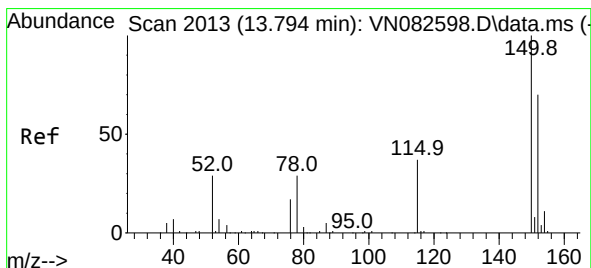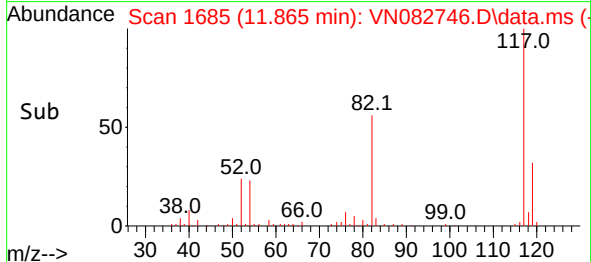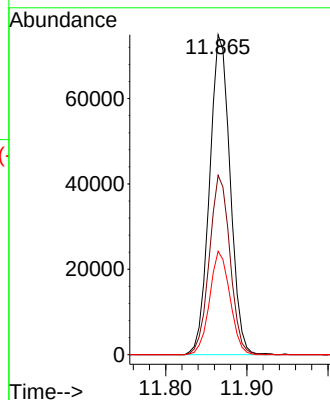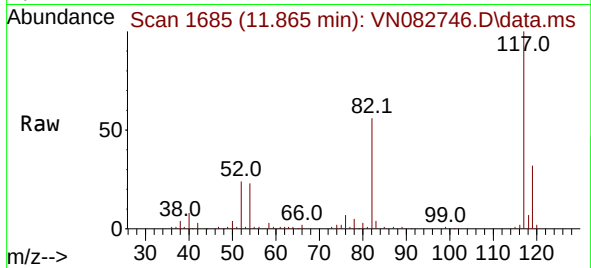

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 2013
Delta R.T. -0.000 min
Lab File: VN082746.D
Acq: 28 Jun 2024 14:32

Tgt Ion:152 Resp: 53953
Ion Ratio Lower Upper
152 100
115 61.6 30.6 91.6
150 155.7 0.0 348.6

