
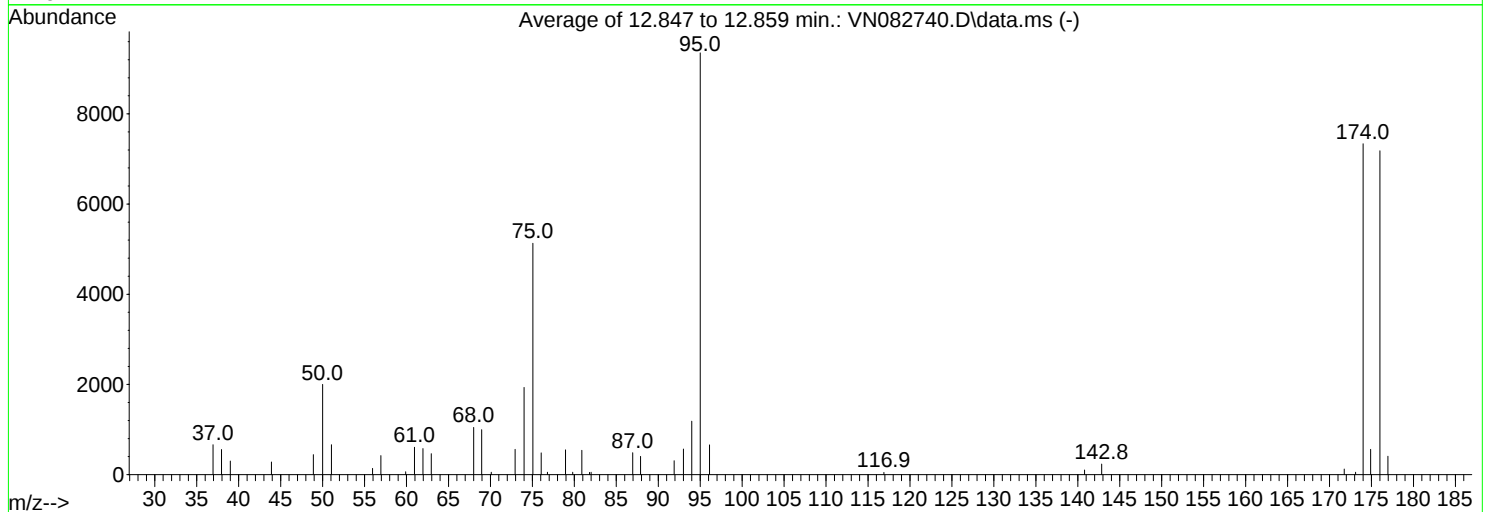


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062824\
Data File : VN082740.D
Acq On : 28 Jun 2024 08:31
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N062724W.M
Title : SW846 8260
Last Update : Fri Jun 28 06:02:21 2024

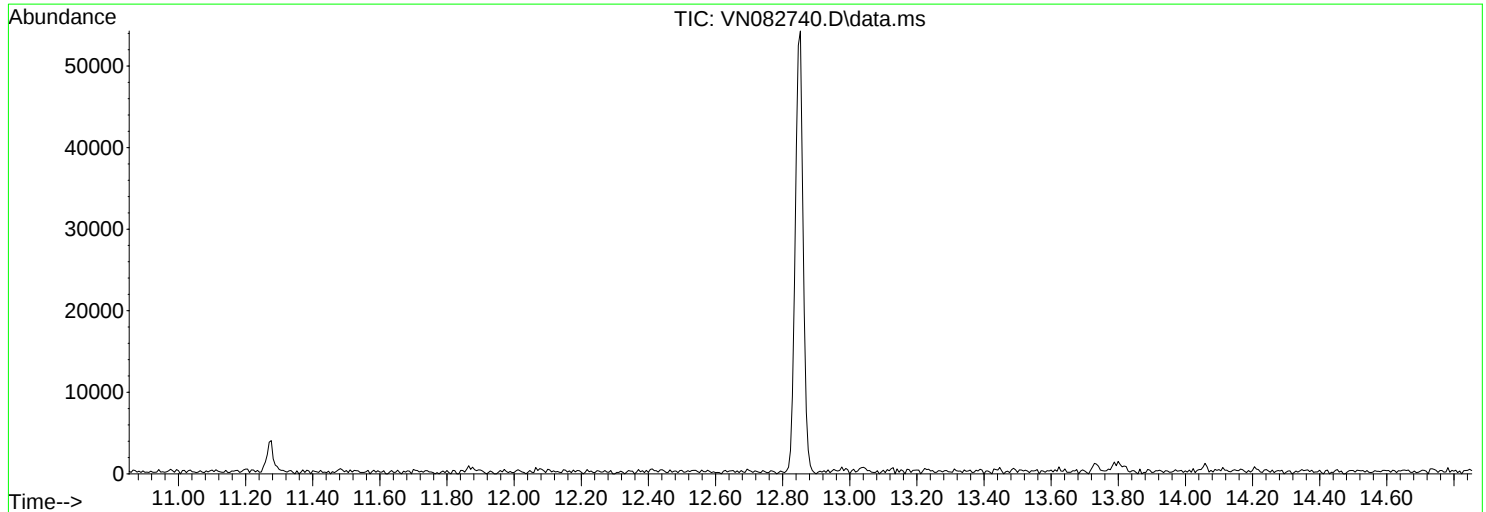

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.4	2000	PASS
75	95	30	60	54.9	5130	PASS
95	95	100	100	100.0	9352	PASS
96	95	5	9	7.1	661	PASS
173	174	0.00	2	0.7	53	PASS
174	95	50	100	78.4	7335	PASS
175	174	5	9	7.6	560	PASS
176	174	95	101	97.9	7181	PASS
177	176	5	9	5.7	408	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.95	662	61.95	577	79.80	55	116.90	51
37.95	557	62.95	465	80.90	541	140.80	104
39.00	303	68.00	1048	81.80	50	142.85	23
43.90	282	68.95	996	82.00	53	171.75	12
48.90	444	70.10	52	86.95	487	173.10	53
50.00	2000	72.95	559	87.90	403	174.00	7335
51.05	664	74.00	1932	91.90	307	174.90	560
55.95	137	75.05	5130	93.00	566	176.00	7181
56.95	424	76.05	484	94.00	1186	176.95	408
59.90	64	76.80	52	95.00	9352		
60.95	606	78.95	551	96.10	661		

Instrument :

MSVOA_N

ClientSampleId :

BFB