

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN072821\
 Data File : VN067953.D
 Acq On : 28 Jul 2021 15:13
 Operator : JC/MD
 Sample : M3195-01
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Jul 29 02:51:45 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070721W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jul 07 16:18:53 2021
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.088	168	301500	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.971	114	566110	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.747	117	538560	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.678	152	200552	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.440	65	231557	50.818	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	= 101.640%	
35) Dibromofluoromethane	8.024	113	175418	51.287	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	= 102.580%	
50) Toluene-d8	10.443	98	710502	49.628	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	= 99.260%	
62) 4-Bromofluorobenzene	12.733	95	236349	46.733	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	= 93.460%	
Target Compounds						
					Qvalue	
3) Chloromethane	2.301	50	927	0.228	ug/l	93
5) Bromomethane	2.869	94	1477	Below Cal	#	64
6) Chloroethane	3.049	64	93	Below Cal	#	44
7) Trichlorofluoromethane	3.376	101	88	Below Cal	#	18
11) Tert butyl alcohol	5.385	59	775	1.184	ug/l #	71
13) Acrolein	4.036	56	365	Below Cal	#	32
16) Acetone	4.296	43	10305	7.187	ug/l	99
18) Methyl Acetate	4.865	43	2392	0.594	ug/l	96
20) Methylene Chloride	5.101	84	1848	Below Cal	#	70
25) 2-Butanone	7.353	43	2283	0.959	ug/l	96
29) Tetrahydrofuran	7.694	42	61975	39.584	ug/l	93
31) Cyclohexane	8.091	56	8186	1.281	ug/l #	15
36) 1,1-Dichloropropene	8.088	75	26961	5.127	ug/l #	52
37) Ethyl Acetate	7.353	43	2283	0.448	ug/l #	69
38) Carbon Tetrachloride	8.091	117	33138	6.389	ug/l #	17
41) Methacrylonitrile	7.694	41	39032	14.905	ug/l #	48
43) Isopropyl Acetate	8.657	43	5242	0.585	ug/l #	58
49) 1,4-Dioxane	9.671	88	185	34.404	ug/l #	20
51) 4-Methyl-2-Pentanone	10.330	43	2401	0.436	ug/l #	75
59) 2-Hexanone	11.098	43	4988	1.298	ug/l	67
60) Dibromochloromethane	10.977	129	24	2.362	ug/l #	11
67) Ethyl Benzene	11.848	91	6107	0.303	ug/l	93
68) m/p-Xylenes	11.958	106	5276	0.693	ug/l	99
69) o-Xylene	12.283	106	11938	1.594	ug/l	90
71) Bromoform	12.717	173	133	3.212	ug/l #	1
76) 1,2,3-Trichloropropane	12.733	75	130303	31.815	ug/l #	100
80) 1,3,5-Trimethylbenzene	13.061	105	10469	0.798	ug/l	88
81) trans-1,4-Dichloro-2-b...	12.733	75	130303	102.575	ug/l #	6
84) 1,2,4-Trimethylbenzene	13.369	105	7369	0.574	ug/l	97
89) n-Butylbenzene	13.935	91	2425	0.226	ug/l #	82
90) Hexachloroethane	14.217	117	3697	1.783	ug/l #	16
93) 1,2,4-Trichlorobenzene	15.260	180	1427	3.079	ug/l #	23
95) Naphthalene	15.507	128	8693	3.844	ug/l #	90
96) 1,2,3-Trichlorobenzene	15.702	180	1559	3.094	ug/l #	1

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN072821\
Data File : VN067953.D
Acq On : 28 Jul 2021 15:13
Operator : JC/MD
Sample : M3195-01
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: Jul 29 02:51:45 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070721W.M
Quant Title : SW846 8260
QLast Update : Wed Jul 07 16:18:53 2021
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


(#)=qualifier out of range (m)=manual integration (+)=signals summed						

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN072821\
Data File : VN067953.D
Acq On : 28 Jul 2021 15:13
Operator : JC/MD
Sample : M3195-01
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: Jul 29 02:51:45 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070721W.M
Quant Title : SW846 8260
QLast Update : Wed Jul 07 16:18:53 2021
Response via : Initial Calibration

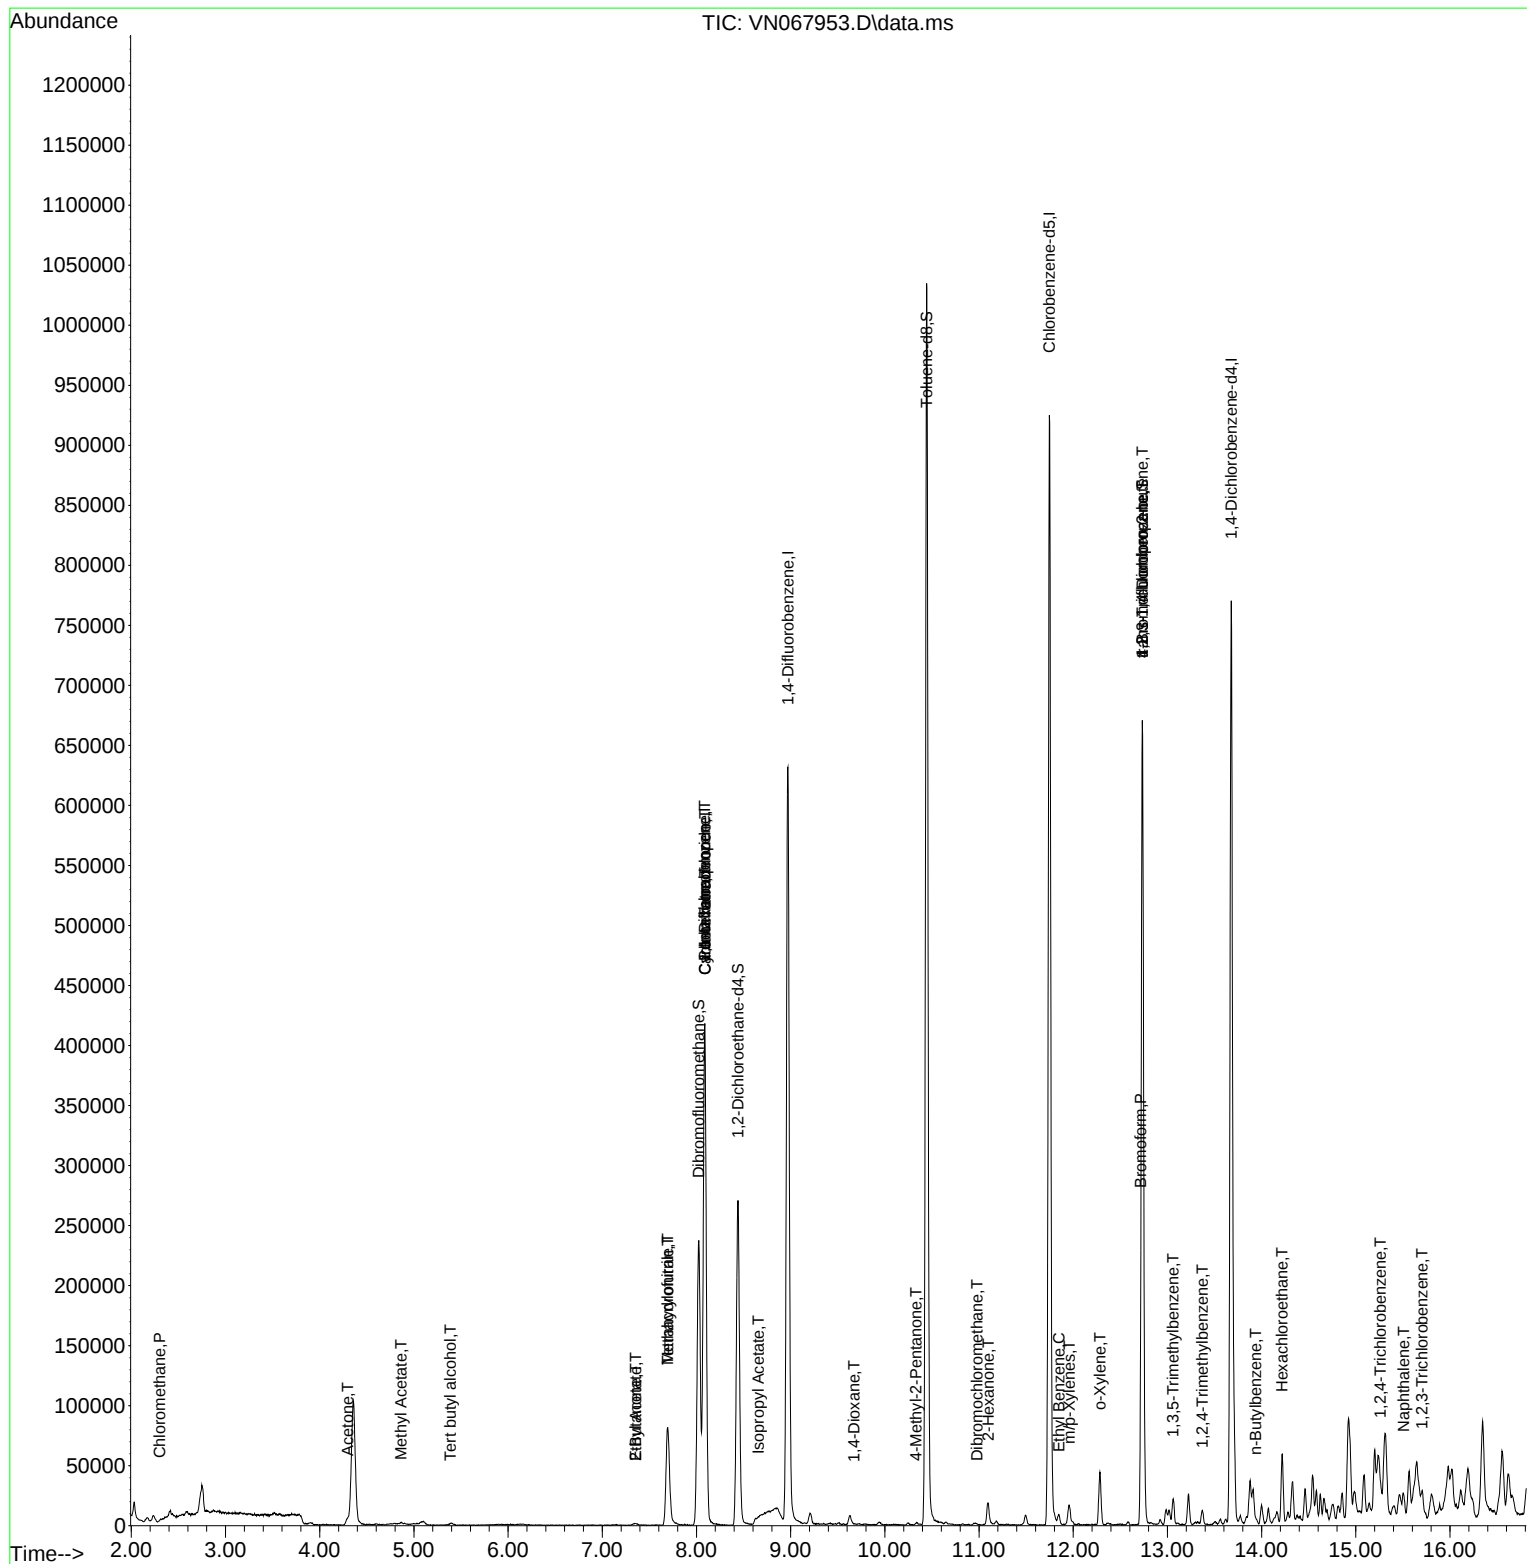



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 8.088 min Scan# 2274

Delta R.T. 0.002 min

Lab File: VN067953.D





Acq: 28 Jul 2021 15:13

Tgt Ion:168 Resp: 301500

Ion Ratio Lower Upper

168 100

99 62.9 62.9 94.3

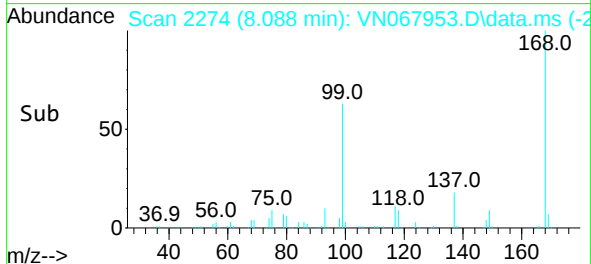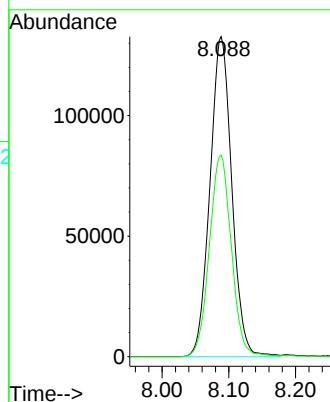

#3

Chloromethane

Concen: 0.228 ug/l

RT: 2.301 min Scan# 116

Delta R.T. -0.000 min

Lab File: VN067953.D




Acq: 28 Jul 2021 15:13


Tgt Ion: 50 Resp: 927

Ion Ratio Lower Upper

50 100


52 28.0 25.6 38.4

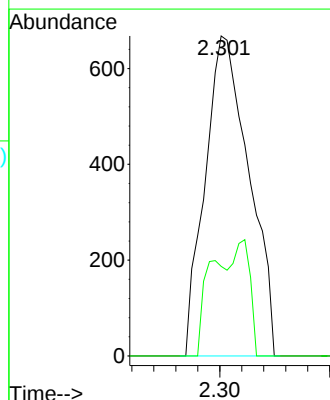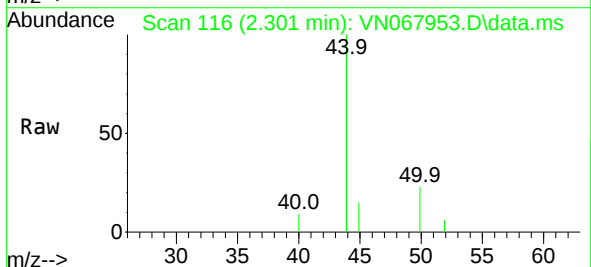






#5
Bromomethane
Concen: Below Cal
RT: 2.869 min Scan# 328
Delta R.T. 0.037 min
Lab File: VN067953.D
Acq: 28 Jul 2021 15:13

Instrument :
MSVOA_N
ClientSampled :







Tgt Ion: 94 Resp: 1477
Ion Ratio Lower Upper
94 100
96 58.1 73.7 110.5#



#6
Chloroethane
Concen: Below Cal
RT: 3.049 min Scan# 395
Delta R.T. 0.043 min
Lab File: VN067953.D
Acq: 28 Jul 2021 15:13

Tgt Ion: 64 Resp: 93
Ion Ratio Lower Upper
64 100
66 0.0 24.7 37.1#


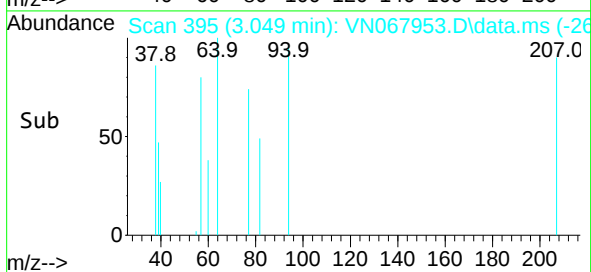






#7
Trichlorofluoromethane
Concen: Below Cal
RT: 3.376 min Scan# 517
Delta R.T. 0.011 min
Lab File: VN067953.D
Acq: 28 Jul 2021 15:13




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:101 Resp: 88
Ion Ratio Lower Upper
101 100
103 0.0 51.2 76.8#

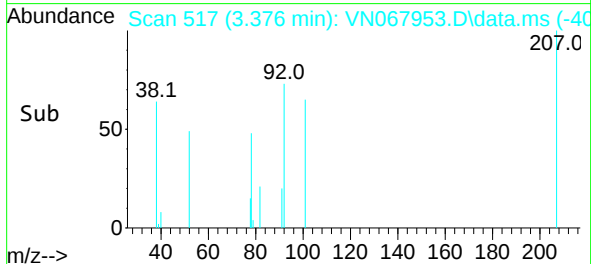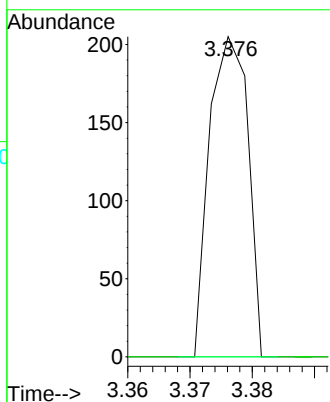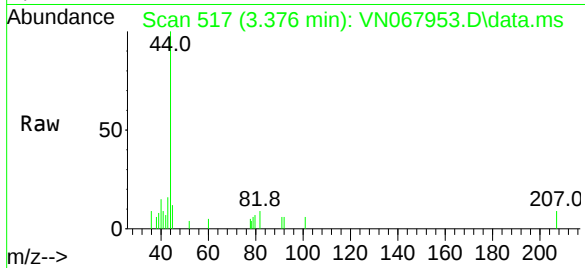

#11
Tert butyl alcohol
Concen: 1.184 ug/l
RT: 5.385 min Scan# 1266
Delta R.T. -0.005 min
Lab File: VN067953.D
Acq: 28 Jul 2021 15:13

Tgt Ion: 59 Resp: 775
Ion Ratio Lower Upper
59 100
57 0.0 8.7 13.1#



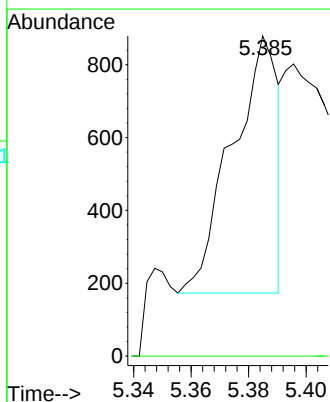
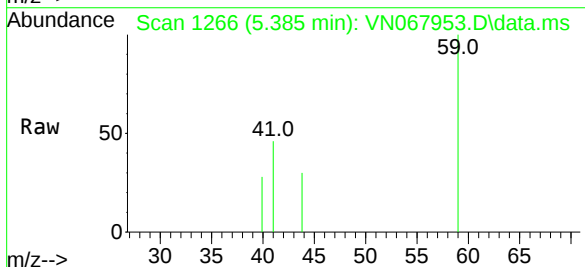




#13
Acrolein
Concen: Below Cal
RT: 4.036 min Scan# 763
Delta R.T. -0.003 min
Lab File: VN067953.D
Acq: 28 Jul 2021 15:13




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 56 Resp: 365
Ion Ratio Lower Upper
56 100
55 14.8 57.4 86.0#

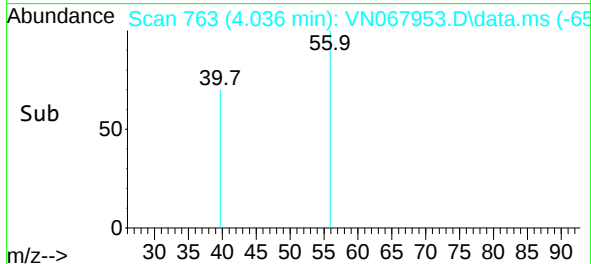

#16
Acetone
Concen: 7.187 ug/l
RT: 4.296 min Scan# 860
Delta R.T. 0.008 min
Lab File: VN067953.D
Acq: 28 Jul 2021 15:13

Tgt Ion: 43 Resp: 10305
Ion Ratio Lower Upper
43 100
58 26.9 21.2 31.8

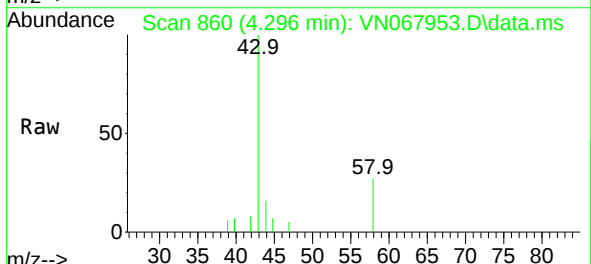

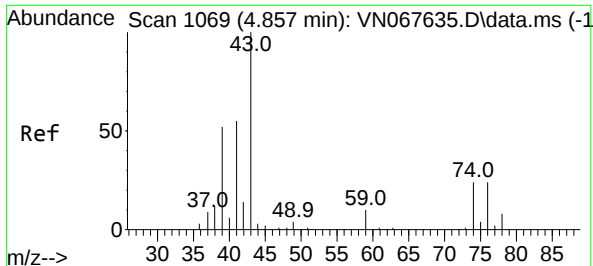

#18

Methyl Acetate

Concen: 0.594 ug/l

RT: 4.865 min Scan# 1072

Delta R.T. 0.008 min

Lab File: VN067953.D





Acq: 28 Jul 2021 15:13

Tgt Ion: 43 Resp: 2392

Ion Ratio Lower Upper

43 100

74 19.9 17.4 26.0

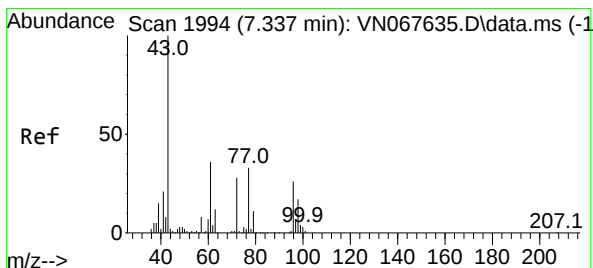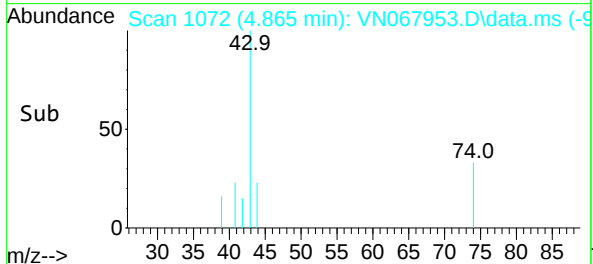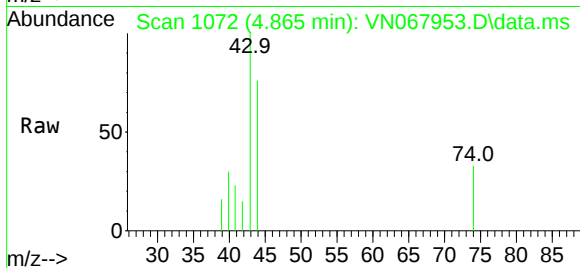

#25

2-Butanone

Concen: 0.959 ug/l

RT: 7.353 min Scan# 2000

Delta R.T. 0.016 min

Lab File: VN067953.D




Acq: 28 Jul 2021 15:13


Tgt Ion: 43 Resp: 2283

Ion Ratio Lower Upper

43 100

72 22.6 19.7 29.5

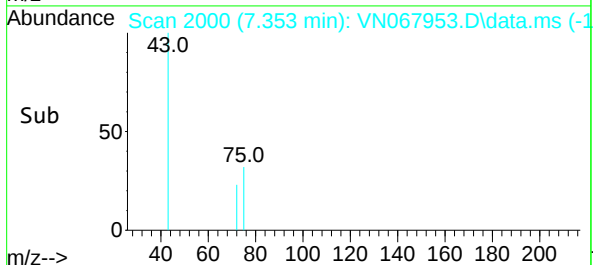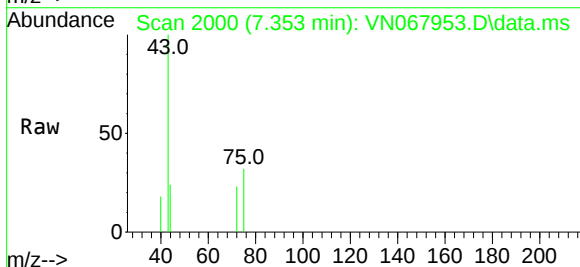



#29

Tetrahydrofuran

Concen: 39.584 ug/l


RT: 7.694 min Scan# 2127

Delta R.T. 0.005 min




Lab File: VN067953.D

Acq: 28 Jul 2021 15:13

Instrument :
MSVOA_N
ClientSampleId :



Tgt Ion:	42	Resp:	61975
Ion	Ratio	Lower	Upper
42	100		
72	43.9	32.8	49.2
71	44.3	31.2	46.8

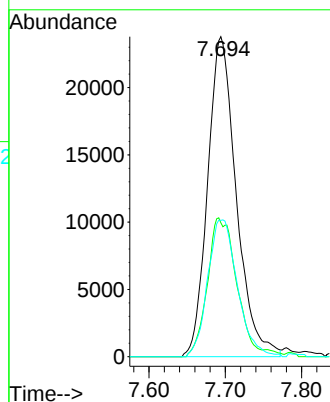

#31

Cyclohexane

Concen: 1.281 ug/l




RT: 8.091 min Scan# 2275


Delta R.T. -0.003 min

Lab File: VN067953.D

Acq: 28 Jul 2021 15:13

Tgt Ion:	56	Resp:	8186
Ion	Ratio	Lower	Upper
56	100		
69	139.3	27.3	40.9#
84	119.9	64.9	97.3#


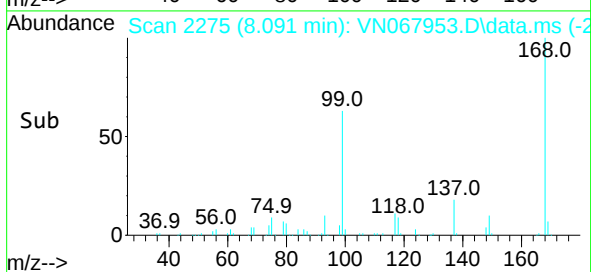
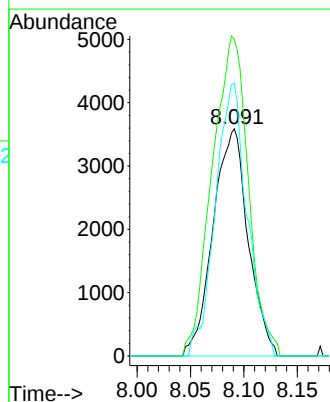





#33
 1,2-Dichloroethane-d4
 Concen: 50.818 ug/l
 RT: 8.440 min Scan# 2405
 Delta R.T. -0.000 min
 Lab File: VN067953.D
 Acq: 28 Jul 2021 15:13




Instrument :
 MSVOA_N
 ClientSampleId :


Tgt Ion: 65 Resp: 231557
 Ion Ratio Lower Upper
 65 100
 67 50.2 0.0 98.6

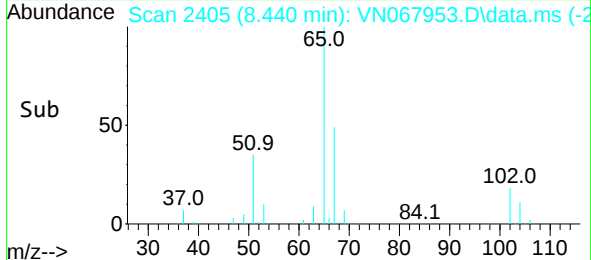

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.971 min Scan# 2603
 Delta R.T. 0.003 min
 Lab File: VN067953.D
 Acq: 28 Jul 2021 15:13

Tgt Ion: 114 Resp: 566110
 Ion Ratio Lower Upper
 114 100
 63 20.6 0.0 49.0
 88 15.1 0.0 36.6


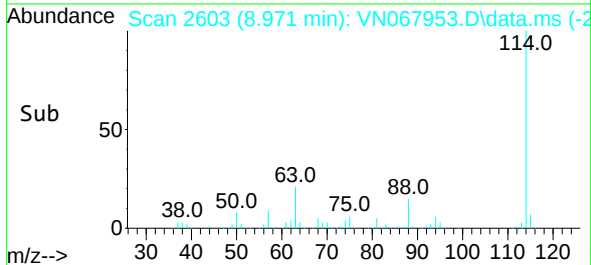

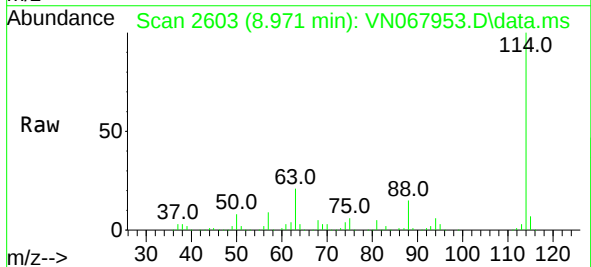




#35
Dibromofluoromethane
Concen: 51.287 ug/l
RT: 8.024 min Scan# 2250
Delta R.T. 0.003 min
Lab File: VN067953.D
Acq: 28 Jul 2021 15:13




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:113 Resp: 175418
Ion Ratio Lower Upper
113 100
111 102.1 83.8 125.8
192 15.6 13.4 20.0

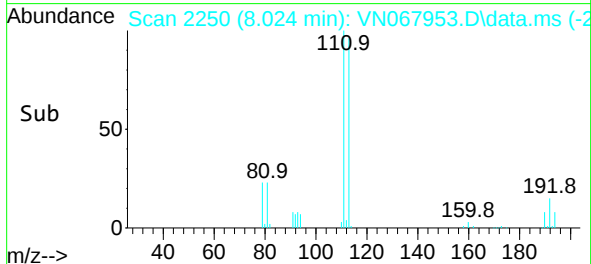

#36
1,1-Dichloropropene
Concen: 5.127 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. -0.134 min
Lab File: VN067953.D
Acq: 28 Jul 2021 15:13

Tgt Ion: 75 Resp: 26961
Ion Ratio Lower Upper
75 100
110 9.0 15.7 47.0#
77 0.0 24.6 37.0#




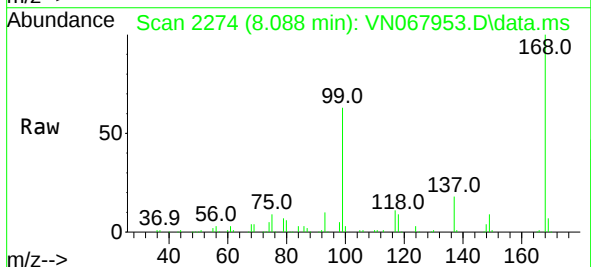


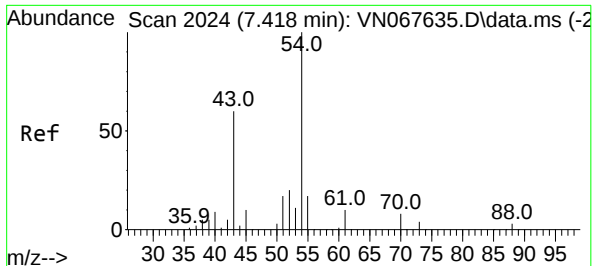

#37
Ethyl Acetate
Concen: 0.448 ug/l
RT: 7.353 min Scan# 2000
Delta R.T. -0.065 min
Lab File: VN067953.D
Acq: 28 Jul 2021 15:13




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:	43	Resp:	2283
Ion	Ratio	Lower	Upper
43	100		
61	0.0	10.6	16.0#
70	0.0	8.1	12.1#

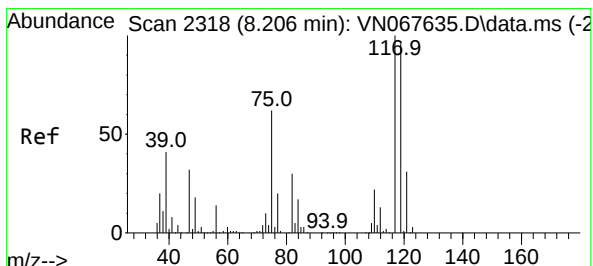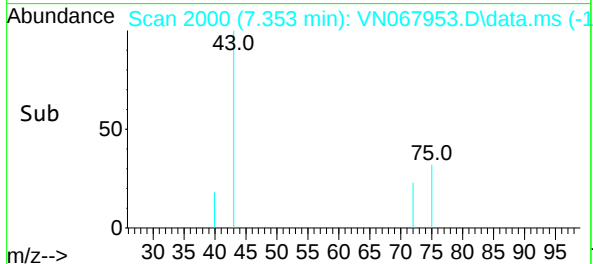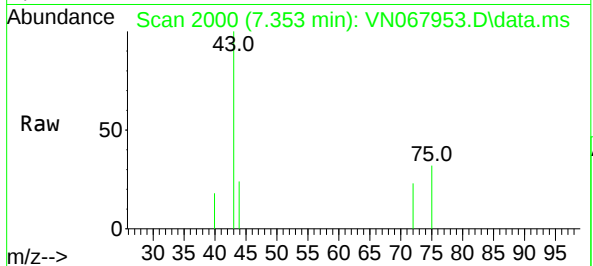

#38
Carbon Tetrachloride
Concen: 6.389 ug/l
RT: 8.091 min Scan# 2275
Delta R.T. -0.115 min
Lab File: VN067953.D
Acq: 28 Jul 2021 15:13

Tgt Ion:	117	Resp:	33138
Ion	Ratio	Lower	Upper
117	100		
119	5.1	75.4	113.2#
121	0.0	23.5	35.3#


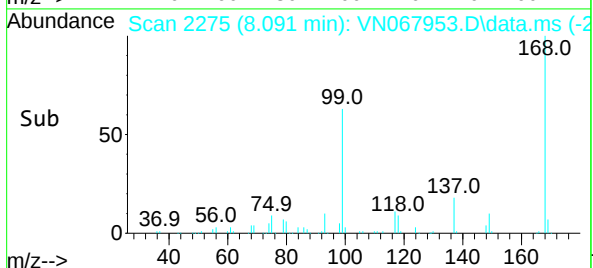
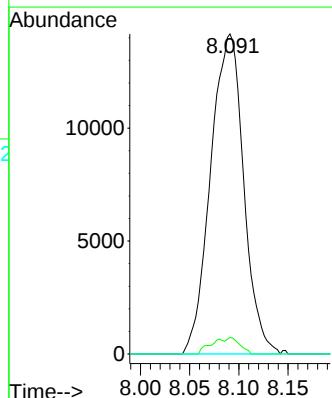
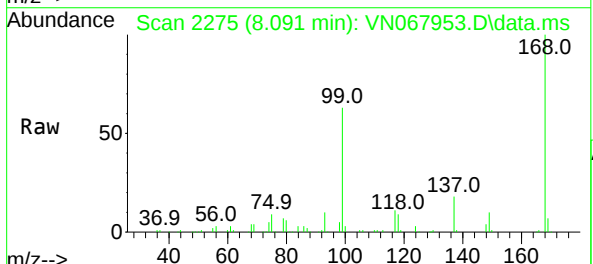


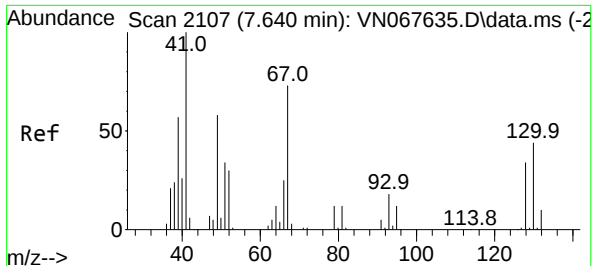

#41
Methacrylonitrile
Concen: 14.905 ug/l
RT: 7.694 min Scan# 2127
Delta R.T. 0.054 min
Lab File: VN067953.D
Acq: 28 Jul 2021 15:13




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:	41	Resp:	39032
Ion	Ratio	Lower	Upper
41	100		
39	53.5	47.6	71.4
67	0.0	57.7	86.5#
52	0.0	26.2	39.4#

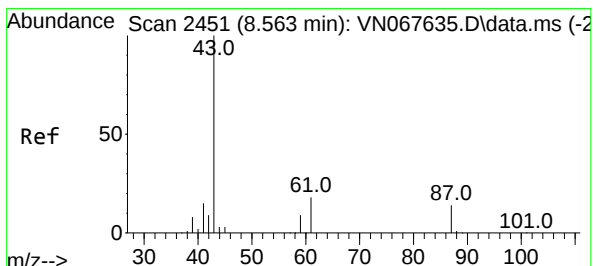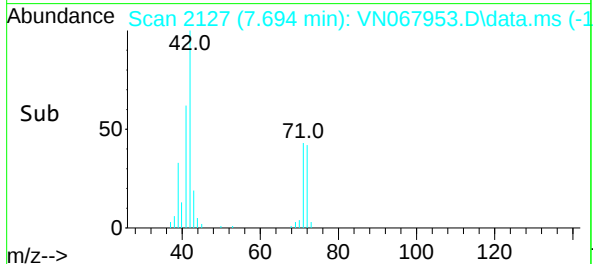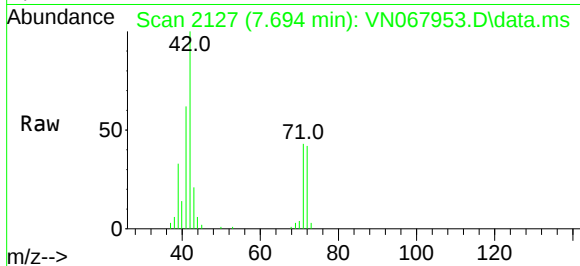

#43
Isopropyl Acetate
Concen: 0.585 ug/l
RT: 8.657 min Scan# 2486
Delta R.T. 0.094 min
Lab File: VN067953.D
Acq: 28 Jul 2021 15:13

Tgt Ion:	43	Resp:	5242
Ion	Ratio	Lower	Upper
43	100		
61	0.0	19.0	28.4#
87	0.0	9.5	14.3#


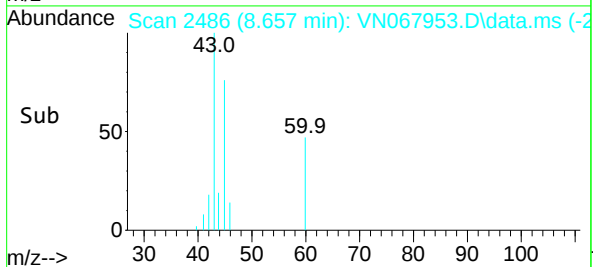

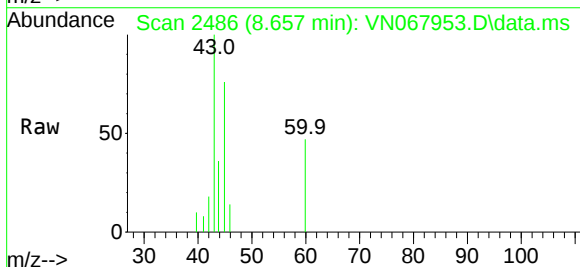




#49
1,4-Dioxane
Concen: 34.404 ug/l
RT: 9.671 min Scan# 2864
Delta R.T. 0.100 min
Lab File: VN067953.D
Acq: 28 Jul 2021 15:13




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 88 Resp: 185
Ion Ratio Lower Upper
88 100
43 0.0 28.8 43.2#
58 0.0 60.4 90.6#

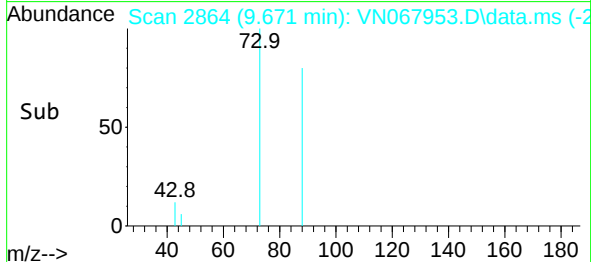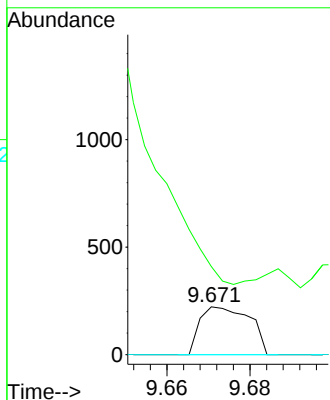

#50
Toluene-d8
Concen: 49.628 ug/l
RT: 10.443 min Scan# 3152
Delta R.T. 0.000 min
Lab File: VN067953.D
Acq: 28 Jul 2021 15:13

Tgt Ion: 98 Resp: 710502
Ion Ratio Lower Upper
98 100
100 64.3 51.7 77.5


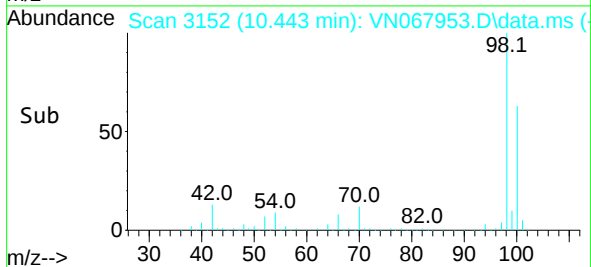
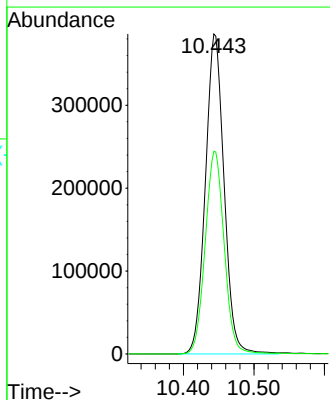
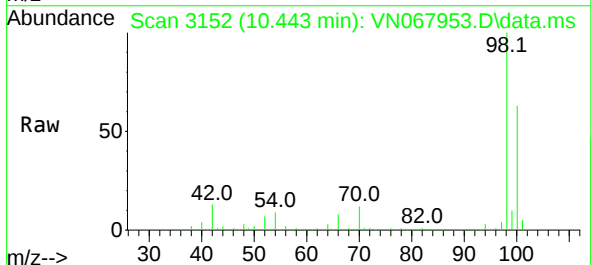




#51
4-Methyl-2-Pentanone
Concen: 0.436 ug/l
RT: 10.330 min Scan# 3110
Delta R.T. -0.003 min
Lab File: VN067953.D
Acq: 28 Jul 2021 15:13




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 43 Resp: 2401
Ion Ratio Lower Upper
43 100
58 21.2 28.6 43.0#



#59
2-Hexanone
Concen: 1.298 ug/l
RT: 11.098 min Scan# 3396
Delta R.T. 0.011 min
Lab File: VN067953.D
Acq: 28 Jul 2021 15:13

Tgt Ion: 43 Resp: 4988
Ion Ratio Lower Upper
43 100
58 26.6 24.7 74.1









#60
Dibromochloromethane
Concen: 2.362 ug/l
RT: 10.977 min Scan# 3351
Delta R.T. -0.265 min
Lab File: VN067953.D
Acq: 28 Jul 2021 15:13




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:129 Resp: 24
Ion Ratio Lower Upper
129 100
127 0.0 38.6 115.8#

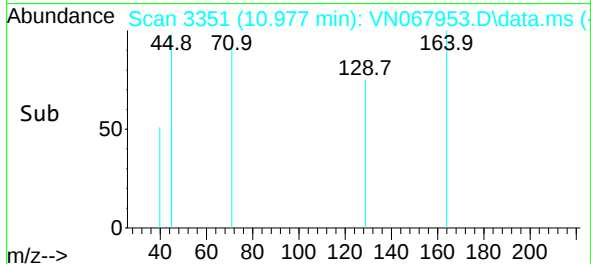

#62
4-Bromofluorobenzene
Concen: 46.733 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. 0.000 min
Lab File: VN067953.D
Acq: 28 Jul 2021 15:13

Tgt Ion: 95 Resp: 236349
Ion Ratio Lower Upper
95 100
174 71.7 0.0 122.0
176 68.6 0.0 117.6




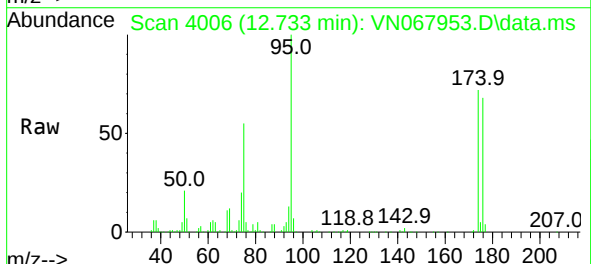




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.747 min Scan# 3638
Delta R.T. 0.000 min
Lab File: VN067953.D
Acq: 28 Jul 2021 15:13




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:117 Resp: 538560
Ion Ratio Lower Upper
117 100
82 55.5 53.1 79.7
119 31.7 25.5 38.3

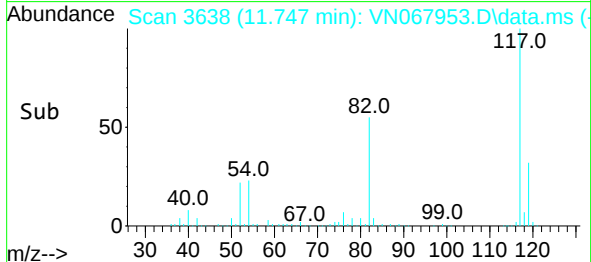

#67
Ethyl Benzene
Concen: 0.303 ug/l
RT: 11.848 min Scan# 3676
Delta R.T. 0.002 min
Lab File: VN067953.D
Acq: 28 Jul 2021 15:13

Tgt Ion: 91 Resp: 6107
Ion Ratio Lower Upper
91 100
106 33.2 23.4 35.0


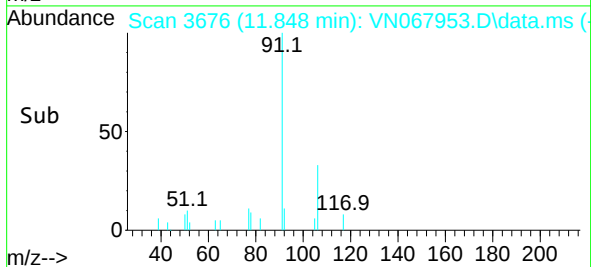

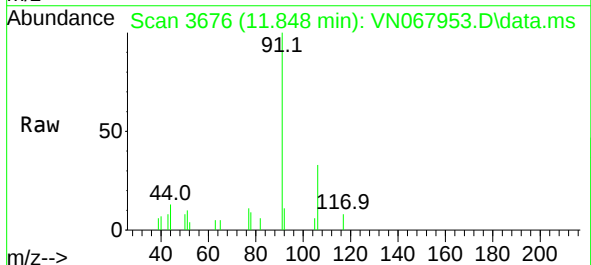


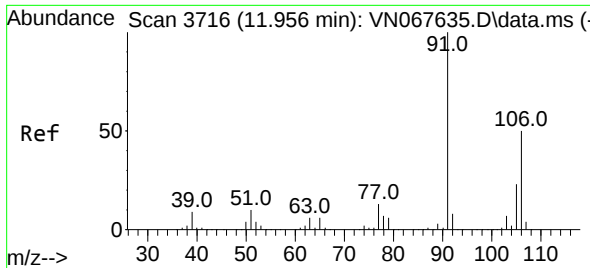

#68
m/p-Xylenes
Concen: 0.693 ug/l
RT: 11.958 min Scan# 3717
Delta R.T. 0.002 min
Lab File: VN067953.D
Acq: 28 Jul 2021 15:13




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:106 Resp: 5276
Ion Ratio Lower Upper
106 100
91 224.3 180.6 270.8

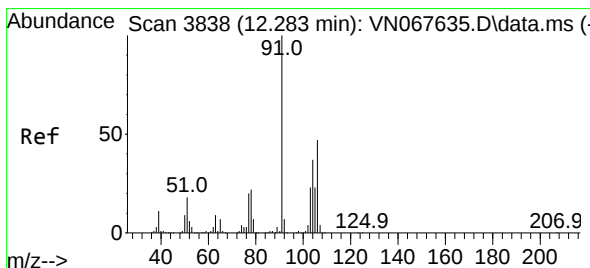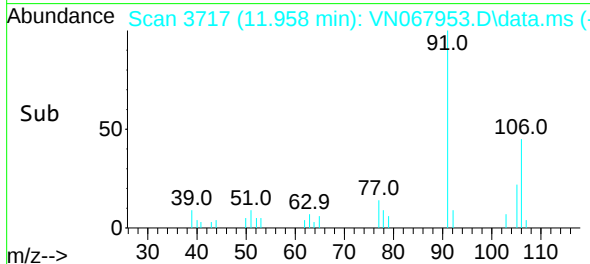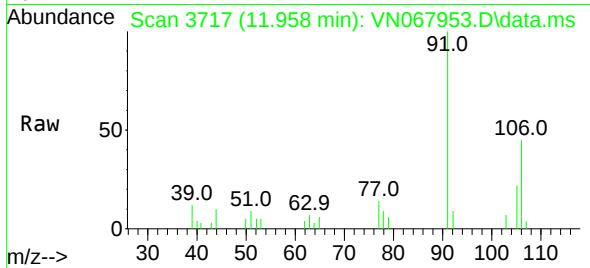

#69
o-Xylene
Concen: 1.594 ug/l
RT: 12.283 min Scan# 3838
Delta R.T. -0.000 min
Lab File: VN067953.D
Acq: 28 Jul 2021 15:13

Tgt Ion:106 Resp: 11938
Ion Ratio Lower Upper
106 100
91 219.2 118.3 354.9


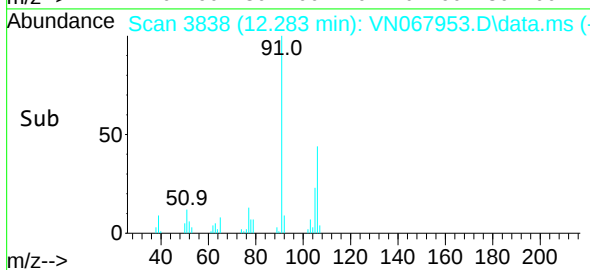

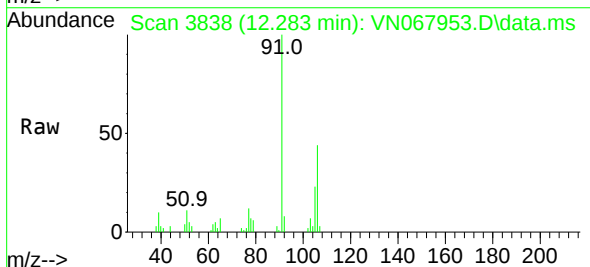


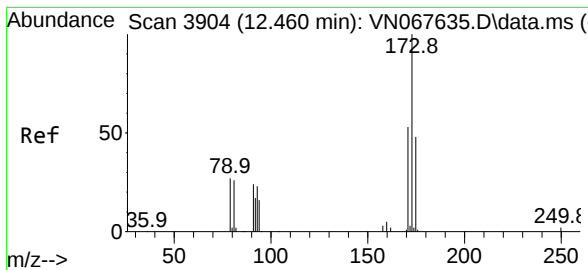

#71
Bromoform
Concen: 3.212 ug/l
RT: 12.717 min Scan# 4000
Delta R.T. 0.257 min
Lab File: VN067953.D
Acq: 28 Jul 2021 15:13




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:173 Resp: 133
Ion Ratio Lower Upper
173 100
175 8985.0 23.9 71.8#
254 0.0 0.0 0.0

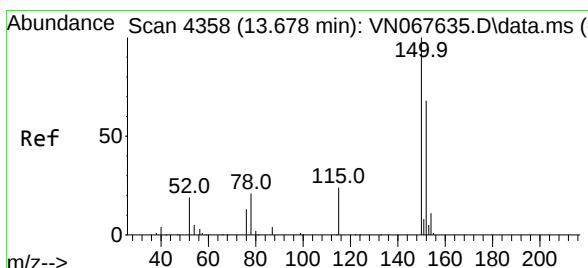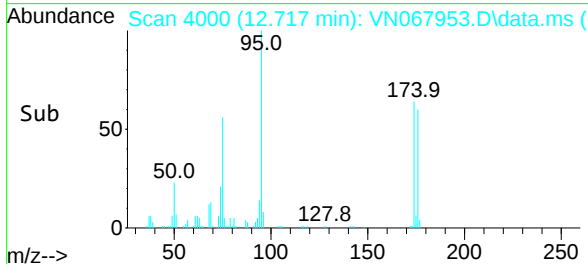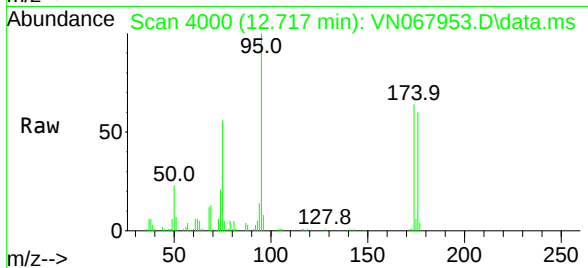

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.678 min Scan# 4358
Delta R.T. 0.000 min
Lab File: VN067953.D
Acq: 28 Jul 2021 15:13

Tgt Ion:152 Resp: 200552
Ion Ratio Lower Upper
152 100
115 62.8 36.1 108.5
150 158.1 0.0 351.8


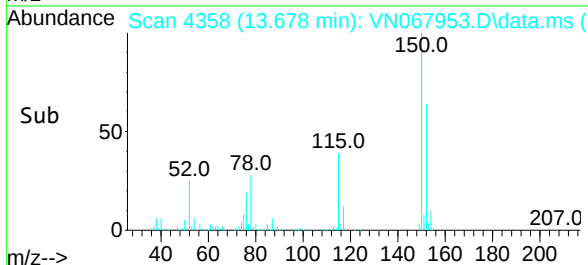

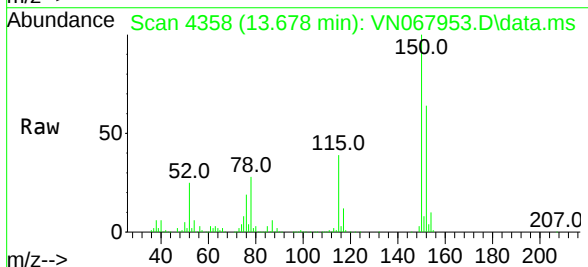




#76
1,2,3-Trichloropropane
Concen: 31.815 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. -0.151 min
Lab File: VN067953.D
Acq: 28 Jul 2021 15:13




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 75 Resp: 130303
Ion Ratio Lower Upper
75 100
77 1.2 0.0 0.0#

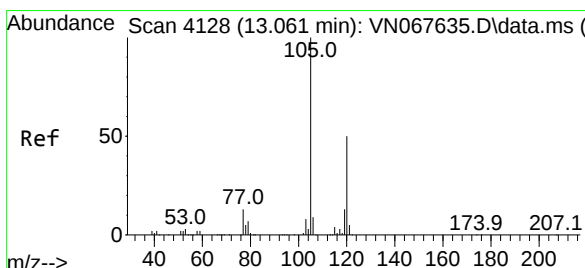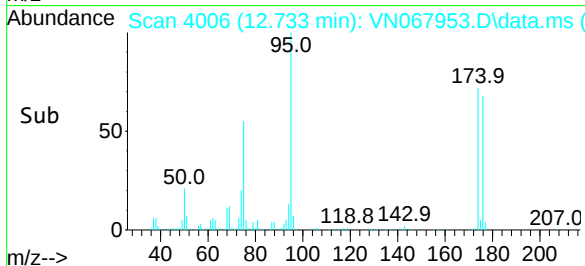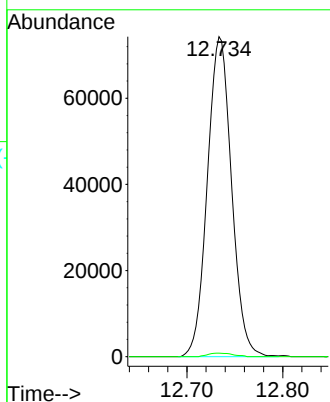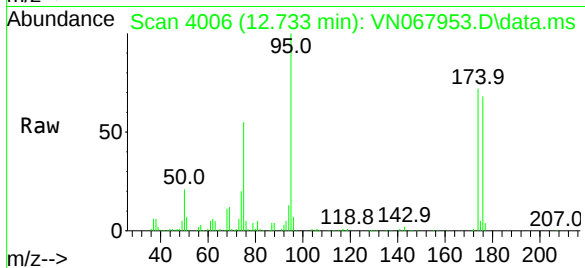

#80
1,3,5-Trimethylbenzene
Concen: 0.798 ug/l
RT: 13.061 min Scan# 4128
Delta R.T. -0.000 min
Lab File: VN067953.D
Acq: 28 Jul 2021 15:13


Tgt Ion:105 Resp: 10469
Ion Ratio Lower Upper
105 100
120 52.4 22.2 66.6

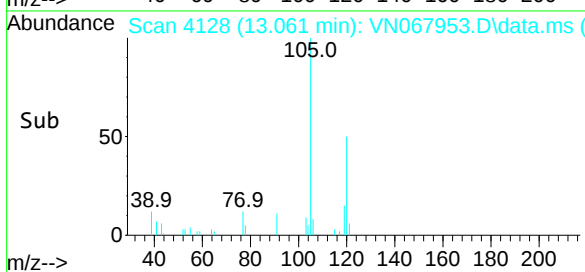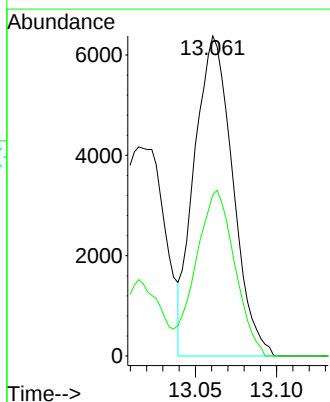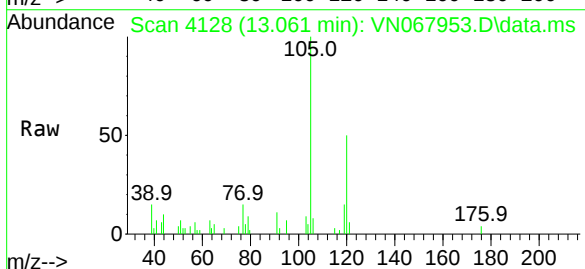






#81
 trans-1,4-Dichloro-2-butene
 Concen: 102.575 ug/l
 RT: 12.733 min Scan# 4006
 Delta R.T. 0.104 min
 Lab File: VN067953.D
 Acq: 28 Jul 2021 15:13


Instrument :
 MSVOA_N
 ClientSampled :





Tgt Ion: 75 Resp: 130303
 Ion Ratio Lower Upper
 75 100
 53 0.0 87.6 131.4#
 89 0.0 37.8 56.8#




#84
 1,2,4-Trimethylbenzene
 Concen: 0.574 ug/l
 RT: 13.369 min Scan# 4243
 Delta R.T. -0.003 min
 Lab File: VN067953.D
 Acq: 28 Jul 2021 15:13



Tgt Ion: 105 Resp: 7369
 Ion Ratio Lower Upper
 105 100
 120 43.3 20.6 61.8









#89
n-Butylbenzene
Concen: 0.226 ug/l
RT: 13.935 min Scan# 4454
Delta R.T. -0.011 min
Lab File: VN067953.D
Acq: 28 Jul 2021 15:13




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 91 Resp: 2425
Ion Ratio Lower Upper
91 100
92 47.2 25.7 77.1
134 0.0 11.2 33.6#

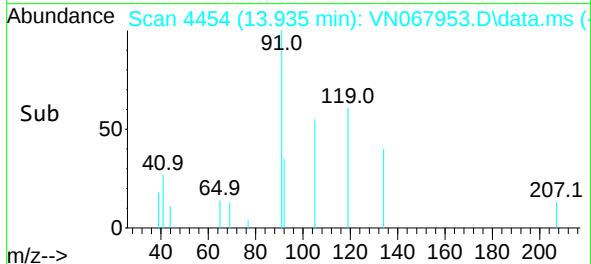

#90
Hexachloroethane
Concen: 1.783 ug/l
RT: 14.217 min Scan# 4559
Delta R.T. 0.003 min
Lab File: VN067953.D
Acq: 28 Jul 2021 15:13

Tgt Ion: 117 Resp: 3697
Ion Ratio Lower Upper
117 100
201 0.0 33.5 100.5#


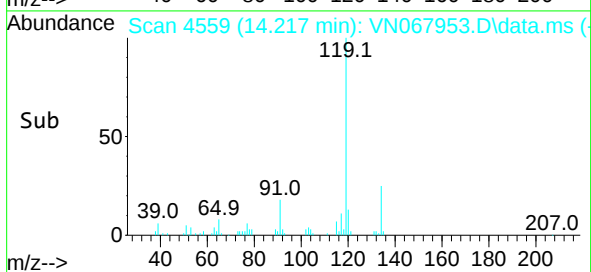






#93
1,2,4-Trichlorobenzene
Concen: 3.079 ug/l
RT: 15.260 min Scan# 4948
Delta R.T. -0.005 min
Lab File: VN067953.D
Acq: 28 Jul 2021 15:13




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:180 Resp: 1427
Ion Ratio Lower Upper
180 100
182 78.1 47.5 142.5
145 172.5 17.2 51.6#

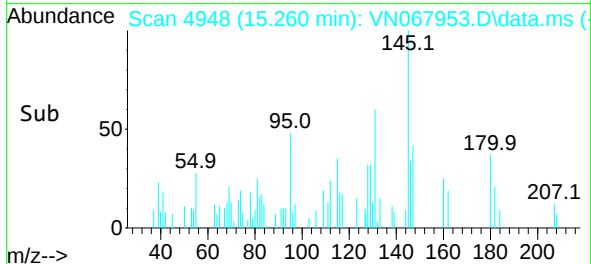

#95
Naphthalene
Concen: 3.844 ug/l
RT: 15.507 min Scan# 5040
Delta R.T. -0.002 min
Lab File: VN067953.D
Acq: 28 Jul 2021 15:13


Tgt Ion:128 Resp: 8693
Ion Ratio Lower Upper
128 100
127 18.8 10.6 15.8#
129 12.5 8.6 12.8

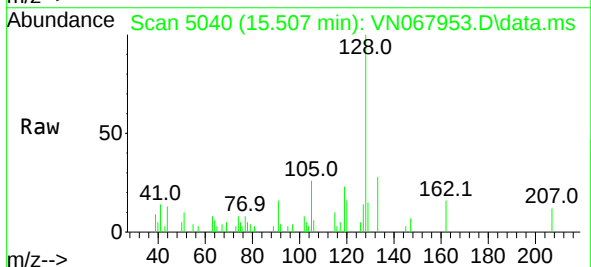



#96
 1,2,3-Trichlorobenzene
 Concen: 3.094 ug/l
 RT: 15.702 min Scan# 5113
 Delta R.T. 0.000 min
 Lab File: VN067953.D
 Acq: 28 Jul 2021 15:13

Instrument :
 MSVOA_N
 ClientSampled :



Tgt Ion:	180	Resp:	1559
Ion	Ratio	Lower	Upper
180	100		
182	38.8	47.8	143.3#
145	344.5	18.2	54.6#

