
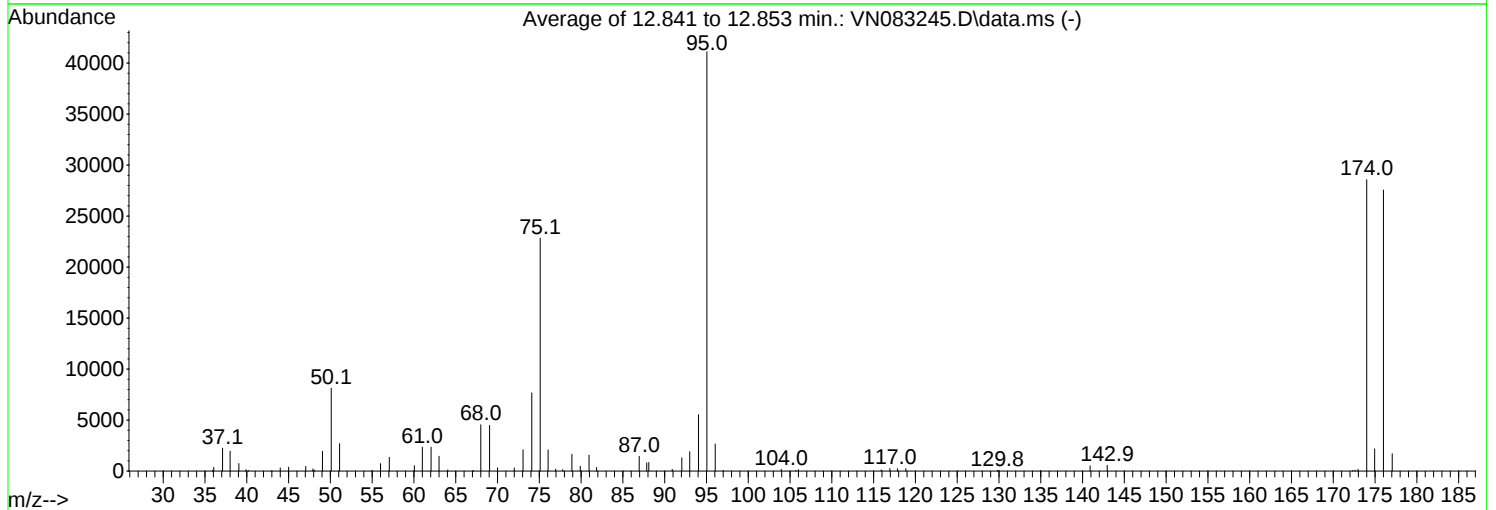


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN081324\
Data File : VN083245.D
Acq On : 13 Aug 2024 09:54
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N080724W.M
Title : SW846 8260
Last Update : Thu Aug 08 06:30:41 2024

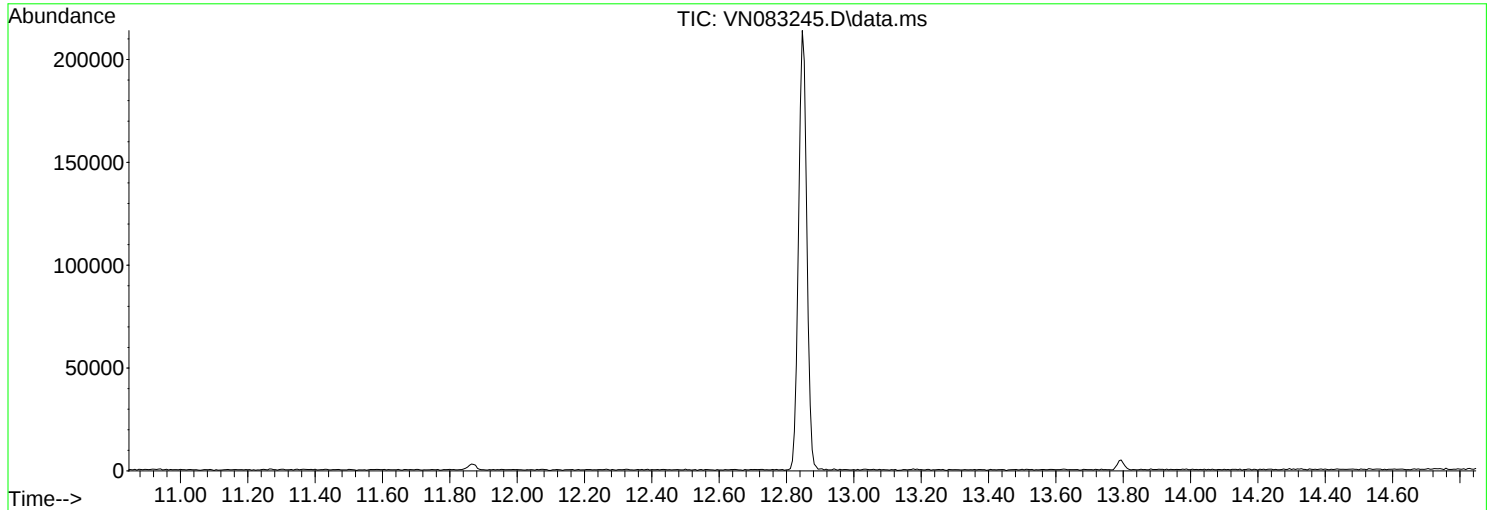

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	8125	PASS
75	95	30	60	55.6	22840	PASS
95	95	100	100	100.0	41112	PASS
96	95	5	9	6.5	2659	PASS
173	174	0.00	2	0.6	179	PASS
174	95	50	100	69.5	28568	PASS
175	174	5	9	7.6	2175	PASS
176	174	95	101	96.5	27557	PASS
177	176	5	9	6.1	1693	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	68	47.90	210	63.00	1458	76.95	195
36.05	358	48.10	98	64.05	118	77.80	144
37.10	2247	49.05	1950	67.10	64	78.90	1656
38.00	1949	50.10	8125	68.00	4540	79.90	479
39.05	734	51.10	2692	69.05	4480	80.95	1575
39.90	138	55.00	56	70.00	319	81.85	350
40.20	58	56.00	736	72.00	308	86.95	1446
43.00	53	57.05	1352	73.05	2093	87.85	807
44.00	320	60.05	528	74.10	7670	88.10	848
45.00	388	61.00	2341	75.10	22840	90.90	168
47.05	462	62.05	2343	76.05	2077	92.05	1299

Average of 12.841 to 12.853 min.: VN083245.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
93.00	1900	118.85	243	176.00	27557		
94.05	5531	129.80	78	177.05	1693		
95.05	41112	130.00	66				
96.05	2659	135.00	63				
97.00	60	140.90	521				
103.95	168	142.95	563				
105.70	64	172.30	51				
106.00	143	172.60	92				
115.90	113	172.95	179				
116.95	254	174.00	28568				
117.85	233	174.95	2175				

Instrument :

MSVOA_N

ClientSampleId :

BFB