
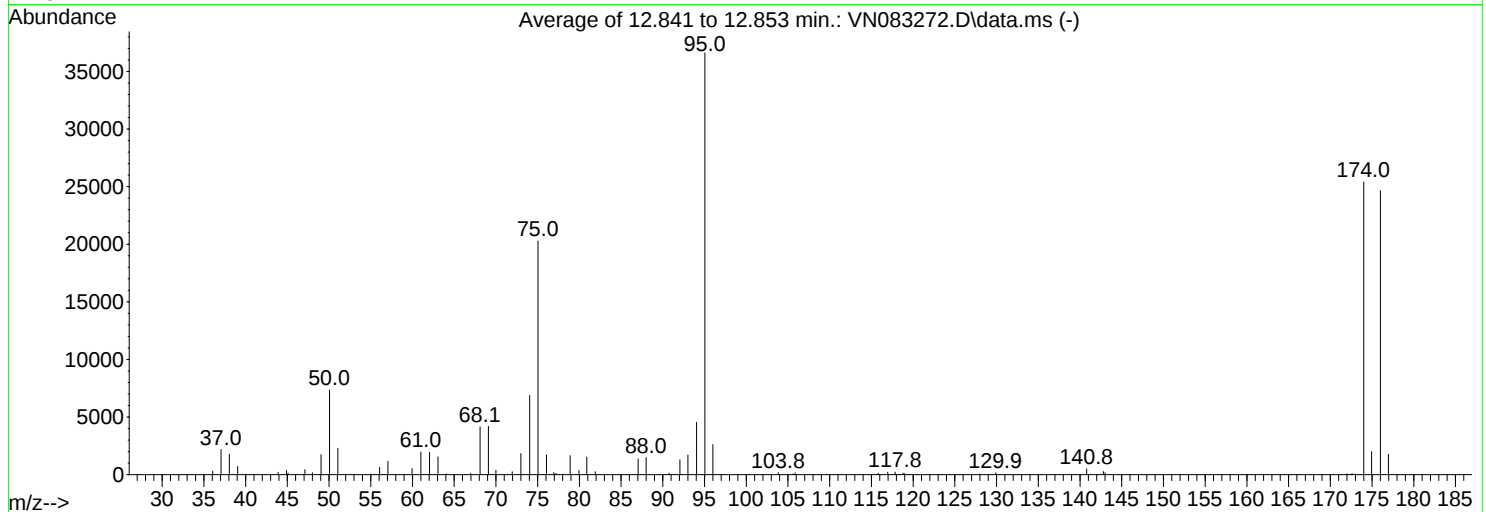


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN081324\
Data File : VN083272.D
Acq On : 14 Aug 2024 01:50
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N080724W.M
Title : SW846 8260
Last Update : Thu Aug 08 06:30:41 2024

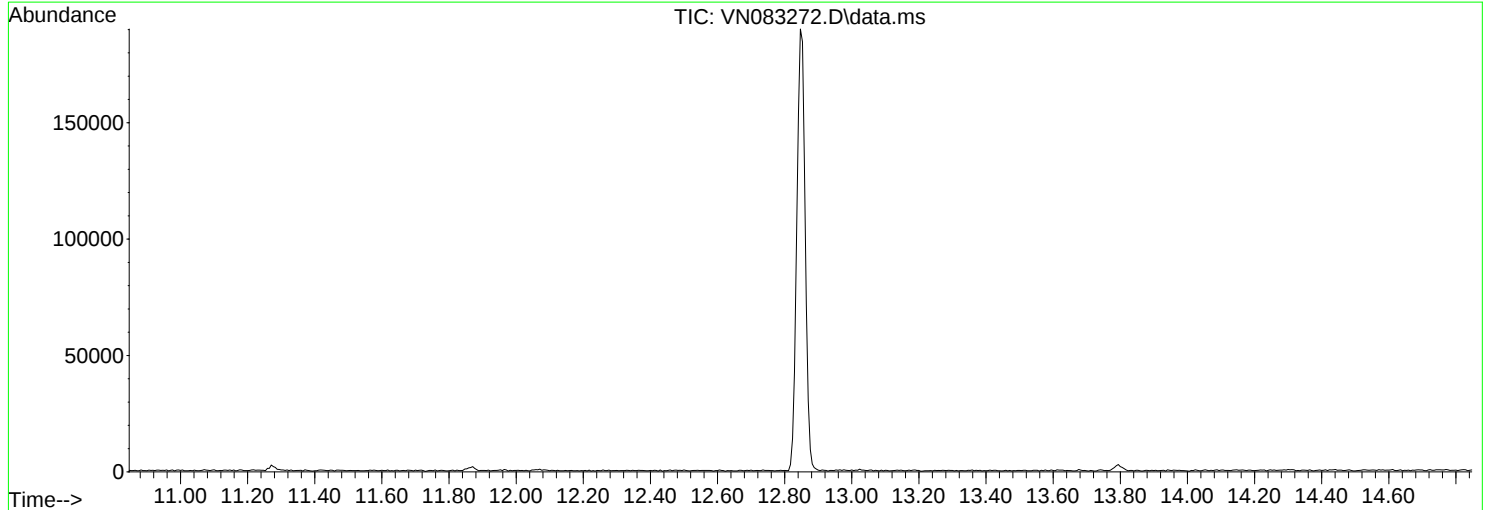

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.1	7351	PASS
75	95	30	60	55.4	20288	PASS
95	95	100	100	100.0	36619	PASS
96	95	5	9	7.1	2607	PASS
173	174	0.00	2	0.3	70	PASS
174	95	50	100	69.4	25411	PASS
175	174	5	9	7.8	1990	PASS
176	174	95	101	97.0	24656	PASS
177	176	5	9	7.2	1769	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	304	50.05	7351	66.95	131	78.00	61
37.05	2182	51.05	2285	68.10	4160	78.90	164
38.05	1778	52.00	55	69.10	4190	79.95	36
39.05	703	55.00	52	70.00	395	80.90	152
39.95	57	56.05	621	71.95	255	81.90	256
43.90	204	57.05	1149	73.00	1841	87.05	1364
44.90	366	59.95	529	74.05	6877	88.00	1485
45.10	136	61.00	1956	75.05	20288	90.75	131
47.10	433	62.05	1932	76.05	1709	92.05	1293
48.00	163	63.05	1545	76.95	184	93.00	1711
49.05	1737	64.10	68	77.20	111	94.05	4548

Average of 12.841 to 12.853 min.: VN083272.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
95.05	36619	129.90	167				
96.00	2607	140.80	498				
103.85	176	142.80	265				
105.60	50	143.00	172				
105.85	155	172.00	66				
115.80	128	172.60	99				
116.95	215	173.00	70				
117.85	220	174.00	25411				
118.80	134	174.95	1990				
119.00	102	176.00	24656				
127.90	73	176.95	1769				

Instrument :

MSVOA_N

ClientSampleId :

BFB