

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN081924\
 Data File : VN083368.D
 Acq On : 19 Aug 2024 12:21
 Operator : JC\MD
 Sample : VN0819MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0819MBL01

Quant Time: Aug 20 04:43:33 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N080724W.M
 Quant Title : SW846 8260
 QLast Update : Thu Aug 08 06:30:41 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.224	168	111668	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	220576	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	230647	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	103931	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.577	65	97792	61.525	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 123.040%	
35) Dibromofluoromethane	8.165	113	80454	58.436	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 116.880%	
50) Toluene-d8	10.565	98	290917	56.645	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 113.300%#	
62) 4-Bromofluorobenzene	12.847	95	117344	58.607	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	= 117.220%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN081924\
Data File : VN083368.D
Acq On : 19 Aug 2024 12:21
Operator : JC\MD
Sample : VN0819MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0819MBL01

Quant Time: Aug 20 04:43:33 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N080724W.M
Quant Title : SW846 8260
QLast Update : Thu Aug 08 06:30:41 2024
Response via : Initial Calibration




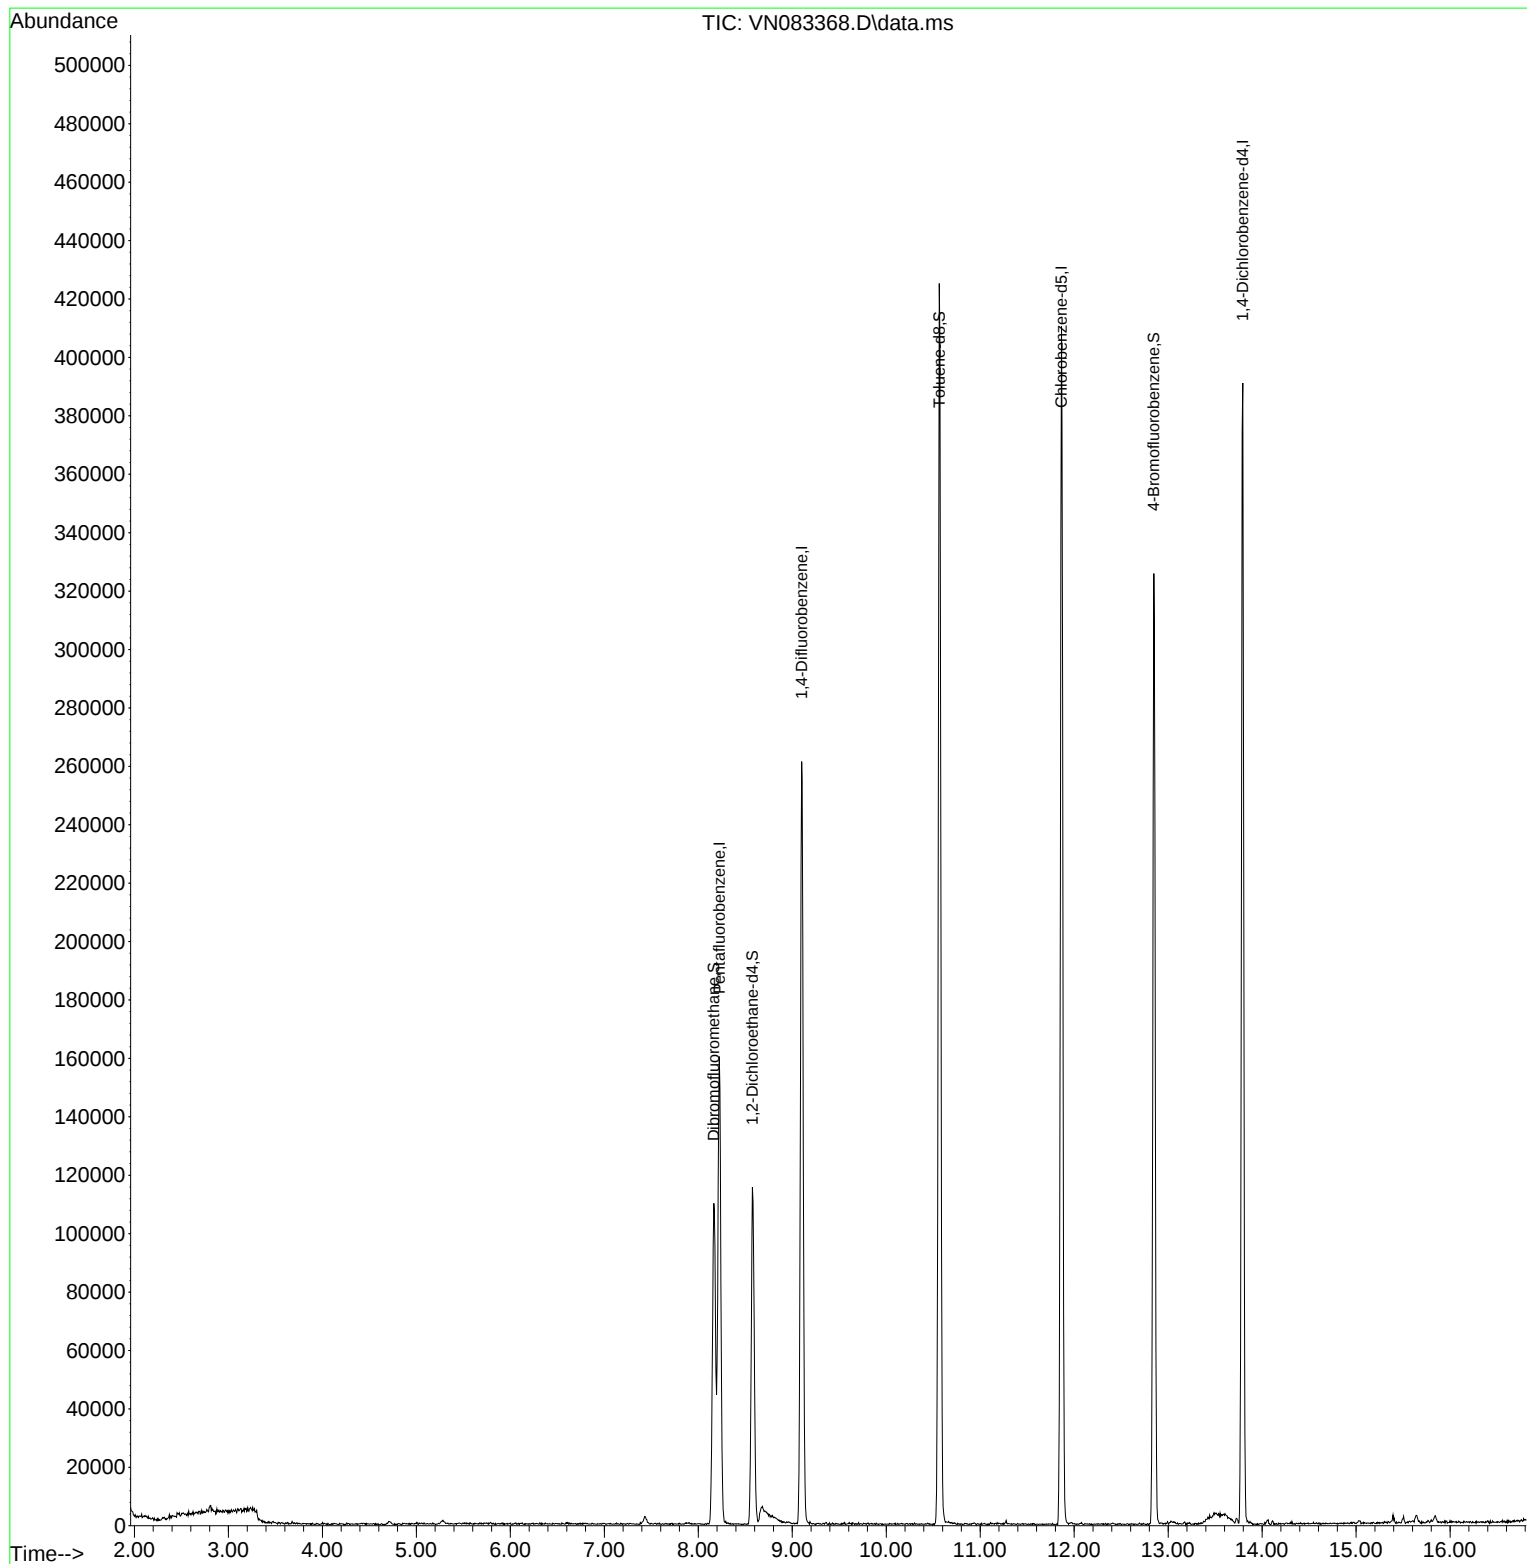


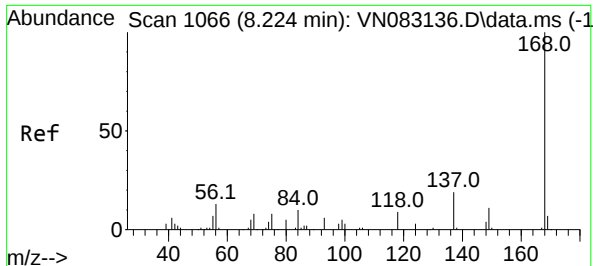

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 1106
Delta R.T. -0.000 min
Lab File: VN083368.D
Acq: 19 Aug 2024 12:21




Instrument :
MSVOA_N
ClientSampleId :
VN0819MBL01


Tgt Ion:168 Resp: 111668
Ion Ratio Lower Upper
168 100
99 65.7 48.2 72.4

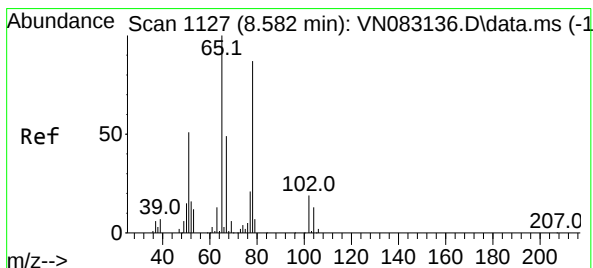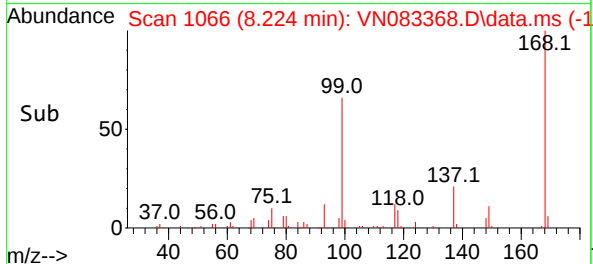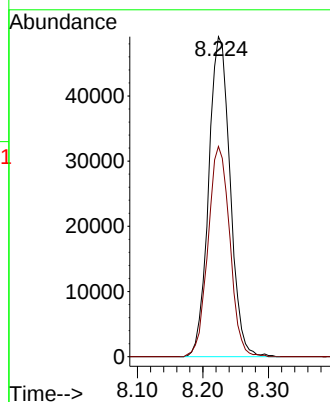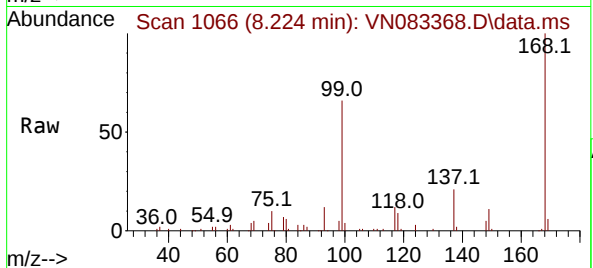

#33
1,2-Dichloroethane-d4
Concen: 61.525 ug/l
RT: 8.577 min Scan# 1126
Delta R.T. -0.005 min
Lab File: VN083368.D
Acq: 19 Aug 2024 12:21

Tgt Ion: 65 Resp: 97792
Ion Ratio Lower Upper
65 100
67 49.9 0.0 104.4

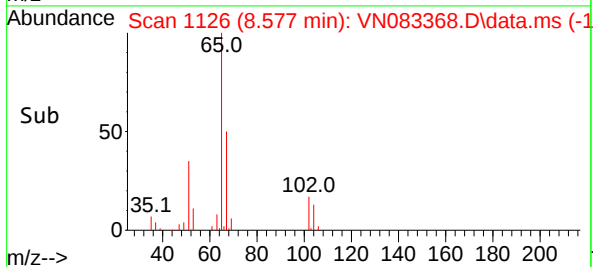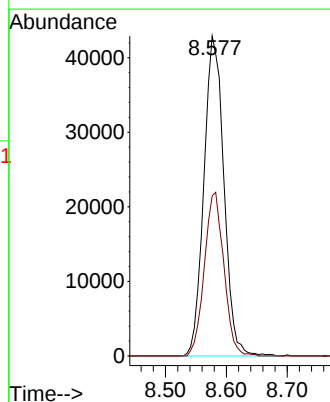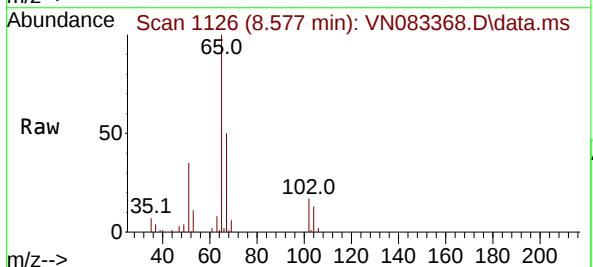

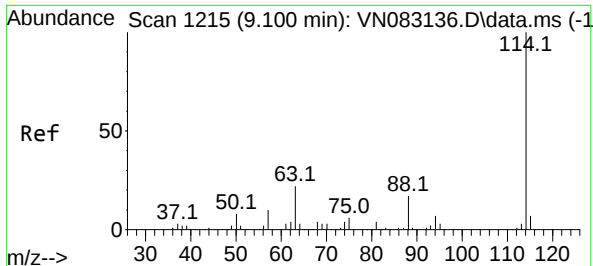

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.100 min Scan# 1

Delta R.T. -0.000 min

Lab File: VN083368.D

Acq: 19 Aug 2024 12:21

Instrument :

MSVOA_N

ClientSampleId :

VN0819MBL01





Tgt Ion:114 Resp: 220576

Ion Ratio Lower Upper

114 100

63 21.5 0.0 44.6

88 17.3 0.0 31.4

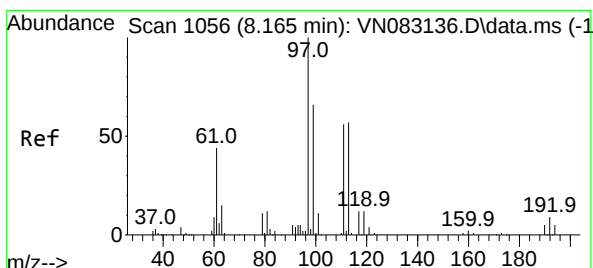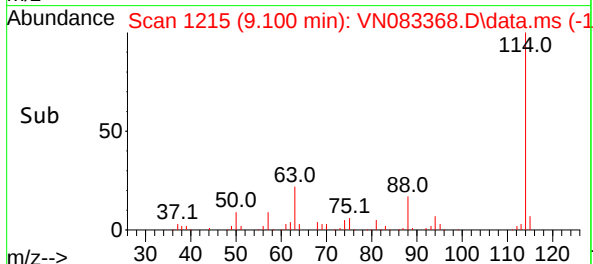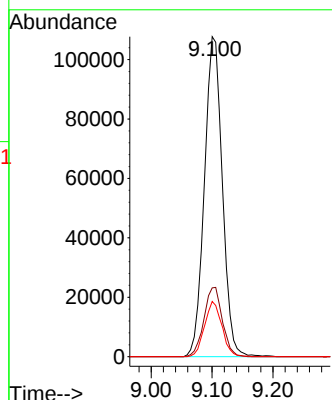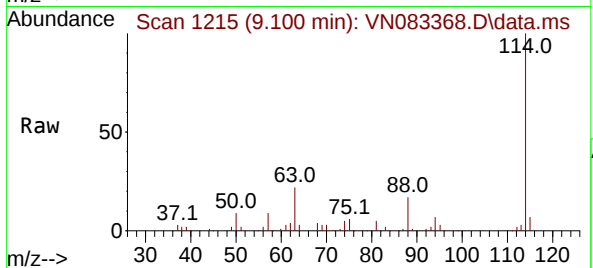

#35

Dibromofluoromethane

Concen: 58.436 ug/l

RT: 8.165 min Scan# 1056

Delta R.T. -0.000 min

Lab File: VN083368.D

Acq: 19 Aug 2024 12:21




Tgt Ion:113 Resp: 80454


Ion Ratio Lower Upper

113 100

111 101.4 82.4 123.6

192 17.5 14.9 22.3


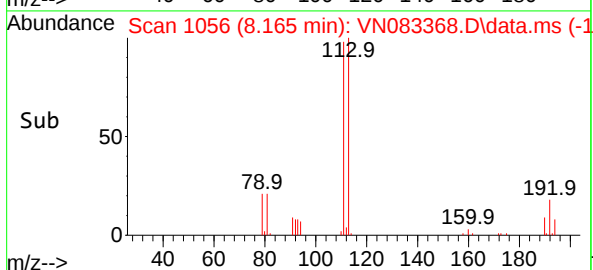
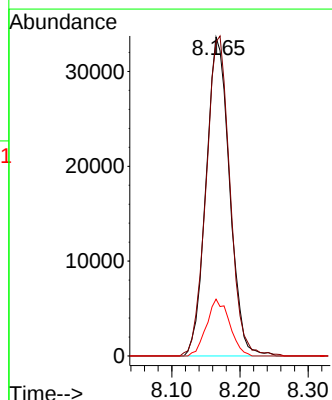
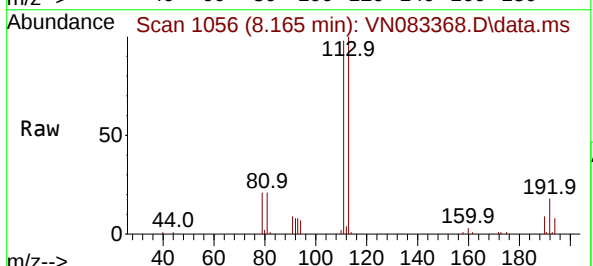


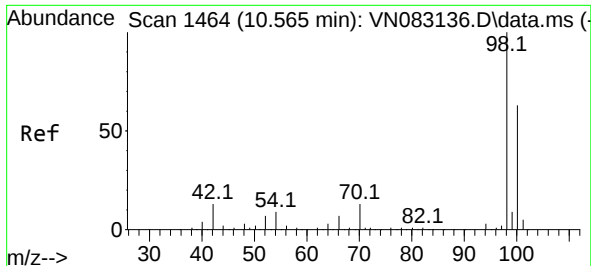

#50
Toluene-d8
Concen: 56.645 ug/l
RT: 10.565 min Scan# 1464
Delta R.T. -0.000 min
Lab File: VN083368.D
Acq: 19 Aug 2024 12:21




Instrument :
MSVOA_N
ClientSampleId :
VN0819MBL01


Tgt Ion: 98 Resp: 290917
Ion Ratio Lower Upper
98 100
100 64.6 51.5 77.3

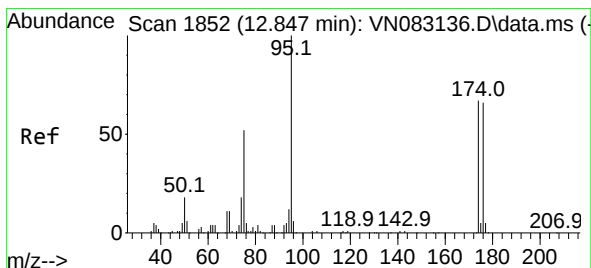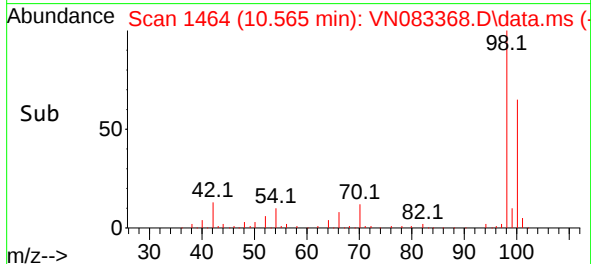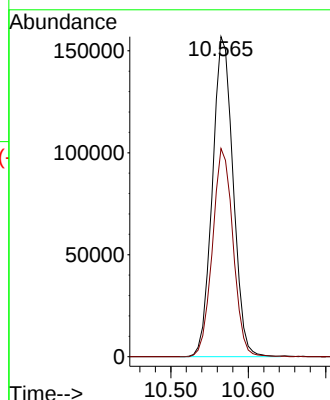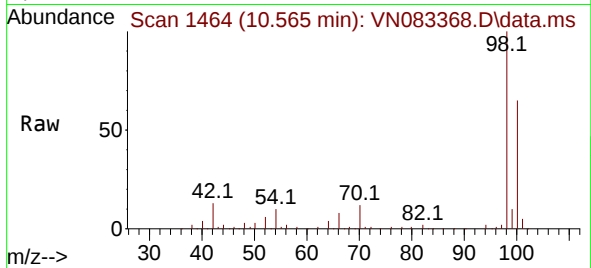

#62
4-Bromofluorobenzene
Concen: 58.607 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. -0.000 min
Lab File: VN083368.D
Acq: 19 Aug 2024 12:21

Tgt Ion: 95 Resp: 117344
Ion Ratio Lower Upper
95 100
174 70.5 0.0 159.2
176 67.9 0.0 147.6

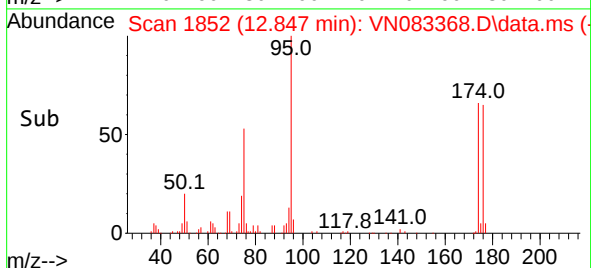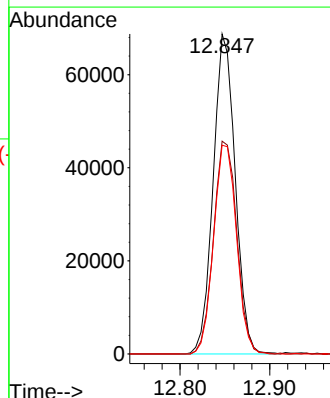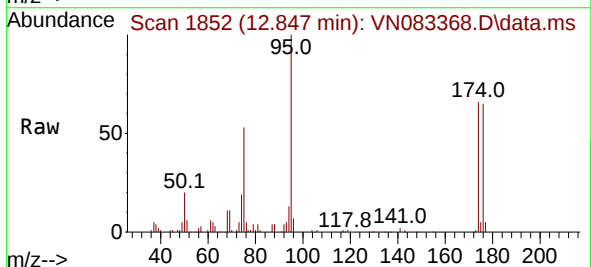

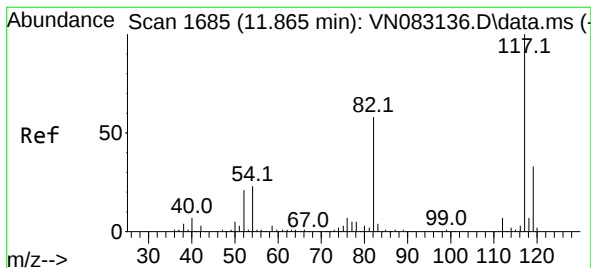

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.865 min Scan# 1

Delta R.T. -0.000 min

Lab File: VN083368.D

Acq: 19 Aug 2024 12:21

Instrument :

MSVOA_N

ClientSampleId :

VN0819MBL01





Tgt Ion:117 Resp: 230647

Ion Ratio Lower Upper

117 100

82 60.8 47.5 71.3

119 33.8 25.6 38.4

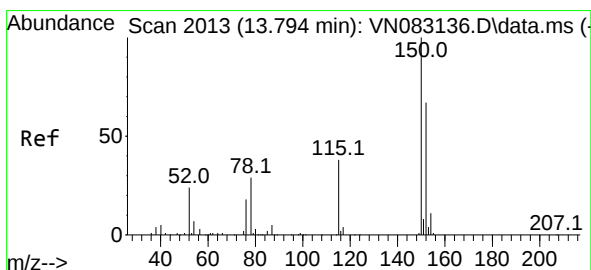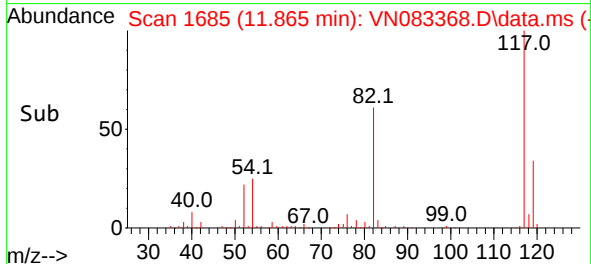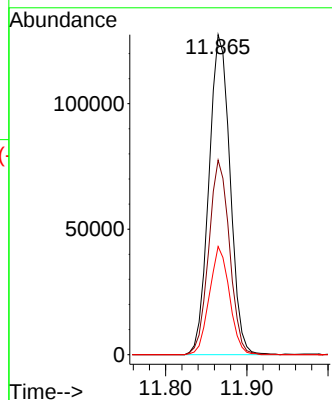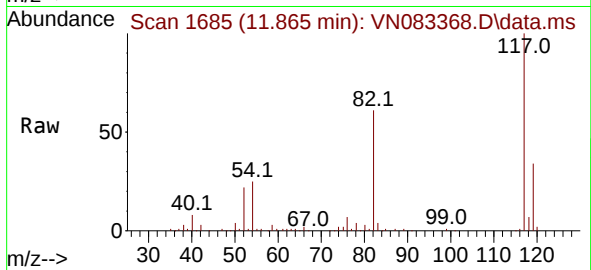

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.794 min Scan# 2013

Delta R.T. -0.000 min

Lab File: VN083368.D

Acq: 19 Aug 2024 12:21

Tgt Ion:152 Resp: 103931

Ion Ratio Lower Upper

152 100

115 63.4 30.6 91.6

150 155.5 0.0 348.6

