

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN081924\
 Data File : VN083369.D
 Acq On : 19 Aug 2024 13:37
 Operator : JC\MD
 Sample : VN0819WBL01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0819WBL01

Quant Time: Aug 20 04:43:59 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N080724W.M
 Quant Title : SW846 8260
 QLast Update : Thu Aug 08 06:30:41 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.224	168	144938	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	283183	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	290527	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	134032	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.583	65	105966	51.364	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 102.720%	
35) Dibromofluoromethane	8.171	113	85532	48.390	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 96.780%	
50) Toluene-d8	10.565	98	319405	48.443	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 96.880%	
62) 4-Bromofluorobenzene	12.847	95	132664	51.610	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	= 103.220%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN081924\
Data File : VN083369.D
Acq On : 19 Aug 2024 13:37
Operator : JC\MD
Sample : VN0819WBL01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0819WBL01

Quant Time: Aug 20 04:43:59 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N080724W.M
Quant Title : SW846 8260
QLast Update : Thu Aug 08 06:30:41 2024
Response via : Initial Calibration




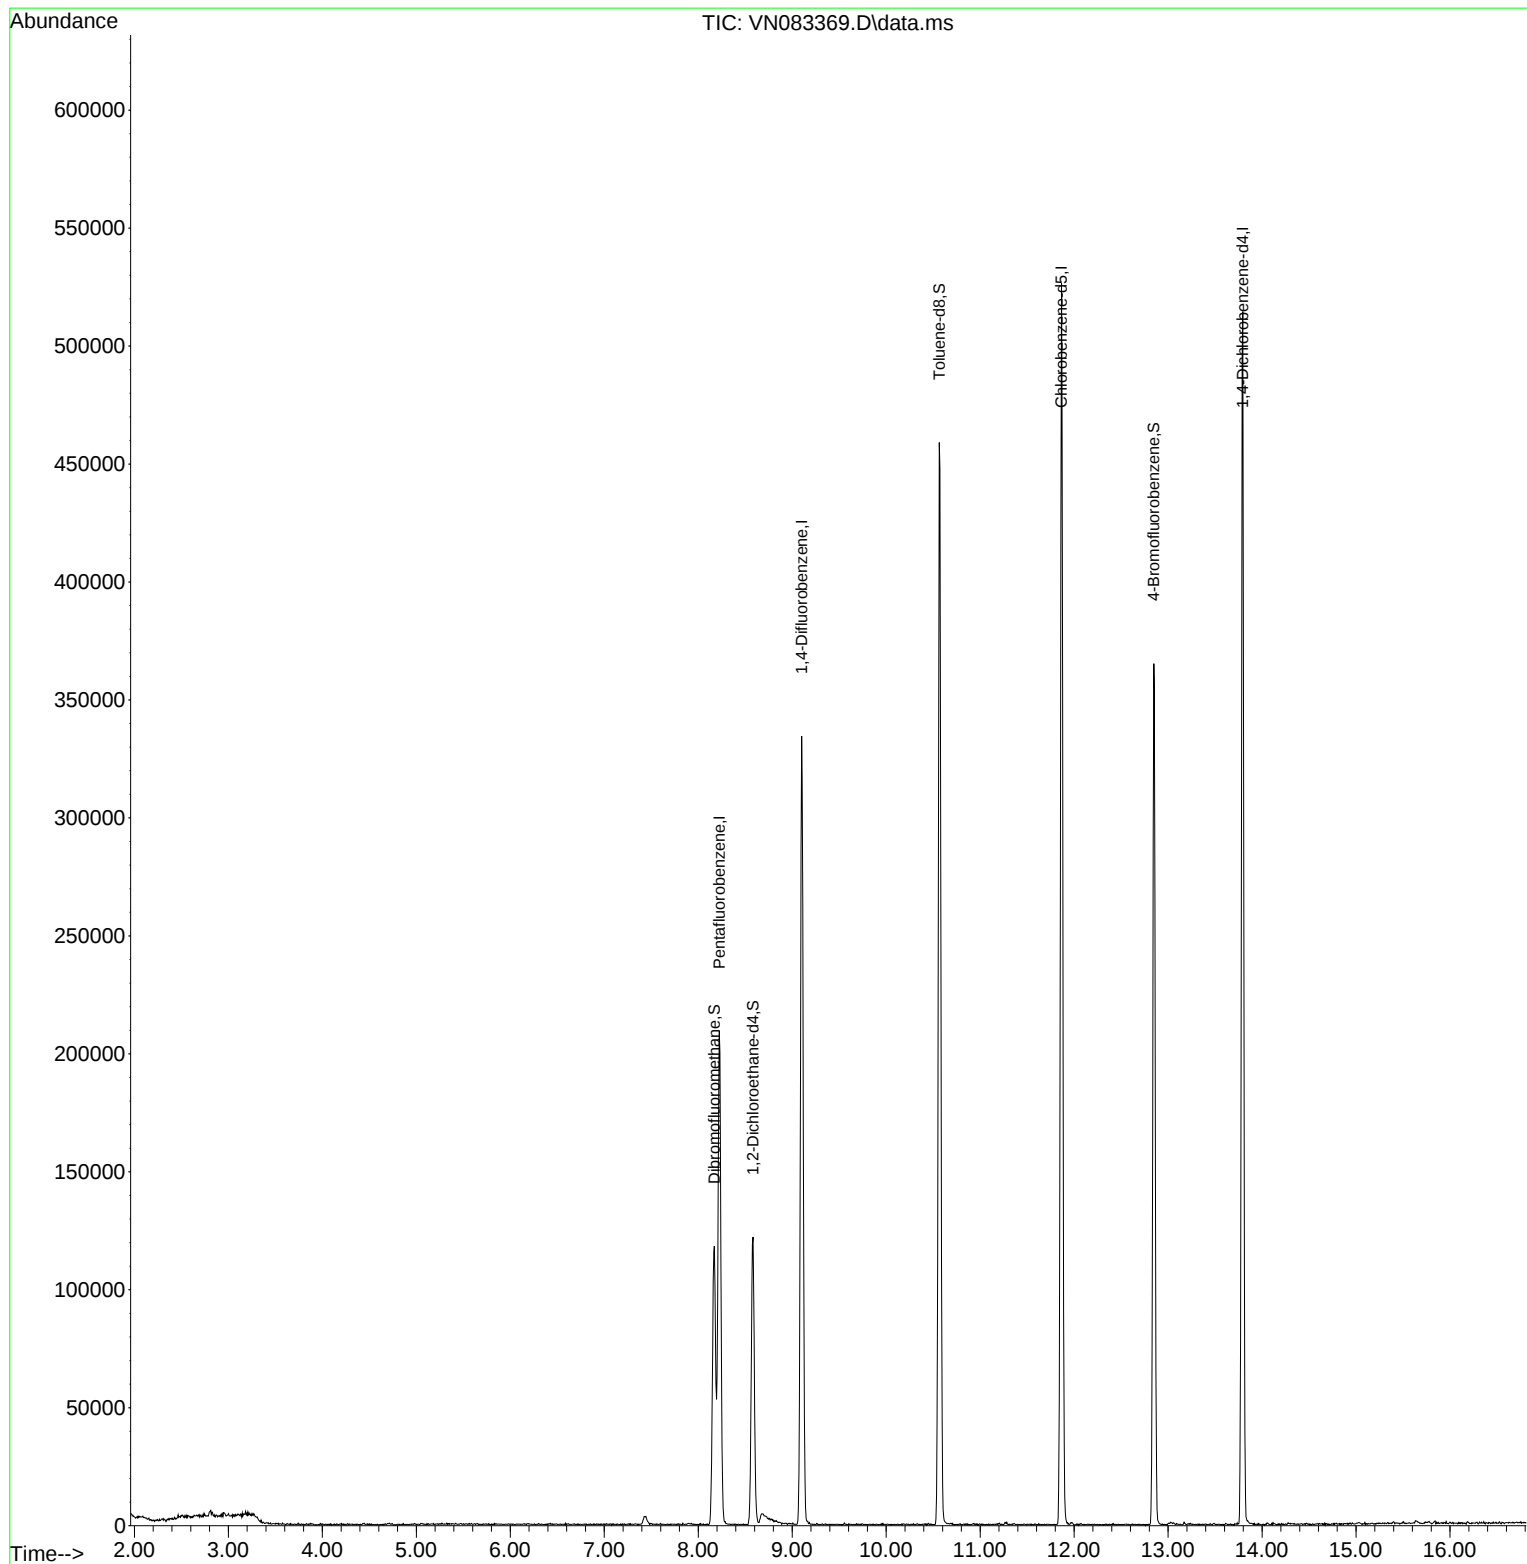


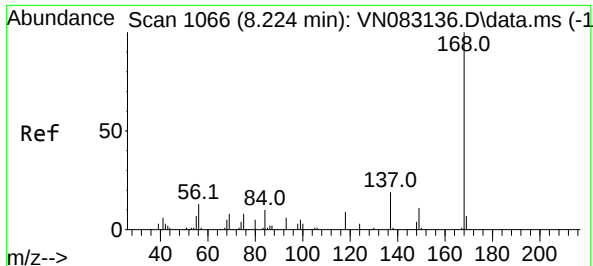

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. 0.000 min
Lab File: VN083369.D
Acq: 19 Aug 2024 13:37




Instrument :
MSVOA_N
ClientSampleId :
VN0819WBL01


Tgt Ion:168 Resp: 144938
Ion Ratio Lower Upper
168 100
99 68.6 48.2 72.4

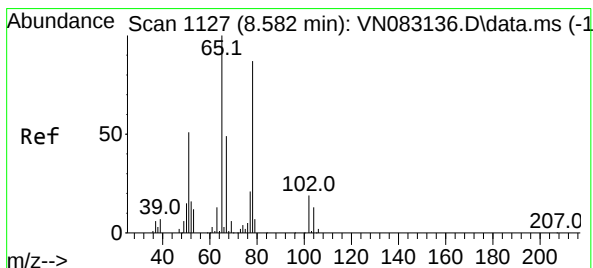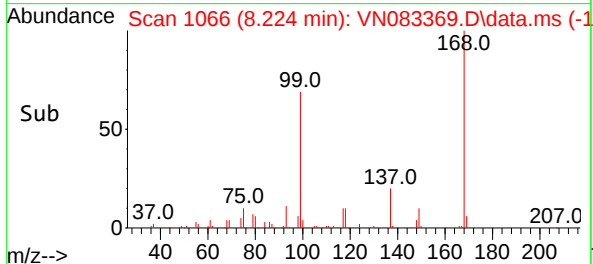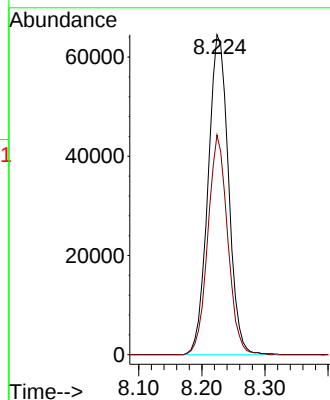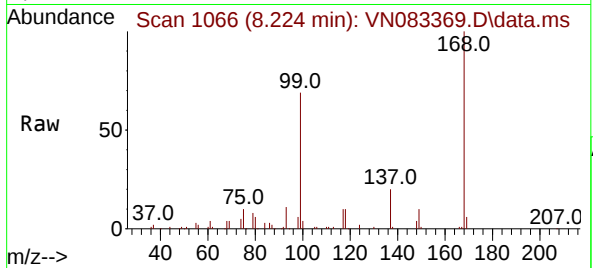

#33
1,2-Dichloroethane-d4
Concen: 51.364 ug/l
RT: 8.583 min Scan# 1127
Delta R.T. 0.001 min
Lab File: VN083369.D
Acq: 19 Aug 2024 13:37

Tgt Ion: 65 Resp: 105966
Ion Ratio Lower Upper
65 100
67 49.6 0.0 104.4

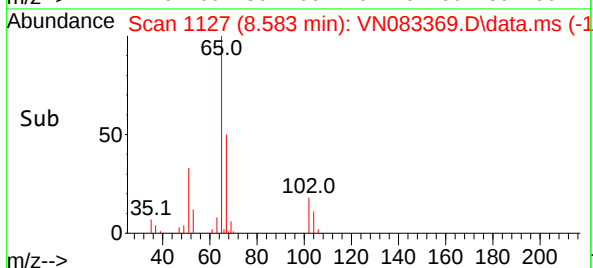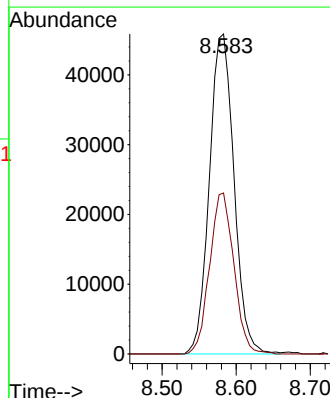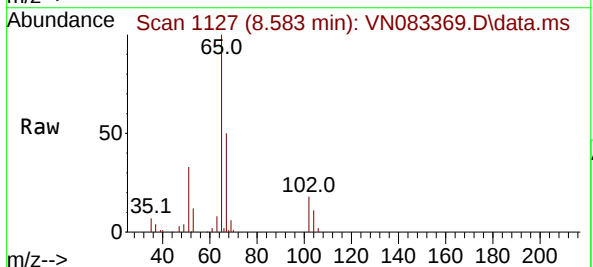

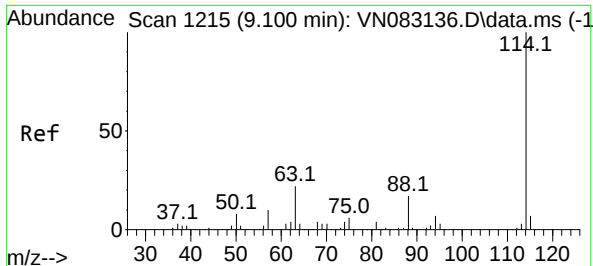

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.100 min Scan# 1

Delta R.T. 0.000 min

Lab File: VN083369.D

Acq: 19 Aug 2024 13:37

Instrument :

MSVOA_N

ClientSampleId :

VN0819WBL01





Tgt Ion:114 Resp: 283183

Ion Ratio Lower Upper

114 100

63 22.1 0.0 44.6

88 17.5 0.0 31.4

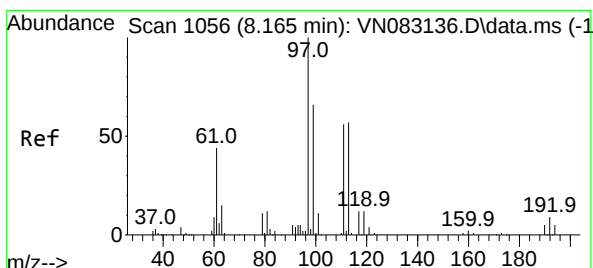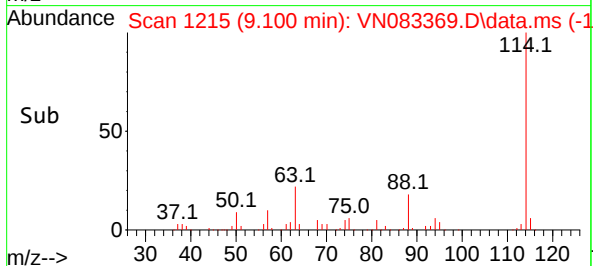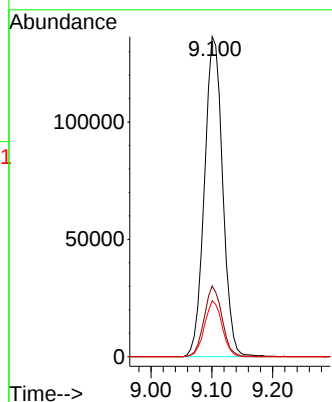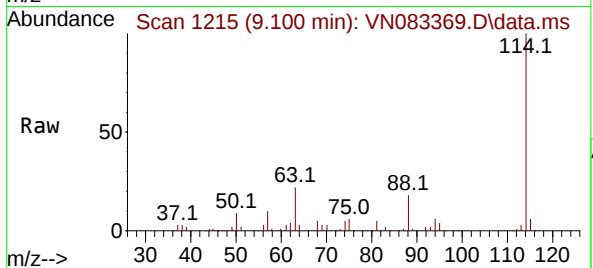

#35

Dibromofluoromethane

Concen: 48.390 ug/l

RT: 8.171 min Scan# 1057

Delta R.T. 0.006 min

Lab File: VN083369.D

Acq: 19 Aug 2024 13:37




Tgt Ion:113 Resp: 85532


Ion Ratio Lower Upper

113 100

111 103.4 82.4 123.6

192 16.9 14.9 22.3


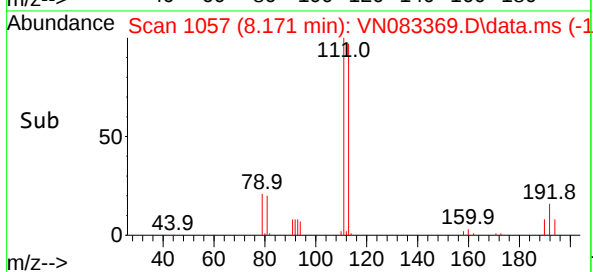
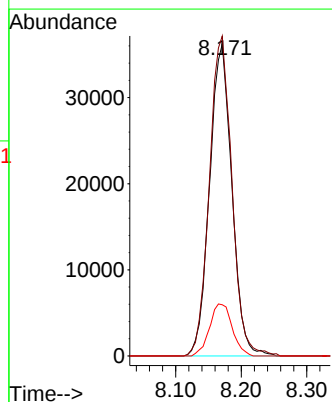
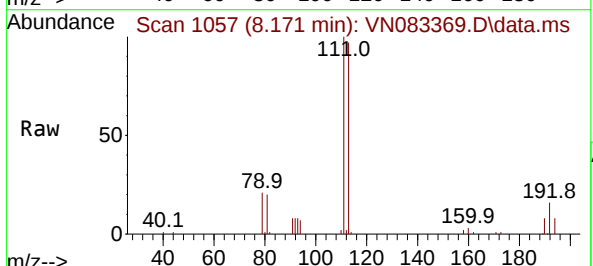


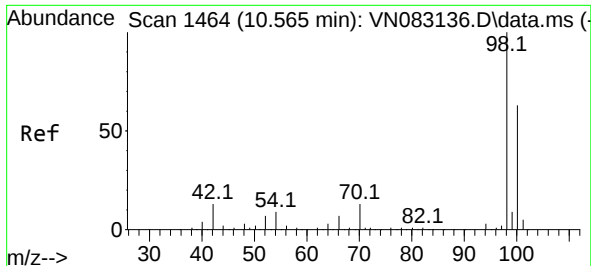

#50
Toluene-d8
Concen: 48.443 ug/l
RT: 10.565 min Scan# 1464
Delta R.T. 0.000 min
Lab File: VN083369.D
Acq: 19 Aug 2024 13:37




Instrument :
MSVOA_N
ClientSampleId :
VN0819WBL01


Tgt Ion: 98 Resp: 319405
Ion Ratio Lower Upper
98 100
100 64.1 51.5 77.3

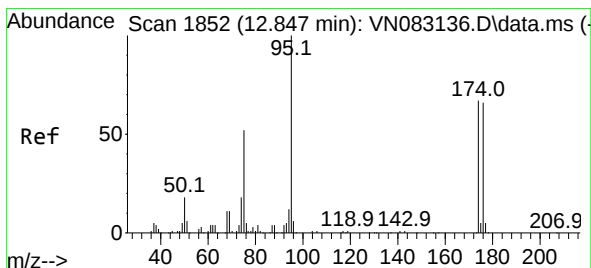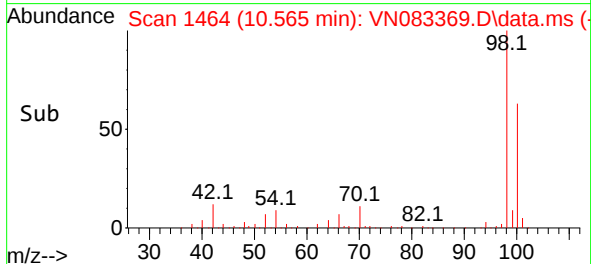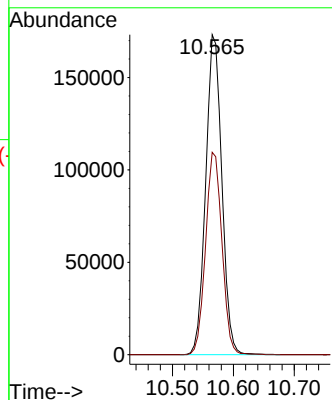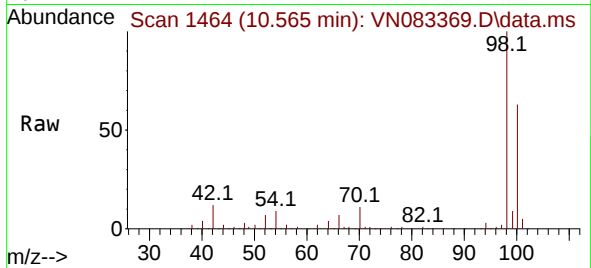

#62
4-Bromofluorobenzene
Concen: 51.610 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. 0.000 min
Lab File: VN083369.D
Acq: 19 Aug 2024 13:37

Tgt Ion: 95 Resp: 132664
Ion Ratio Lower Upper
95 100
174 70.4 0.0 159.2
176 67.5 0.0 147.6


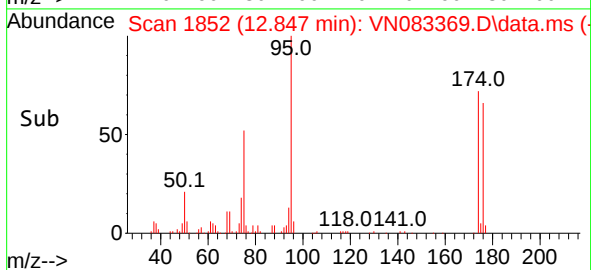
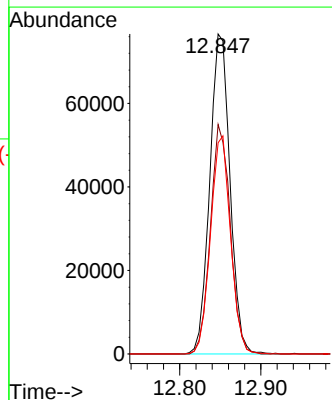
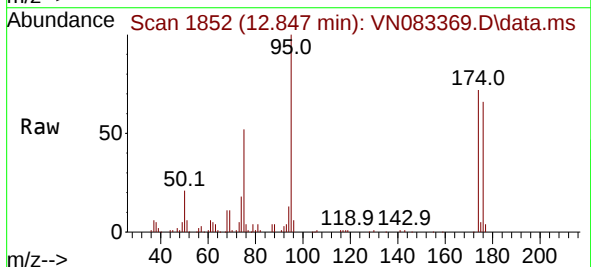


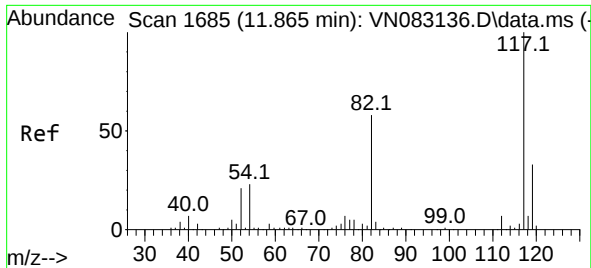

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 1
Delta R.T. 0.000 min
Lab File: VN083369.D
Acq: 19 Aug 2024 13:37

Instrument :
MSVOA_N
ClientSampleId :
VN0819WBL01

Tgt Ion:117 Resp: 290527
Ion Ratio Lower Upper
117 100
82 59.2 47.5 71.3
119 31.8 25.6 38.4

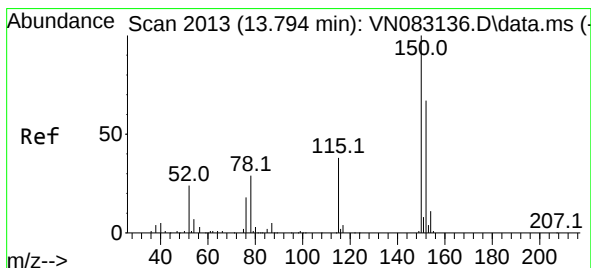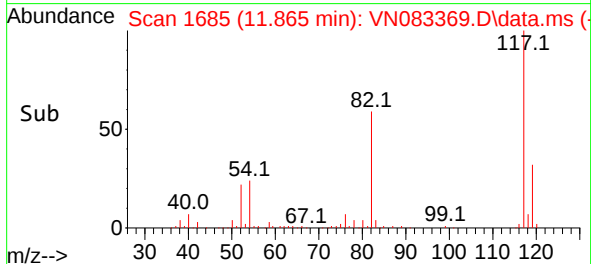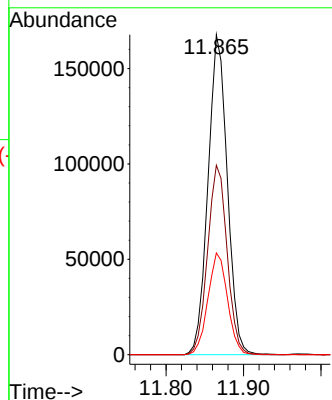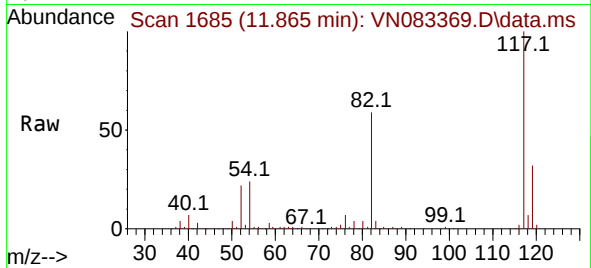

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 2013
Delta R.T. 0.000 min
Lab File: VN083369.D
Acq: 19 Aug 2024 13:37

Tgt Ion:152 Resp: 134032
Ion Ratio Lower Upper
152 100
115 63.6 30.6 91.6
150 159.0 0.0 348.6

