
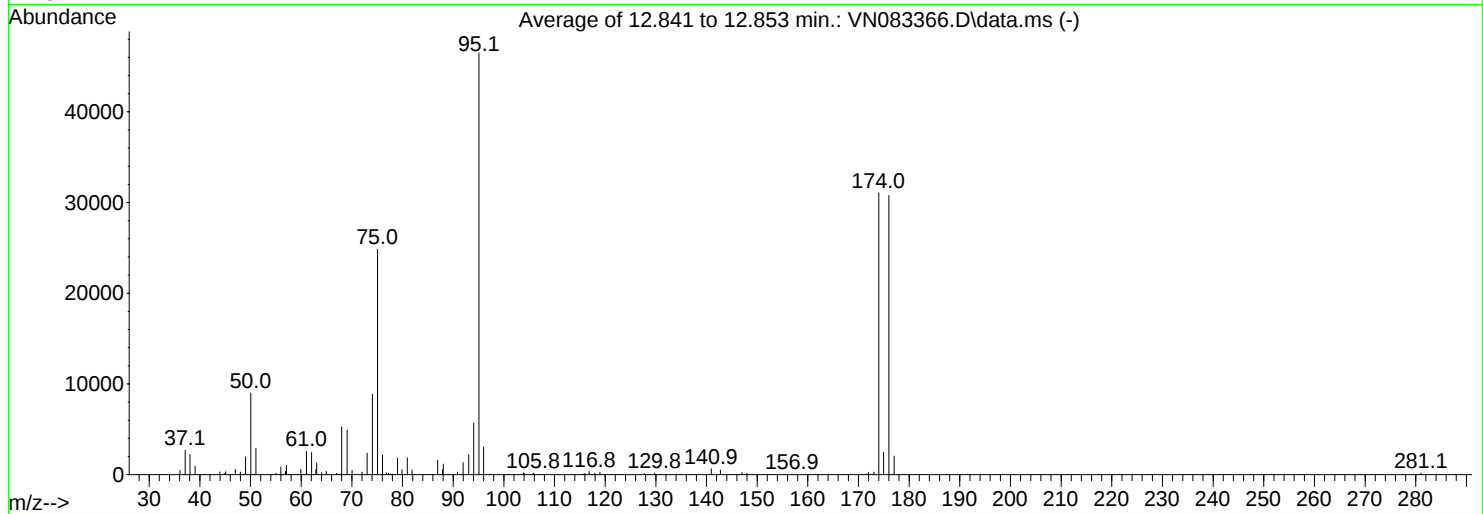


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN081924\
Data File : VN083366.D
Acq On : 19 Aug 2024 10:59
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N080724W.M
Title : SW846 8260
Last Update : Thu Aug 08 06:30:41 2024

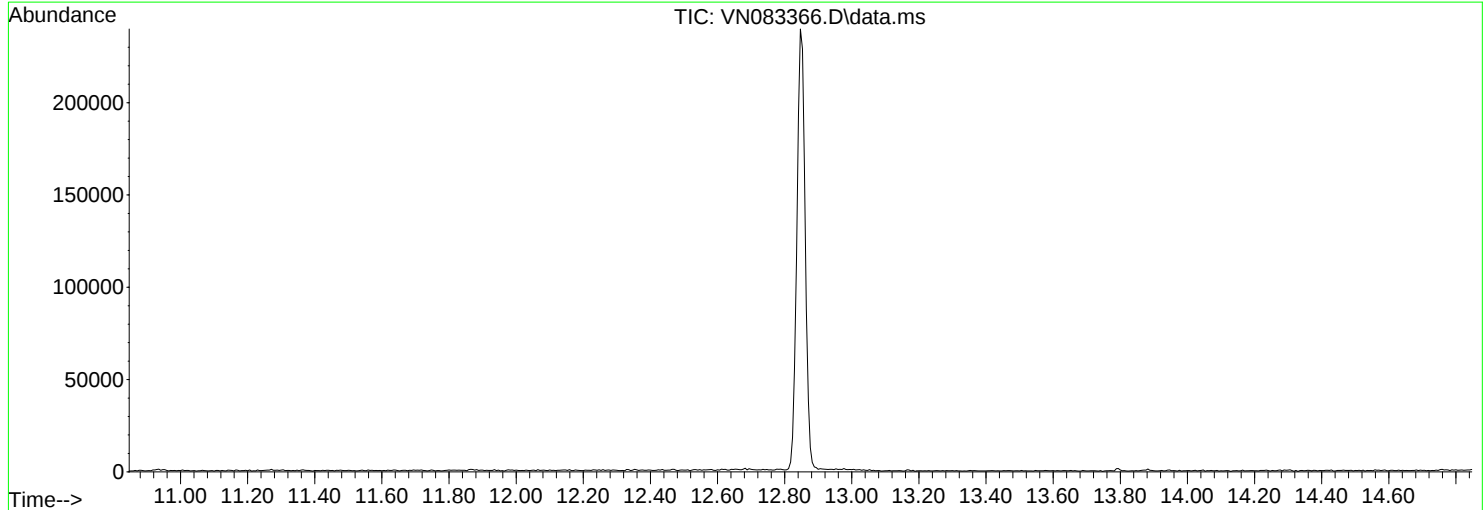

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.3	8998	PASS
75	95	30	60	53.4	24840	PASS
95	95	100	100	100.0	46504	PASS
96	95	5	9	6.5	3046	PASS
173	174	0.00	2	0.9	278	PASS
174	95	50	100	66.8	31069	PASS
175	174	5	9	8.0	2479	PASS
176	174	95	101	99.1	30787	PASS
177	176	5	9	6.7	2054	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	467	51.05	2889	64.05	254	76.80	211
37.10	2698	52.00	59	64.95	328	77.25	171
38.05	2226	55.00	162	67.00	142	77.70	7
39.05	939	56.00	831	68.00	5275	78.00	7
43.95	303	56.90	352	69.05	4917	79.00	1822
44.80	120	57.10	1016	70.05	484	79.90	543
45.10	324	59.95	578	72.00	283	80.95	1852
47.00	589	61.05	2573	73.00	2369	81.90	494
48.00	281	62.05	2433	74.05	8860	86.95	1573
49.00	1950	62.90	569	75.05	24840	87.90	554
50.05	8998	63.05	1293	76.05	2189	88.05	1166

Average of 12.841 to 12.853 min.: VN083366.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
90.85	274	115.70	53	156.90	60		
91.95	1350	116.00	116	171.60	72		
93.05	2204	116.85	336	172.00	245		
94.05	5680	117.95	158	173.05	278		
95.10	46504	118.95	272	174.00	31069		
96.00	3046	127.75	126	174.95	2479		
97.10	54	129.75	155	176.00	30787		
103.85	211	140.95	646	177.05	2054		
104.10	99	142.75	521	281.05	182		
105.70	59	147.00	225				
105.85	152	148.00	170				

Instrument :

MSVOA_N

ClientSampleId :

BFB