
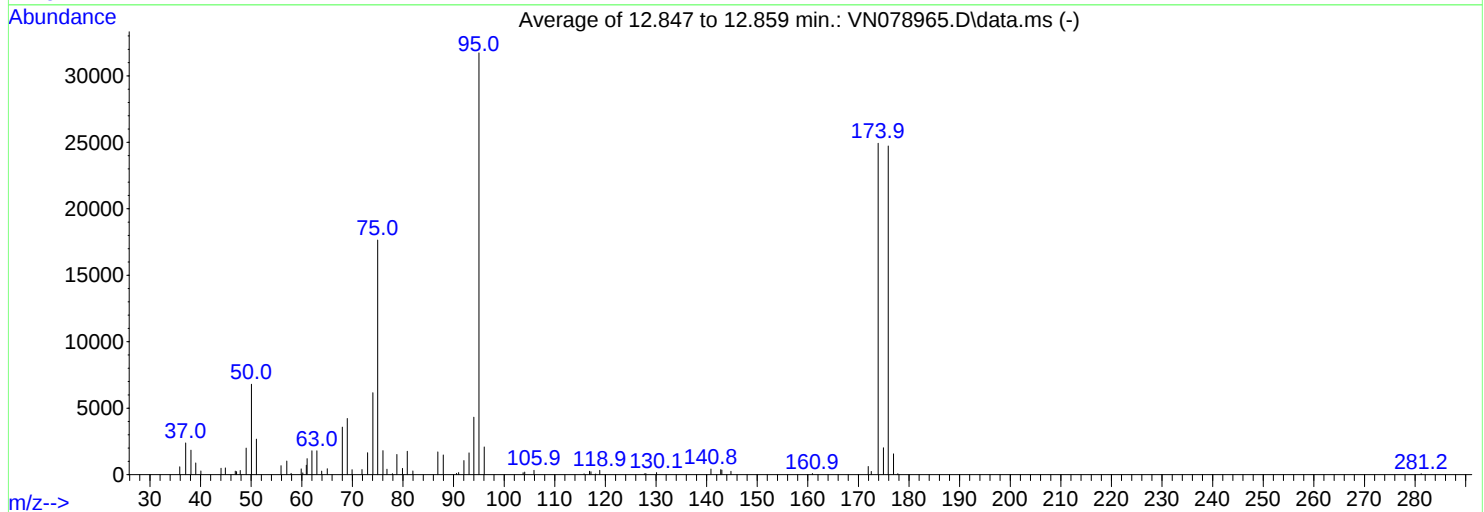


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN082123\  
Data File : VN078965.D  
Acq On : 21 Aug 2023 09:16  
Operator : JC\MD  
Sample : BFB  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N081523W.M  
Title : SW846 8260  
Last Update : Wed Aug 16 02:42:02 2023

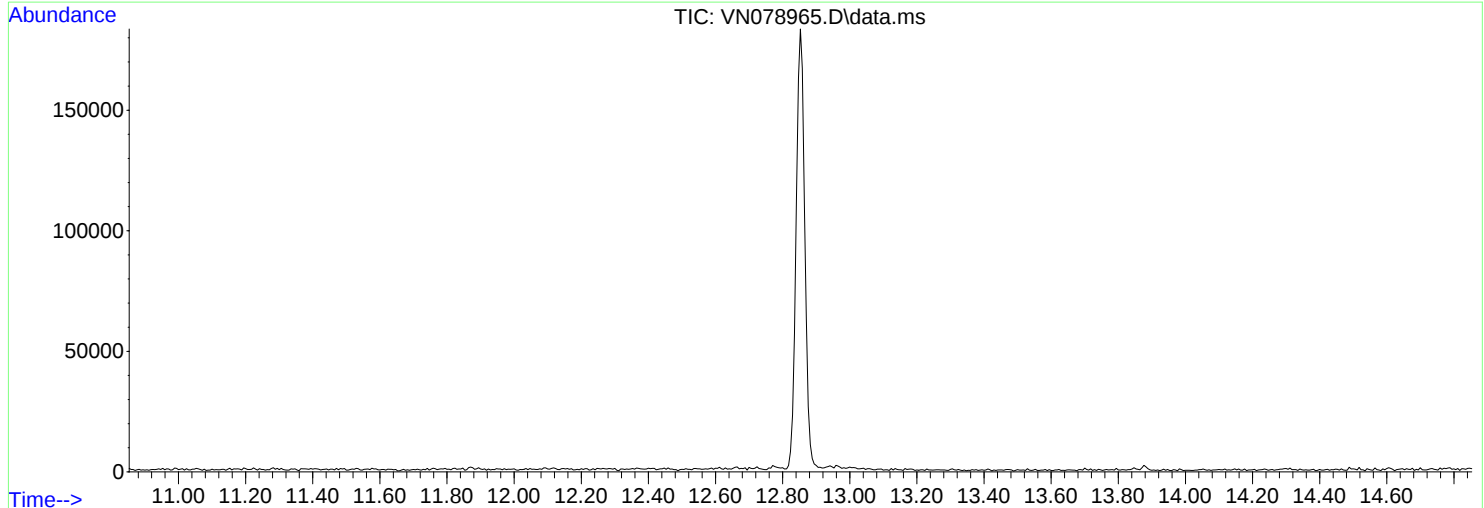

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 21.4         | 6802       | PASS                |
| 75             | 95              | 30              | 60              | 55.6         | 17643      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 31731      | PASS                |
| 96             | 95              | 5               | 9               | 6.6          | 2080       | PASS                |
| 173            | 174             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 174            | 95              | 50              | 100             | 78.6         | 24928      | PASS                |
| 175            | 174             | 5               | 9               | 8.1          | 2027       | PASS                |
| 176            | 174             | 95              | 101             | 99.2         | 24731      | PASS                |
| 177            | 176             | 5               | 9               | 6.3          | 1565       | PASS                |

BFB

Modified:subtracted

| m/z   | abund. | m/z   | abund. | m/z   | abund. | m/z   | abund. |
|-------|--------|-------|--------|-------|--------|-------|--------|
| 35.90 | 593    | 50.05 | 6802   | 63.95 | 263    | 77.90 | 61     |
| 37.05 | 2383   | 51.05 | 2671   | 65.05 | 446    | 78.80 | 151    |
| 38.10 | 1844   | 55.90 | 675    | 68.00 | 3575   | 79.90 | 47     |
| 39.05 | 880    | 57.05 | 1020   | 69.00 | 4227   | 80.85 | 175    |
| 40.05 | 272    | 57.90 | 93     | 69.95 | 370    | 81.95 | 280    |
| 44.05 | 479    | 59.90 | 438    | 71.90 | 385    | 86.90 | 1715   |
| 44.90 | 511    | 60.20 | 139    | 73.00 | 1648   | 87.95 | 1477   |
| 46.85 | 261    | 60.90 | 716    | 74.05 | 6165   | 90.60 | 96     |
| 47.10 | 225    | 61.05 | 1207   | 75.00 | 17643  | 91.00 | 157    |
| 47.85 | 316    | 62.00 | 1797   | 76.05 | 1807   | 92.05 | 1061   |
| 49.00 | 2002   | 63.00 | 1799   | 76.85 | 410    | 93.05 | 1642   |

Average of 12.847 to 12.859 min.: VN078965.D\data.ms

BFB

Modified:subtracted

| m/z    | abund. | m/z    | abund. | m/z    | abund. | m/z | abund. |
|--------|--------|--------|--------|--------|--------|-----|--------|
| 94.00  | 4322   | 127.70 | 63     | 174.95 | 2027   |     |        |
| 95.00  | 31731  | 128.00 | 90     | 175.90 | 24731  |     |        |
| 96.05  | 2080   | 130.10 | 157    | 176.95 | 1565   |     |        |
| 103.75 | 146    | 140.85 | 421    | 177.80 | 69     |     |        |
| 104.05 | 195    | 142.80 | 370    | 281.20 | 71     |     |        |
| 105.90 | 327    | 143.00 | 346    |        |        |     |        |
| 115.80 | 58     | 144.80 | 254    |        |        |     |        |
| 116.85 | 257    | 160.90 | 85     |        |        |     |        |
| 117.15 | 217    | 171.95 | 621    |        |        |     |        |
| 118.10 | 52     | 172.55 | 245    |        |        |     |        |
| 118.90 | 324    | 173.90 | 24928  |        |        |     |        |

Instrument :  
MSVOA\_N  
ClientSampleId :  
BFB