
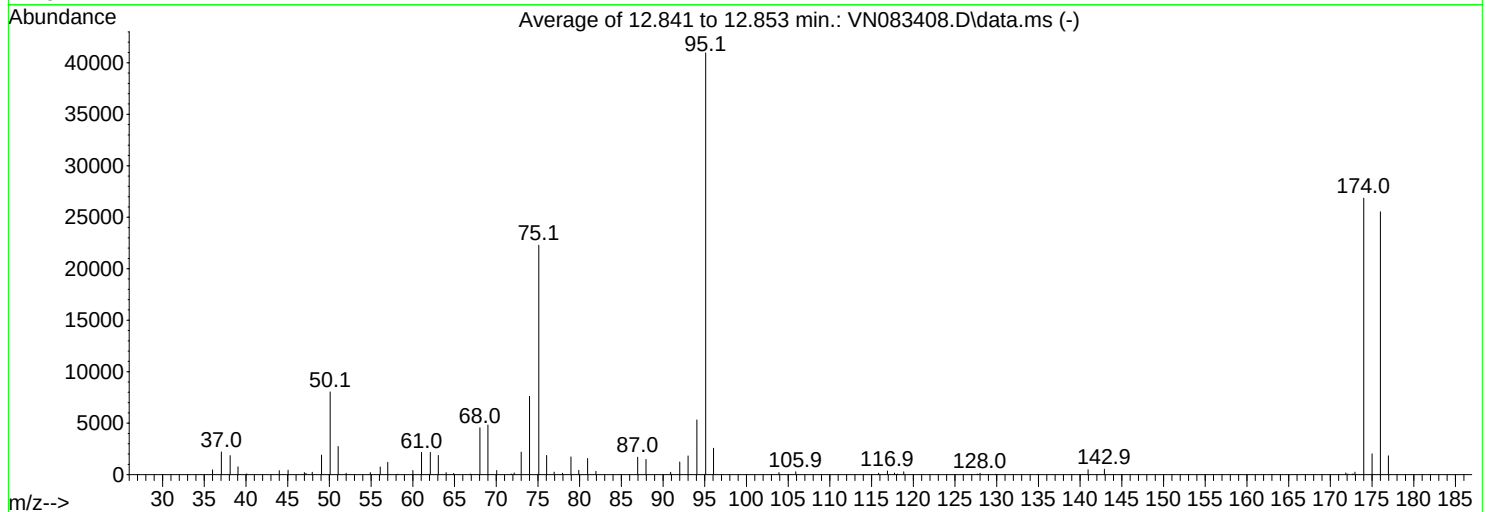


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN082124\
Data File : VN083408.D
Acq On : 21 Aug 2024 10:38
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N080724W.M
Title : SW846 8260
Last Update : Thu Aug 08 06:30:41 2024

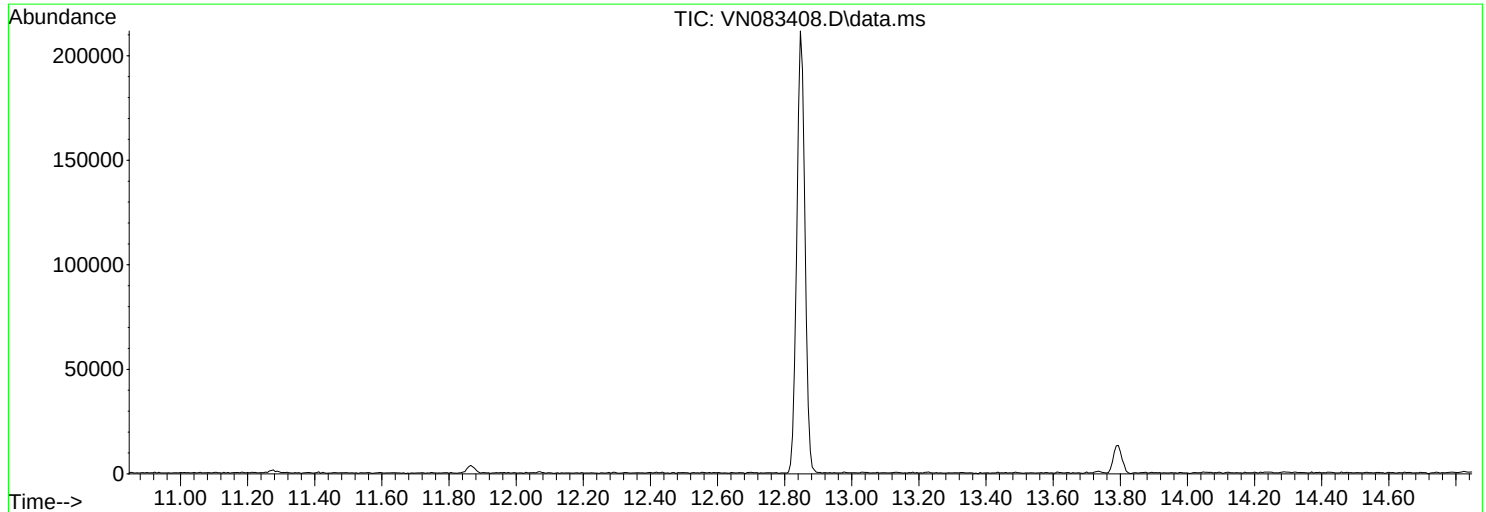

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	8030	PASS
75	95	30	60	54.4	22293	PASS
95	95	100	100	100.0	40968	PASS
96	95	5	9	6.3	2561	PASS
173	174	0.00	2	0.9	255	PASS
174	95	50	100	65.6	26861	PASS
175	174	5	9	7.5	2027	PASS
176	174	95	101	95.1	25541	PASS
177	176	5	9	7.2	1834	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	473	50.10	8030	64.00	206	76.05	1861
37.05	2203	51.05	2739	64.90	119	76.95	241
38.10	1857	52.00	139	66.90	59	77.95	131
39.05	757	54.90	210	68.05	4560	78.95	1731
40.10	81	56.10	740	69.00	4821	79.90	417
44.00	386	57.00	1203	70.05	400	80.95	1574
45.05	434	58.20	51	71.80	64	81.95	329
47.00	201	60.00	406	72.15	166	86.95	1703
47.20	123	61.05	2161	73.00	2192	87.95	1485
47.95	226	62.10	2160	74.00	7609	90.90	228
49.05	1894	63.05	1873	75.10	22293	92.00	1233

Average of 12.841 to 12.853 min.: VN083408.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
93.00	1813	127.70	59	176.00	25541		
94.05	5311	128.00	134	176.95	1834		
95.10	40968	129.90	53				
96.05	2561	140.95	479				
103.90	205	142.90	536				
105.90	274	171.85	166				
115.85	141	172.10	70				
116.90	364	172.70	76				
117.75	153	172.95	255				
118.10	62	174.00	26861				
118.85	282	175.00	2027				

Instrument :

MSVOA_N

ClientSampleId :

BFB