

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN082224\
 Data File : VN083426.D
 Acq On : 22 Aug 2024 10:53
 Operator : JC\MD
 Sample : VN0822WBL01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0822WBL01

Quant Time: Aug 23 01:38:42 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N080724W.M
 Quant Title : SW846 8260
 QLast Update : Thu Aug 08 06:30:41 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.224	168	142322	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	288957	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	306835	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	145694	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.577	65	109671	54.137	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	108.280%
35) Dibromofluoromethane	8.165	113	88398	49.012	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	98.020%
50) Toluene-d8	10.565	98	317440	47.183	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	94.360%
62) 4-Bromofluorobenzene	12.847	95	144169	54.965	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	109.940%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN082224\
Data File : VN083426.D
Acq On : 22 Aug 2024 10:53
Operator : JC\MD
Sample : VN0822WBL01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0822WBL01

Quant Time: Aug 23 01:38:42 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N080724W.M
Quant Title : SW846 8260
QLast Update : Thu Aug 08 06:30:41 2024
Response via : Initial Calibration




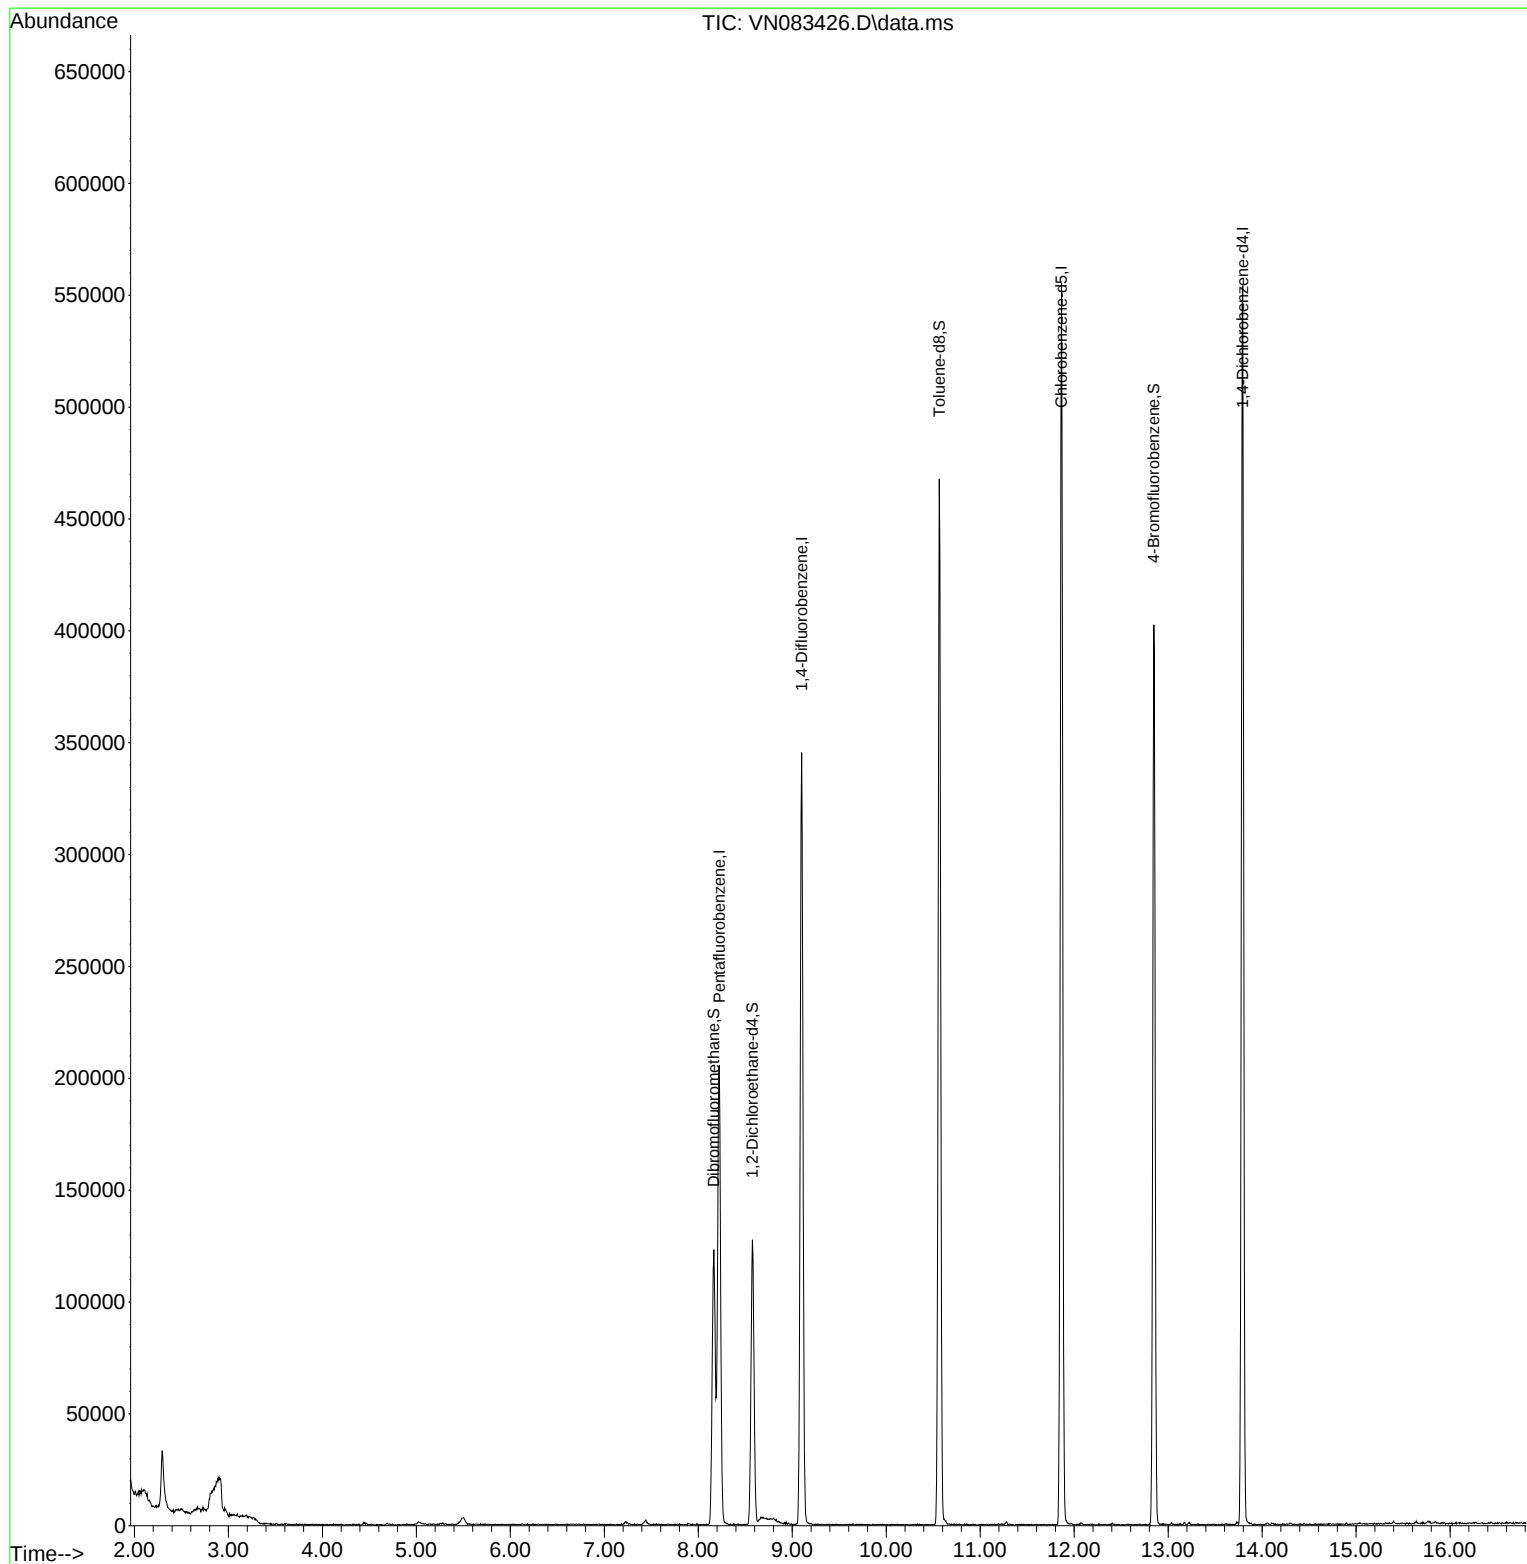


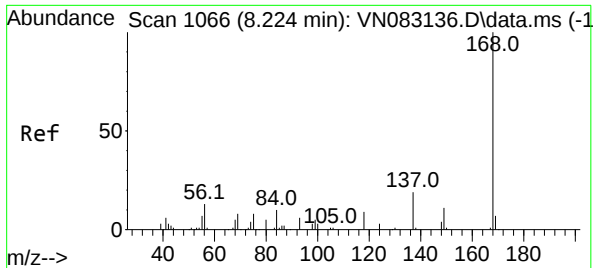

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.000 min
Lab File: VN083426.D
Acq: 22 Aug 2024 10:53




Instrument :
MSVOA_N
ClientSampleId :
VN0822WBL01


Tgt Ion:168 Resp: 142322
Ion Ratio Lower Upper
168 100
99 65.8 48.2 72.4

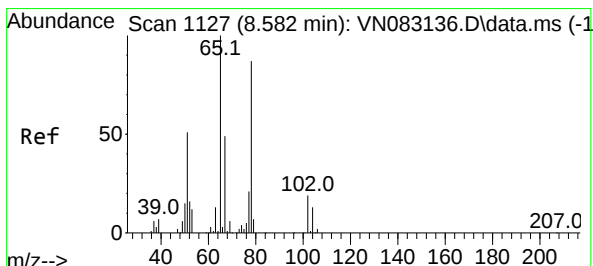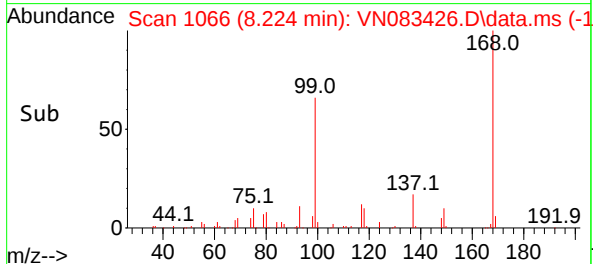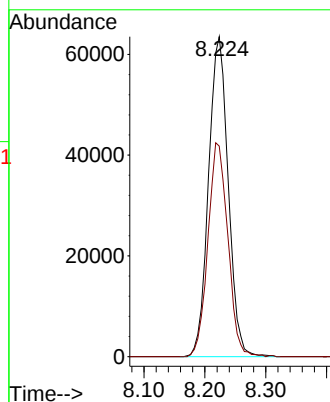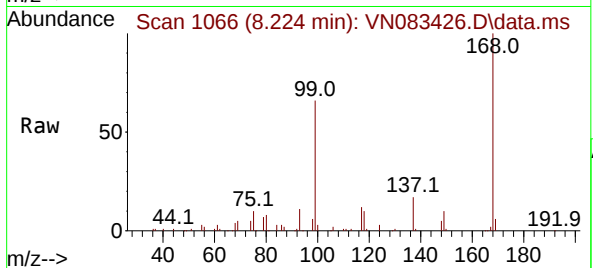

#33
1,2-Dichloroethane-d4
Concen: 54.137 ug/l
RT: 8.577 min Scan# 1126
Delta R.T. -0.005 min
Lab File: VN083426.D
Acq: 22 Aug 2024 10:53

Tgt Ion: 65 Resp: 109671
Ion Ratio Lower Upper
65 100
67 50.0 0.0 104.4

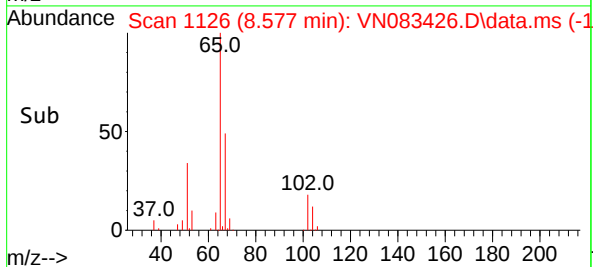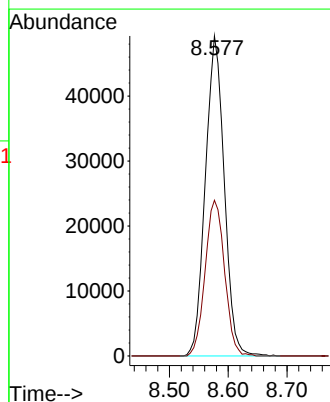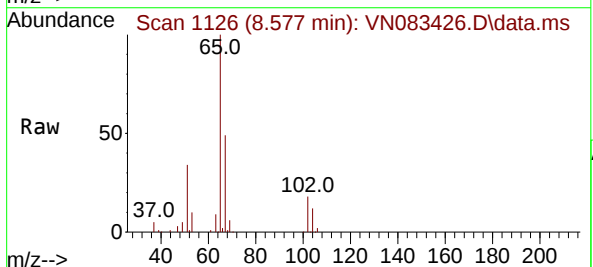

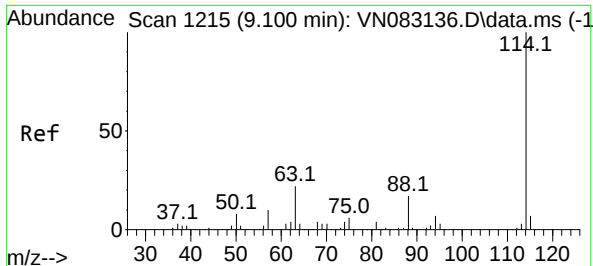

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.100 min Scan# 1

Delta R.T. -0.000 min

Lab File: VN083426.D

Acq: 22 Aug 2024 10:53

Instrument :

MSVOA_N

ClientSampleId :

VN0822WBL01





Tgt Ion:114 Resp: 288957

Ion Ratio Lower Upper

114 100

63 23.2 0.0 44.6

88 17.7 0.0 31.4

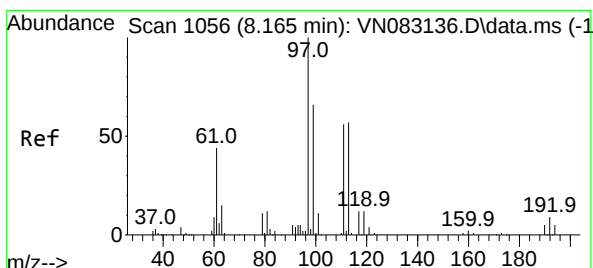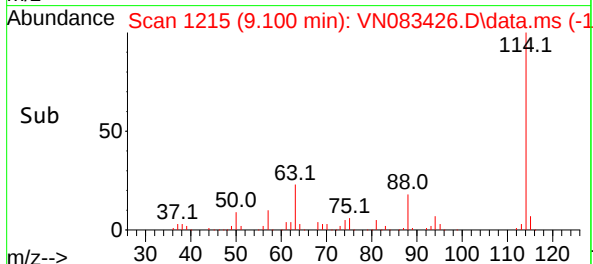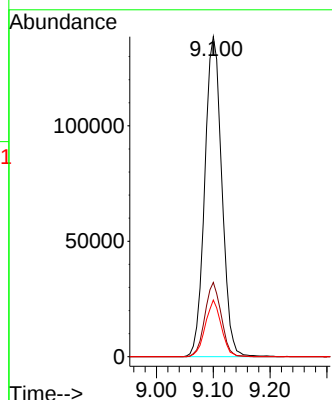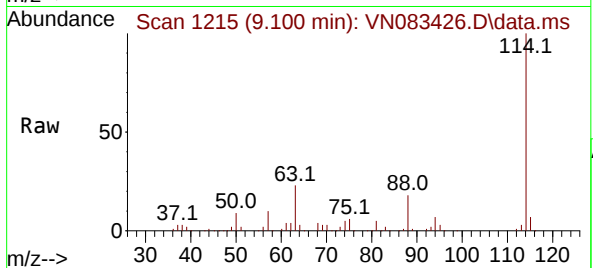

#35

Dibromofluoromethane

Concen: 49.012 ug/l

RT: 8.165 min Scan# 1056

Delta R.T. -0.000 min

Lab File: VN083426.D

Acq: 22 Aug 2024 10:53




Tgt Ion:113 Resp: 88398


Ion Ratio Lower Upper

113 100

111 102.4 82.4 123.6

192 16.9 14.9 22.3


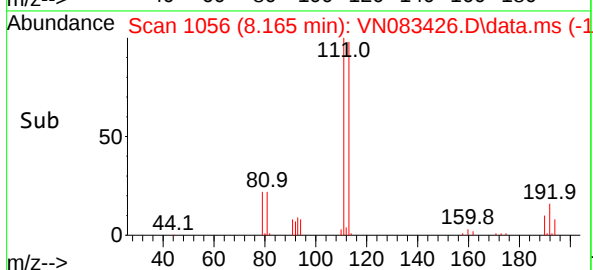
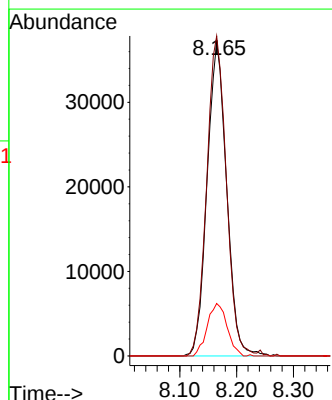
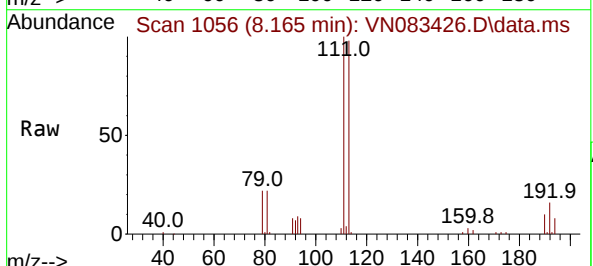


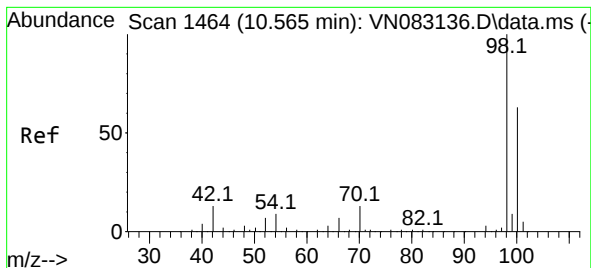

#50
Toluene-d8
Concen: 47.183 ug/l
RT: 10.565 min Scan# 1464
Delta R.T. -0.000 min
Lab File: VN083426.D
Acq: 22 Aug 2024 10:53




Instrument :
MSVOA_N
ClientSampleId :
VN0822WBL01


Tgt Ion: 98 Resp: 317440
Ion Ratio Lower Upper
98 100
100 64.9 51.5 77.3

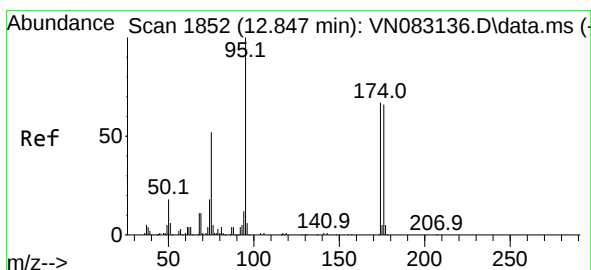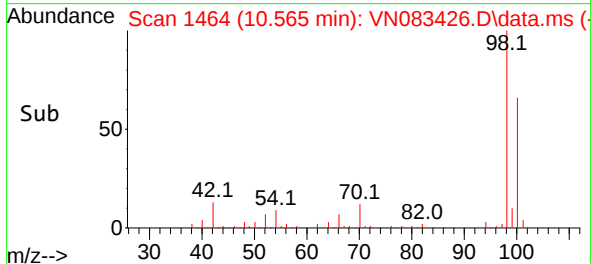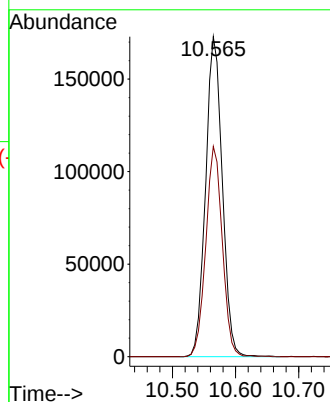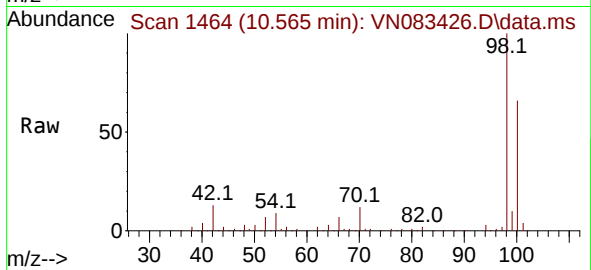

#62
4-Bromofluorobenzene
Concen: 54.965 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. -0.000 min
Lab File: VN083426.D
Acq: 22 Aug 2024 10:53

Tgt Ion: 95 Resp: 144169
Ion Ratio Lower Upper
95 100
174 71.2 0.0 159.2
176 67.8 0.0 147.6

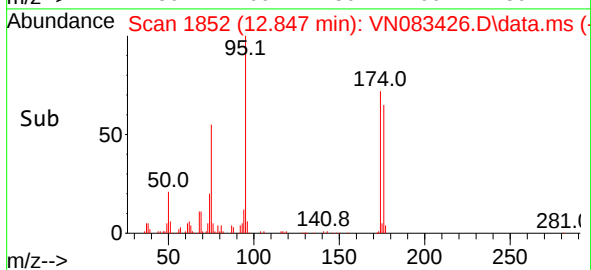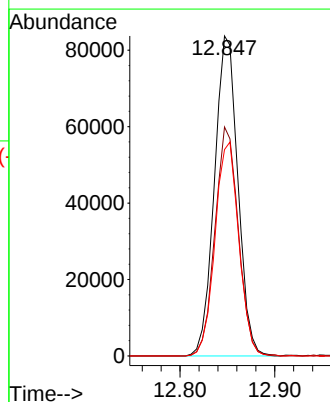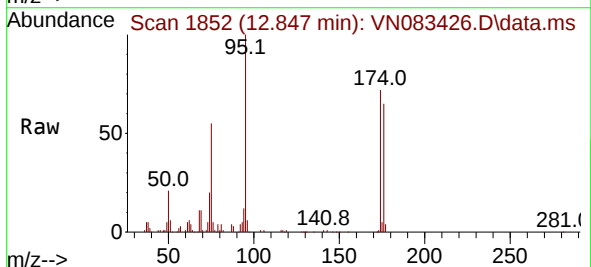

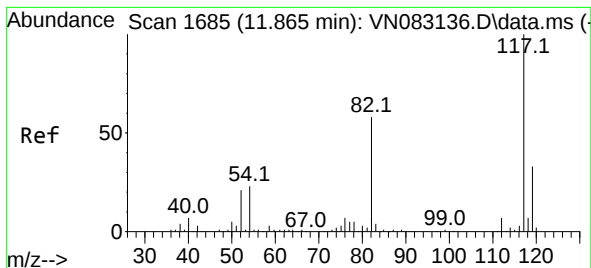

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.865 min Scan# 1

Delta R.T. -0.000 min

Lab File: VN083426.D

Acq: 22 Aug 2024 10:53

Instrument :

MSVOA_N

ClientSampleId :

VN0822WBL01





Tgt Ion:117 Resp: 306835

Ion Ratio Lower Upper

117 100

82 61.4 47.5 71.3

119 30.5 25.6 38.4

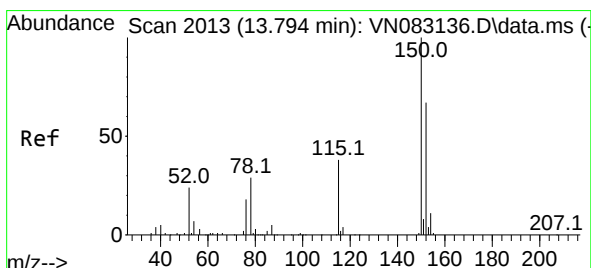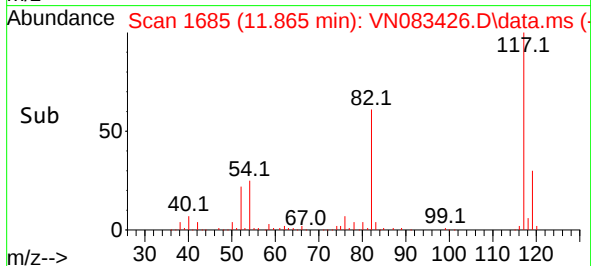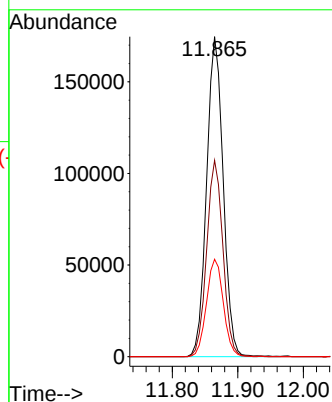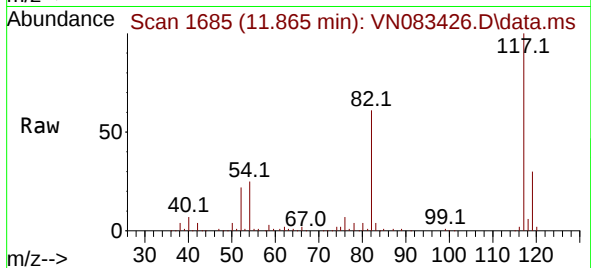

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.794 min Scan# 2013

Delta R.T. -0.000 min

Lab File: VN083426.D

Acq: 22 Aug 2024 10:53

Tgt Ion:152 Resp: 145694

Ion Ratio Lower Upper

152 100

115 64.8 30.6 91.6

150 157.0 0.0 348.6

