

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN082224\
 Data File : VN083429.D
 Acq On : 22 Aug 2024 12:32
 Operator : JC\MD
 Sample : VIBLK
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VIBLK

Quant Time: Aug 23 01:39:51 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N080724W.M
 Quant Title : SW846 8260
 QLast Update : Thu Aug 08 06:30:41 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.224	168	126928	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	259691	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	266909	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.788	152	120949	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.577	65	98164	54.334	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	108.660%
35) Dibromofluoromethane	8.165	113	78351	48.337	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	96.680%
50) Toluene-d8	10.565	98	277332	45.867	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	91.740%
62) 4-Bromofluorobenzene	12.847	95	123426	52.360	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	104.720%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN082224\
Data File : VN083429.D
Acq On : 22 Aug 2024 12:32
Operator : JC\MD
Sample : VIBLK
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VIBLK


Quant Time: Aug 23 01:39:51 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N080724W.M
Quant Title : SW846 8260
QLast Update : Thu Aug 08 06:30:41 2024
Response via : Initial Calibration

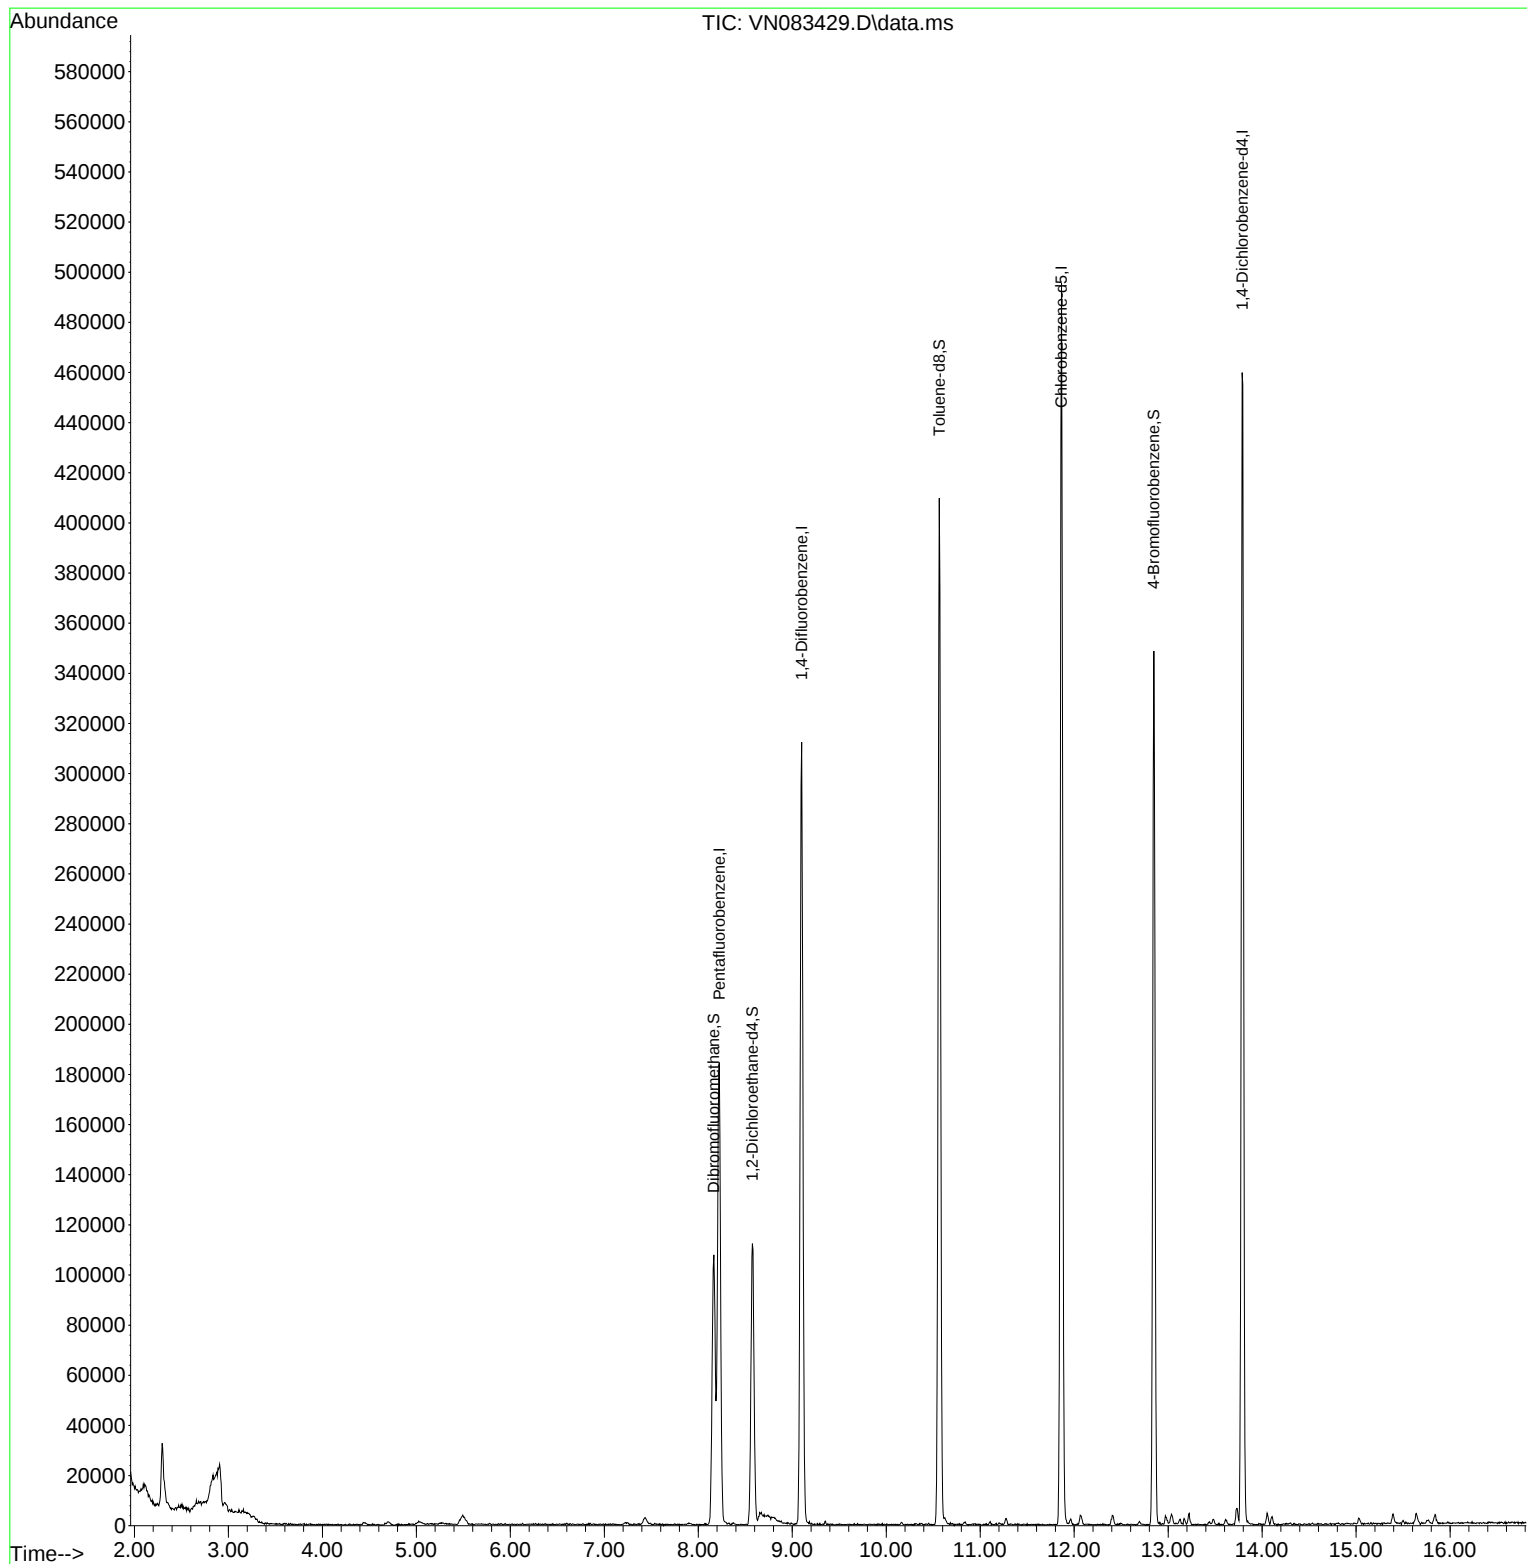





#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.000 min
Lab File: VN083429.D
Acq: 22 Aug 2024 12:32

Instrument :
MSVOA_N
ClientSampleId :
VIBLK



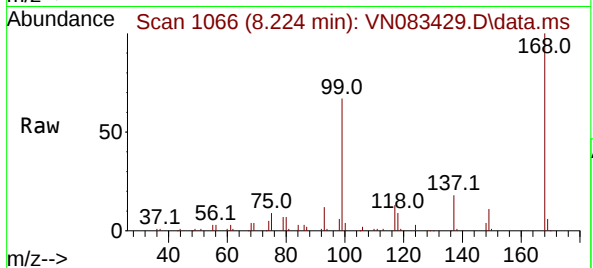


Tgt Ion:168 Resp: 126928
Ion Ratio Lower Upper
168 100
99 67.0 48.2 72.4

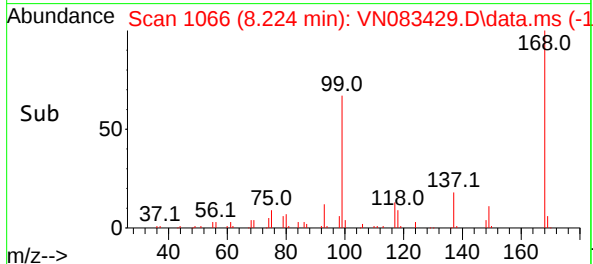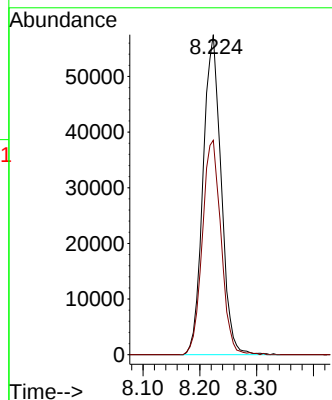

#33
1,2-Dichloroethane-d4
Concen: 54.334 ug/l
RT: 8.577 min Scan# 1126
Delta R.T. -0.005 min
Lab File: VN083429.D
Acq: 22 Aug 2024 12:32

Tgt Ion: 65 Resp: 98164
Ion Ratio Lower Upper
65 100
67 50.8 0.0 104.4

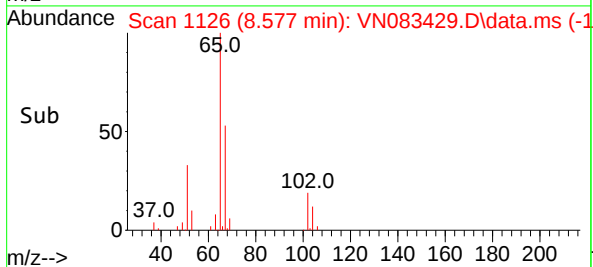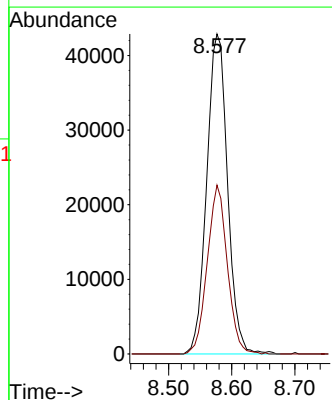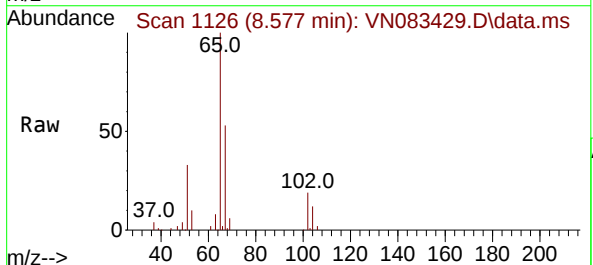



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.100 min Scan# 1

Delta R.T. 0.000 min

Lab File: VN083429.D

Acq: 22 Aug 2024 12:32

Instrument :

MSVOA_N

ClientSampleId :

VIBLK





Tgt Ion:114 Resp: 259691

Ion Ratio Lower Upper

114 100

63 22.7 0.0 44.6

88 17.4 0.0 31.4

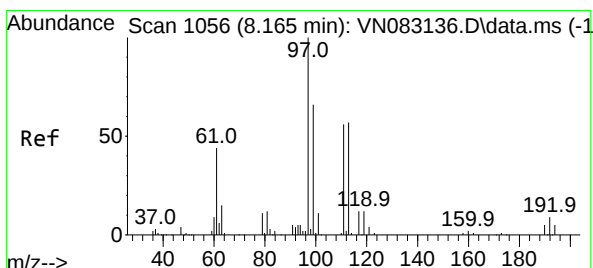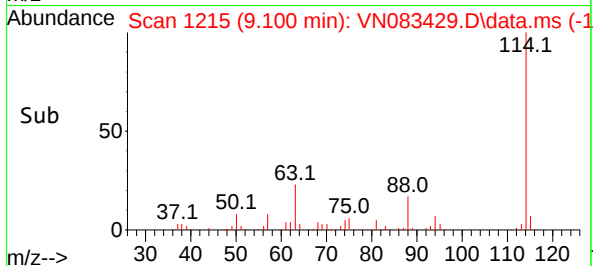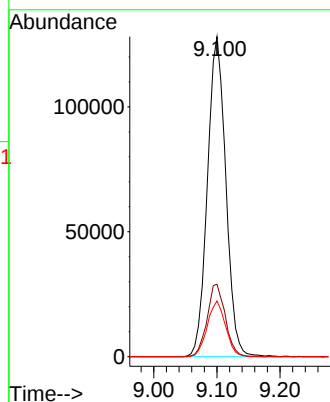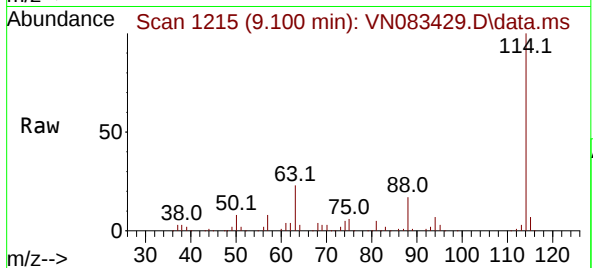

#35

Dibromofluoromethane

Concen: 48.337 ug/l

RT: 8.165 min Scan# 1056

Delta R.T. -0.000 min

Lab File: VN083429.D

Acq: 22 Aug 2024 12:32




Tgt Ion:113 Resp: 78351


Ion Ratio Lower Upper

113 100

111 103.6 82.4 123.6

192 16.7 14.9 22.3


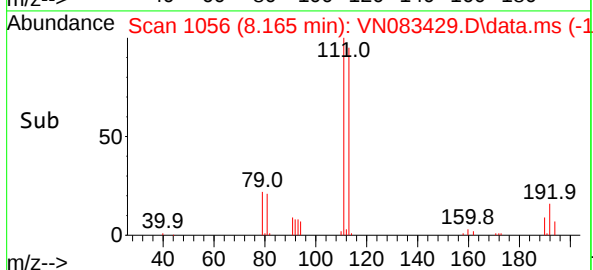
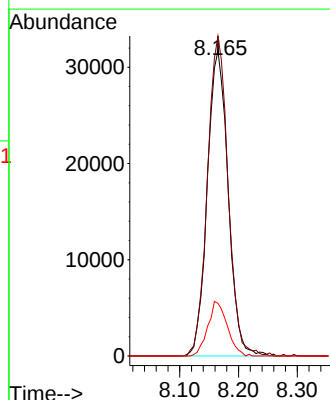
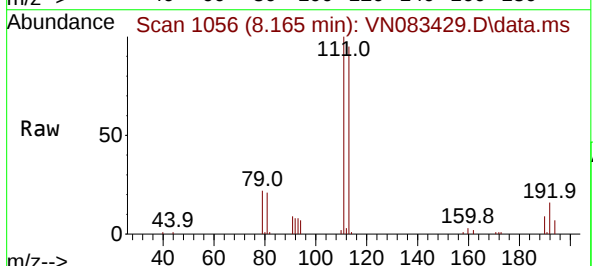


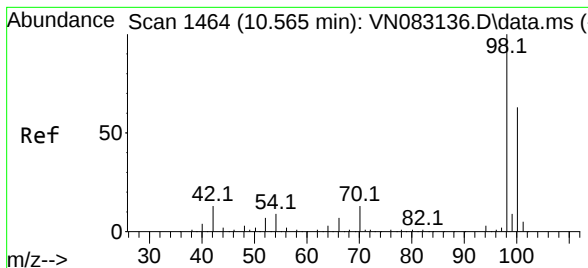

#50
Toluene-d8
Concen: 45.867 ug/l
RT: 10.565 min Scan# 1464
Delta R.T. -0.000 min
Lab File: VN083429.D
Acq: 22 Aug 2024 12:32




Instrument :
MSVOA_N
ClientSampleId :
VIBLK


Tgt Ion: 98 Resp: 277332
Ion Ratio Lower Upper
98 100
100 65.4 51.5 77.3

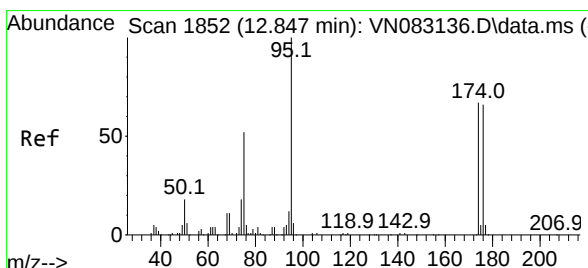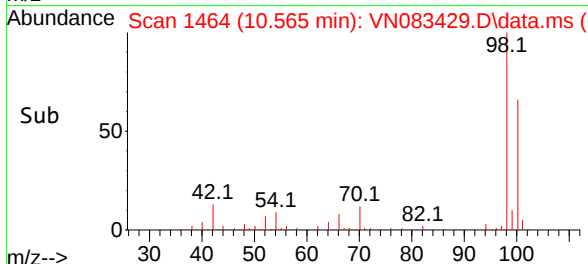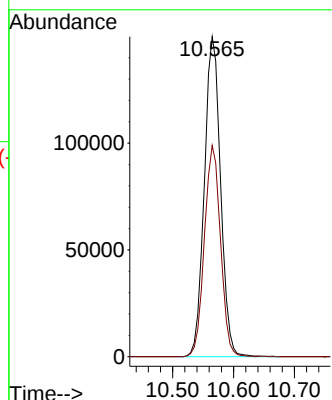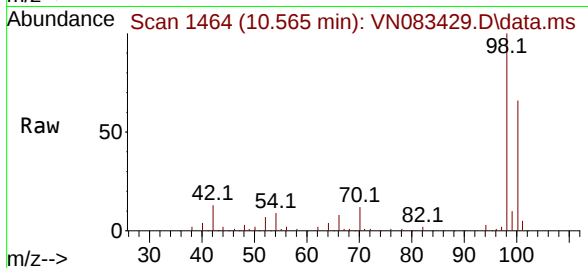

#62
4-Bromofluorobenzene
Concen: 52.360 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. -0.000 min
Lab File: VN083429.D
Acq: 22 Aug 2024 12:32

Tgt Ion: 95 Resp: 123426
Ion Ratio Lower Upper
95 100
174 70.2 0.0 159.2
176 66.8 0.0 147.6


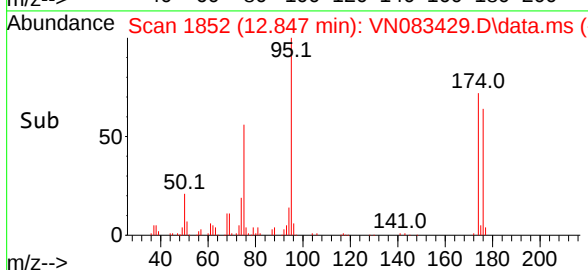
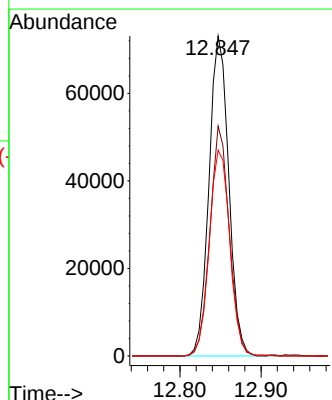
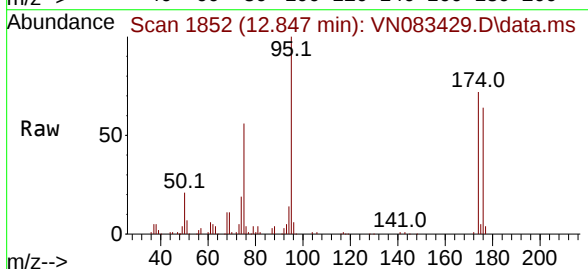


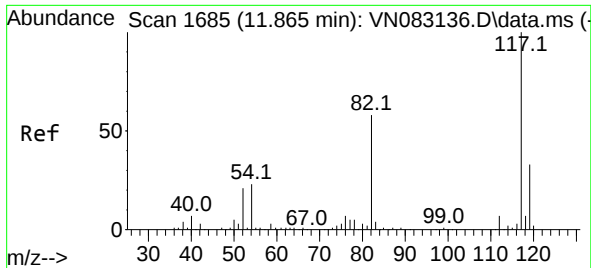

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 117
Delta R.T. 0.000 min
Lab File: VN083429.D
Acq: 22 Aug 2024 12:32

Instrument :
MSVOA_N
ClientSampleId :
VIBLK

Tgt Ion:117 Resp: 266909
Ion Ratio Lower Upper
117 100
82 61.4 47.5 71.3
119 32.2 25.6 38.4

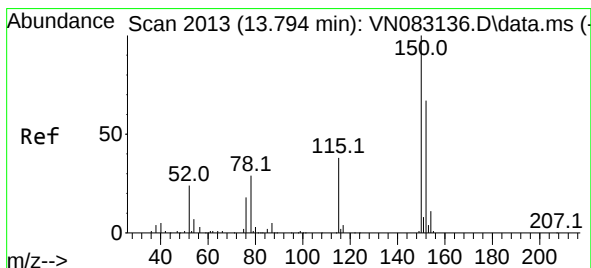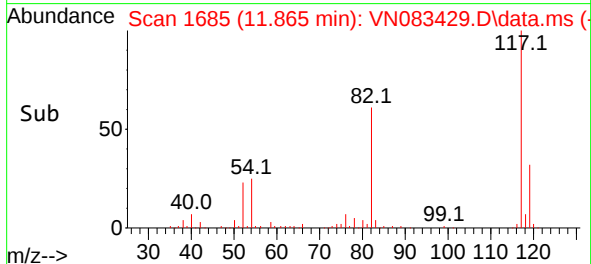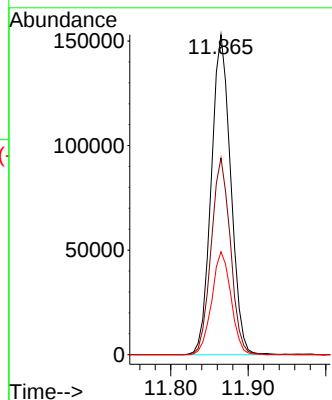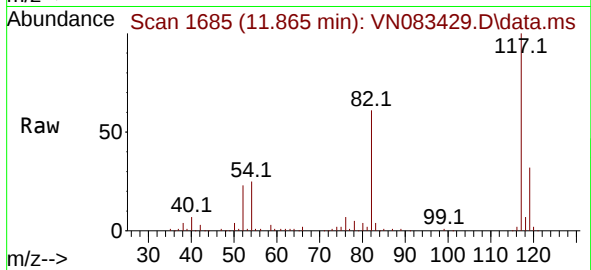

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.788 min Scan# 2012
Delta R.T. -0.006 min
Lab File: VN083429.D
Acq: 22 Aug 2024 12:32

Tgt Ion:152 Resp: 120949
Ion Ratio Lower Upper
152 100
115 64.4 30.6 91.6
150 160.6 0.0 348.6

