
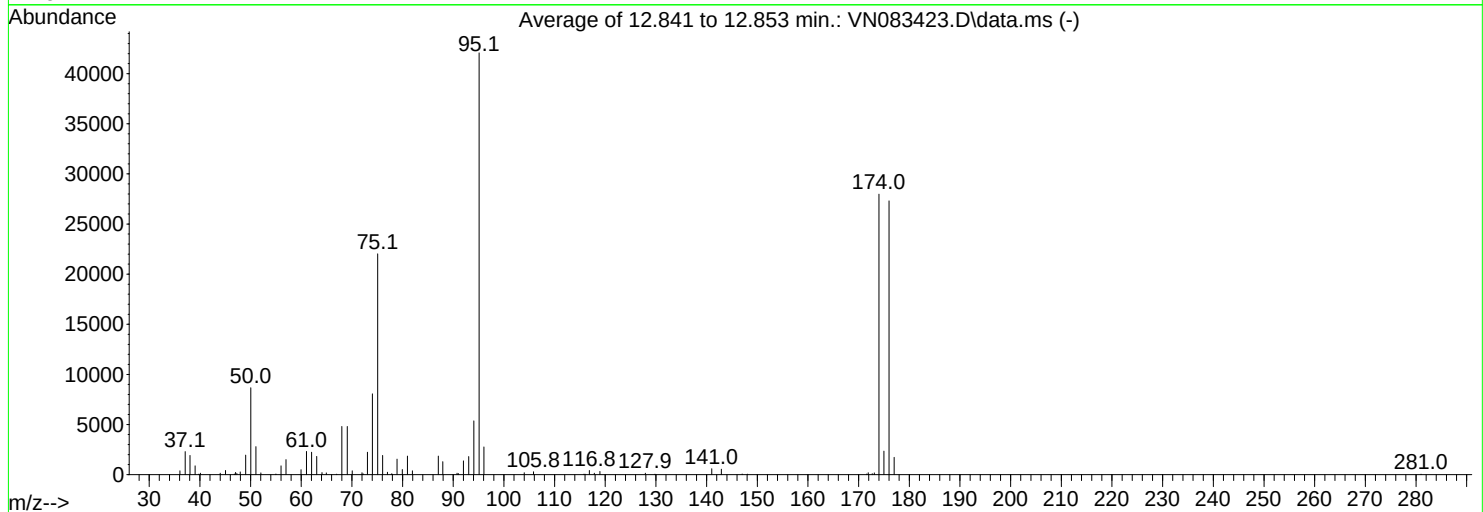


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN082224\
Data File : VN083423.D
Acq On : 22 Aug 2024 08:18
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N080724W.M
Title : SW846 8260
Last Update : Thu Aug 08 06:30:41 2024

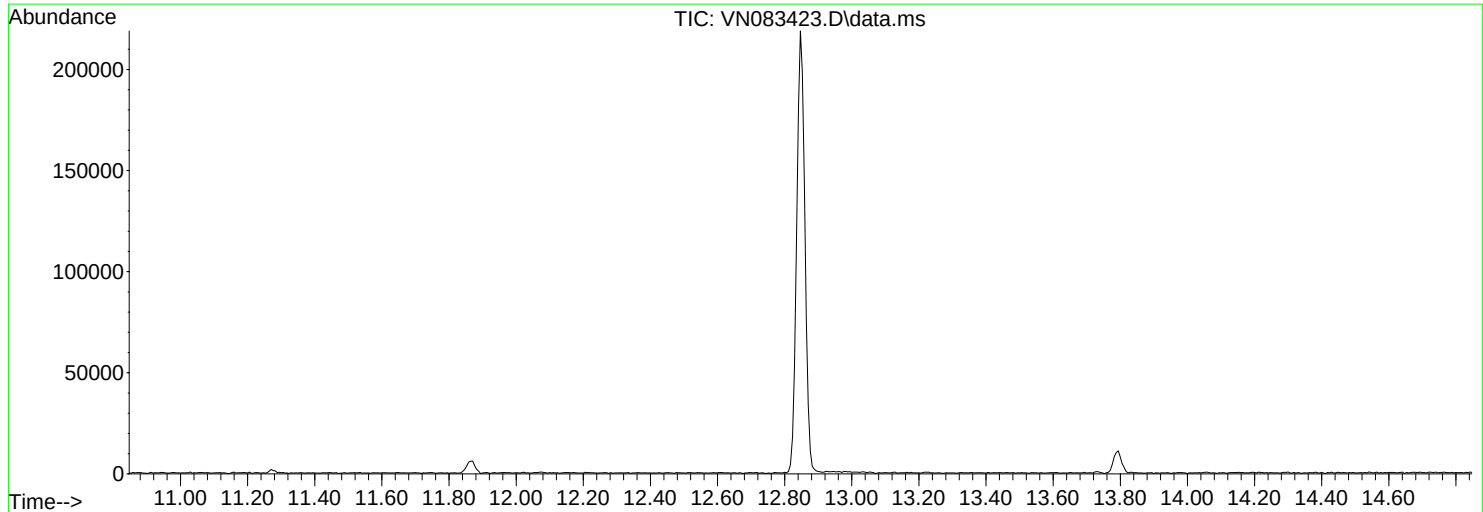

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.6	8665	PASS
75	95	30	60	52.4	22035	PASS
95	95	100	100	100.0	42077	PASS
96	95	5	9	6.6	2758	PASS
173	174	0.00	2	0.6	179	PASS
174	95	50	100	66.5	27987	PASS
175	174	5	9	8.4	2344	PASS
176	174	95	101	97.6	27315	PASS
177	176	5	9	6.3	1729	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	384	47.95	267	63.05	1816	75.10	2203
37.10	2301	49.05	1946	64.10	206	76.05	1921
38.05	1921	50.05	8665	64.95	172	77.00	241
39.05	883	51.05	2799	67.00	56	77.80	80
39.80	52	52.05	183	68.00	4801	78.00	52
40.10	138	55.00	60	69.10	4798	78.90	1545
44.00	138	56.00	872	70.05	387	79.95	518
45.05	419	57.00	1507	72.00	190	80.95	1859
46.80	69	59.95	495	72.20	80	81.95	376
47.05	222	61.05	2313	73.05	2234	87.05	1856
47.30	113	62.05	2231	74.05	8064	87.95	1299

Average of 12.841 to 12.853 min.: VN083423.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
90.75	141	116.85	408	172.70	99		
91.00	108	117.85	138	173.10	179		
92.00	1380	118.95	314	174.00	27987		
93.05	1803	127.90	142	175.00	2344		
94.05	5363	129.80	53	176.00	27315		
95.10	42077	141.00	598	177.00	1729		
96.05	2758	142.90	547	281.00	51		
104.00	186	147.00	66				
105.85	295	148.10	56				
115.80	52	171.60	71				
116.00	50	171.90	199				

Instrument :

MSVOA_N

ClientSampleId :

BFB