
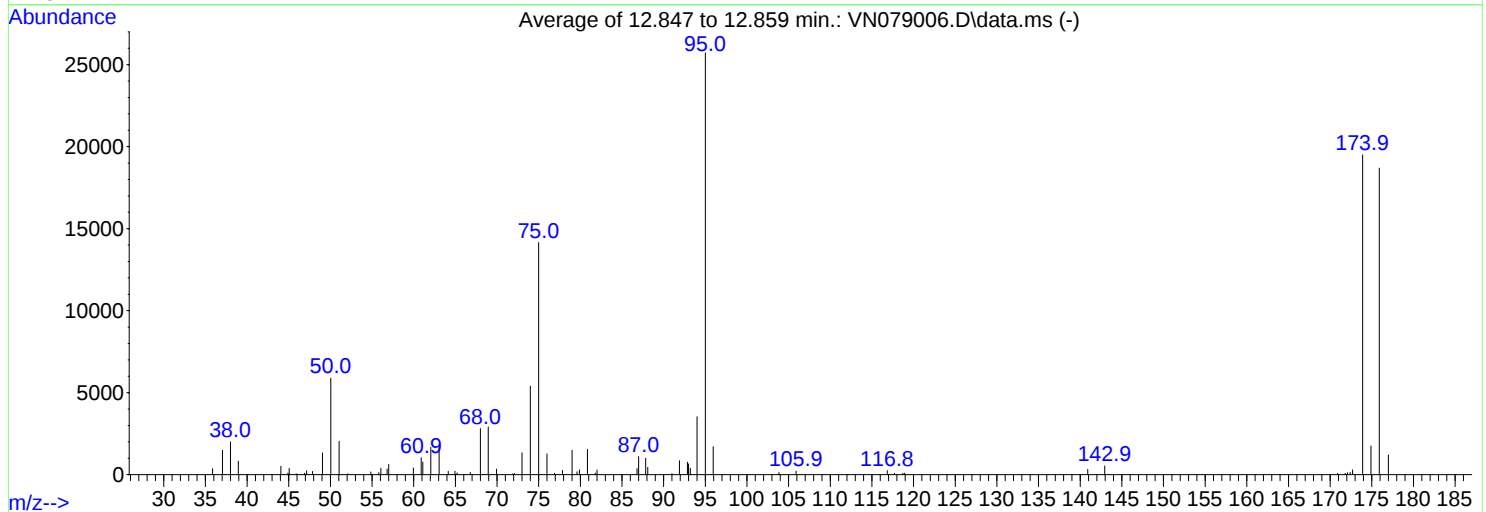


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN082323\
Data File : VN079006.D
Acq On : 23 Aug 2023 08:46
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N081523W.M
Title : SW846 8260
Last Update : Wed Aug 16 02:42:02 2023

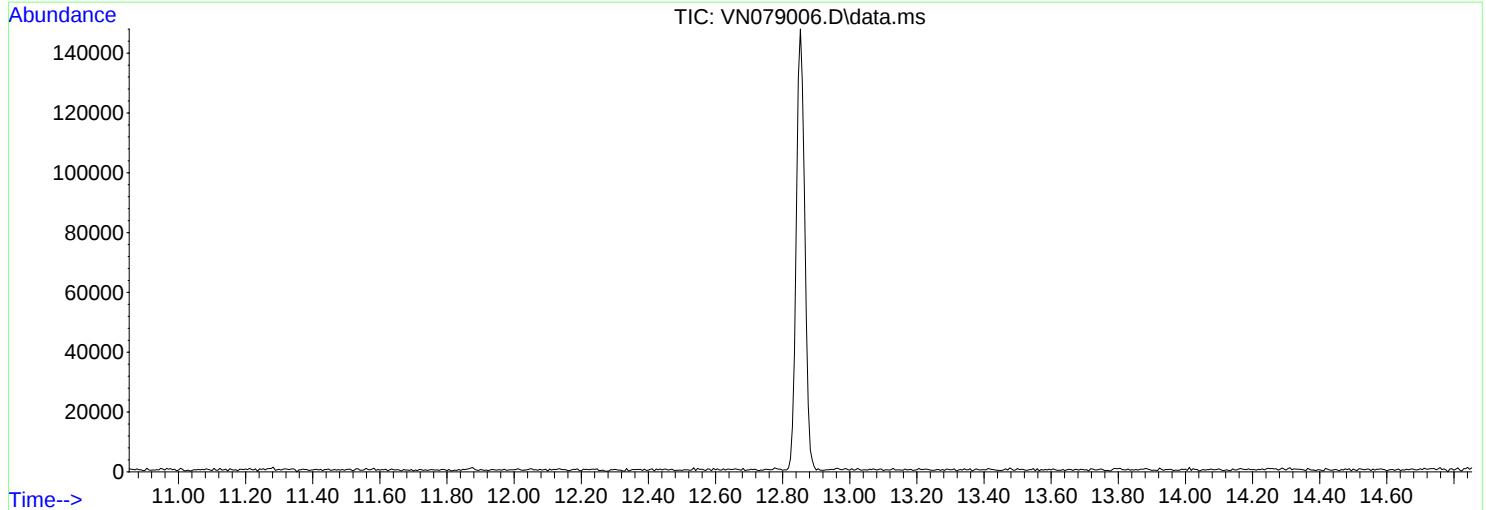

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	22.9	5880	PASS
75	95	30	60	55.0	14157	PASS
95	95	100	100	100.0	25720	PASS
96	95	5	9	6.6	1705	PASS
173	174	0.00	2	1.5	291	PASS
174	95	50	100	75.8	19504	PASS
175	174	5	9	9.0	1748	PASS
176	174	95	101	95.9	18696	PASS
177	176	5	9	6.4	1202	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.85	361	49.05	1331	61.10	772	72.10	64
37.05	1488	50.05	5880	62.05	1667	73.00	134
38.00	2004	51.05	2036	63.05	1738	74.00	539
38.95	815	52.10	61	64.15	207	75.00	1415
44.05	508	54.85	162	64.95	213	76.00	1271
44.90	93	55.80	132	65.20	107	76.90	86
45.05	379	56.05	390	66.80	134	77.85	260
45.90	63	56.80	345	68.00	2808	79.00	1479
46.90	84	57.00	626	68.95	2905	79.60	173
47.15	235	59.95	411	69.95	339	79.90	297
47.85	191	60.90	1032	71.90	55	80.85	1544

Average of 12.847 to 12.859 min.: VN079006.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
81.80	99	94.00	3530	170.90	75		
82.00	281	95.00	25720	171.80	87		
86.80	371	95.95	1705	172.10	118		
87.00	1102	103.85	126	172.40	144		
87.85	996	105.90	211	172.70	291		
88.10	438	116.85	241	173.90	19504		
91.00	57	117.70	81	174.90	1748		
91.90	847	118.70	76	175.90	18696		
92.85	763	118.90	89	177.00	1202		
93.00	656	140.90	322				
93.20	390	142.95	527				

Instrument :

MSVOA_N

ClientSampleId :

BFB