
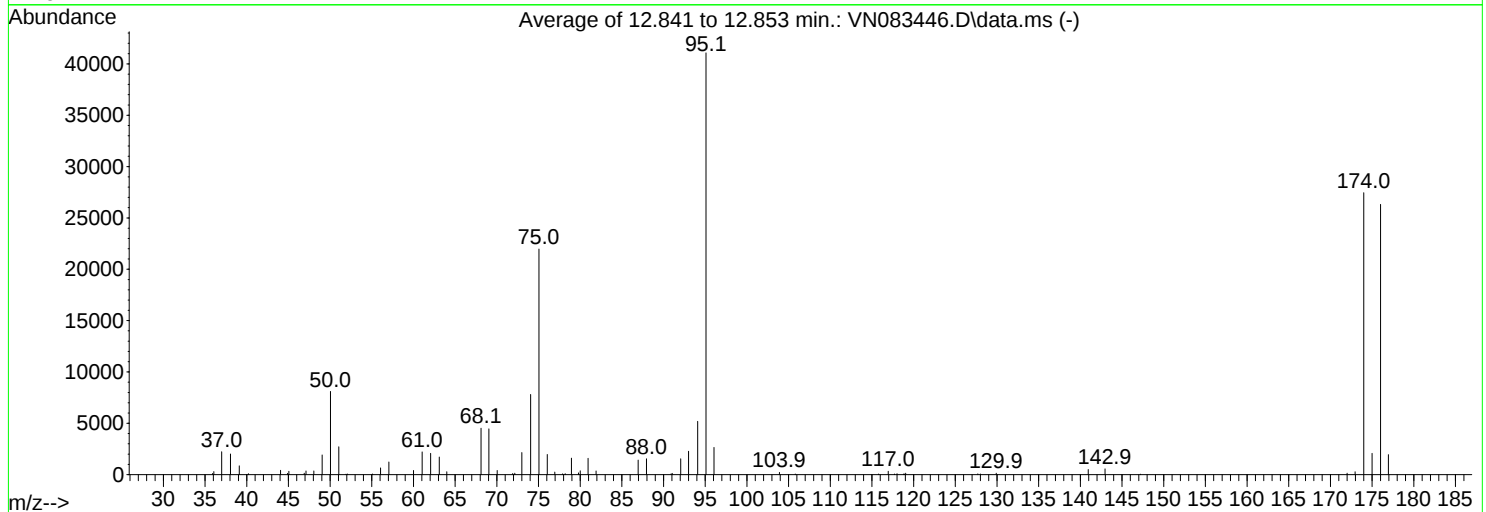


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN082324\
Data File : VN083446.D
Acq On : 23 Aug 2024 08:15
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N080724W.M
Title : SW846 8260
Last Update : Thu Aug 08 06:30:41 2024

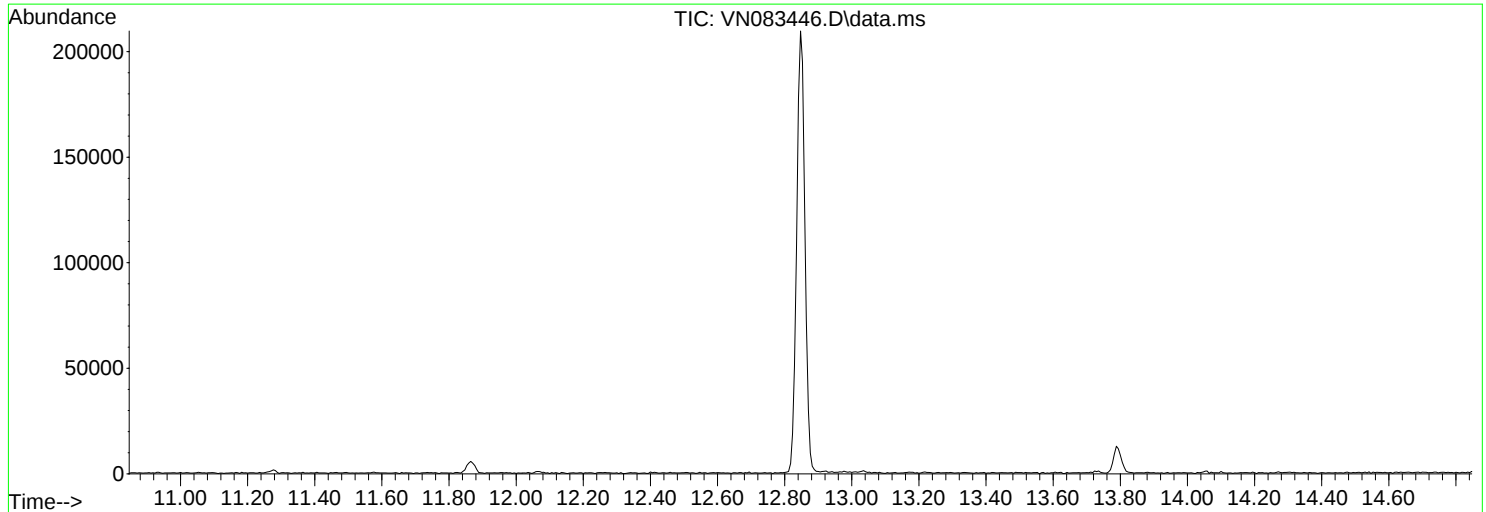

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	8097	PASS
75	95	30	60	53.5	21973	PASS
95	95	100	100	100.0	41075	PASS
96	95	5	9	6.4	2647	PASS
173	174	0.00	2	1.0	284	PASS
174	95	50	100	66.9	27459	PASS
175	174	5	9	7.5	2070	PASS
176	174	95	101	95.9	26320	PASS
177	176	5	9	7.4	1955	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	113	47.10	354	61.05	2215	75.05	2197
36.05	296	48.05	361	62.05	2068	76.05	1961
37.00	2229	49.05	1923	63.10	1716	76.95	257
38.05	2004	50.05	8097	64.00	276	77.90	7
39.10	863	51.05	2719	68.10	4527	78.20	89
40.00	22	51.90	52	69.05	4455	78.95	1605
40.20	101	52.10	67	70.05	410	79.80	172
44.05	422	55.10	66	71.90	114	80.00	382
44.90	124	56.05	660	72.15	144	80.95	1582
45.05	328	57.05	1224	73.00	2154	81.90	358
46.90	142	60.00	401	74.05	7810	86.95	1427

Average of 12.841 to 12.853 min.: VN083446.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
87.95	1545	116.95	335	147.20	53		
90.90	75	117.70	65	172.00	143		
91.05	127	118.00	92	172.95	284		
92.05	1550	118.80	58	174.00	27459		
93.00	2279	118.90	67	175.00	2070		
94.10	5190	119.05	142	176.00	26320		
95.10	41075	127.70	83	176.95	1955		
96.05	2647	128.00	56				
103.90	222	129.90	139				
105.80	65	140.95	498				
115.80	67	142.95	569				

Instrument :

MSVOA_N

ClientSampleId :

BFB