
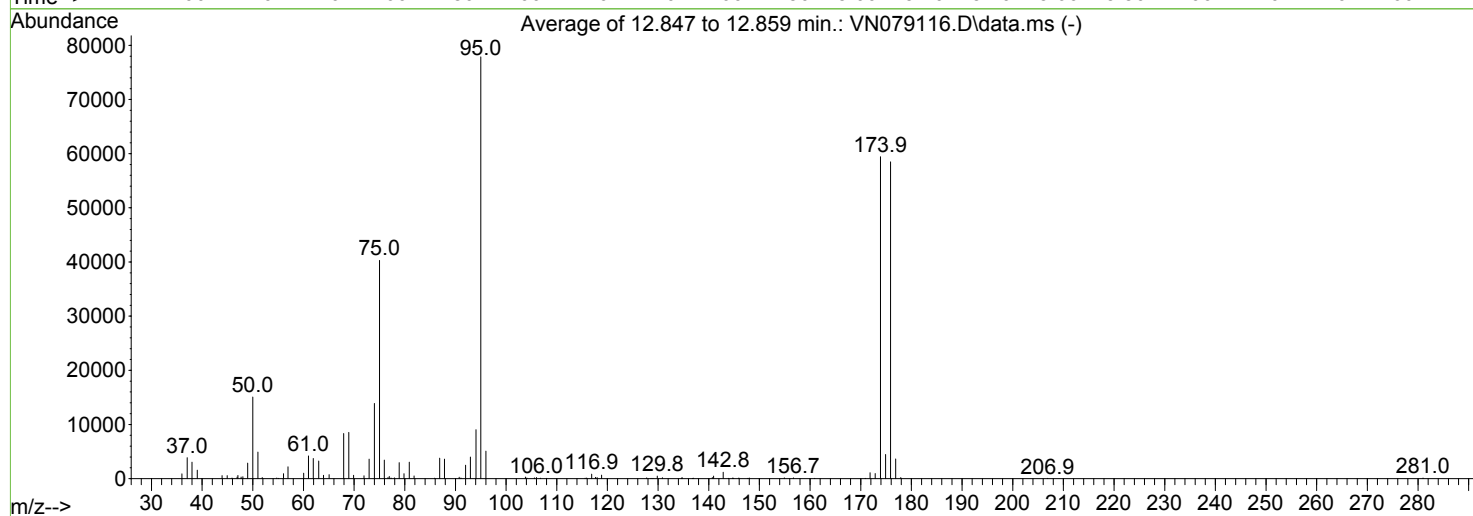


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN090123\
 Data File : VN079116.D
 Acq On : 01 Sep 2023 10:08
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N081523W.M
 Title : SW846 8260
 Last Update : Wed Aug 16 02:42:02 2023

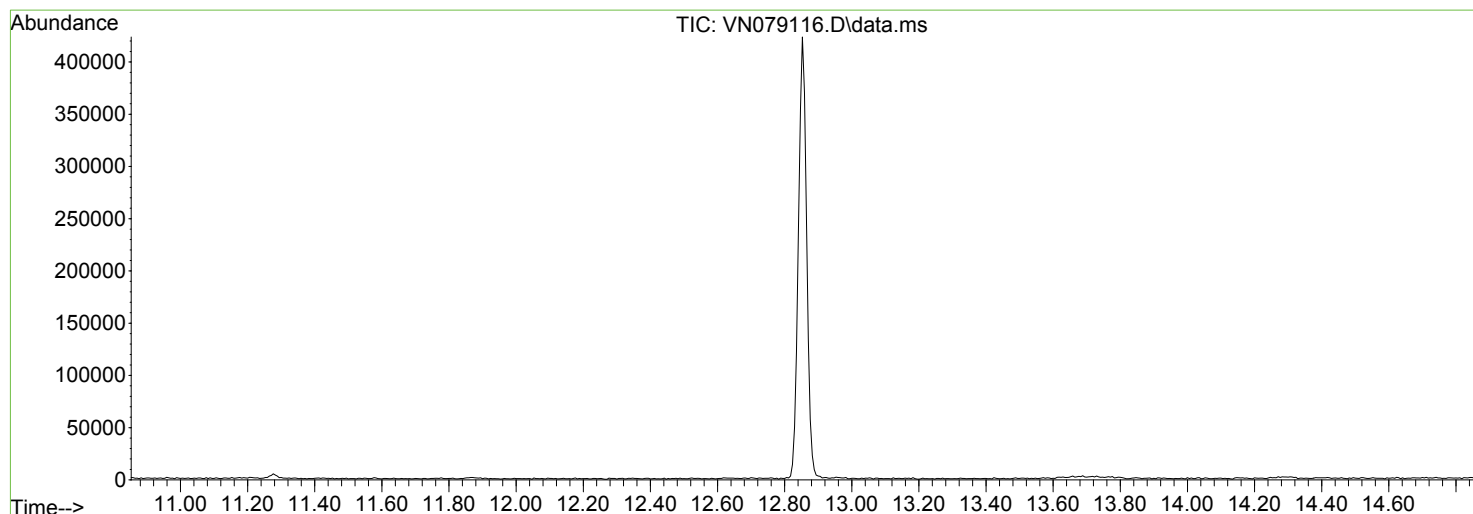

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	15060	PASS
75	95	30	60	51.8	40304	PASS
95	95	100	100	100.0	77875	PASS
96	95	5	9	6.5	5092	PASS
173	174	0.00	2	1.6	950	PASS
174	95	50	100	76.3	59443	PASS
175	174	5	9	7.5	4450	PASS
176	174	95	101	98.4	58488	PASS
177	176	5	9	6.2	3645	PASS

Average of 12.847 to 12.859 min.: VN079116.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	881	48.05	347	61.95	3733	75.95	342
37.05	3866	49.00	2859	63.00	3248	76.70	20
38.00	3045	50.00	15060	63.95	622	76.95	40
39.05	1556	51.00	4908	65.05	738	77.30	11
39.95	38	51.85	214	67.95	8337	77.95	161
43.95	576	54.75	118	68.95	8536	78.90	2969
44.95	575	55.10	58	69.90	608	79.85	927
45.90	117	56.05	922	71.95	542	80.90	3035
46.90	298	56.95	2191	72.95	3615	81.85	508
47.05	582	60.05	1020	74.00	13888	85.90	77
47.70	287	61.00	4193	75.00	40304	86.90	3781

Average of 12.847 to 12.859 min.: VN079116.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
87.85	3607	106.00	210	129.00	60	144.70	119
90.75	272	106.80	77	129.85	485	144.90	100
91.10	124	108.00	51	130.85	181	145.95	118
92.00	2488	115.60	107	134.60	114	147.70	62
92.95	3991	115.90	109	134.75	178	148.00	116
94.05	9034	116.90	820	136.80	64	154.90	138
95.00	77875	117.65	252	137.00	80	156.70	147
96.00	5092	117.95	219	140.70	219	160.90	61
103.80	310	118.85	644	140.95	485	170.90	73
104.10	111	127.75	163	142.85	1177	171.85	1110
105.60	139	128.60	62	143.90	68	172.85	950

Average of 12.847 to 12.859 min.: VN079116.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
173.90	59443						
174.90	4450						
175.90	58488						
176.90	3645						
177.90	221						
206.90	53						
281.00	130						

Instrument :

MSVOA_N

ClientSampleId :

BFB