
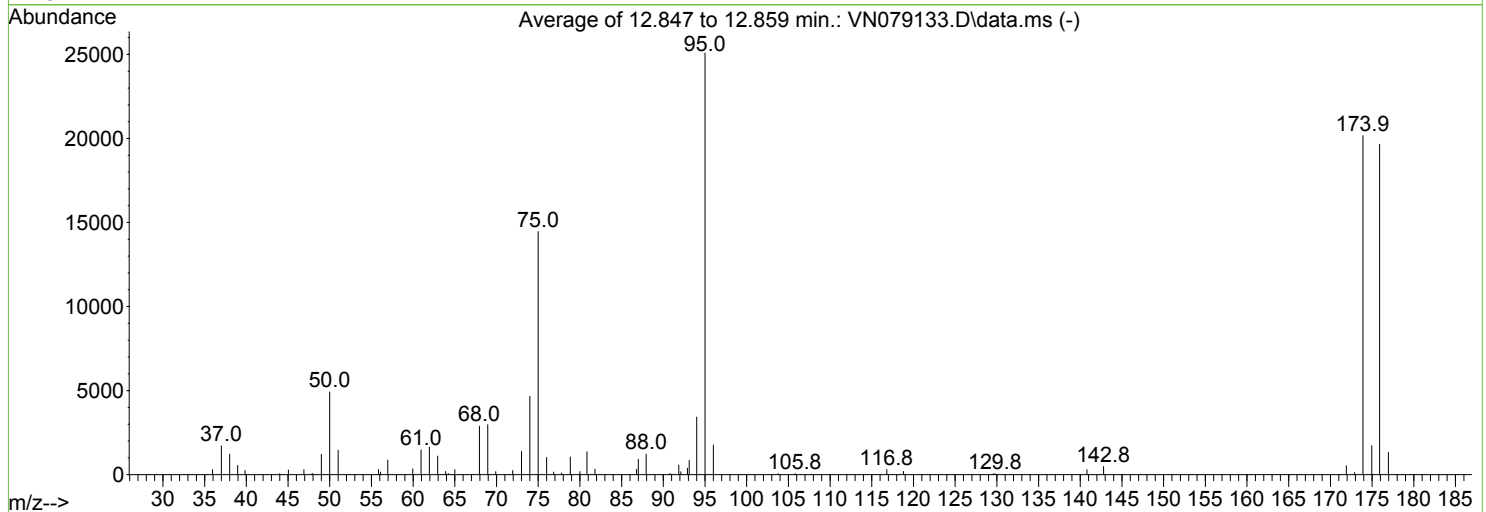


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN090223\
Data File : VN079133.D
Acq On : 02 Sep 2023 10:28
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N081523W.M
Title : SW846 8260
Last Update : Wed Aug 16 02:42:02 2023

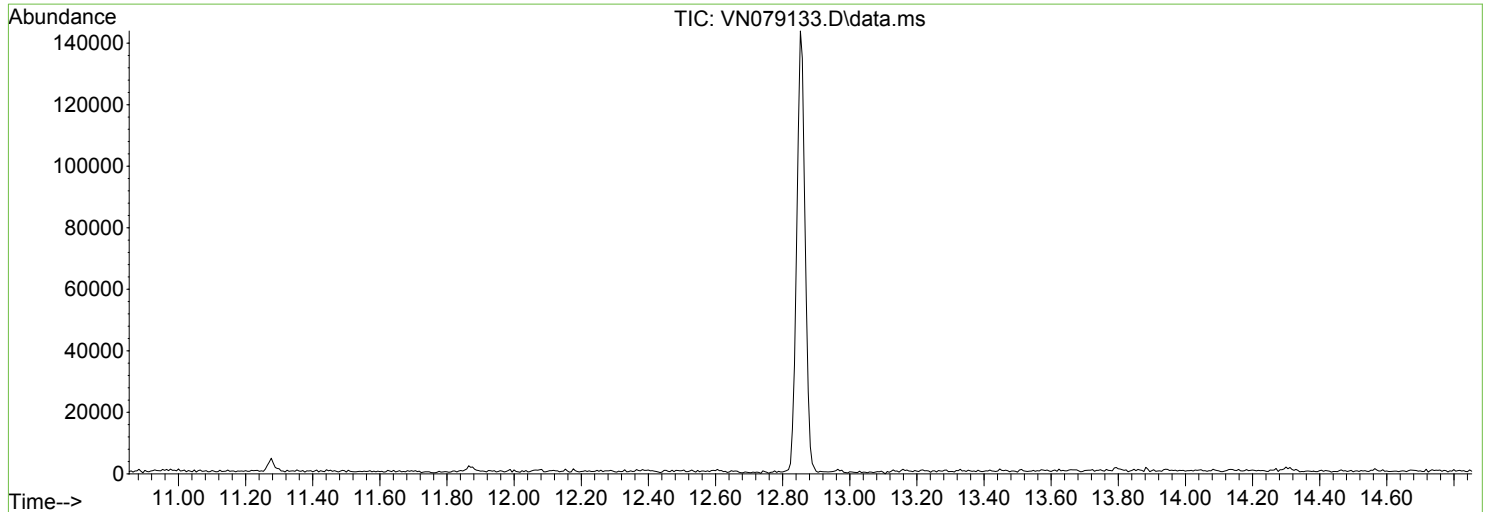

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	4923	PASS
75	95	30	60	57.6	14456	PASS
95	95	100	100	100.0	25091	PASS
96	95	5	9	7.0	1758	PASS
173	174	0.00	2	0.6	122	PASS
174	95	50	100	80.4	20165	PASS
175	174	5	9	8.6	1725	PASS
176	174	95	101	97.5	19656	PASS
177	176	5	9	6.7	1322	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	296	51.00	1459	67.95	2883	80.00	173
37.00	1714	55.85	307	68.95	2972	80.85	136
38.00	1222	56.10	156	69.90	184	81.80	32
38.95	557	56.95	867	71.95	252	86.80	32
39.85	250	59.95	345	73.00	1380	87.00	917
44.00	53	60.95	1480	74.00	4668	87.95	1218
45.05	278	61.95	1641	75.00	14456	90.80	63
46.90	301	62.95	1105	76.00	1020	91.85	570
47.90	74	63.90	190	76.85	149	92.10	172
49.00	1206	64.20	64	77.80	91	92.90	382
50.00	4923	65.00	299	78.85	1047	93.10	846

Average of 12.847 to 12.859 min.: VN079133.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
94.00	3429	171.90	532				
95.00	25091	172.90	122				
96.00	1758	173.90	20165				
103.80	57	174.95	1725				
105.80	59	175.90	19656				
116.80	309	176.95	1322				
118.80	195						
129.60	56						
129.80	60						
140.80	300						
142.80	490						

Instrument :

MSVOA_N

ClientSampleId :

BFB