




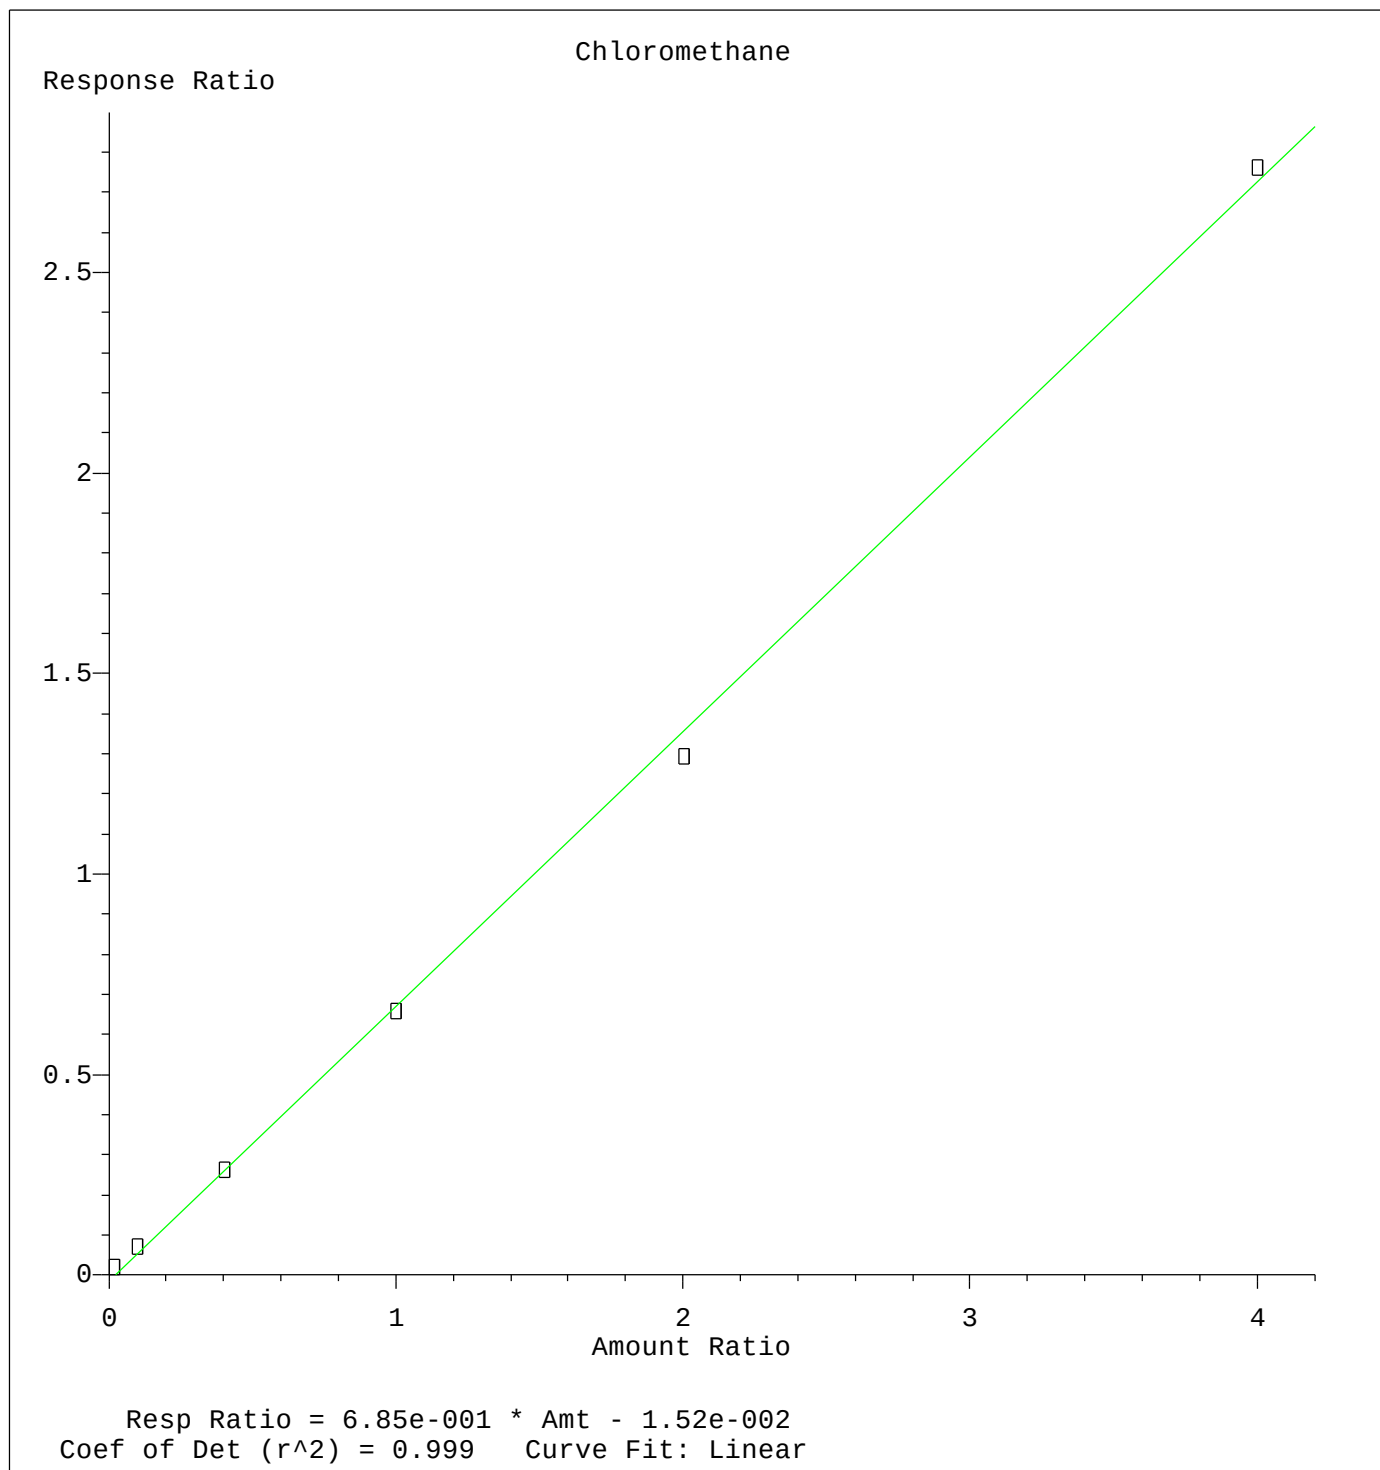


Method Name: W:\HPCHEM1\MSVOA_N\METHODS\82N091515W.M
Calibration Table Last Updated: Tue Sep 15 21:12:09 2015

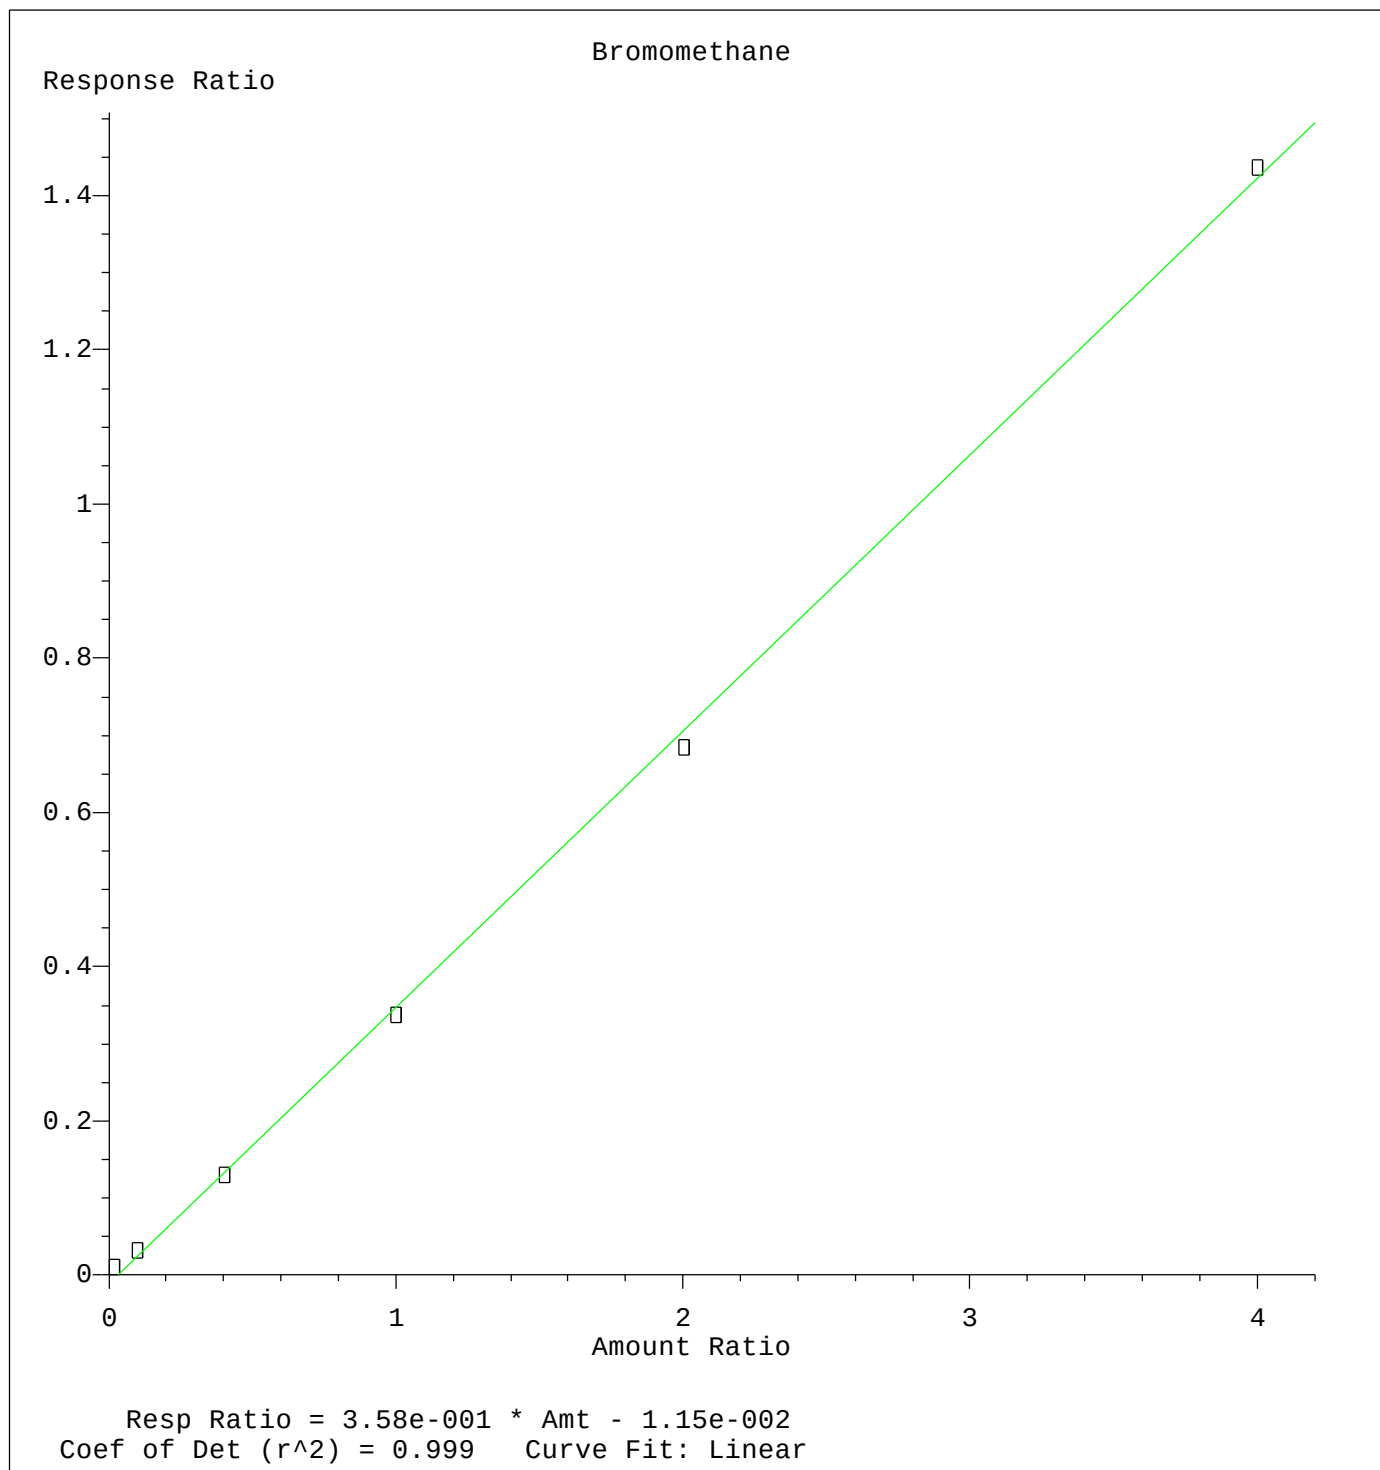

Method Name: W:\HPCHEM1\MSVOA_N\METHODS\82N091515W.M
Calibration Table Last Updated: Tue Sep 15 21:12:09 2015

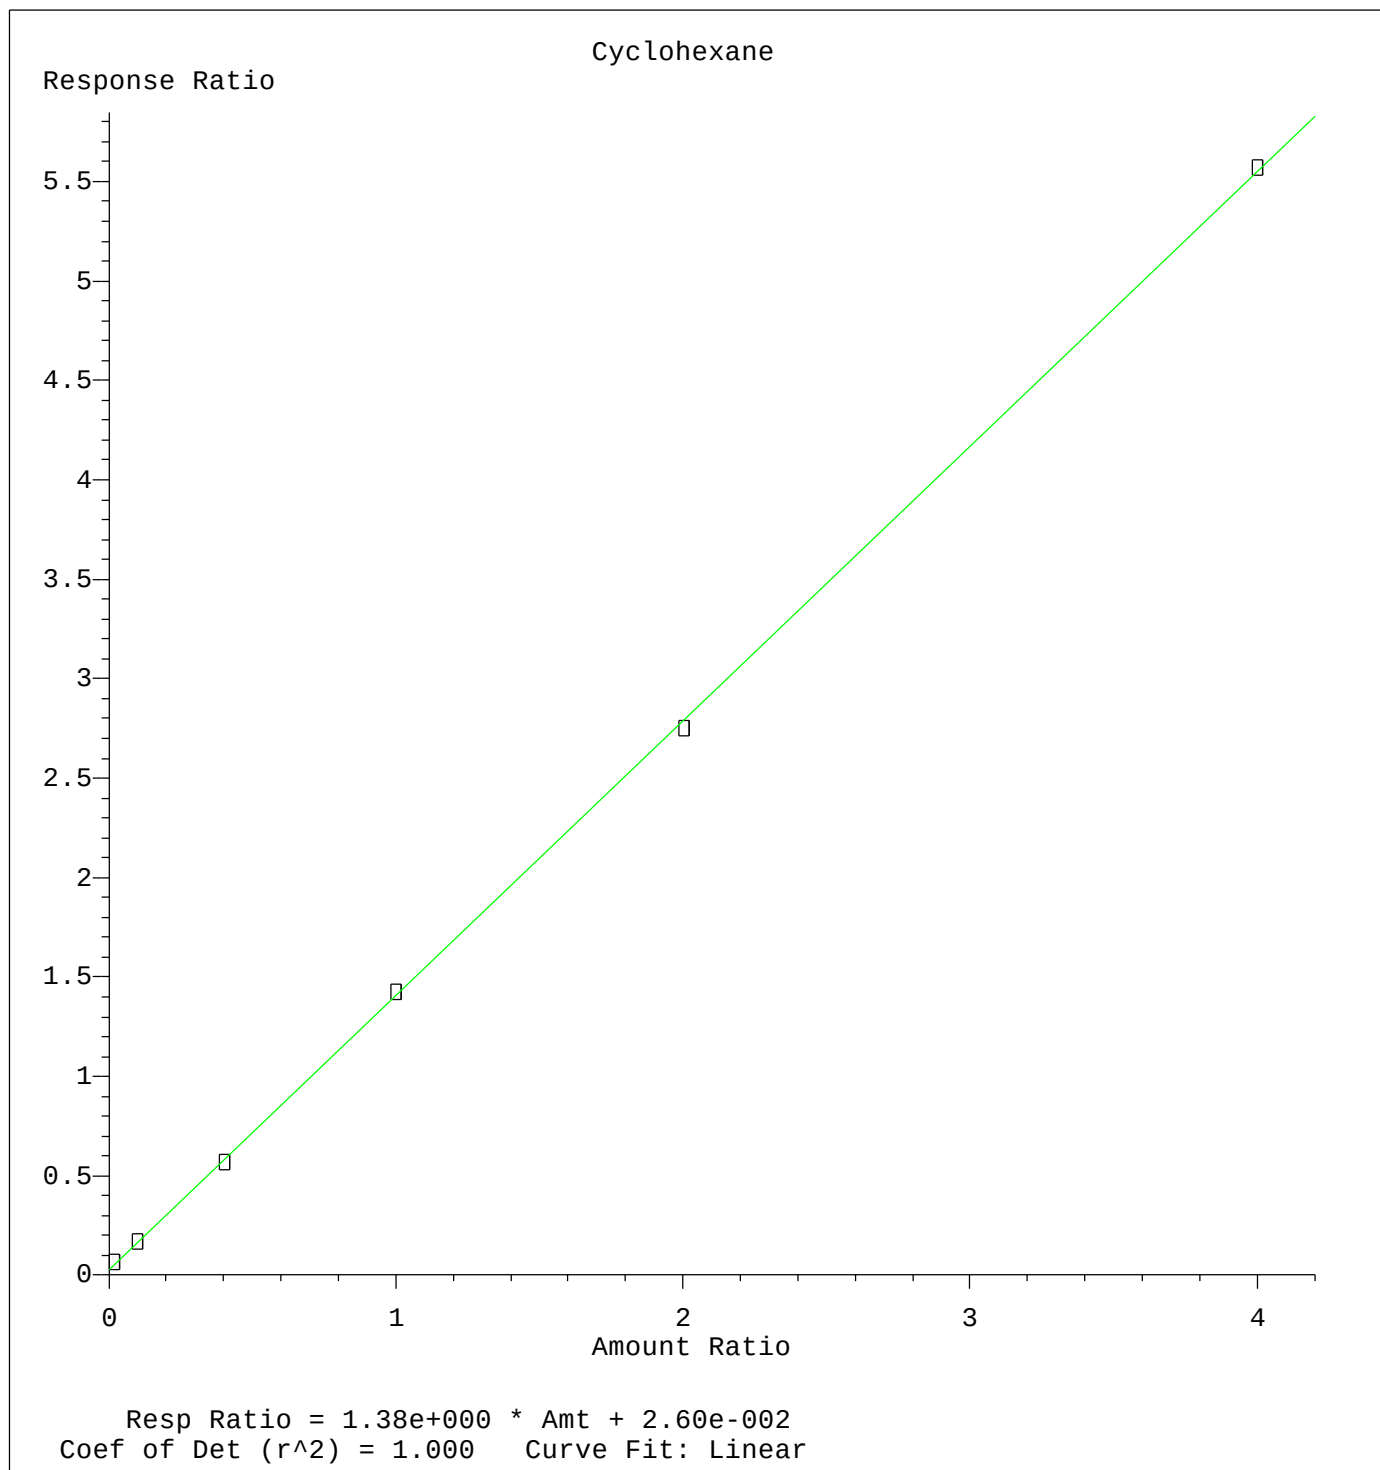


Method Name: W:\HPCHEM1\MSVOA_N\METHODS\82N091515W.M
Calibration Table Last Updated: Tue Sep 15 21:12:09 2015

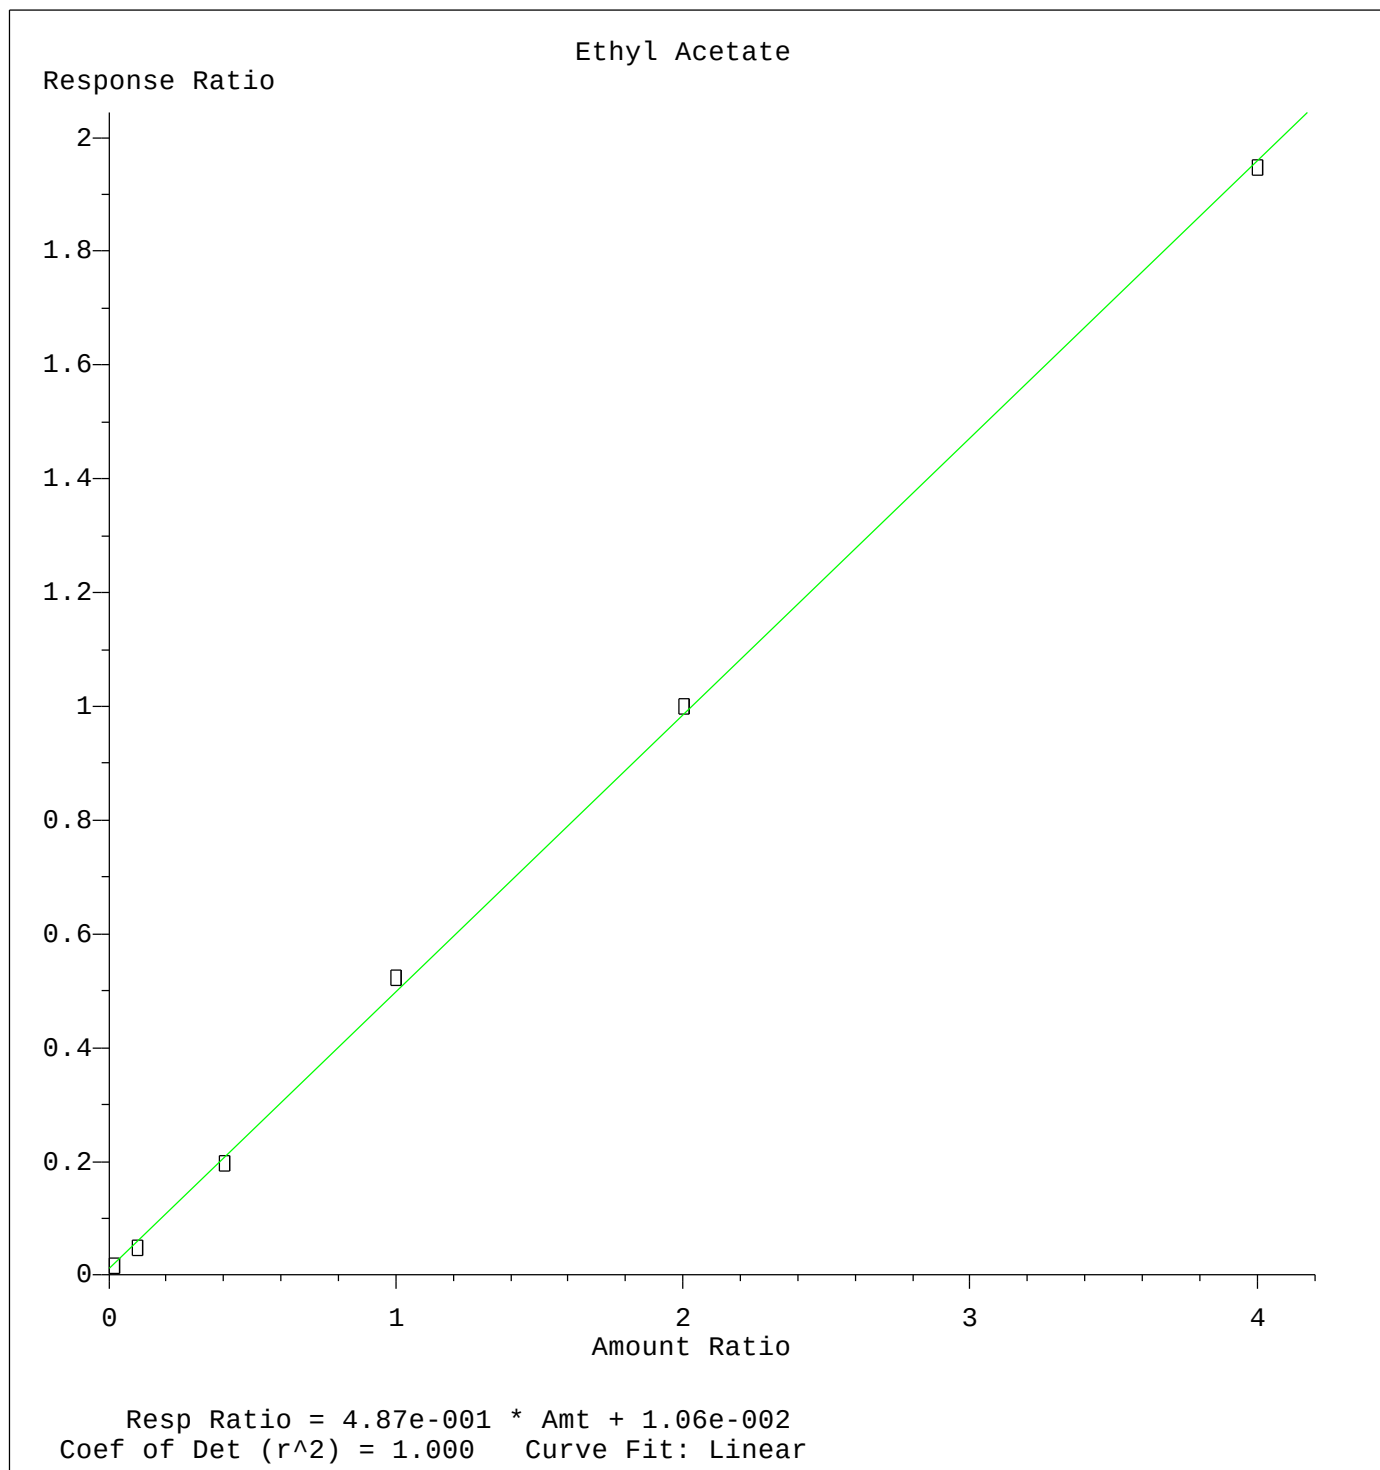

Method Name: W:\HPCHEM1\MSVOA_N\METHODS\82N091515W.M
Calibration Table Last Updated: Tue Sep 15 21:12:09 2015

1,1,2,2-Tetrachloroethane

Response Ratio

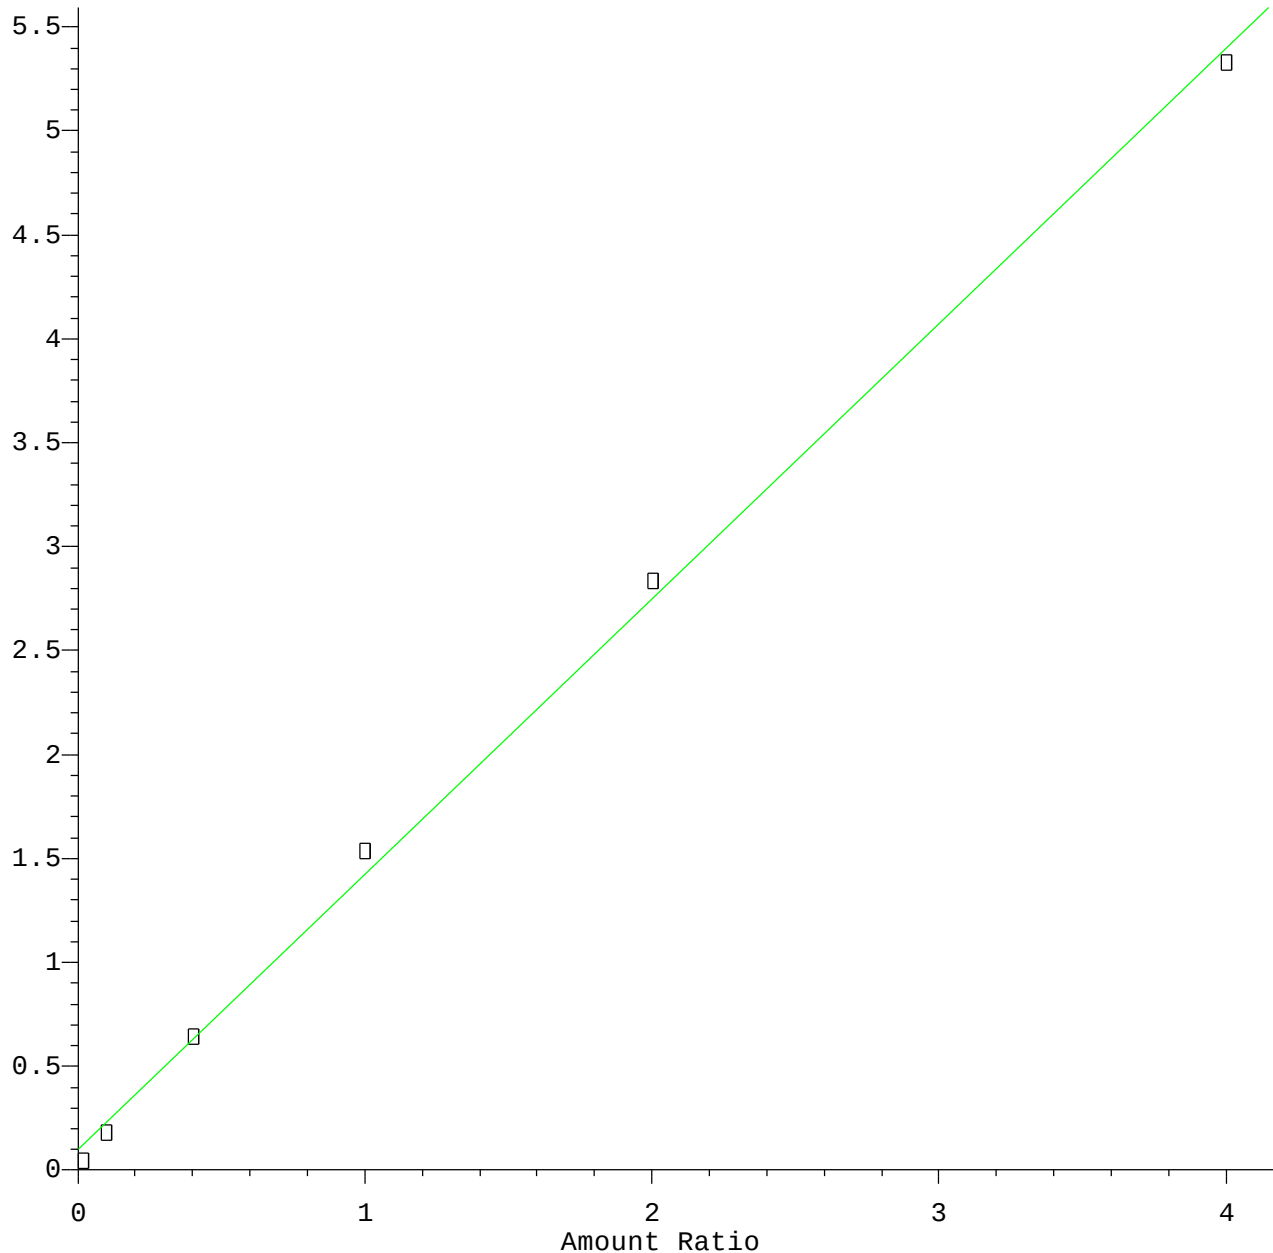


Resp Ratio = 1.32e+000 * Amt + 9.80e-002
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: W:\HPCHEM1\MSVOA_N\METHODS\82N091515W.M
Calibration Table Last Updated: Tue Sep 15 21:12:09 2015

1,2-Dibromo-3-Chloropropane

Response Ratio

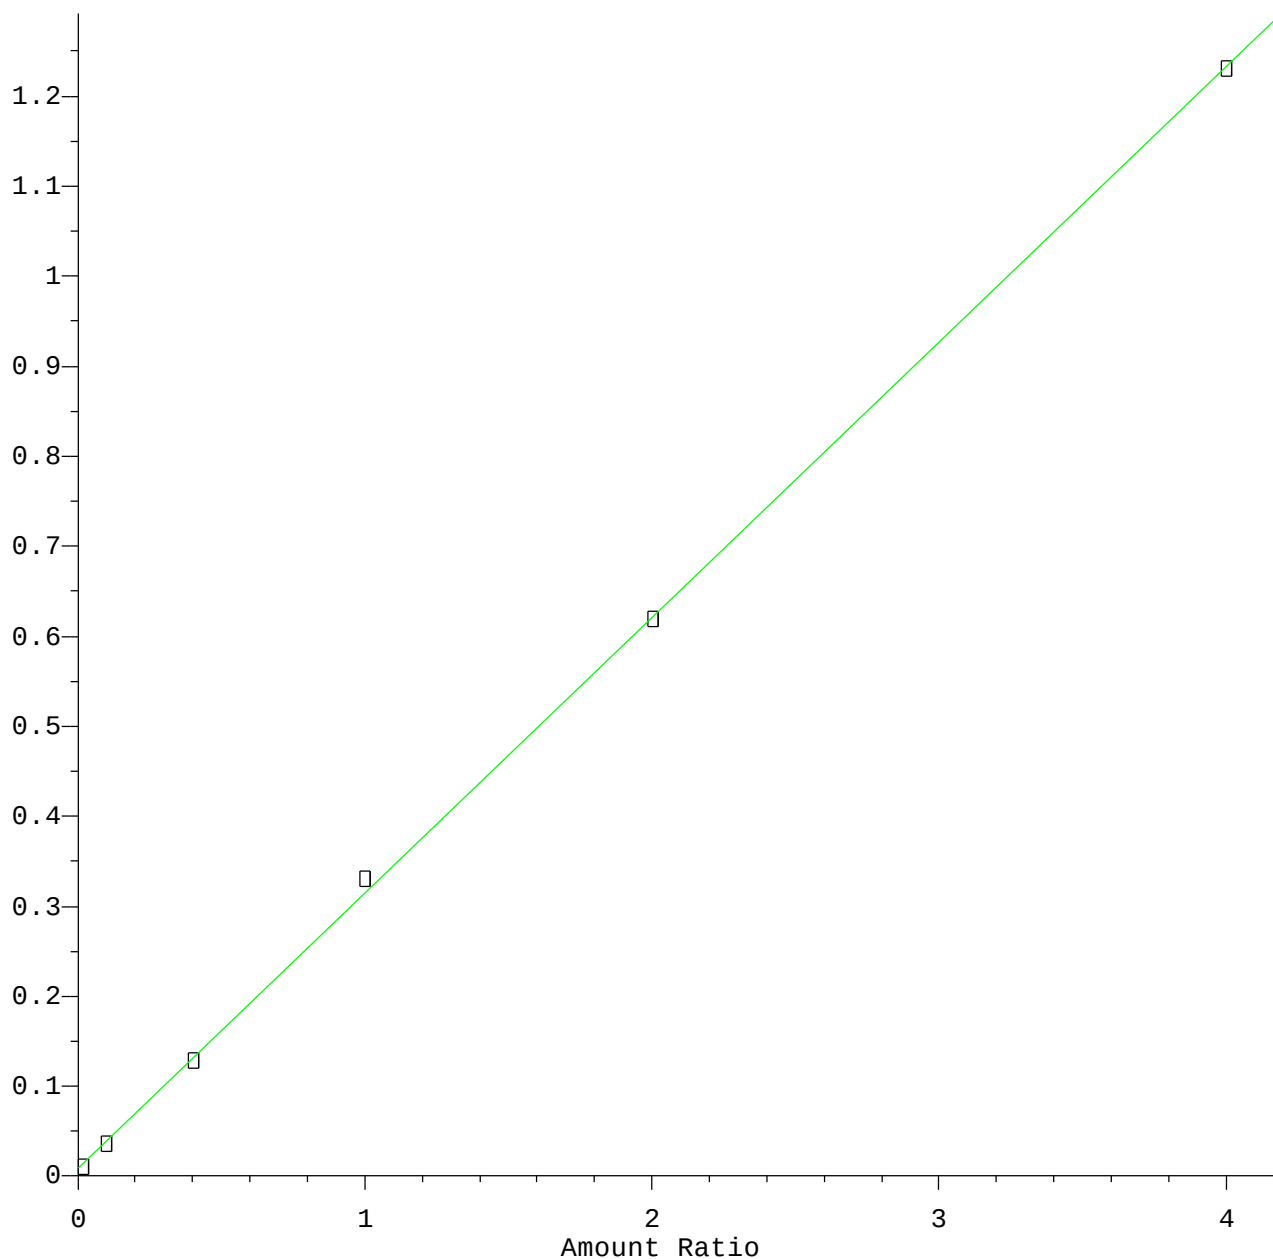

Resp Ratio = $3.06 \times 10^{-1} \times \text{Amt} + 8.67 \times 10^{-3}$
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: W:\HPCHEM1\MSVOA_N\METHODS\82N091515W.M
Calibration Table Last Updated: Tue Sep 15 21:12:09 2015