

Data Path : W:\HPCHEM1\MSVOA N\DATA\VN091515\
 Data File : VN027182.D
 Acq On : 16 Sep 2015 00:43
 Operator : MD\FY
 Sample : G3612-09
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 FIELDBLANK

Quant Time: Sep 16 03:56:24 2015
 Quant Method : W:\HPCHEM1\MSVOA_N\METHODS\82N091515W.M
 Quant Title : SW846 8260
 QLast Update : Tue Sep 15 21:12:09 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.75	168	811426	50.00	ug/l	0.00
35) 1,4-Difluorobenzene	8.68	114	1417264	50.00	ug/l	0.00
64) Chlorobenzene-d5	11.52	117	1174278	50.00	ug/l	0.00
73) 1,4-Dichlorobenzene-d4	13.47	152	408049	50.00	ug/l	0.00

System Monitoring Compounds						
34) 1,2-Dichloroethane-d4	8.12	65	784055	47.16	ug/l	0.00
Spiked Amount	50.000		Recovery	=	94.32%	
36) Dibromofluoromethane	7.68	113	511709	52.09	ug/l	0.00
Spiked Amount	50.000		Recovery	=	104.18%	
51) Toluene-d8	10.19	98	2068409	53.77	ug/l	0.00
Spiked Amount	50.000		Recovery	=	107.54%	
63) 4-Bromofluorobenzene	12.52	95	676561	49.55	ug/l	0.00
Spiked Amount	50.000		Recovery	=	99.10%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : W:\HPCHEM1\MSVOA N\DATA\VN091515\
Data File : VN027182.D
Acq On : 16 Sep 2015 00:43
Operator : MD\FY
Sample : G3612-09
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
FIELDBLANK

Quant Time: Sep 16 03:56:24 2015
Quant Method : W:\HPCHEM1\MSVOA_N\METHODS\82N091515W.M
Quant Title : SW846 8260
QLast Update : Tue Sep 15 21:12:09 2015
Response via : Initial Calibration

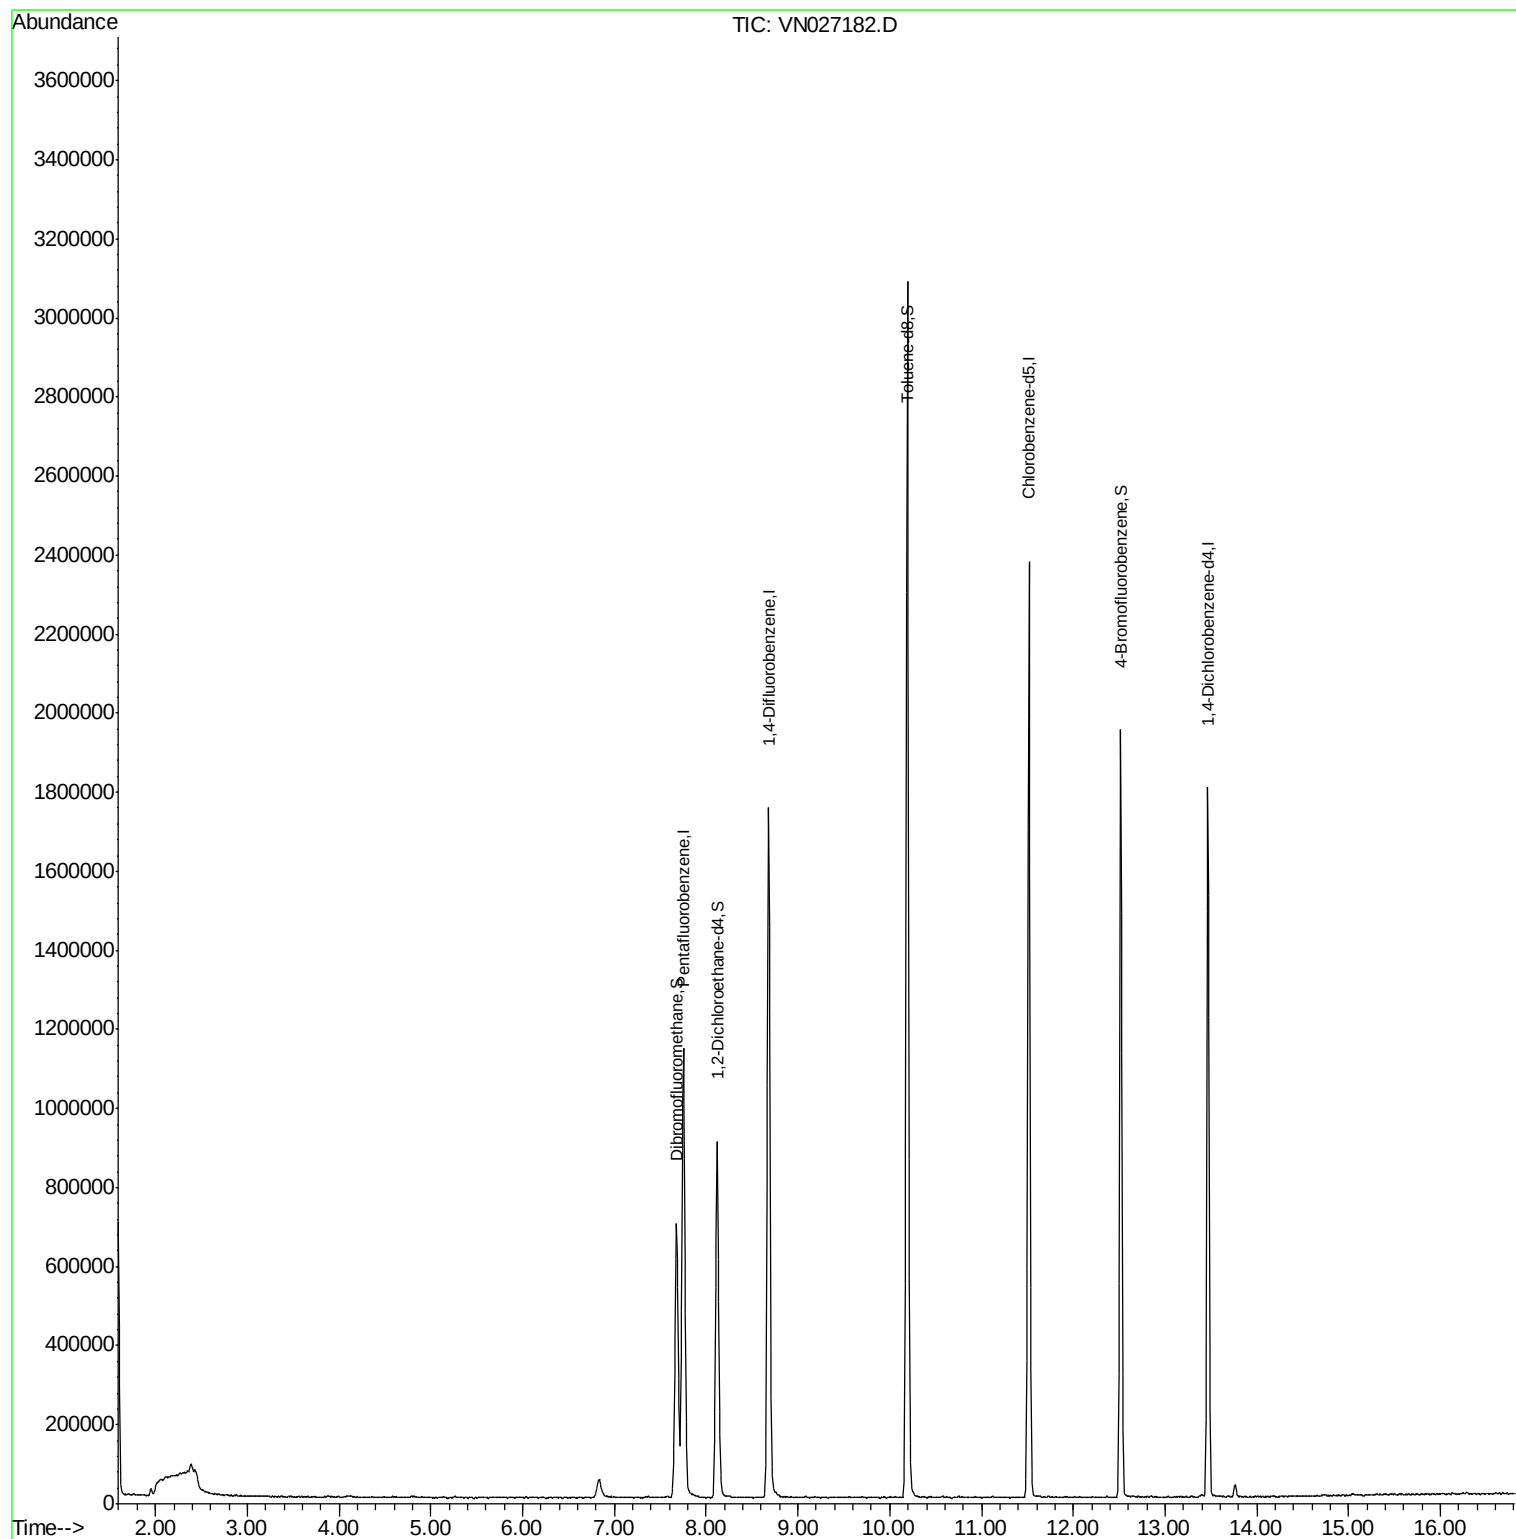

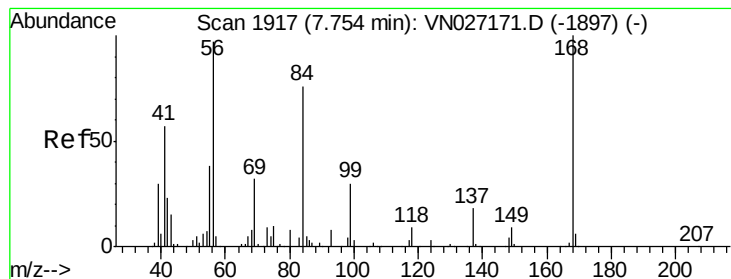

#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 7.75 min Scan# 1917

Delta R.T. 0.00 min

Lab File: VN027182.D

Acq: 16 Sep 2015 00:43

Instrument :

MSVOA_N

ClientSampleId :


FIELDBLANK

Tot Ion:168 Resp: 811426

Ion Ratio Lower Upper

168 100

99 71.5 50.4 75.6

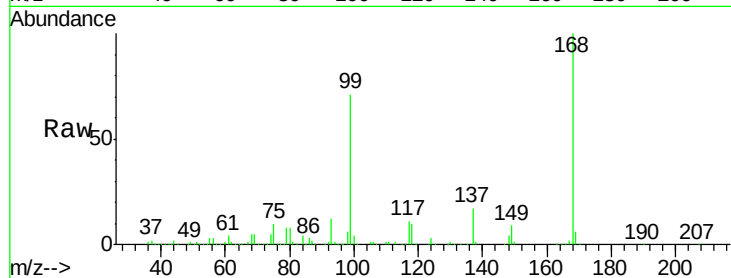

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VN

7.75



300000

200000

100000

0

Time-->

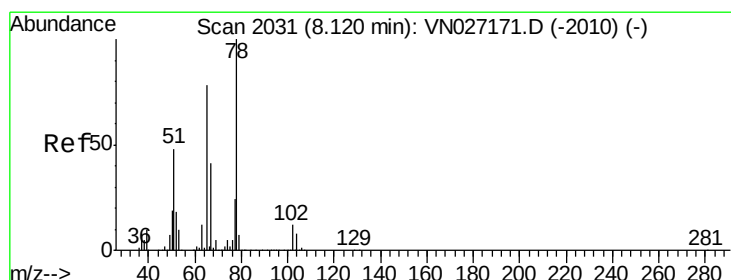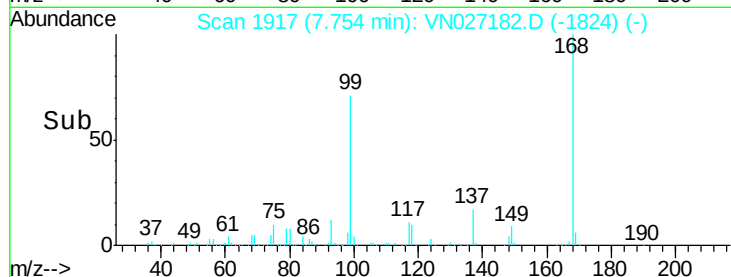

#34

1,2-Dichloroethane-d4

Concen: 47.16 ug/l

RT: 8.12 min Scan# 2031

Delta R.T. 0.00 min

Lab File: VN027182.D


Acq: 16 Sep 2015 00:43

Tgt Ion: 65 Resp: 784055

Ion Ratio Lower Upper

65 100

67 49.9 0.0 110.6

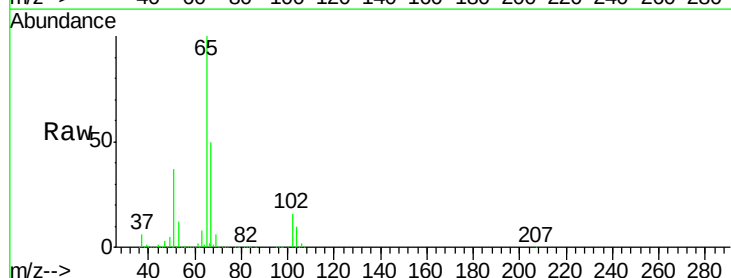

Abundance Ion 64.90 (64.60 to 65.60): VN

Ion 66.90 (66.60 to 67.60): VN

8.12


300000


200000

100000

0

Time-->

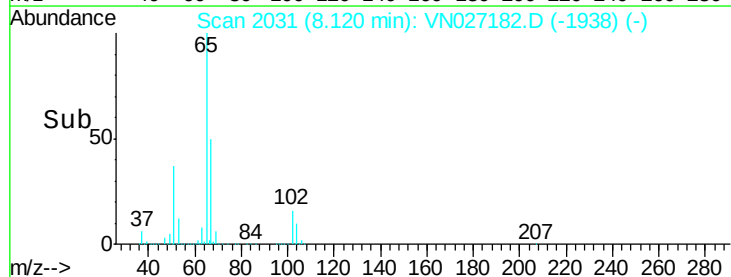


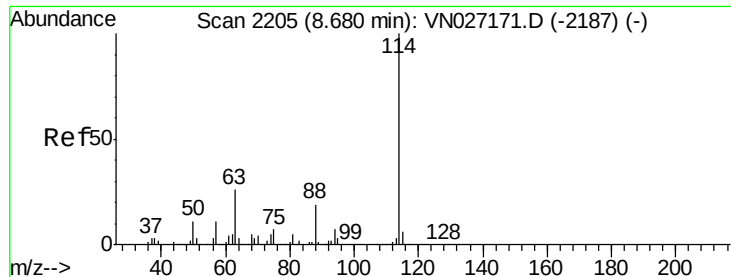




#35
 1,4-Difluorobenzene
 Concen: 50.00 ug/l
 RT: 8.68 min Scan# 2206
 Delta R.T. 0.00 min
 Lab File: VN027182.D
 Acq: 16 Sep 2015 00:43

Instrument :
 MSVOA_N
 ClientSampleId :
 FIELDBLANK

Tot Ion:114 Resp: 1417264
 Ion Ratio Lower Upper
 114 100
 63 25.8 0.0 48.8
 88 17.4 0.0 32.2

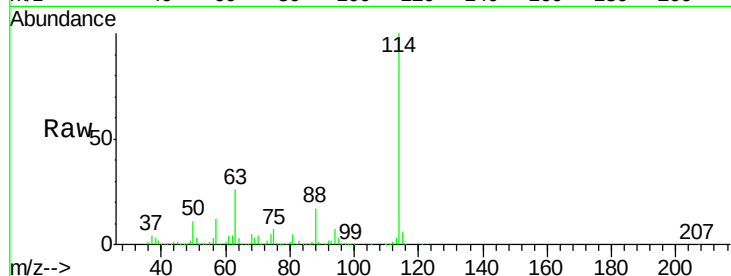


Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): V
 Ion 87.90 (87.60 to 88.60): V

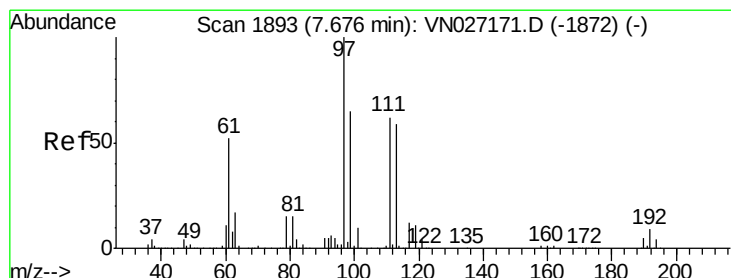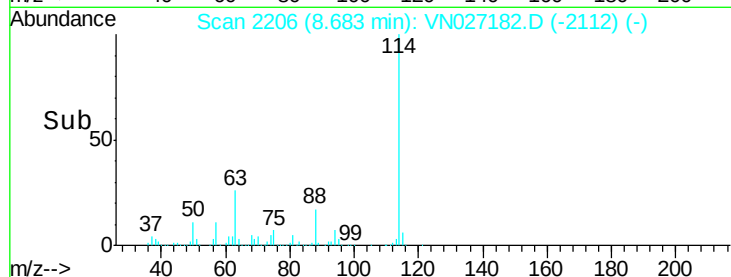
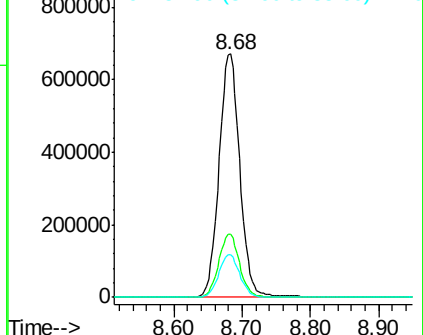



#36
 Dibromofluoromethane
 Concen: 52.09 ug/l
 RT: 7.68 min Scan# 1893
 Delta R.T. 0.00 min
 Lab File: VN027182.D
 Acq: 16 Sep 2015 00:43

Tgt Ion:113 Resp: 511709
 Ion Ratio Lower Upper
 113 100
 111 104.9 83.0 124.4
 192 16.1 14.1 21.1

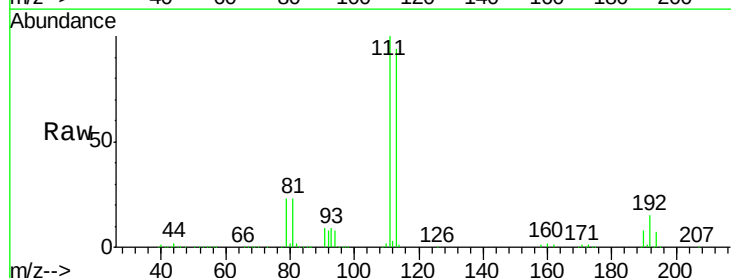

Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V

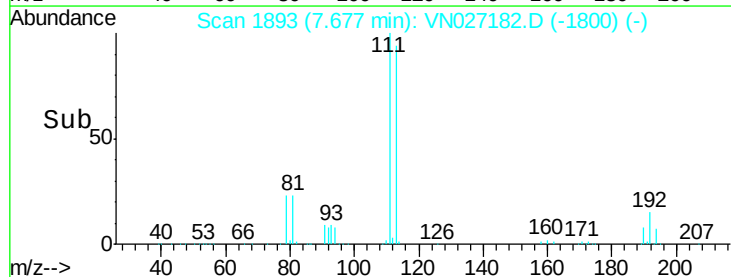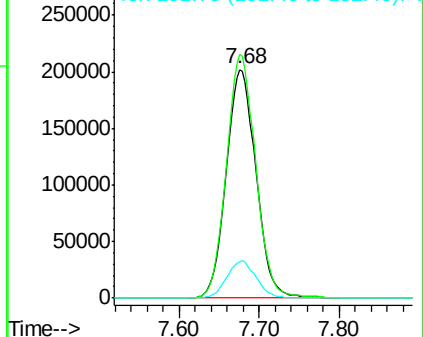

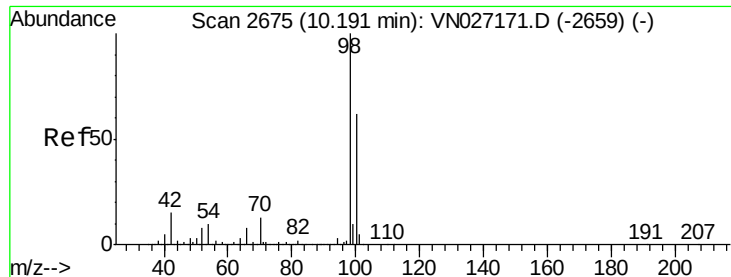

#51

Toluene-d8

Concen: 53.77 ug/l

RT: 10.19 min Scan# 2675

Delta R.T. 0.00 min

Lab File: VN027182.D

Acq: 16 Sep 2015 00:43

Instrument :

MSVOA_N

ClientSampleId :





FIELDBLANK

Tot Ion: 98 Resp: 2068409

Ion Ratio Lower Upper

98 100

100 62.9 50.5 75.7

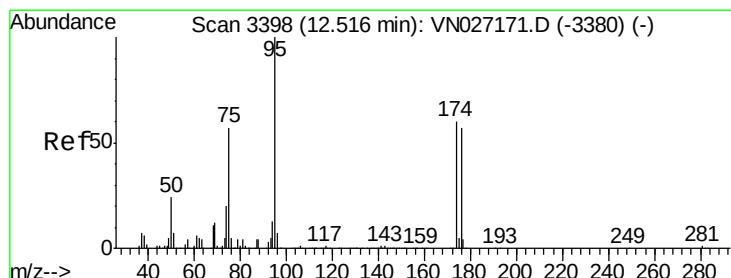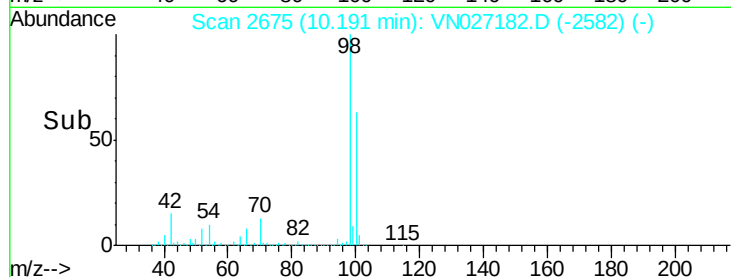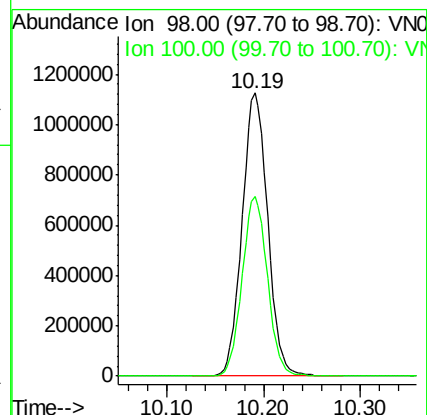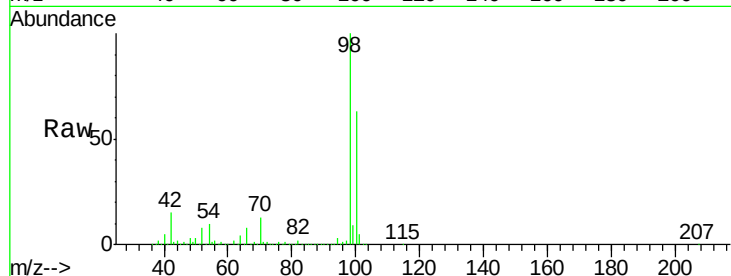

#63

4-Bromofluorobenzene

Concen: 49.55 ug/l

RT: 12.52 min Scan# 3398

Delta R.T. 0.00 min

Lab File: VN027182.D

Acq: 16 Sep 2015 00:43




Tgt Ion: 95 Resp: 676561


Ion Ratio Lower Upper

95 100

174 63.0 0.0 137.0

176 60.1 0.0 130.8


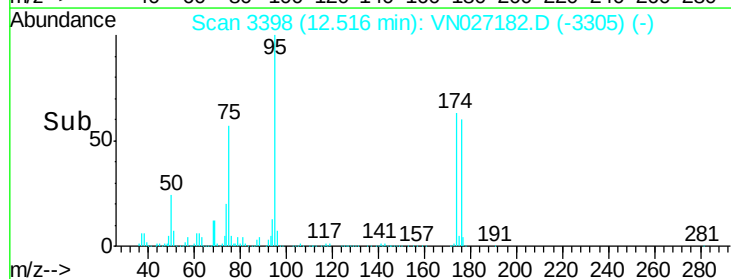
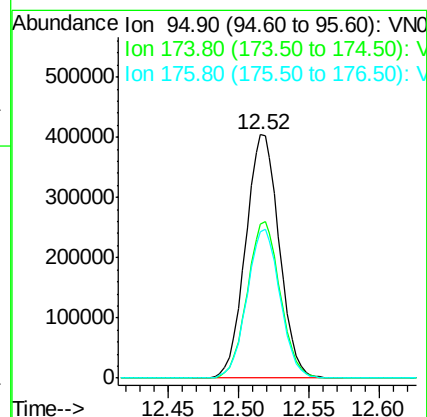
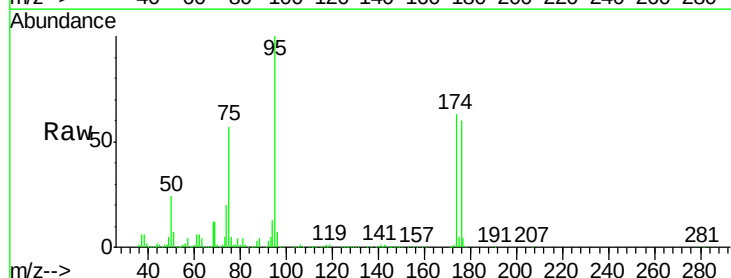


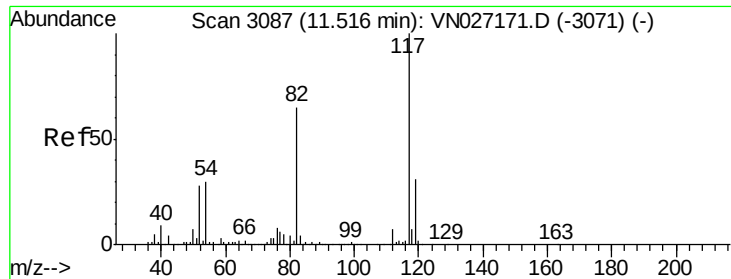

#64
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.52 min Scan# 3087
Delta R.T. 0.00 min
Lab File: VN027182.D
Acq: 16 Sep 2015 00:43

Instrument :
MSVOA_N
ClientSampleId :
FIELDBLANK

Tot Ion:117 Resp: 1174278
Ion Ratio Lower Upper
117 100
82 64.9 49.6 74.4
119 31.9 24.6 36.8

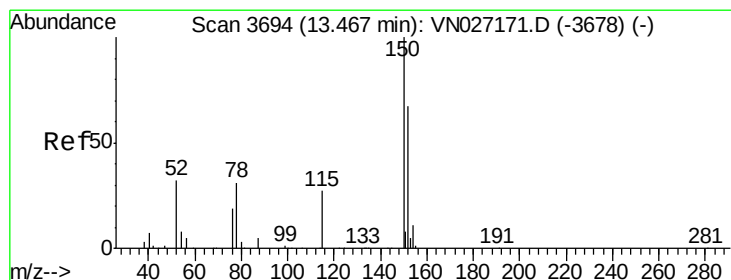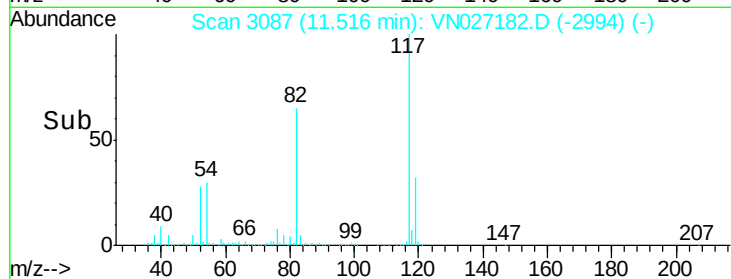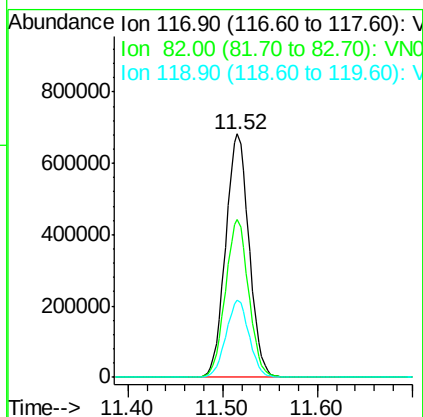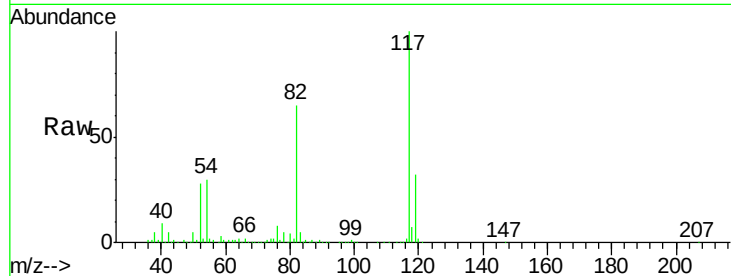

#73
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.47 min Scan# 3694
Delta R.T. 0.00 min
Lab File: VN027182.D
Acq: 16 Sep 2015 00:43

Tgt Ion:152 Resp: 408049
Ion Ratio Lower Upper
152 100
115 66.7 30.8 92.3
150 156.1 0.0 345.0

