


Data Path : W:\HPCHEM1\MSVOA N\DATA\VN091515\
Data File : VN027177.D
Acq On : 15 Sep 2015 21:29
Operator : MD\FY
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_N\METHODS\82N091515W.M
Title : SW846 8260
Last Update : Tue Sep 15 21:12:09 2015

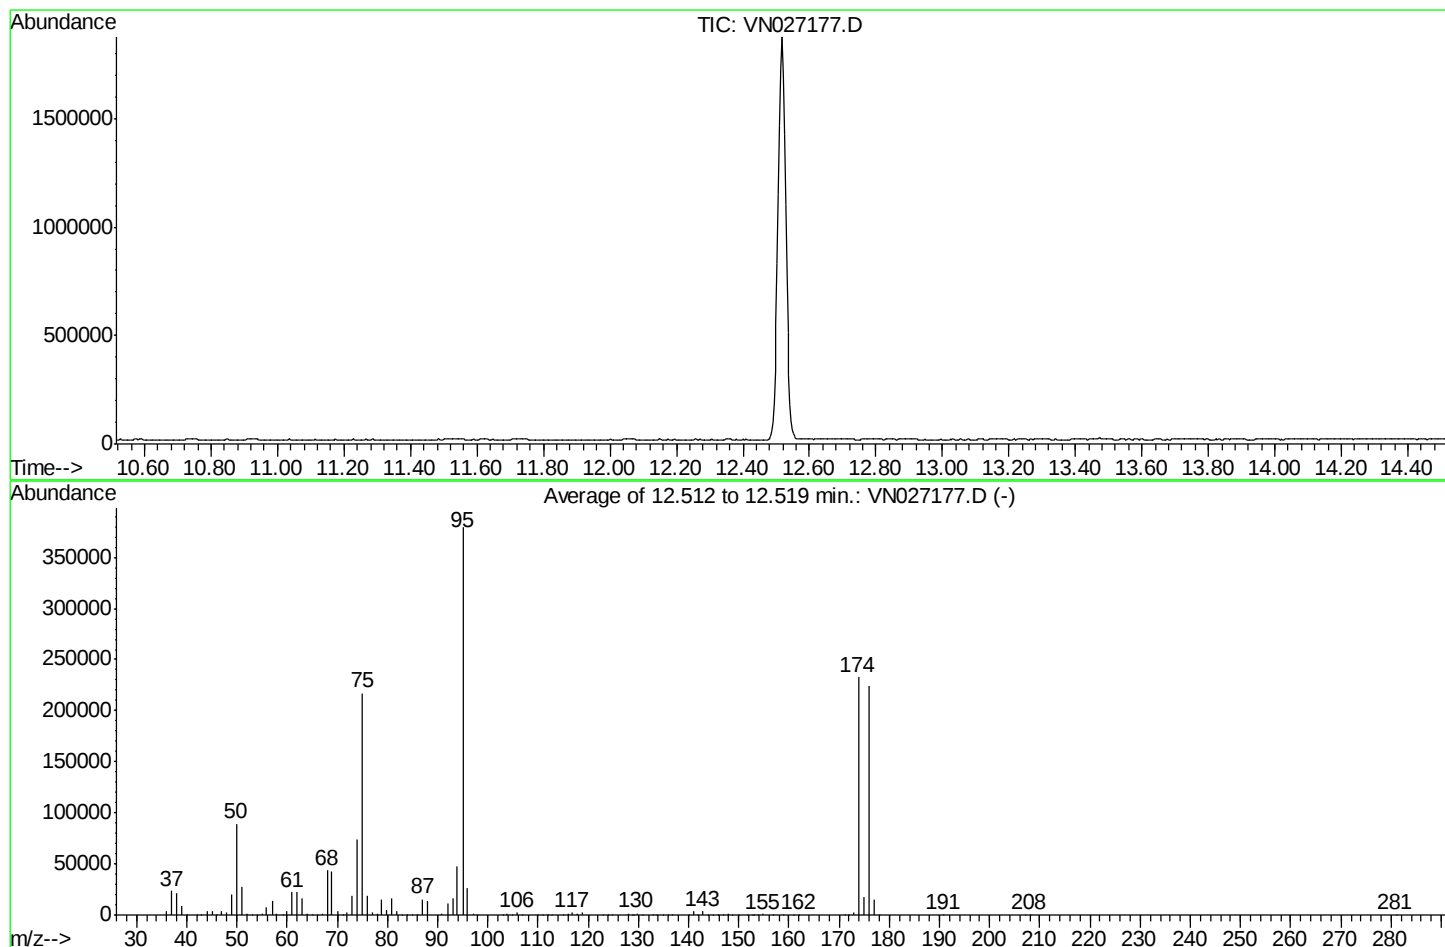

AutoFind: Scans 3397, 3398, 3399; Background Corrected with Scan 3383

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.5	89187	PASS
75	95	30	60	57.2	216874	PASS
95	95	100	100	100.0	379434	PASS
96	95	5	9	6.8	25773	PASS
173	174	0.00	2	0.9	2108	PASS
174	95	50	100	61.3	232490	PASS
175	174	5	9	7.6	17632	PASS
176	174	95	101	96.2	223744	PASS
177	176	5	9	6.6	14817	PASS