

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN091522\
 Data File : VN074491.D
 Acq On : 16 Sep 2022 04:05
 Operator : JC\MD
 Sample : N4630-22
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 WC-17-4-5

Quant Time: Sep 16 07:01:49 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N091522W.M
 Quant Title : SW846 8260
 QLast Update : Thu Sep 15 19:20:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.016	168	373776	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.904	114	720396	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.686	117	725690	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.616	152	323425	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.369	65	270608	42.669	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	85.340%		
35) Dibromofluoromethane	7.951	113	227043	47.444	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	94.880%		
50) Toluene-d8	10.381	98	830225	44.860	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	89.720%		
62) 4-Bromofluorobenzene	12.675	95	327626	51.687	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	103.380%		
Target Compounds						Qvalue
3) Chloromethane	2.263	50	1428	0.466	ug/l #	78
6) Chloroethane	2.740	64	14795	2.958	ug/l #	61
12) 1,1-Dichloroethene	4.110	96	223	0.729	ug/l #	1
13) Acrolein	3.987	56	876	1.161	ug/l #	71
16) Acetone	4.222	43	118528	29.207	ug/l #	88
17) Carbon Disulfide	4.457	76	39230	2.906	ug/l #	92
18) Methyl Acetate	4.781	43	13920	1.104	ug/l #	66
20) Methylene Chloride	5.010	84	22052	3.588	ug/l #	88
21) trans-1,2-Dichloroethene	5.522	96	149	0.456	ug/l #	44
25) 2-Butanone	7.263	43	29241	4.340	ug/l #	82
28) Bromochloromethane	7.757	49	57	Below Cal	#	8
29) Tetrahydrofuran	7.628	42	5412	1.222	ug/l #	73
31) Cyclohexane	8.016	56	12204	1.084	ug/l #	42
36) 1,1-Dichloropropene	8.016	75	36640	4.326	ug/l #	48
37) Ethyl Acetate	7.334	43	62010	4.740	ug/l #	90
38) Carbon Tetrachloride	8.016	117	40043	5.120	ug/l #	15
42) 1,2-Dichloroethane	8.469	62	1897	0.211	ug/l #	74
43) Isopropyl Acetate	8.498	43	219567	10.716	ug/l #	85
48) Methyl methacrylate	9.486	41	12608	1.388	ug/l #	38
49) 1,4-Dioxane	9.510	88	143	0.819	ug/l #	25
51) 4-Methyl-2-Pentanone	10.269	43	24570	1.836	ug/l #	79
54) cis-1,3-Dichloropropene	10.186	75	59898	5.433	ug/l #	75
57) 1,3-Dichloropropane	11.028	76	5186	0.455	ug/l #	44
59) 2-Hexanone	10.998	43	362357	35.475	ug/l #	21
68) m/p-Xylenes	11.898	106	4542	0.367	ug/l	91
69) o-Xylene	12.227	106	5135	0.407	ug/l	68
76) 1,2,3-Trichloropropane	12.675	75	194130	19.500	ug/l #	1
79) 2-Chlorotoluene	12.951	91	9952	0.423	ug/l	94
81) trans-1,4-Dichloro-2-b...	12.675	75	194130	42.088	ug/l #	10
84) 1,2,4-Trimethylbenzene	13.316	105	11392	0.419	ug/l	98
95) Naphthalene	15.439	128	8131	1.873	ug/l #	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN091522\
Data File : VN074491.D
Acq On : 16 Sep 2022 04:05
Operator : JC\MD
Sample : N4630-22
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
WC-17-4-5

Quant Time: Sep 16 07:01:49 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N091522W.M
Quant Title : SW846 8260
QLast Update : Thu Sep 15 19:20:33 2022
Response via : Initial Calibration




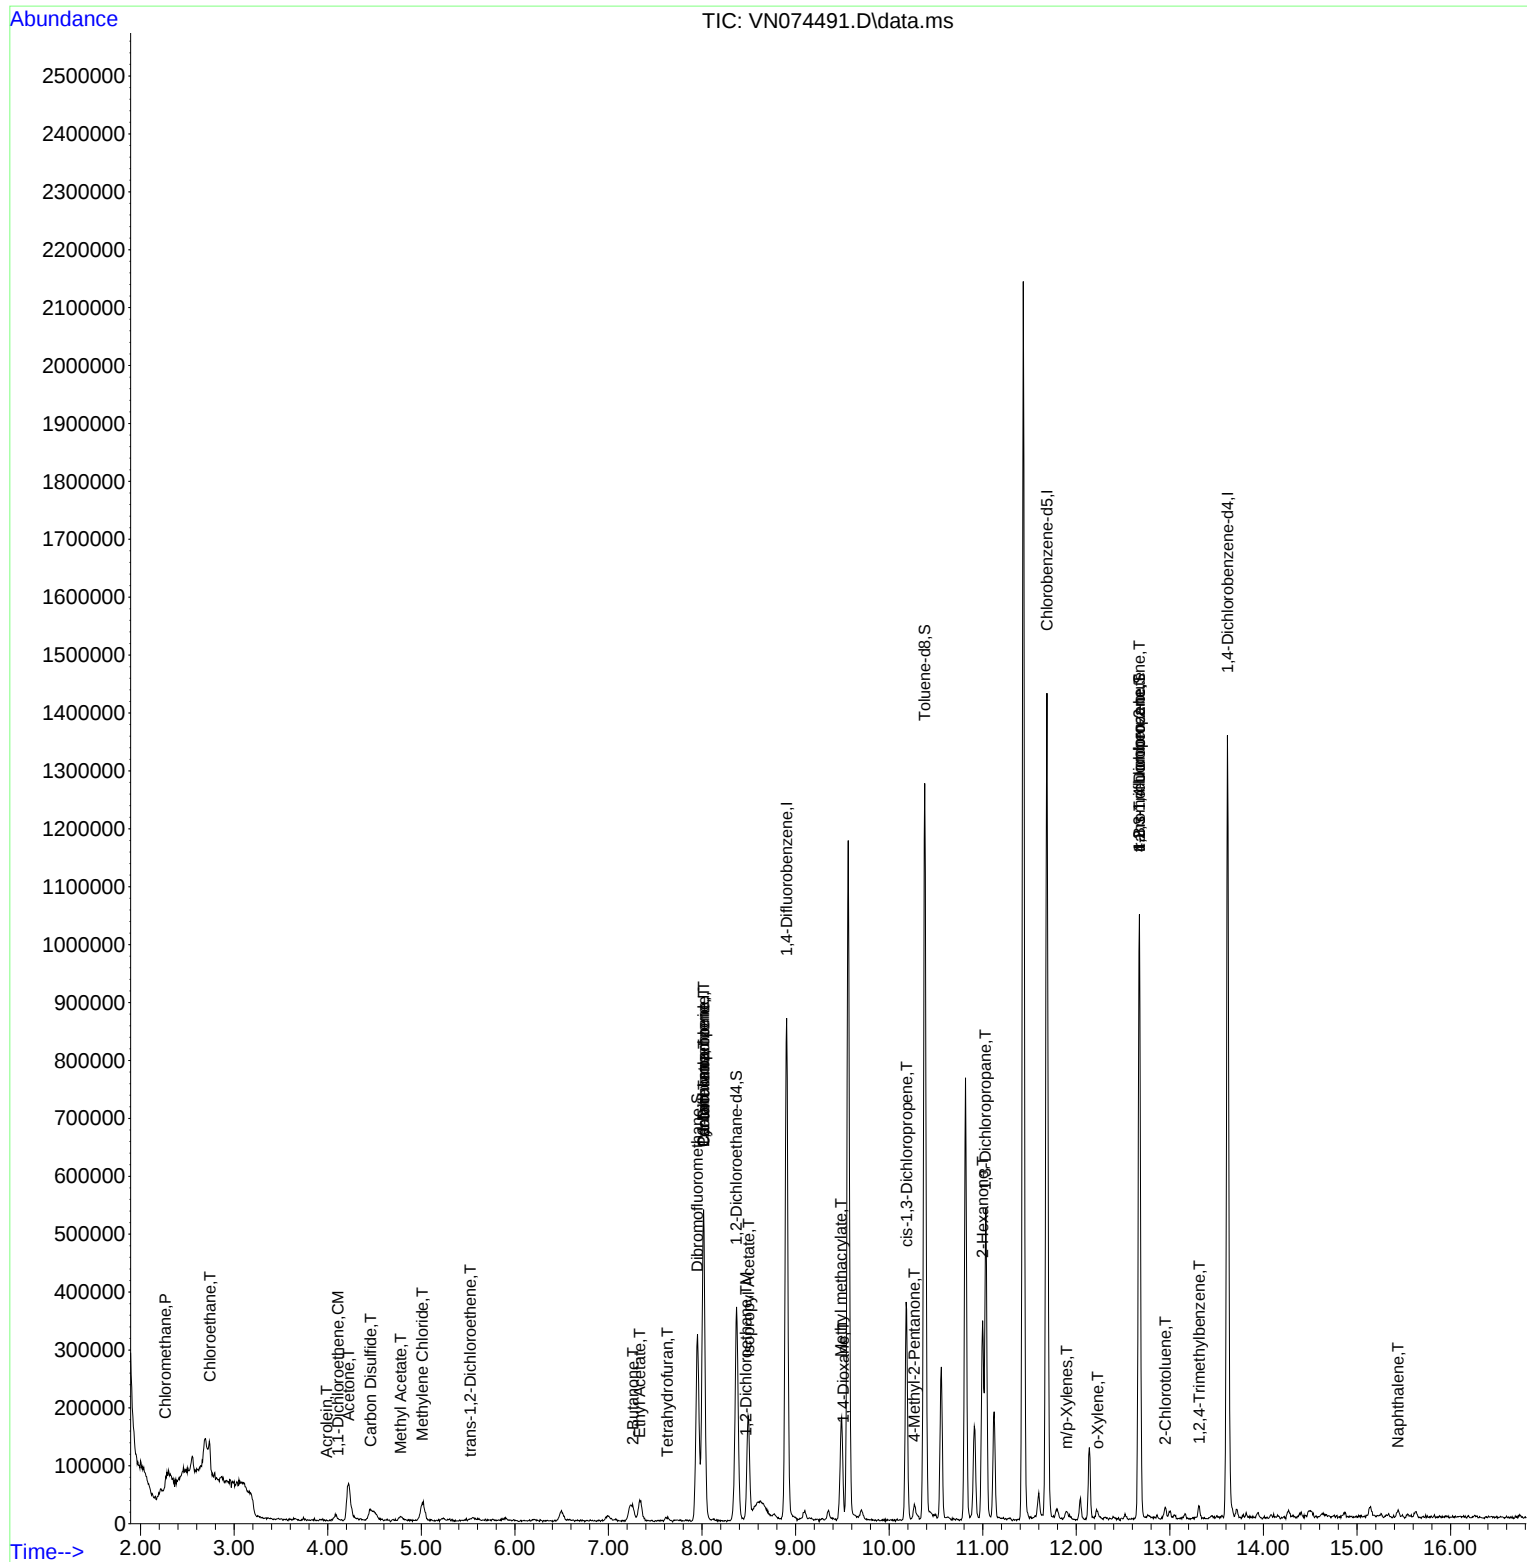




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.016 min Scan# 1042
Delta R.T. -0.000 min
Lab File: VN074491.D
Acq: 16 Sep 2022 04:05




Instrument :
MSVOA_N
ClientSampleId :
WC-17-4-5


Tgt Ion:168 Resp: 373776
Ion Ratio Lower Upper
168 100
99 60.4 42.3 63.5

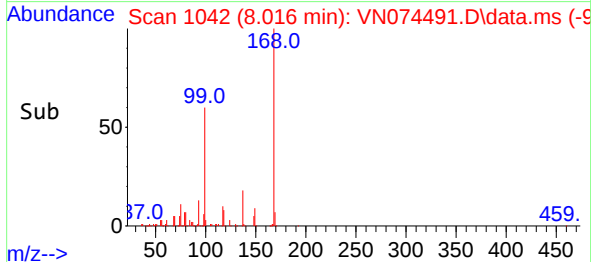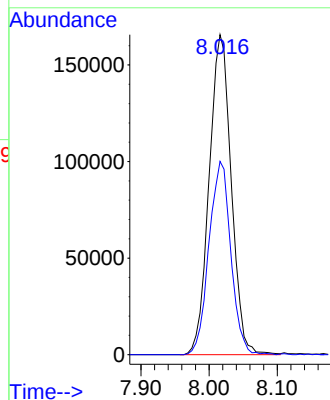

#3
Chloromethane
Concen: 0.466 ug/l
RT: 2.263 min Scan# 64
Delta R.T. 0.000 min
Lab File: VN074491.D
Acq: 16 Sep 2022 04:05

Tgt Ion: 50 Resp: 1428
Ion Ratio Lower Upper
50 100
52 44.4 25.7 38.5#


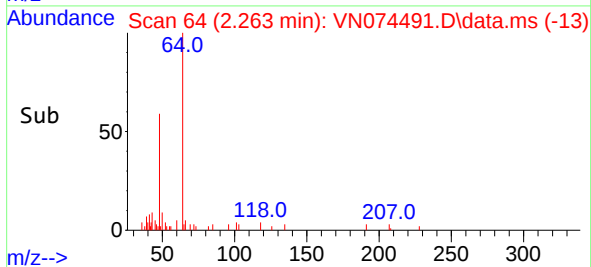
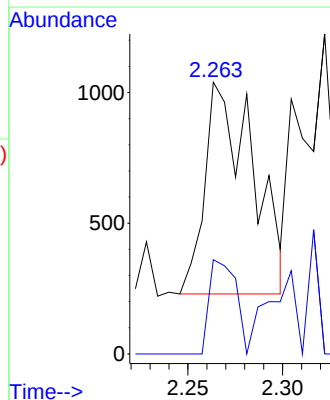
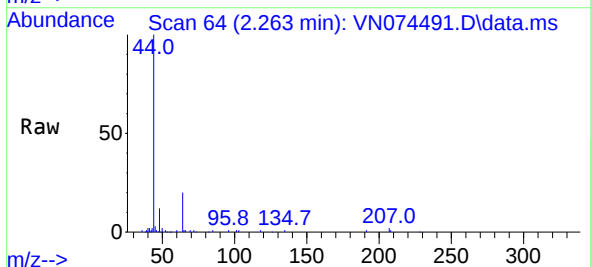




#6
Chloroethane
Concen: 2.958 ug/l
RT: 2.740 min Scan# 14
Delta R.T. -0.211 min
Lab File: VN074491.D
Acq: 16 Sep 2022 04:05




Instrument :
MSVOA_N
ClientSampleId :
WC-17-4-5


Tgt Ion: 64 Resp: 14795
Ion Ratio Lower Upper
64 100
66 11.1 26.2 39.4#



#12
1,1-Dichloroethene
Concen: 0.729 ug/l
RT: 4.110 min Scan# 378
Delta R.T. 0.006 min
Lab File: VN074491.D
Acq: 16 Sep 2022 04:05

Tgt Ion: 96 Resp: 223
Ion Ratio Lower Upper
96 100
61 0.0 127.6 191.4#
98 0.0 51.2 76.8#


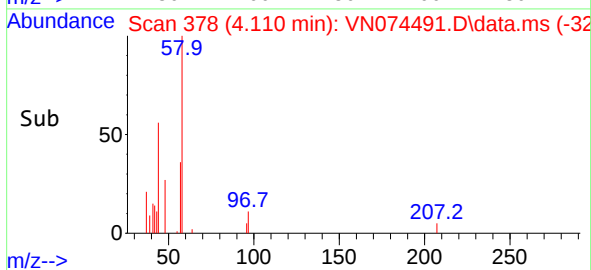






#13
Acrolein
Concen: 1.161 ug/l
RT: 3.987 min Scan# 31
Delta R.T. 0.012 min
Lab File: VN074491.D
Acq: 16 Sep 2022 04:05




Instrument :
MSVOA_N
ClientSampleId :
WC-17-4-5


Tgt Ion: 56 Resp: 876
Ion Ratio Lower Upper
56 100
55 45.2 54.8 82.2#

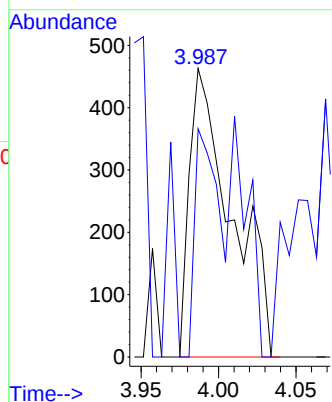

#16
Acetone
Concen: 29.207 ug/l
RT: 4.222 min Scan# 397
Delta R.T. 0.006 min
Lab File: VN074491.D
Acq: 16 Sep 2022 04:05

Tgt Ion: 43 Resp: 118528
Ion Ratio Lower Upper
43 100
58 25.9 26.0 39.0#


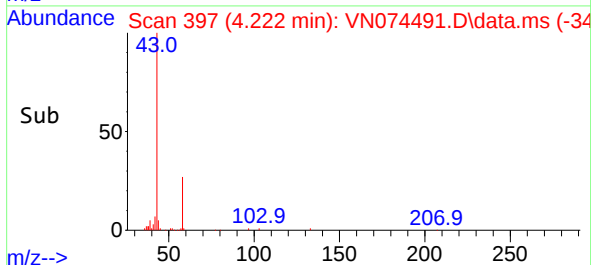

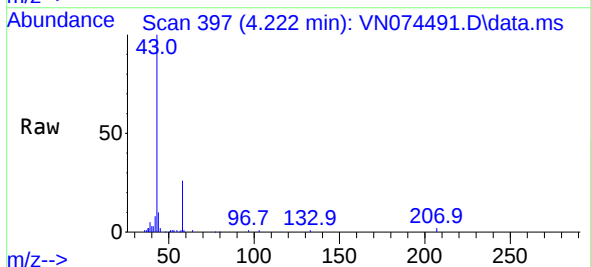




#17
Carbon Disulfide
Concen: 2.906 ug/l
RT: 4.457 min Scan# 41
Delta R.T. 0.000 min
Lab File: VN074491.D
Acq: 16 Sep 2022 04:05




Instrument :
MSVOA_N
ClientSampleId :
WC-17-4-5


Tgt Ion: 76 Resp: 39230
Ion Ratio Lower Upper
76 100
78 12.0 7.2 10.8#

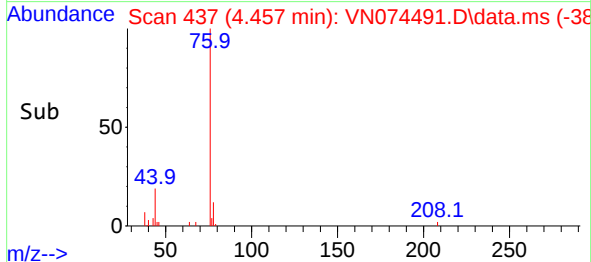

#18
Methyl Acetate
Concen: 1.104 ug/l
RT: 4.781 min Scan# 492
Delta R.T. 0.012 min
Lab File: VN074491.D
Acq: 16 Sep 2022 04:05

Tgt Ion: 43 Resp: 13920
Ion Ratio Lower Upper
43 100
74 9.3 21.6 32.4#


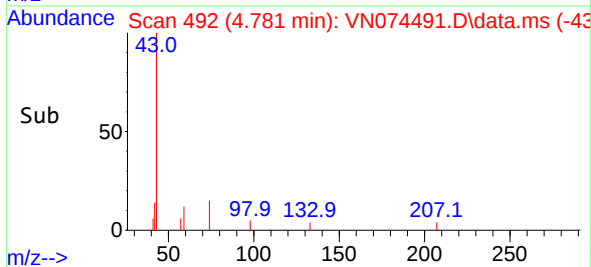

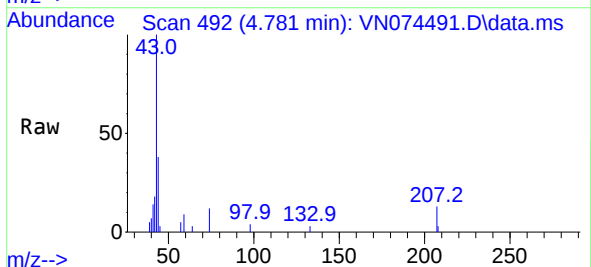




#20
Methylene Chloride
Concen: 3.588 ug/l
RT: 5.010 min Scan# 51
Delta R.T. 0.000 min
Lab File: VN074491.D
Acq: 16 Sep 2022 04:05




Instrument :
MSVOA_N
ClientSampleId :
WC-17-4-5


Tgt Ion:	84	Resp:	22052
Ion	Ratio	Lower	Upper
84	100		
49	109.9	88.3	132.5
51	27.7	28.2	42.2#
86	39.9	50.6	76.0#

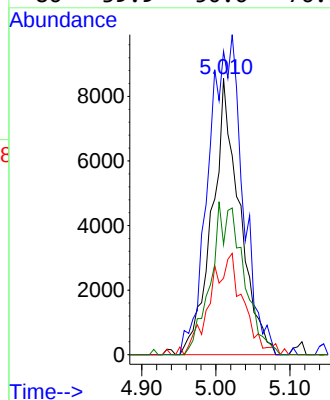

#21
trans-1,2-Dichloroethene
Concen: 0.456 ug/l
RT: 5.522 min Scan# 618
Delta R.T. 0.018 min
Lab File: VN074491.D
Acq: 16 Sep 2022 04:05

Tgt Ion:	96	Resp:	149
Ion	Ratio	Lower	Upper
96	100		
61	81.3	105.8	158.8#
98	0.0	50.3	75.5#

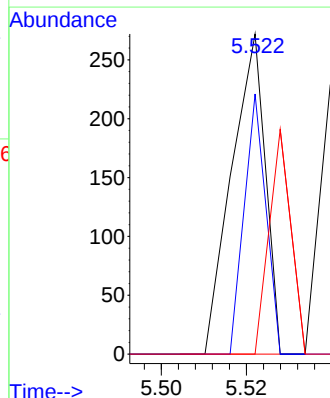



#25

2-Butanone

Concen: 4.340 ug/l

RT: 7.263 min Scan# 913

Delta R.T. 0.006 min

Lab File: VN074491.D

Acq: 16 Sep 2022 04:05

Instrument :

MSVOA_N

ClientSampleId :





WC-17-4-5

Tgt Ion: 43 Resp: 29241

Ion Ratio Lower Upper

43 100

72 20.1 23.7 35.5#

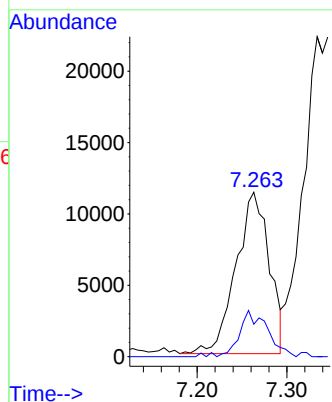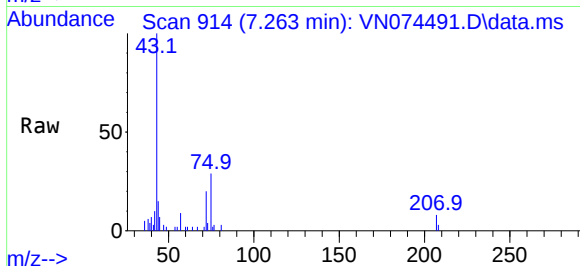

#29

Tetrahydrofuran

Concen: 1.222 ug/l

RT: 7.628 min Scan# 976

Delta R.T. 0.024 min

Lab File: VN074491.D

Acq: 16 Sep 2022 04:05




Tgt Ion: 42 Resp: 5412


Ion Ratio Lower Upper

42 100

72 32.4 39.7 59.5#

71 26.8 36.6 55.0#


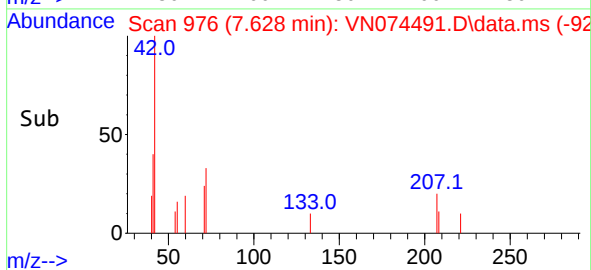

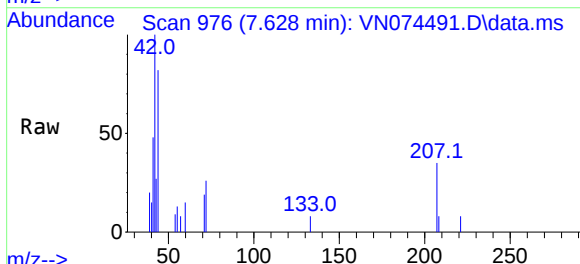




#31
Cyclohexane
Concen: 1.084 ug/l
RT: 8.016 min Scan# 1042
Delta R.T. -0.006 min
Lab File: VN074491.D
Acq: 16 Sep 2022 04:05




Instrument :
MSVOA_N
ClientSampleId :
WC-17-4-5


Tgt Ion: 56 Resp: 12204
Ion Ratio Lower Upper
56 100
69 146.2 27.8 41.8#
84 105.3 76.9 115.3

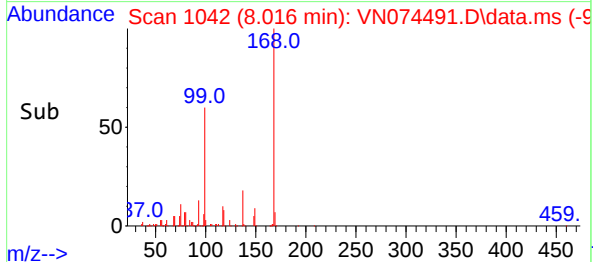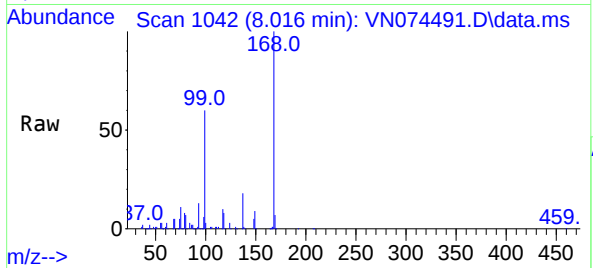

#33
1,2-Dichloroethane-d4
Concen: 42.669 ug/l
RT: 8.369 min Scan# 1102
Delta R.T. -0.000 min
Lab File: VN074491.D
Acq: 16 Sep 2022 04:05

Tgt Ion: 65 Resp: 270608
Ion Ratio Lower Upper
65 100
67 53.5 0.0 104.8

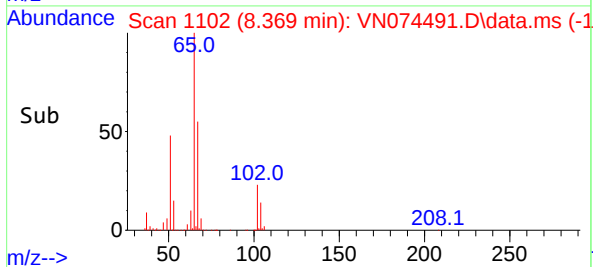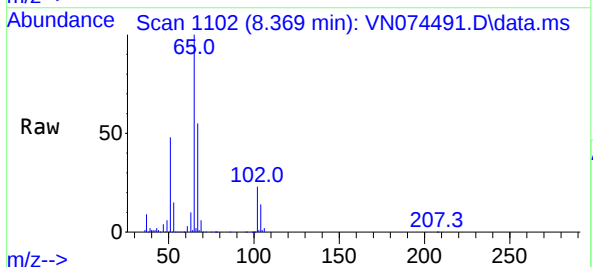







#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.904 min Scan# 1193
Delta R.T. 0.000 min
Lab File: VN074491.D
Acq: 16 Sep 2022 04:05

Instrument :
MSVOA_N
ClientSampleId :
WC-17-4-5

Tgt Ion:114 Resp: 720396




Ion	Ratio	Lower	Upper
114	100		
63	23.9	0.0	40.0
88	15.6	0.0	32.6

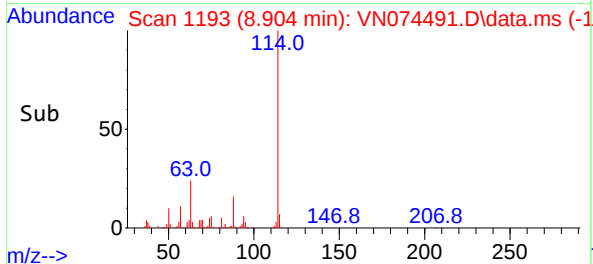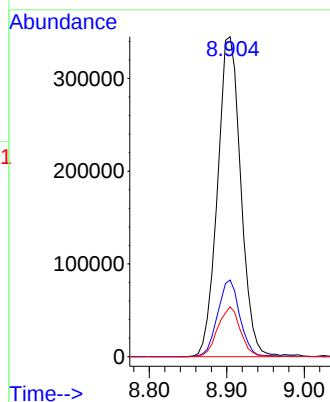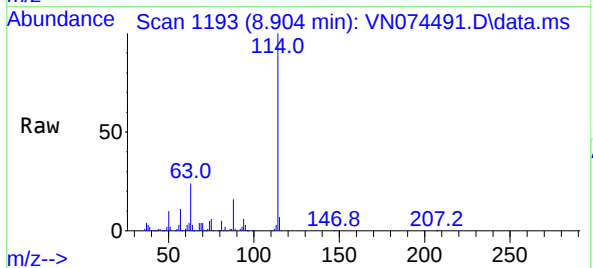


#35
Dibromofluoromethane
Concen: 47.444 ug/l
RT: 7.951 min Scan# 1031
Delta R.T. 0.000 min
Lab File: VN074491.D
Acq: 16 Sep 2022 04:05

Tgt Ion:113 Resp: 227043

Ion	Ratio	Lower	Upper
113	100		
111	103.8	81.4	122.0
192	15.8	17.0	25.6


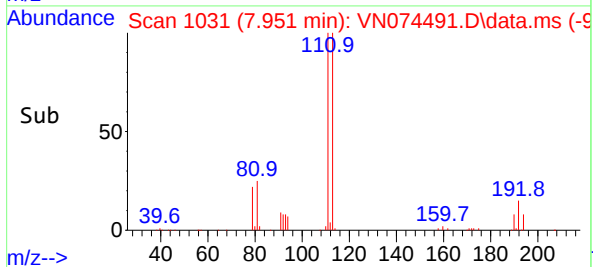
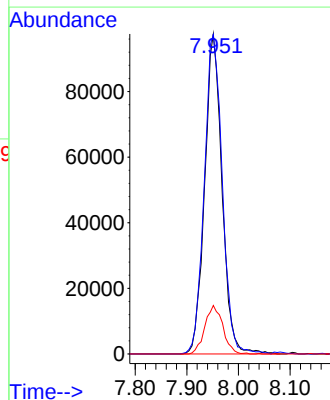
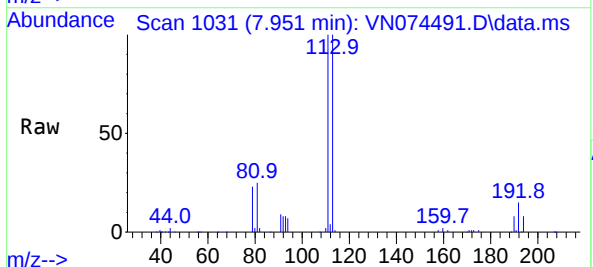




#36
1,1-Dichloropropene
Concen: 4.326 ug/l
RT: 8.016 min Scan# 1042
Delta R.T. -0.135 min
Lab File: VN074491.D
Acq: 16 Sep 2022 04:05




Instrument :
MSVOA_N
ClientSampleId :
WC-17-4-5


Tgt Ion: 75 Resp: 36640
Ion Ratio Lower Upper
75 100
110 8.3 18.3 54.8#
77 0.2 25.1 37.7#

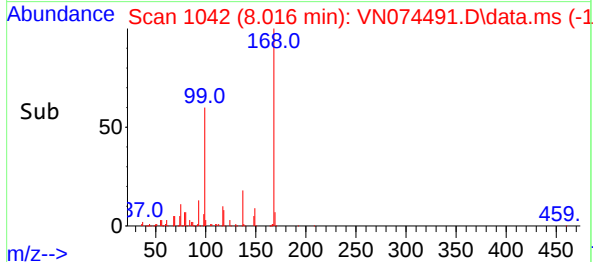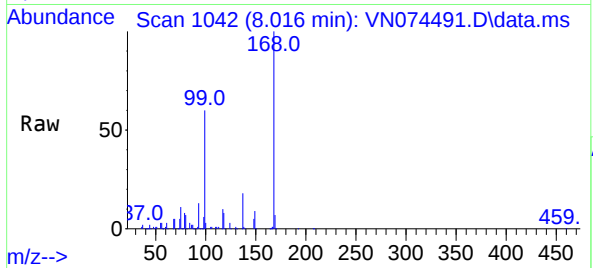

#37
Ethyl Acetate
Concen: 4.740 ug/l
RT: 7.334 min Scan# 926
Delta R.T. -0.000 min
Lab File: VN074491.D
Acq: 16 Sep 2022 04:05

Tgt Ion: 43 Resp: 62010
Ion Ratio Lower Upper
43 100
61 13.0 11.8 17.6
70 5.1 9.3 13.9#


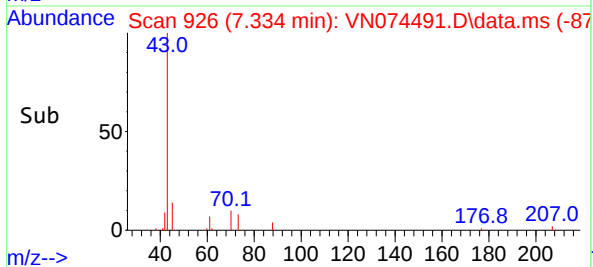

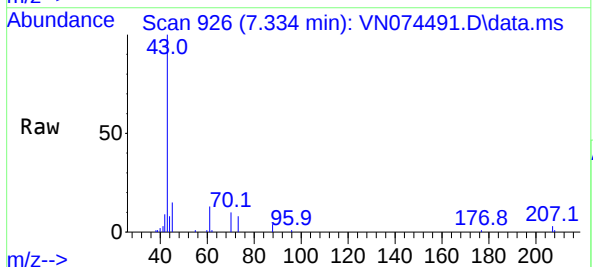




#38
Carbon Tetrachloride
Concen: 5.120 ug/l
RT: 8.016 min Scan# 1042
Delta R.T. -0.117 min
Lab File: VN074491.D
Acq: 16 Sep 2022 04:05




Instrument :
MSVOA_N
ClientSampleId :
WC-17-4-5


Tgt Ion:117 Resp: 40043
Ion Ratio Lower Upper
117 100
119 3.6 75.8 113.8#
121 0.0 24.6 37.0#

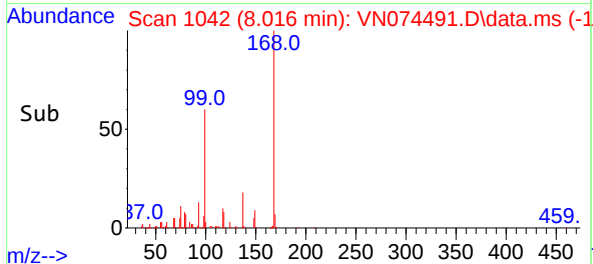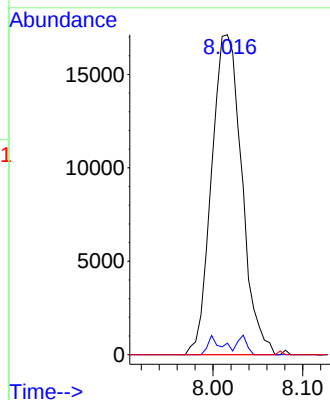

#42
1,2-Dichloroethane
Concen: 0.211 ug/l
RT: 8.469 min Scan# 1119
Delta R.T. 0.006 min
Lab File: VN074491.D
Acq: 16 Sep 2022 04:05

Tgt Ion: 62 Resp: 1897
Ion Ratio Lower Upper
62 100
98 0.0 0.0 19.4

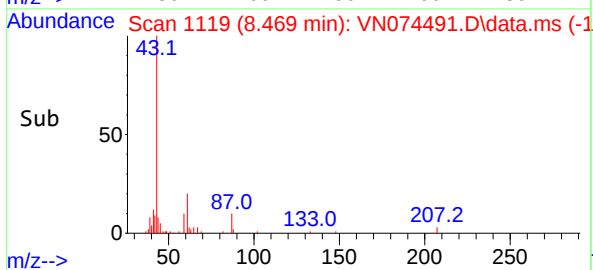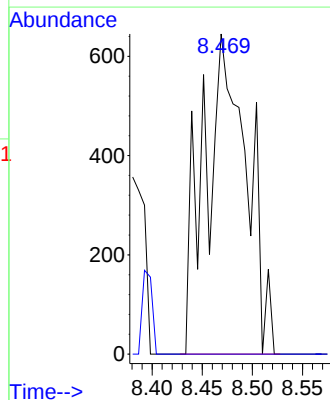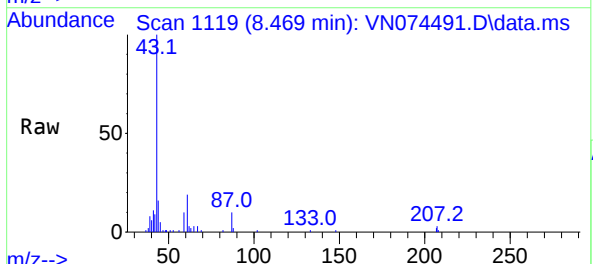




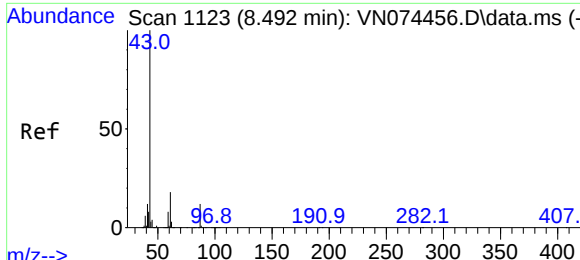


#43
Isopropyl Acetate
Concen: 10.716 ug/l
RT: 8.498 min Scan# 1123
Delta R.T. 0.006 min
Lab File: VN074491.D
Acq: 16 Sep 2022 04:05

Instrument : MSVOA_N
ClientSampleId : WC-17-4-5

Tgt Ion: 43 Resp: 219567




Ion	Ratio	Lower	Upper
43	100		
61	17.5	21.9	32.9#
87	11.8	12.0	18.0#

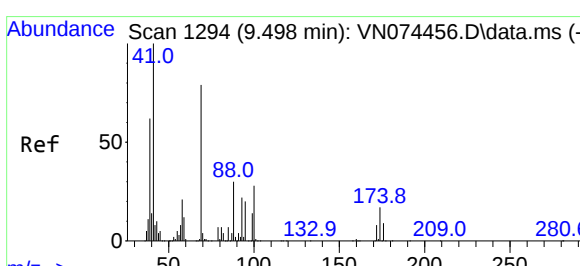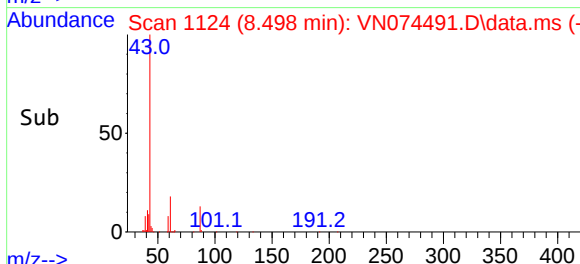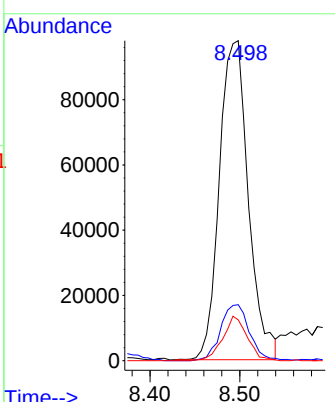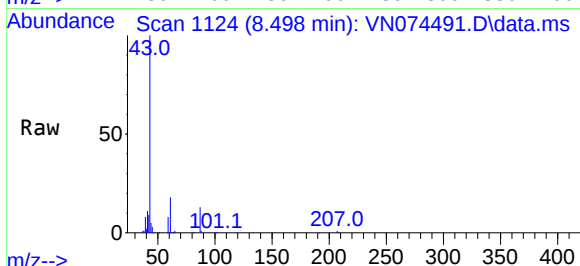


#48
Methyl methacrylate
Concen: 1.388 ug/l
RT: 9.486 min Scan# 1292
Delta R.T. -0.012 min
Lab File: VN074491.D
Acq: 16 Sep 2022 04:05

Tgt Ion: 41 Resp: 12608

Ion	Ratio	Lower	Upper
41	100		
69	0.0	74.7	112.1#
39	52.9	45.6	68.4


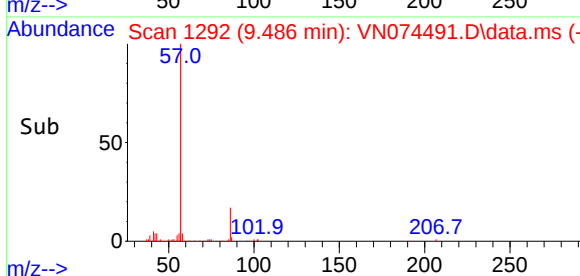
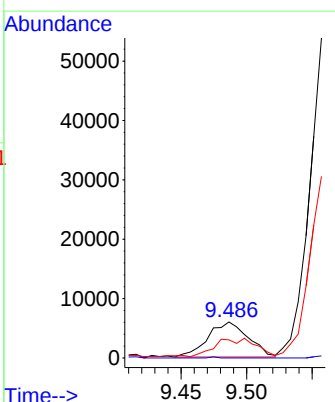
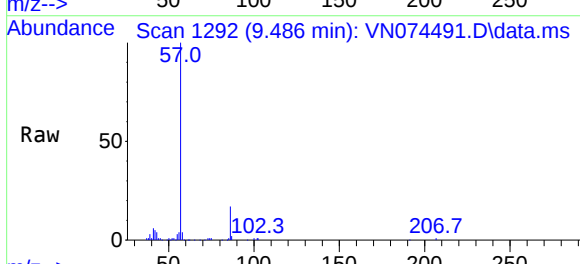




#49
1,4-Dioxane
Concen: 0.819 ug/l
RT: 9.510 min Scan# 11
Delta R.T. 0.006 min
Lab File: VN074491.D
Acq: 16 Sep 2022 04:05




Instrument :
MSVOA_N
ClientSampleId :
WC-17-4-5


Tgt Ion: 88 Resp: 143
Ion Ratio Lower Upper
88 100
43 0.0 20.2 30.4#
58 0.0 54.2 81.4#

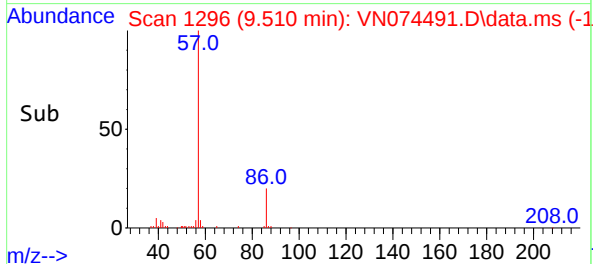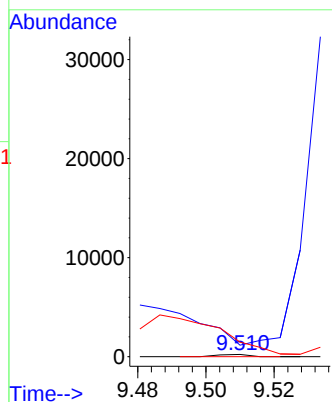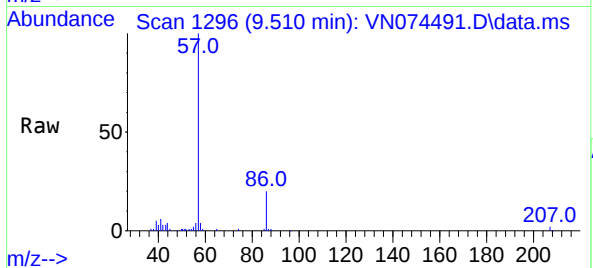

#50
Toluene-d8
Concen: 44.860 ug/l
RT: 10.381 min Scan# 1444
Delta R.T. 0.001 min
Lab File: VN074491.D
Acq: 16 Sep 2022 04:05

Tgt Ion: 98 Resp: 830225
Ion Ratio Lower Upper
98 100
100 64.6 52.6 78.8


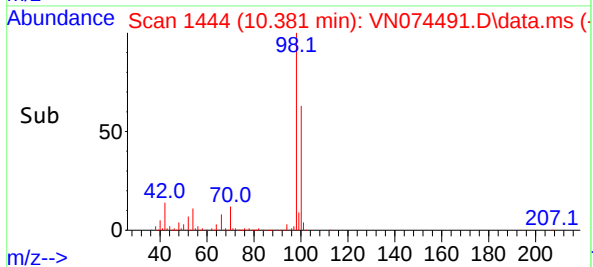
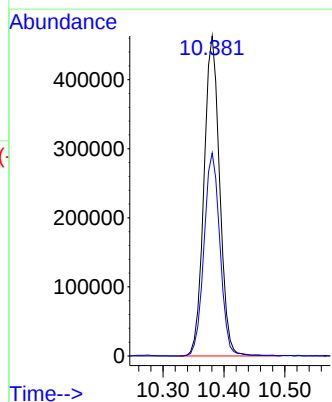
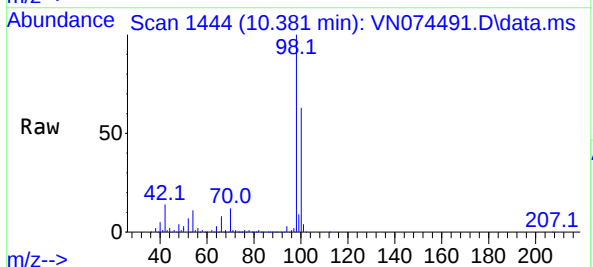


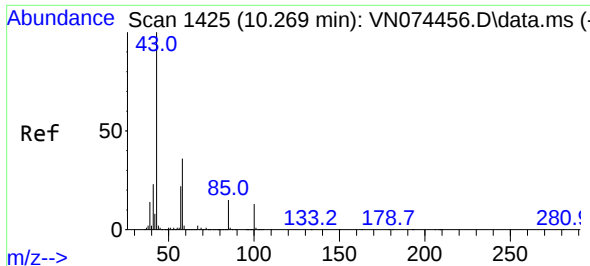

#51
4-Methyl-2-Pentanone
Concen: 1.836 ug/l
RT: 10.269 min Scan# 1425
Delta R.T. -0.000 min
Lab File: VN074491.D
Acq: 16 Sep 2022 04:05




Instrument : MSVOA_N
ClientSampleId : WC-17-4-5


Tgt Ion: 43 Resp: 24570
Ion Ratio Lower Upper
43 100
58 28.9 34.1 51.1#

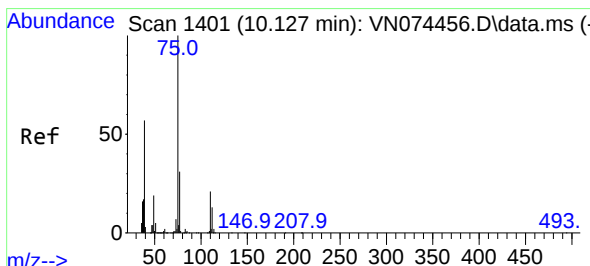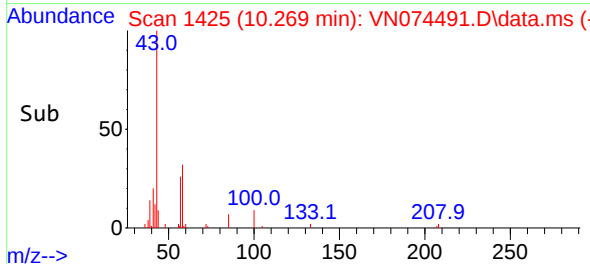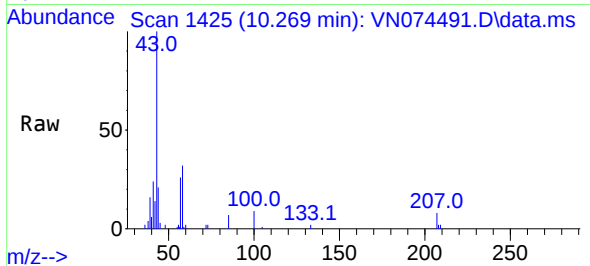

#54
cis-1,3-Dichloropropene
Concen: 5.433 ug/l
RT: 10.186 min Scan# 1411
Delta R.T. 0.059 min
Lab File: VN074491.D
Acq: 16 Sep 2022 04:05

Tgt Ion: 75 Resp: 59898
Ion Ratio Lower Upper
75 100
77 0.8 25.2 37.8#
39 42.4 35.7 53.5

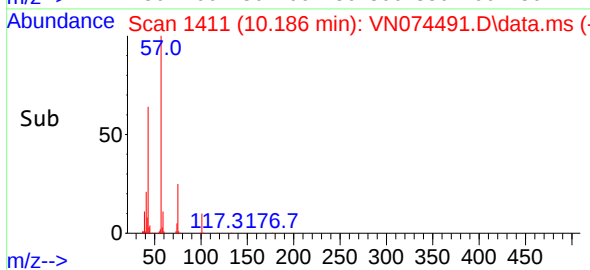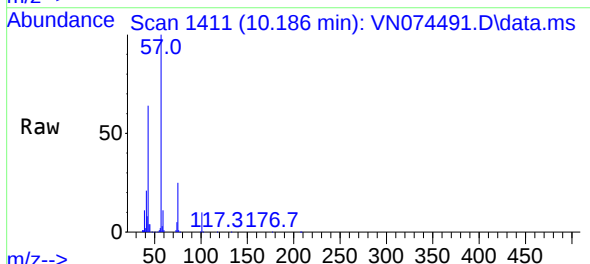



#57

1,3-Dichloropropane

Concen: 0.455 ug/l

RT: 11.028 min Scan# 1549

Delta R.T. 0.042 min

Lab File: VN074491.D

Acq: 16 Sep 2022 04:05

Instrument :

MSVOA_N

ClientSampleId :





WC-17-4-5

Tgt Ion: 76 Resp: 5186

Ion Ratio Lower Upper

76 100

78 1.3 26.2 39.2#

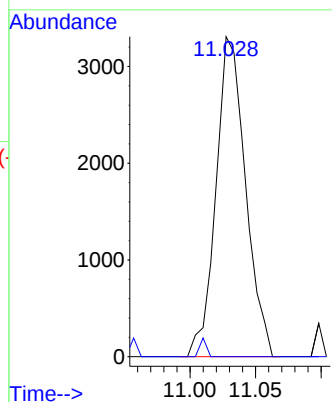

#59

2-Hexanone

Concen: 35.475 ug/l

RT: 10.998 min Scan# 1549

Delta R.T. -0.029 min

Lab File: VN074491.D




Acq: 16 Sep 2022 04:05


Tgt Ion: 43 Resp: 362357

Ion Ratio Lower Upper

43 100

58 0.0 29.7 89.1#


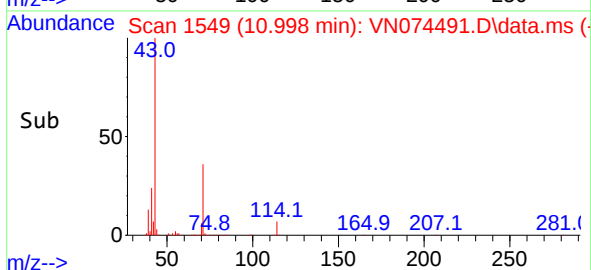
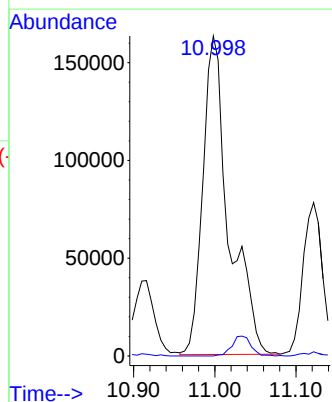





#62
4-Bromofluorobenzene
Concen: 51.687 ug/l
RT: 12.675 min Scan# 1834
Delta R.T. 0.001 min
Lab File: VN074491.D
Acq: 16 Sep 2022 04:05




Instrument :
MSVOA_N
ClientSampleId :
WC-17-4-5


Tgt Ion: 95 Resp: 327626
Ion Ratio Lower Upper
95 100
174 73.4 0.0 167.6
176 70.8 0.0 163.4



#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.686 min Scan# 1666
Delta R.T. 0.000 min
Lab File: VN074491.D
Acq: 16 Sep 2022 04:05

Tgt Ion: 117 Resp: 725690
Ion Ratio Lower Upper
117 100
82 59.0 44.2 66.2
119 31.2 25.4 38.0


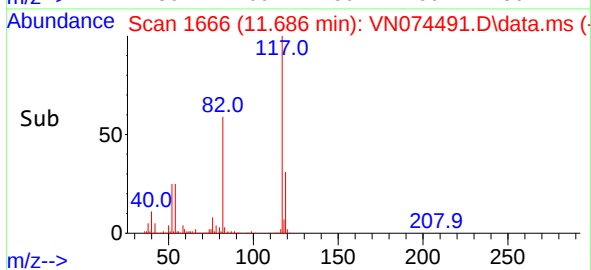






#68
m/p-Xylenes
Concen: 0.367 ug/l
RT: 11.898 min Scan# 1702
Delta R.T. 0.006 min
Lab File: VN074491.D
Acq: 16 Sep 2022 04:05




Instrument :
MSVOA_N
ClientSampleId :
WC-17-4-5


Tgt Ion:106 Resp: 4542
Ion Ratio Lower Upper
106 100
91 212.4 158.9 238.3

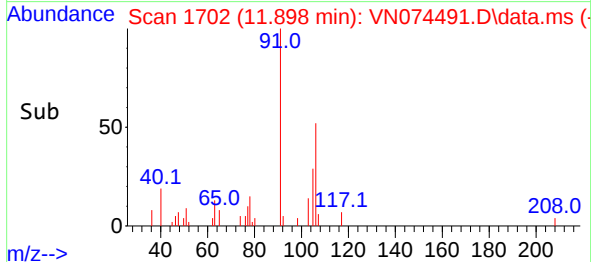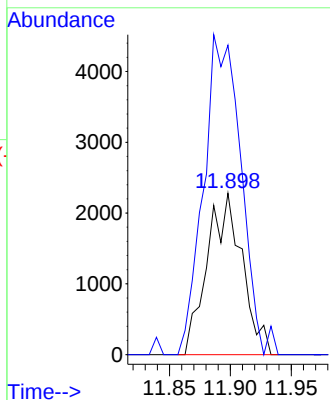

#69
o-Xylene
Concen: 0.407 ug/l
RT: 12.227 min Scan# 1758
Delta R.T. 0.006 min
Lab File: VN074491.D
Acq: 16 Sep 2022 04:05

Tgt Ion:106 Resp: 5135
Ion Ratio Lower Upper
106 100
91 161.8 106.0 318.0


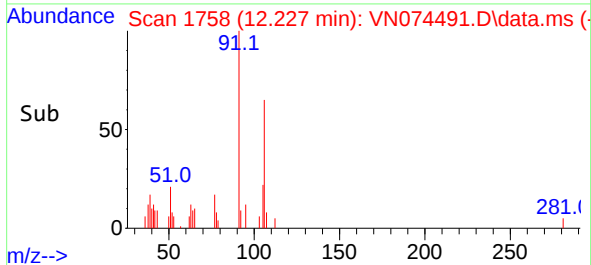
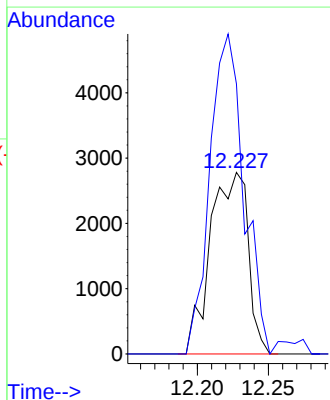
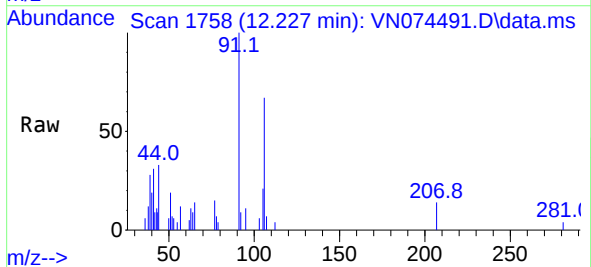


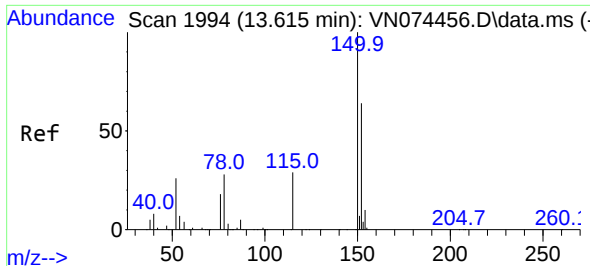

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.616 min Scan# 1994
 Delta R.T. 0.001 min
 Lab File: VN074491.D
 Acq: 16 Sep 2022 04:05




Instrument :
 MSVOA_N
 ClientSampleId :
 WC-17-4-5


Tgt Ion:152 Resp: 323425
 Ion Ratio Lower Upper
 152 100
 115 59.9 28.9 86.7
 150 156.0 0.0 356.2

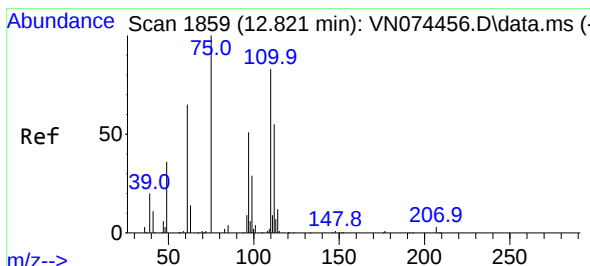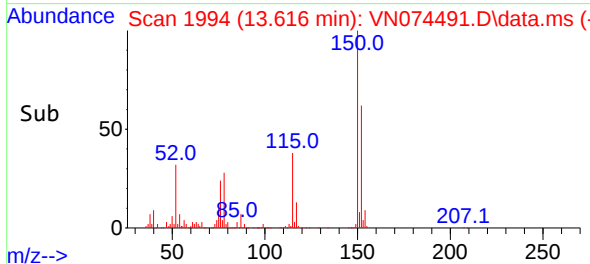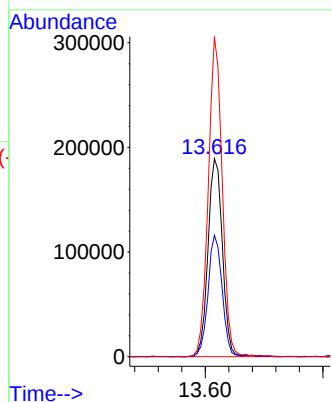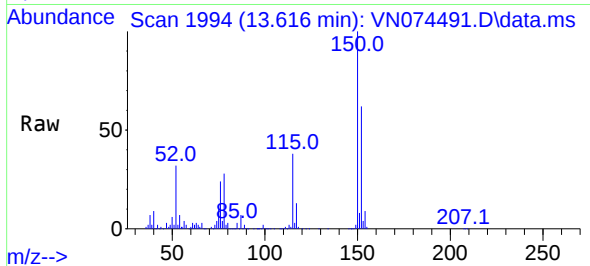

#76
 1,2,3-Trichloropropane
 Concen: 19.500 ug/l
 RT: 12.675 min Scan# 1834
 Delta R.T. -0.146 min
 Lab File: VN074491.D
 Acq: 16 Sep 2022 04:05

Tgt Ion: 75 Resp: 194130
 Ion Ratio Lower Upper
 75 100
 77 1.0 98.5 295.5#


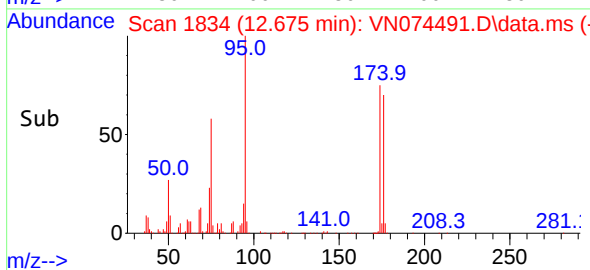

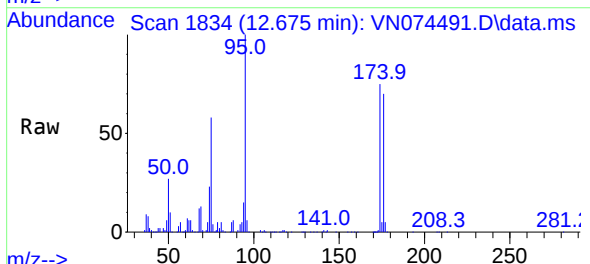




#79
2-Chlorotoluene
Concen: 0.423 ug/l
RT: 12.951 min Scan# 1881
Delta R.T. -0.000 min
Lab File: VN074491.D
Acq: 16 Sep 2022 04:05




Instrument :
MSVOA_N
ClientSampleId :
WC-17-4-5


Tgt Ion: 91 Resp: 9952
Ion Ratio Lower Upper
91 100
126 38.0 17.3 51.9

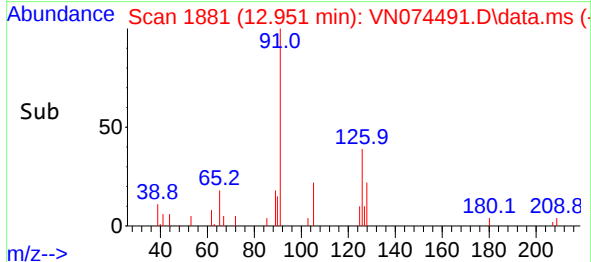

#81
trans-1,4-Dichloro-2-butene
Concen: 42.088 ug/l
RT: 12.675 min Scan# 1834
Delta R.T. 0.105 min
Lab File: VN074491.D
Acq: 16 Sep 2022 04:05

Tgt Ion: 75 Resp: 194130
Ion Ratio Lower Upper
75 100
53 0.0 78.0 117.0#
89 0.0 37.2 55.8#


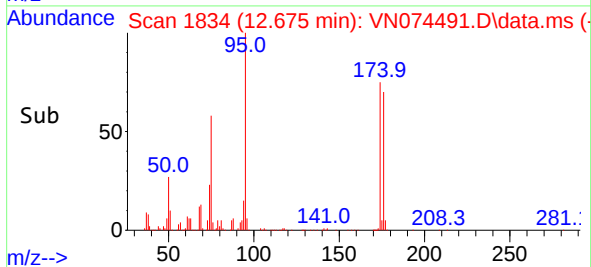

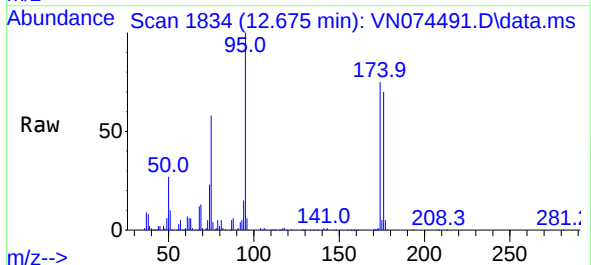




#84
1,2,4-Trimethylbenzene
Concen: 0.419 ug/l
RT: 13.316 min Scan# 1942
Delta R.T. 0.006 min
Lab File: VN074491.D
Acq: 16 Sep 2022 04:05

Instrument :
MSVOA_N
ClientSampleId :
WC-17-4-5

Tgt Ion:105 Resp: 11392
Ion Ratio Lower Upper
105 100
120 47.7 23.3 69.8

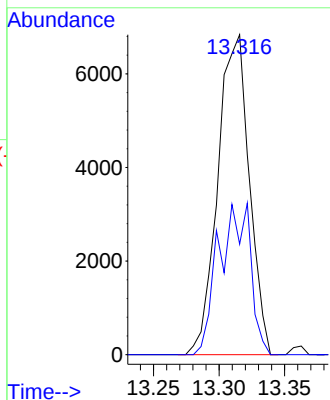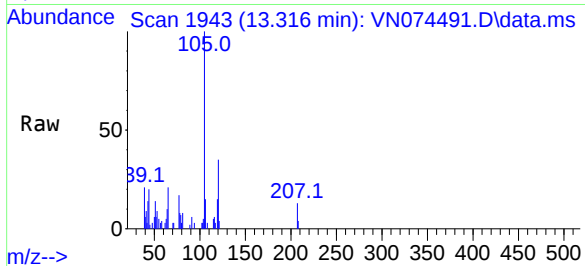

#95
Naphthalene
Concen: 1.873 ug/l
RT: 15.439 min Scan# 2304
Delta R.T. 0.000 min
Lab File: VN074491.D
Acq: 16 Sep 2022 04:05

Tgt Ion:128 Resp: 8131
Ion Ratio Lower Upper
128 100
127 20.6 10.3 15.5#
129 14.4 8.6 13.0#

