
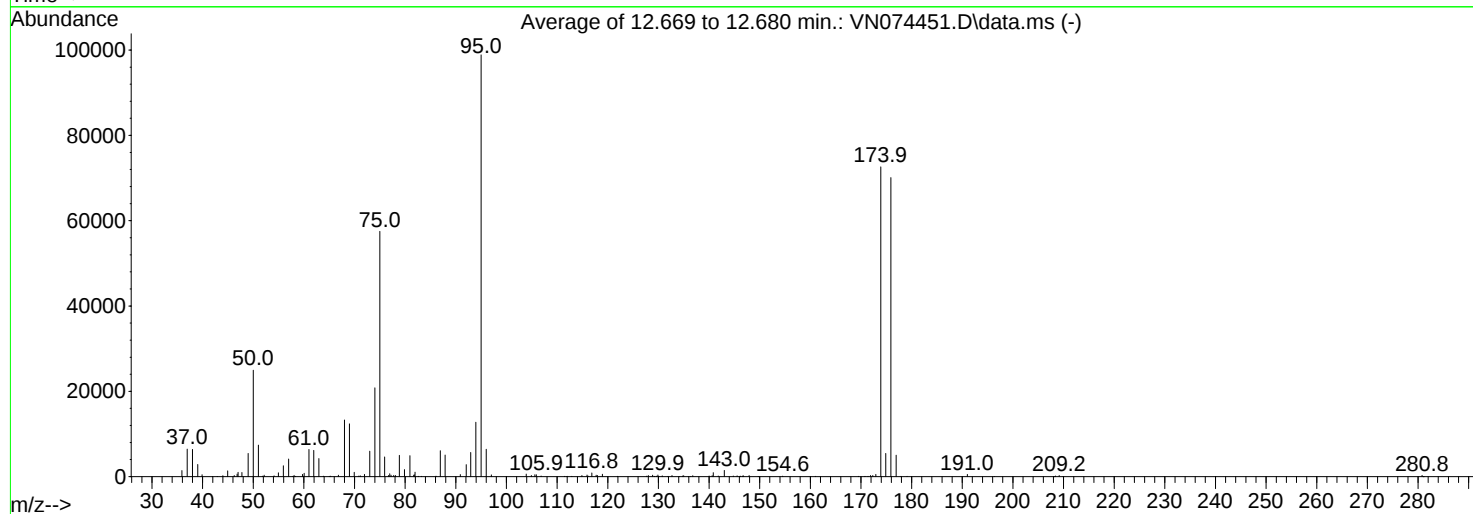


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN091522\
Data File : VN074451.D
Acq On : 15 Sep 2022 09:22
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N091522W.M
Title : SW846 8260
Last Update : Thu Sep 15 19:20:33 2022

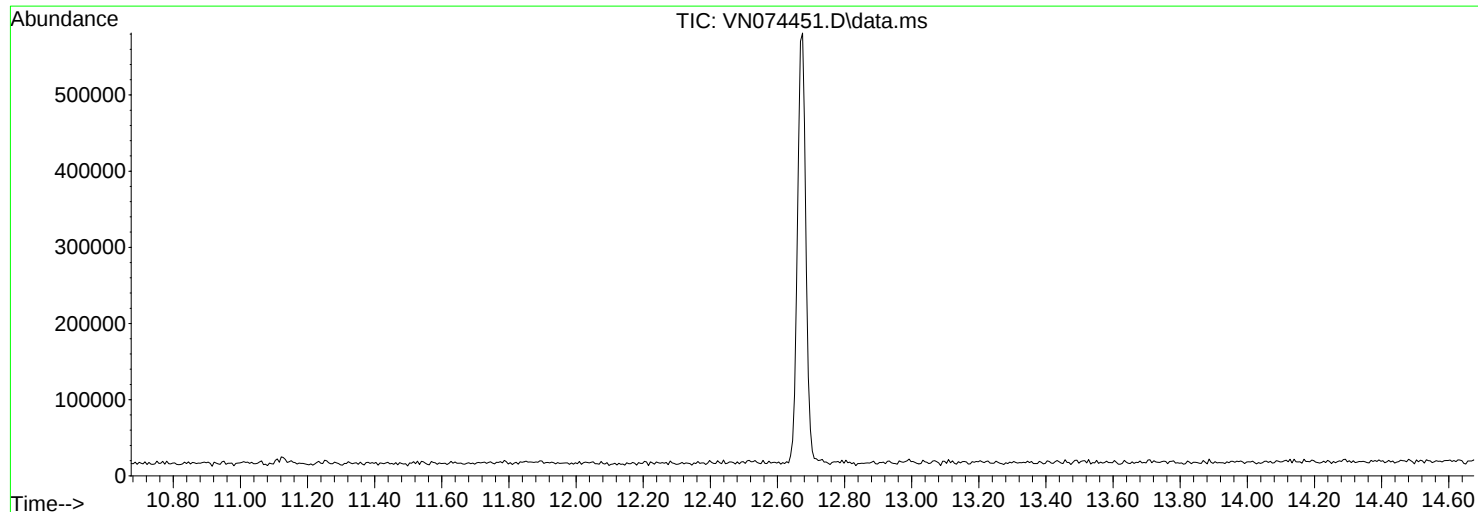

AutoFind: Scans 1833, 1834, 1835; Background Corrected with Scan 1824

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	25.2	24952	PASS
75	95	30	60	58.2	57499	PASS
95	95	100	100	100.0	98877	PASS
96	95	5	9	6.5	6433	PASS
173	174	0.00	2	0.7	528	PASS
174	95	50	100	73.5	72635	PASS
175	174	5	9	7.5	5454	PASS
176	174	95	101	96.5	70107	PASS
177	176	5	9	7.2	5014	PASS