


Data Path : W:\HPCHEM1\MSVOA N\DATA\VN091715\
Data File : VN027267.D
Acq On : 17 Sep 2015 21:12
Operator : MD\FY
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_N\METHODS\82N091515W.M
Title : SW846 8260
Last Update : Tue Sep 15 21:12:09 2015

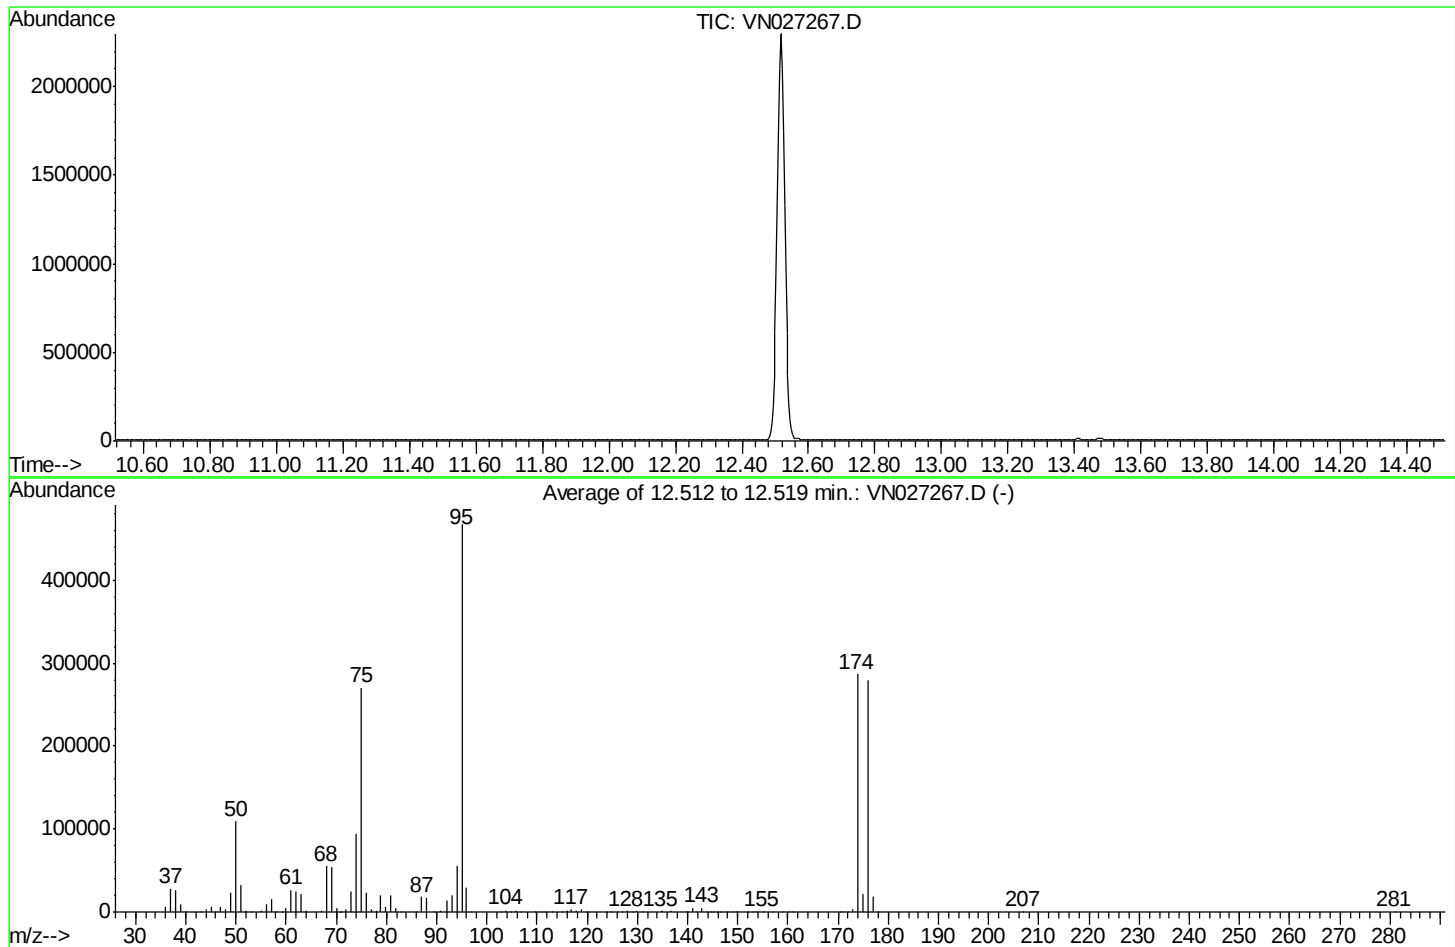

AutoFind: Scans 3397, 3398, 3399; Background Corrected with Scan 3382

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.3	108877	PASS
75	95	30	60	57.8	270037	PASS
95	95	100	100	100.0	467200	PASS
96	95	5	9	6.4	29853	PASS
173	174	0.00	2	1.1	3135	PASS
174	95	50	100	61.4	286741	PASS
175	174	5	9	7.4	21290	PASS
176	174	95	101	97.3	278997	PASS
177	176	5	9	6.8	19021	PASS