




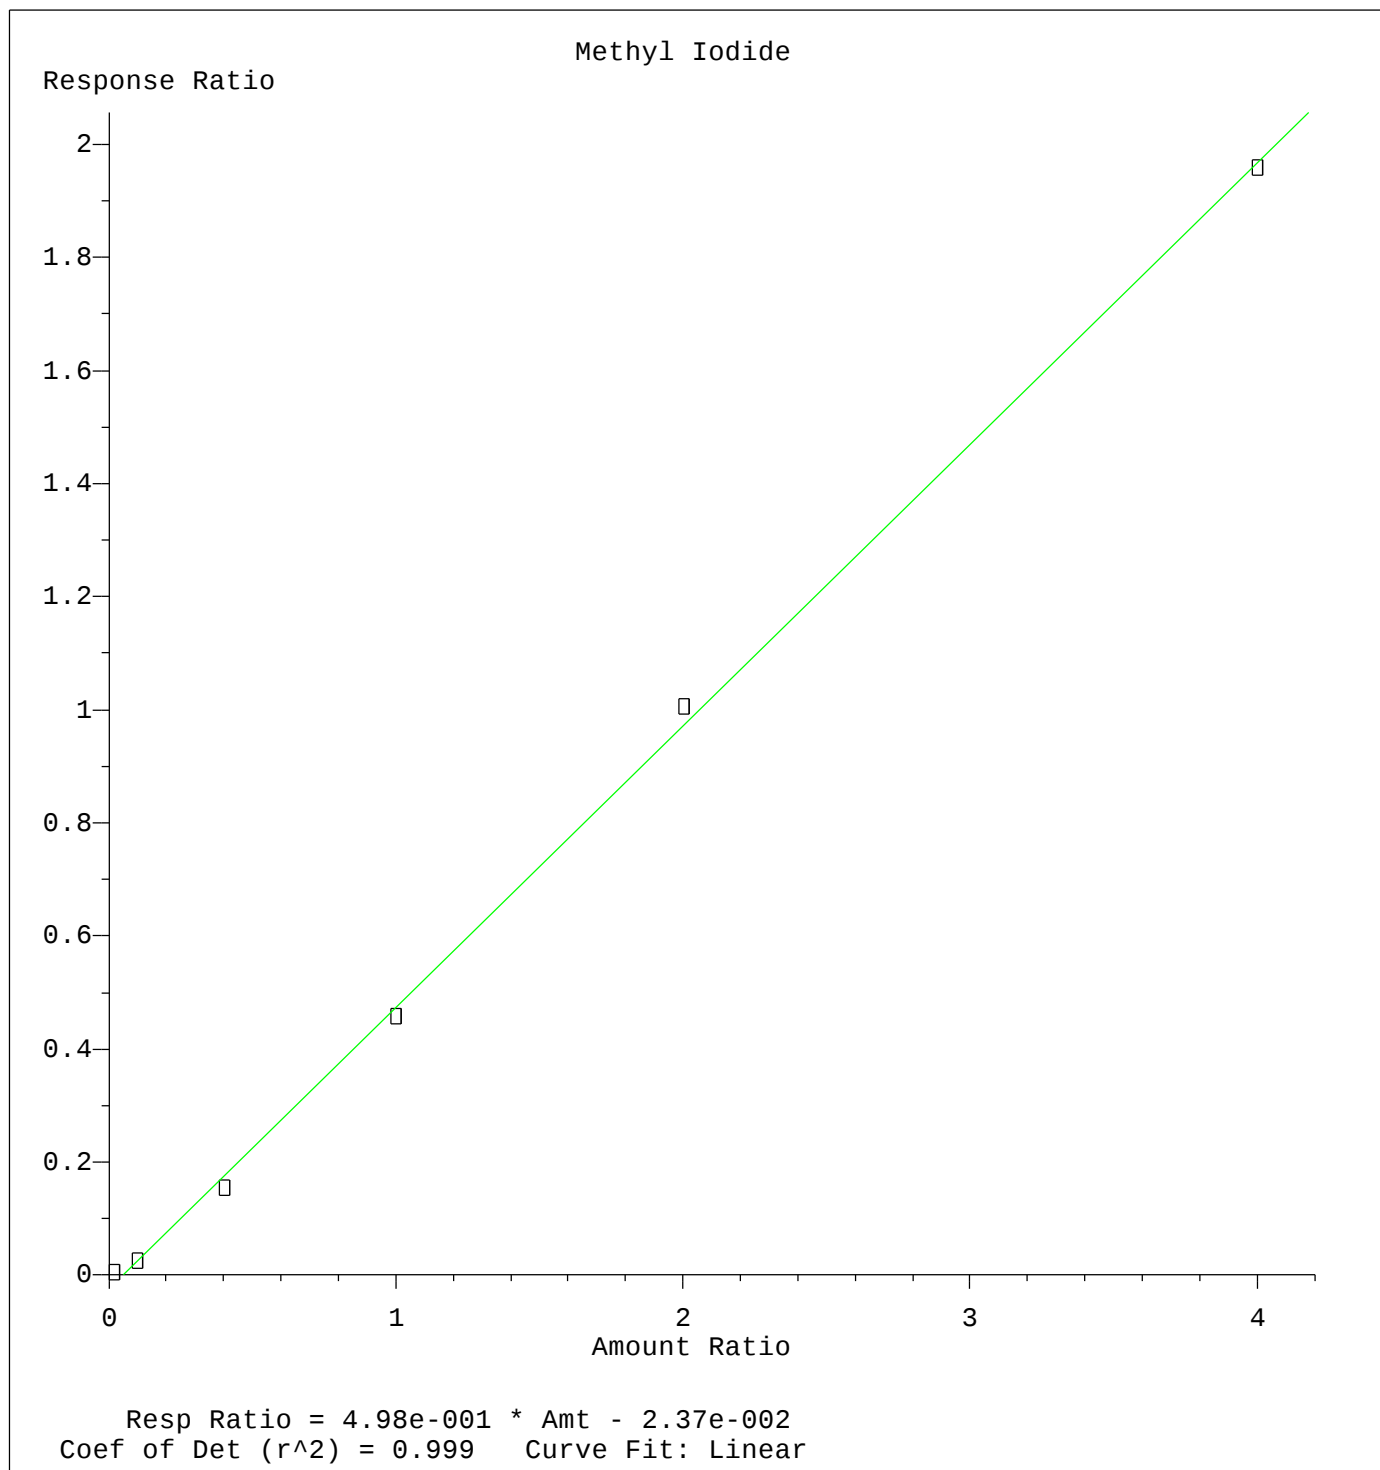

Method Name: W:\HPCHEM1\MSVOA_N\METHODS\82N092115W.M
Calibration Table Last Updated: Mon Sep 21 13:12:32 2015

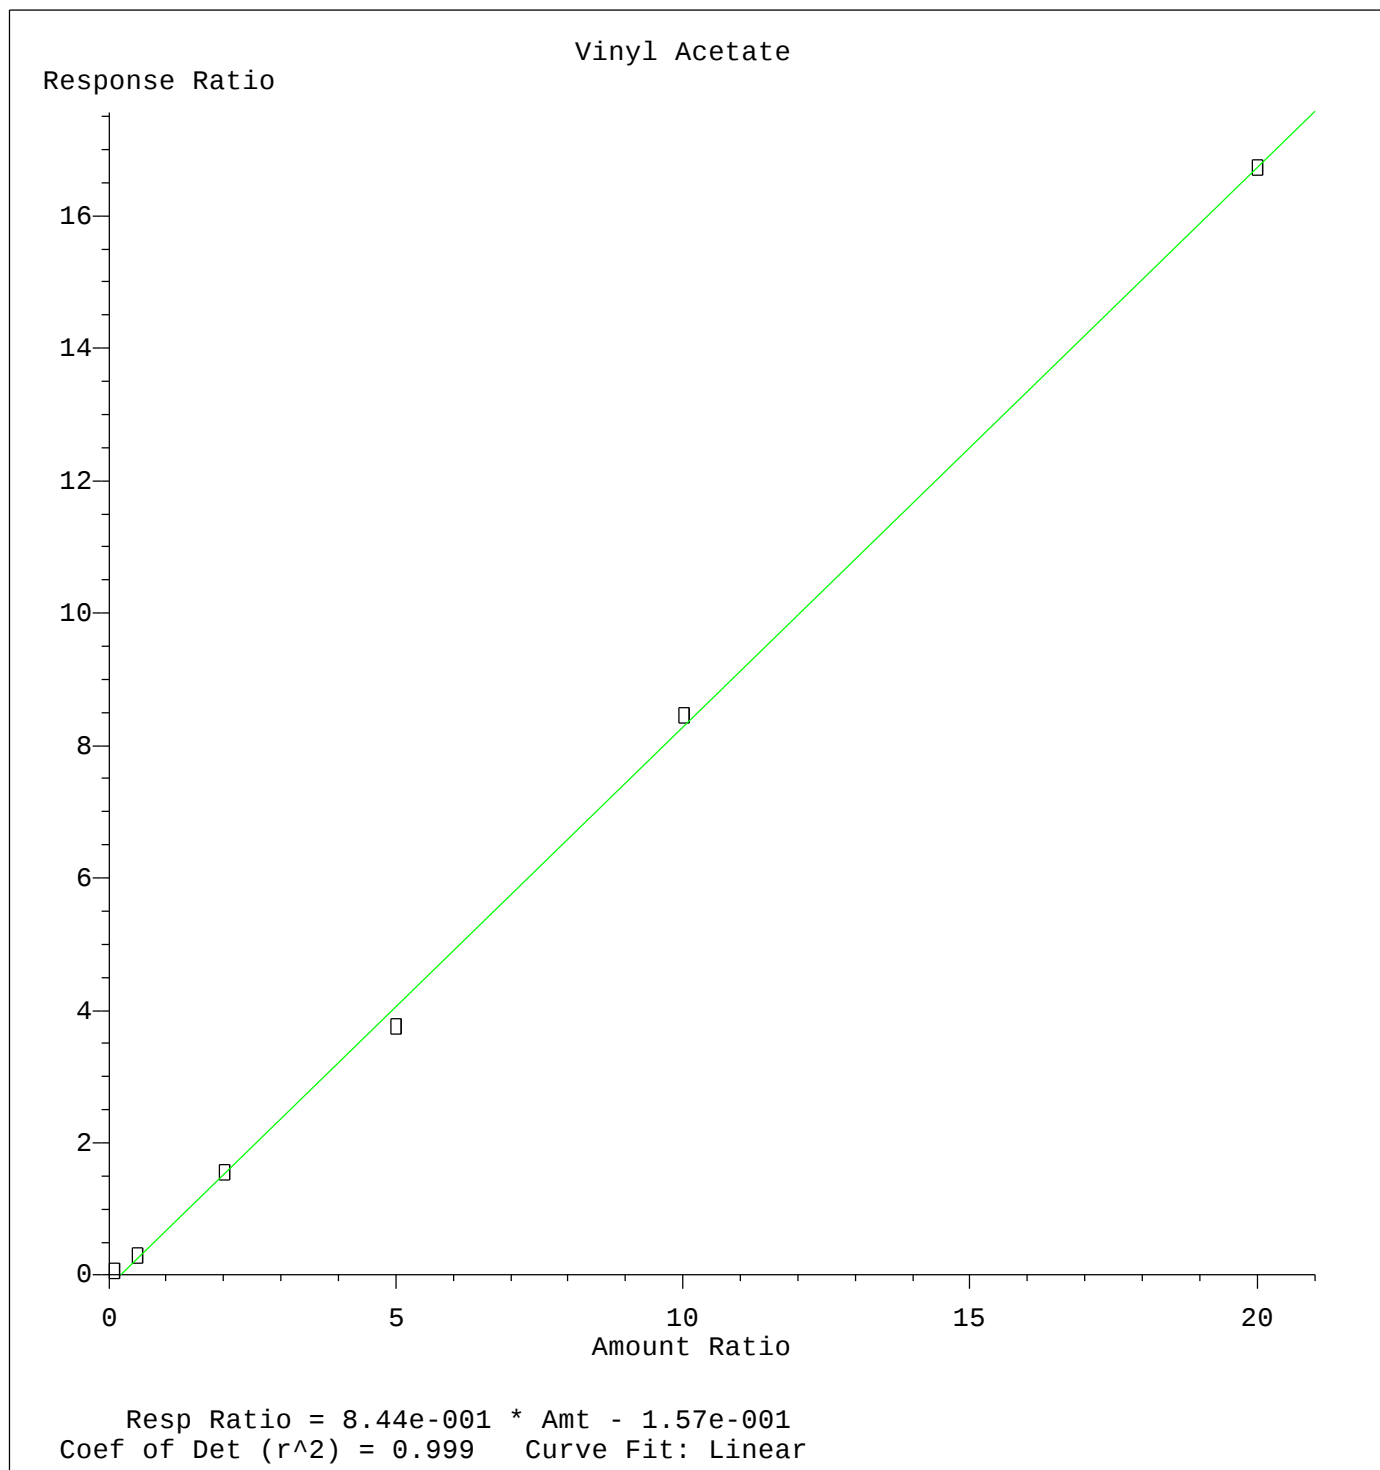


Method Name: W:\HPCHEM1\MSVOA_N\METHODS\82N092115W.M
Calibration Table Last Updated: Mon Sep 21 13:12:32 2015

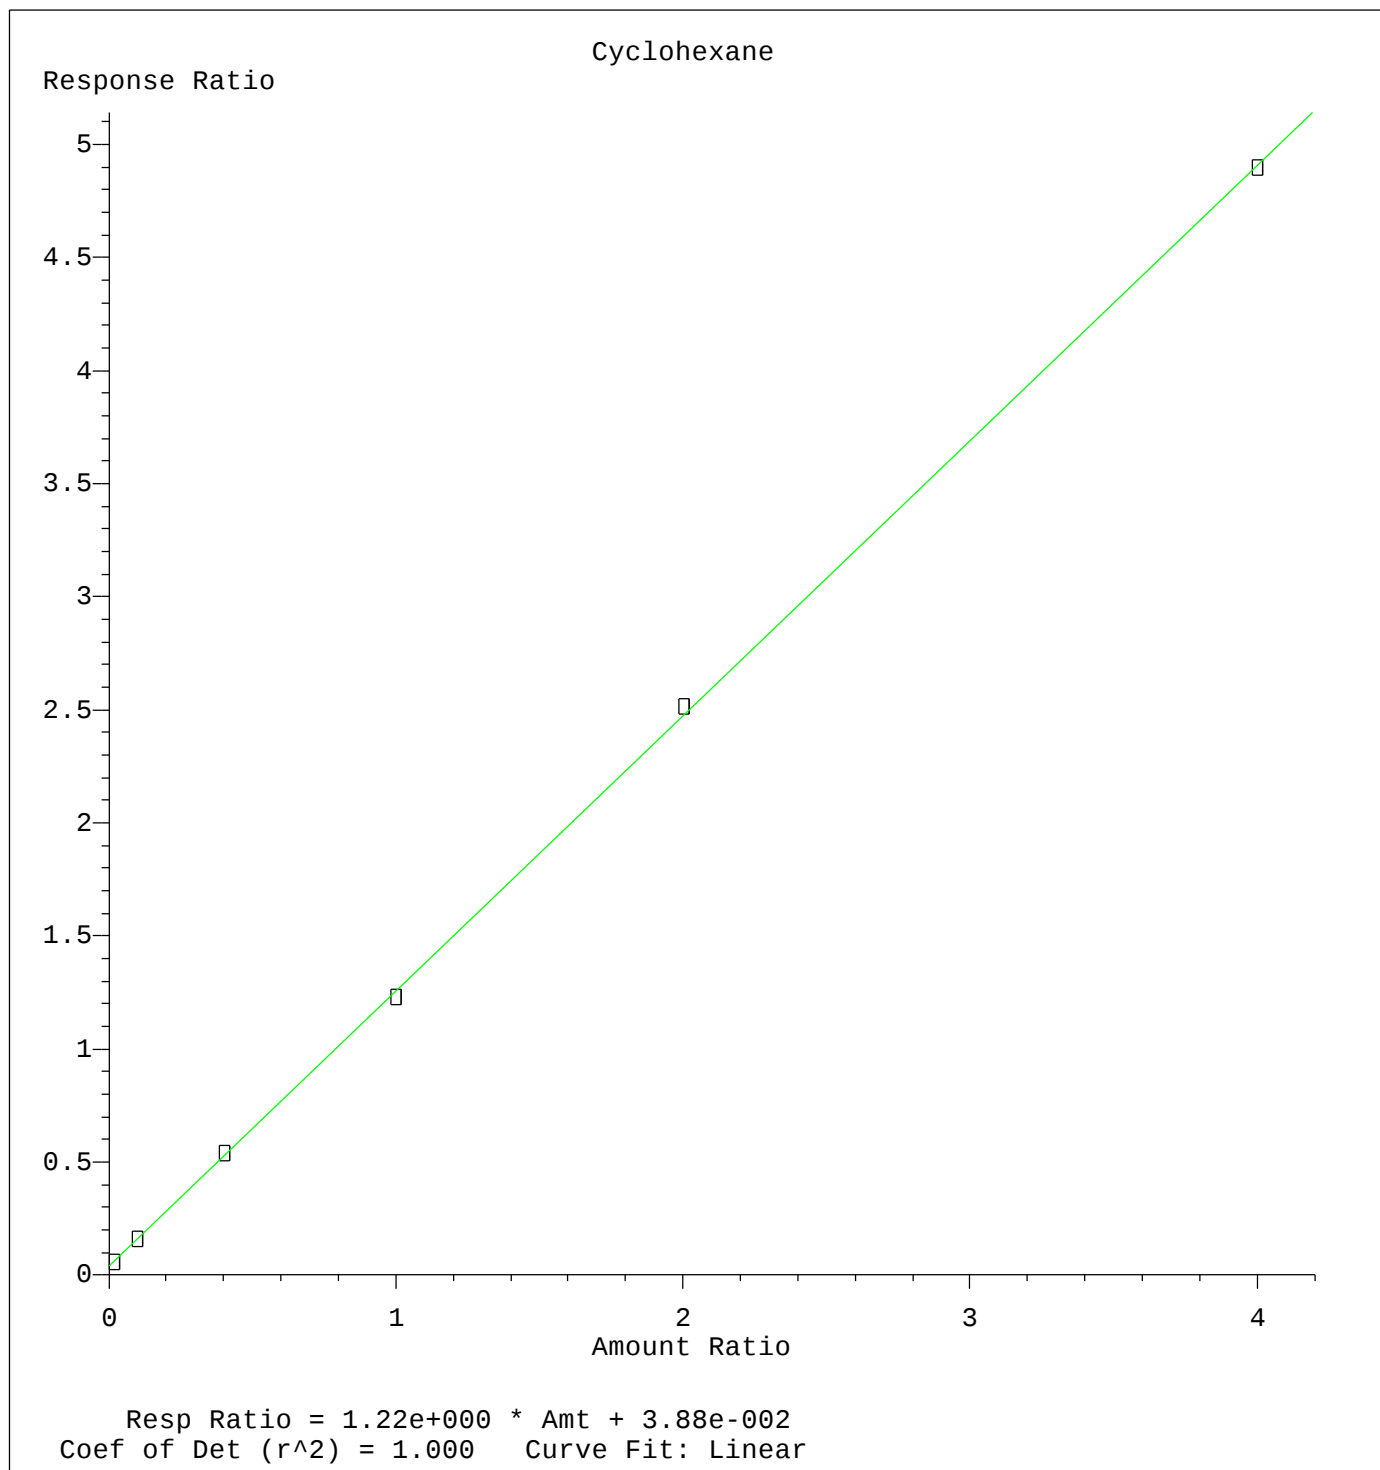

Method Name: W:\HPCHEM1\MSVOA_N\METHODS\82N092115W.M
Calibration Table Last Updated: Mon Sep 21 13:12:32 2015

Naphthalene

Response Ratio

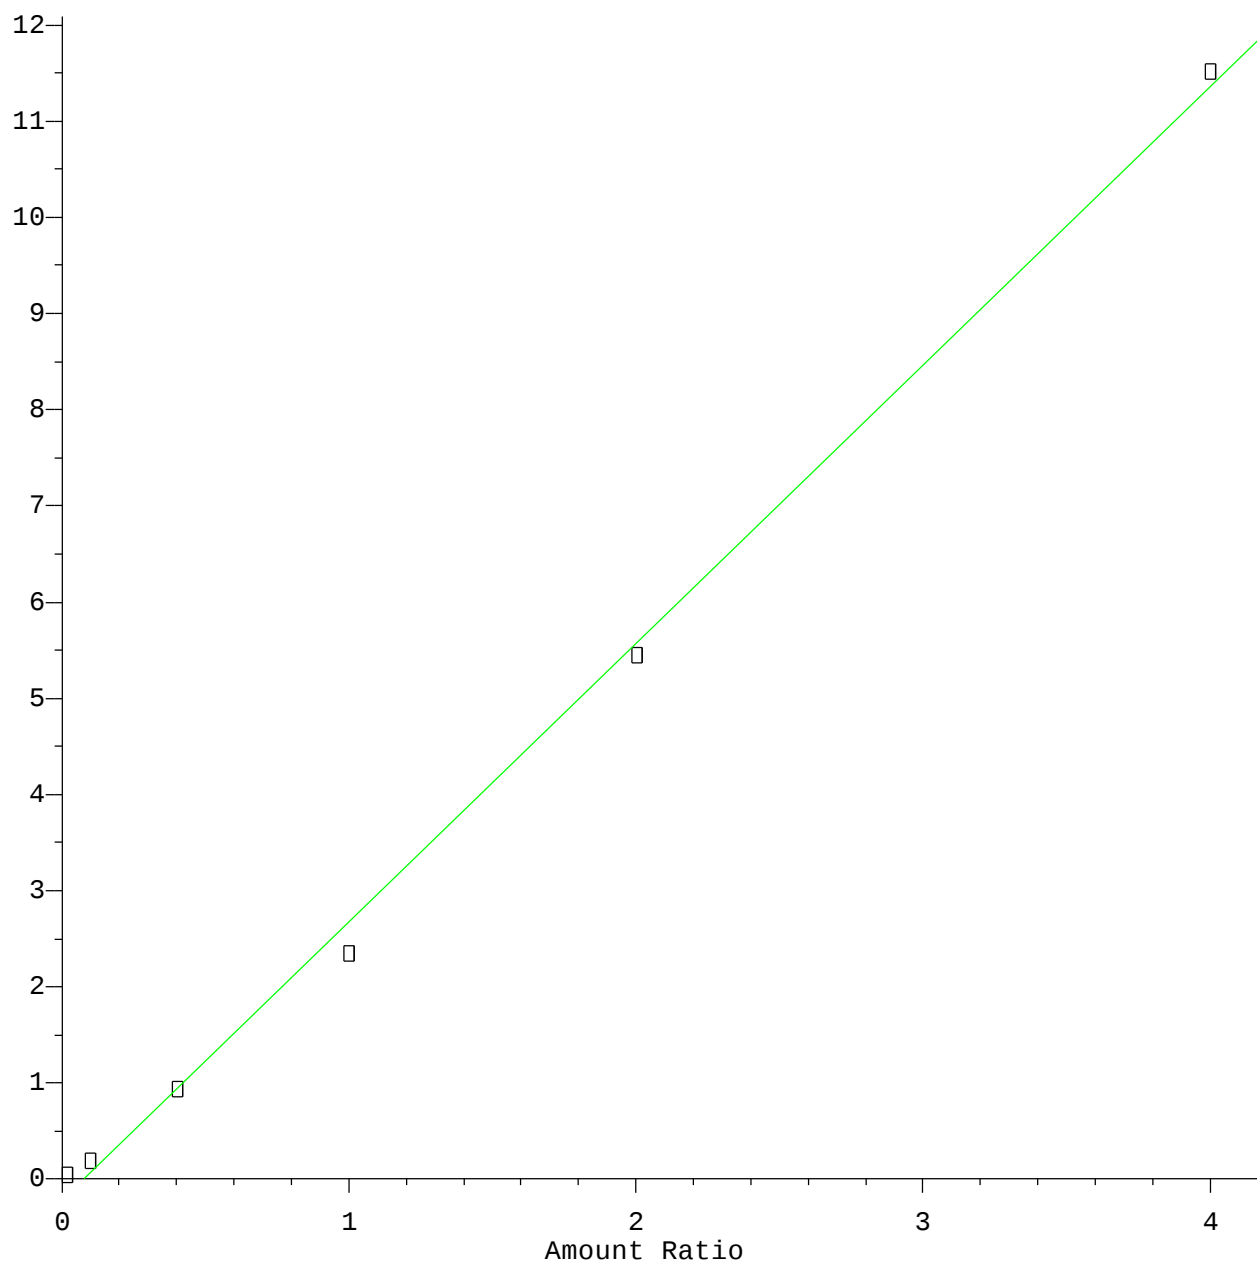

Resp Ratio = 2.90×10^0 * Amt - 2.21×10^{-1}
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: W:\HPCHEM1\MSVOA_N\METHODS\82N092115W.M
Calibration Table Last Updated: Mon Sep 21 13:12:32 2015