

Data Path : W:\HPCHEM1\MSVOA N\DATA\VN092115\
 Data File : VN027332.D
 Acq On : 21 Sep 2015 14:41
 Operator : MD\FY
 Sample : VN0921WBL01
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0921WBL01

Quant Time: Sep 22 01:43:09 2015
 Quant Method : W:\HPCHEM1\MSVOA_N\METHODS\82N092115W.M
 Quant Title : SW846 8260
 QLast Update : Mon Sep 21 13:12:32 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.75	168	527320	50.00	ug/l	0.00
35) 1,4-Difluorobenzene	8.68	114	1057242	50.00	ug/l	0.00
64) Chlorobenzene-d5	11.52	117	1008190	50.00	ug/l	0.00
73) 1,4-Dichlorobenzene-d4	13.47	152	363106	50.00	ug/l	0.00

System Monitoring Compounds						
34) 1,2-Dichloroethane-d4	8.12	65	503955	48.82	ug/l	0.00
Spiked Amount	50.000		Recovery	=	97.64%	
36) Dibromofluoromethane	7.68	113	330403	47.90	ug/l	0.00
Spiked Amount	50.000		Recovery	=	95.80%	
51) Toluene-d8	10.19	98	1385730	51.96	ug/l	0.00
Spiked Amount	50.000		Recovery	=	103.92%	
63) 4-Bromofluorobenzene	12.52	95	539780	55.71	ug/l	0.00
Spiked Amount	50.000		Recovery	=	111.42%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : W:\HPCHEM1\MSVOA N\DATA\VN092115\
Data File : VN027332.D
Acq On : 21 Sep 2015 14:41
Operator : MD\FY
Sample : VN0921WBL01
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0921WBL01

Quant Time: Sep 22 01:43:09 2015
Quant Method : W:\HPCHEM1\MSVOA_N\METHODS\82N092115W.M
Quant Title : SW846 8260
QLast Update : Mon Sep 21 13:12:32 2015
Response via : Initial Calibration

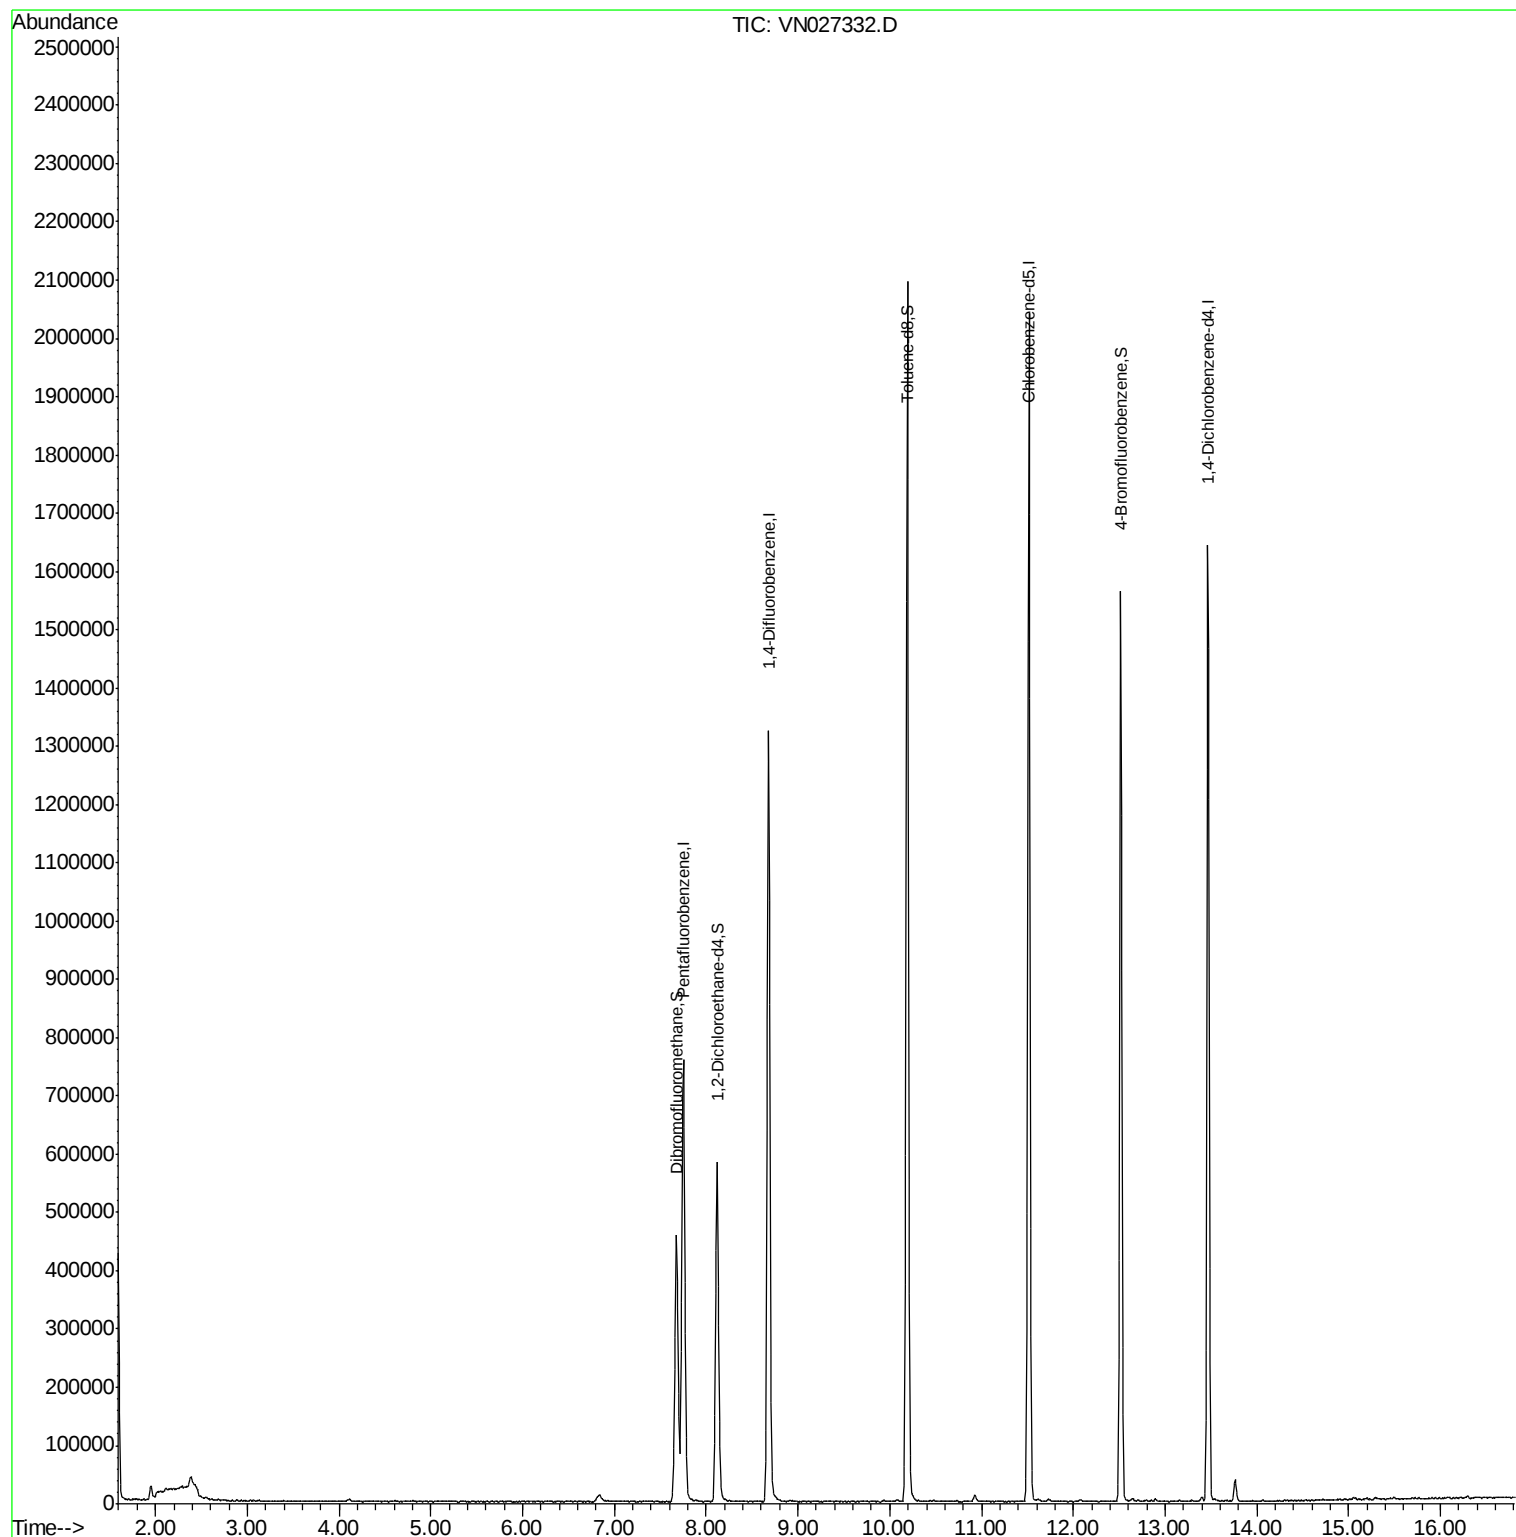

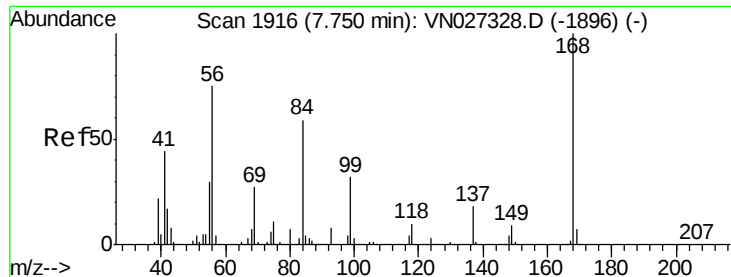

#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 7.75 min Scan# 1917

Delta R.T. 0.00 min

Lab File: VN027332.D

Acq: 21 Sep 2015 14:41

Instrument :

MSVOA_N

ClientSampleId :


VN0921WBL01

Tot Ion:168 Resp: 527320

Ion Ratio Lower Upper

168 100

99 73.5 50.4 75.6

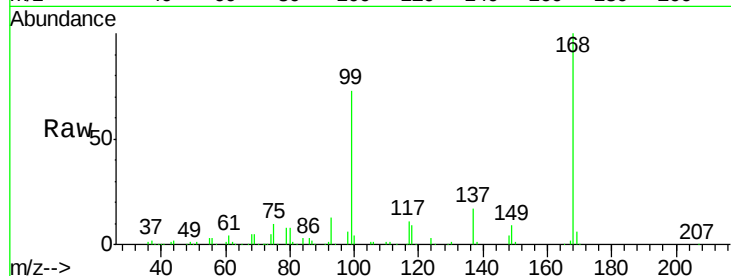

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VN

7.75

250000

200000



150000

100000

50000

0

Time-->

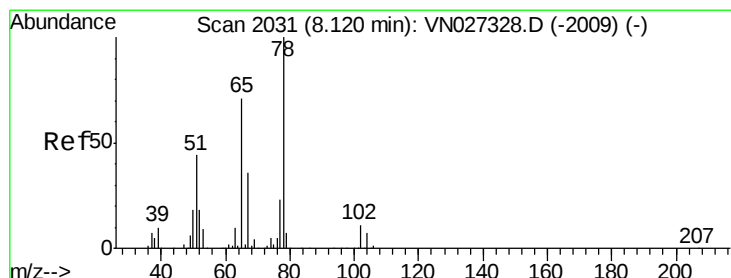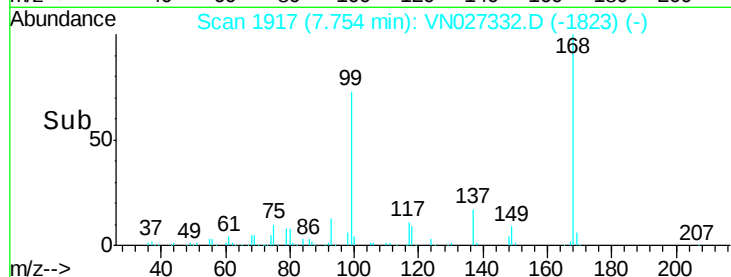

#34

1,2-Dichloroethane-d4

Concen: 48.82 ug/l

RT: 8.12 min Scan# 2031

Delta R.T. 0.00 min

Lab File: VN027332.D


Acq: 21 Sep 2015 14:41

Tgt Ion: 65 Resp: 503955

Ion Ratio Lower Upper

65 100

67 50.5 0.0 110.6

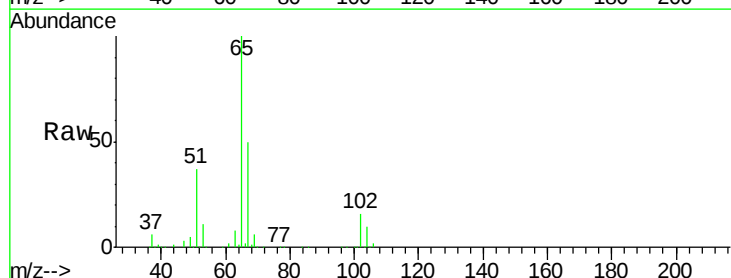

Abundance Ion 64.90 (64.60 to 65.60): VN

Ion 66.90 (66.60 to 67.60): VN

8.12

250000

200000


150000


100000

50000

0

Time-->




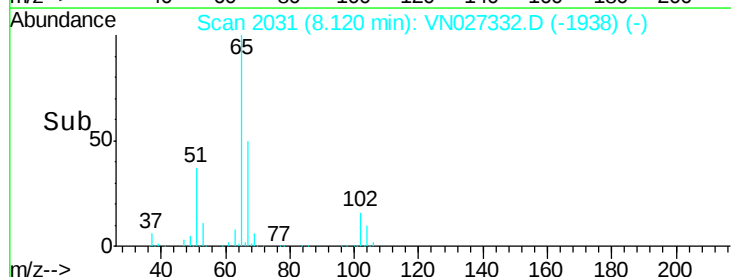


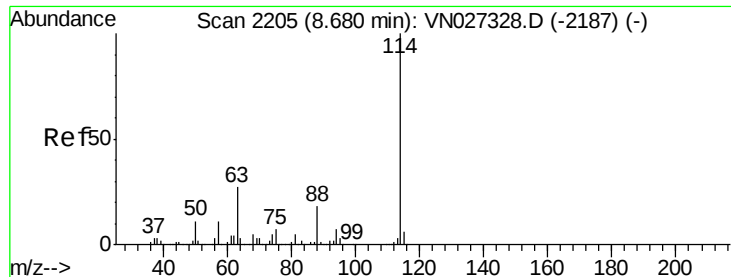

#35
 1,4-Difluorobenzene
 Concen: 50.00 ug/l
 RT: 8.68 min Scan# 2205
 Delta R.T. 0.00 min
 Lab File: VN027332.D
 Acq: 21 Sep 2015 14:41




Instrument :
 MSVOA_N
 ClientSampleId :
 VN0921WBL01


Tot Ion:114 Resp: 1057242
 Ion Ratio Lower Upper
 114 100
 63 25.9 0.0 48.8
 88 18.4 0.0 32.2

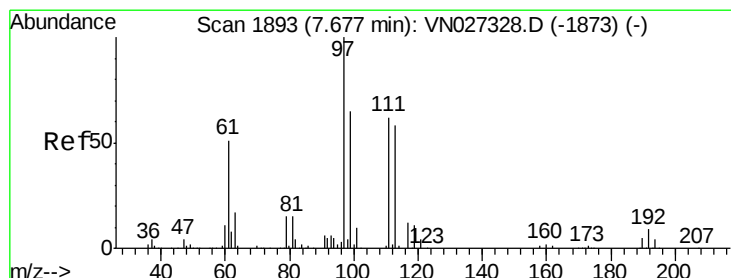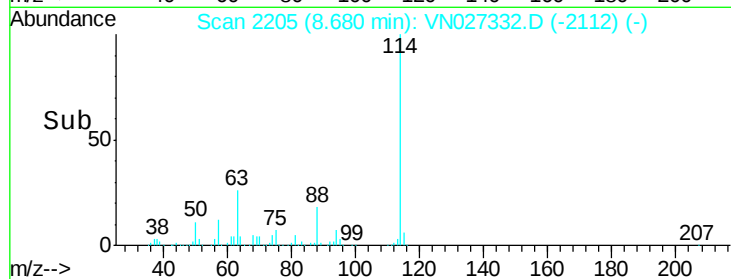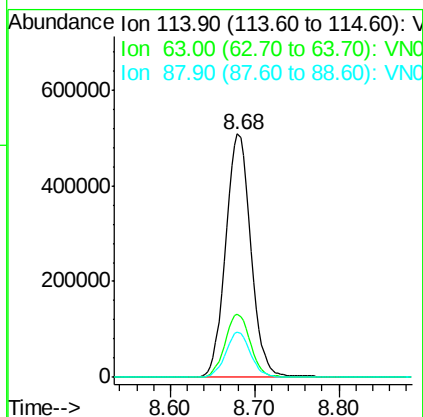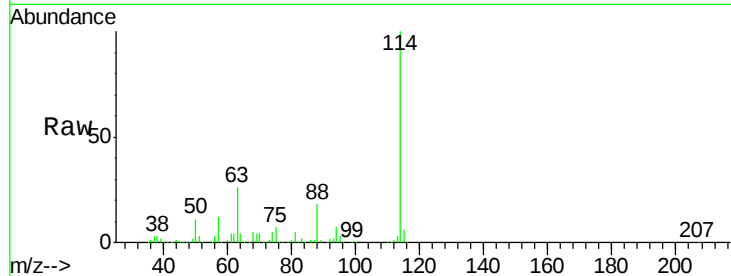

#36
 Dibromofluoromethane
 Concen: 47.90 ug/l
 RT: 7.68 min Scan# 1893
 Delta R.T. 0.00 min
 Lab File: VN027332.D
 Acq: 21 Sep 2015 14:41

Tgt Ion:113 Resp: 330403
 Ion Ratio Lower Upper
 113 100
 111 107.2 83.0 124.4
 192 15.9 14.1 21.1

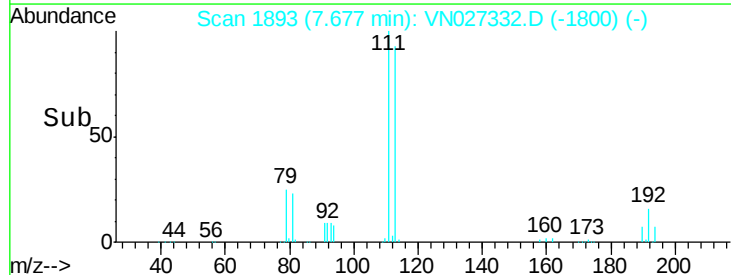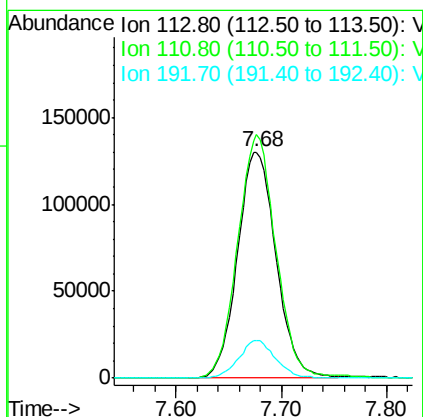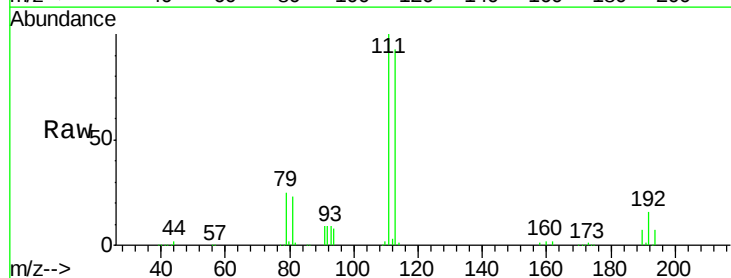

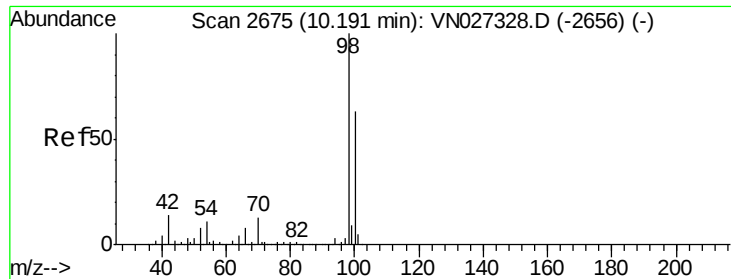

#51

Toluene-d8

Concen: 51.96 ug/l

RT: 10.19 min Scan# 2675

Delta R.T. 0.00 min

Lab File: VN027332.D

Acq: 21 Sep 2015 14:41

Instrument :

MSVOA_N

ClientSampled :





VN0921WBL01

Tot Ion: 98 Resp: 1385730

Ion Ratio Lower Upper

98 100

100 62.4 50.5 75.7

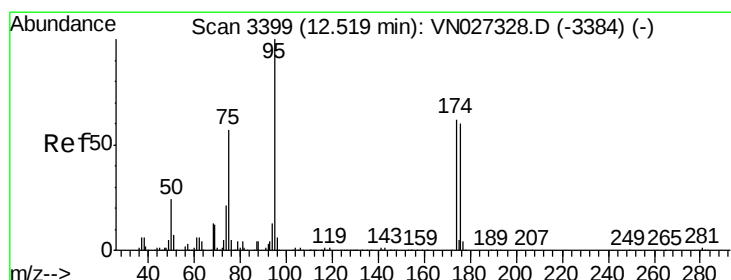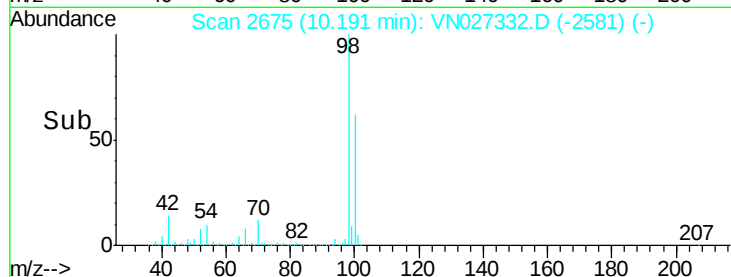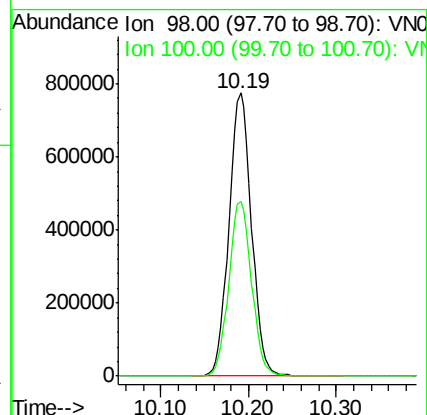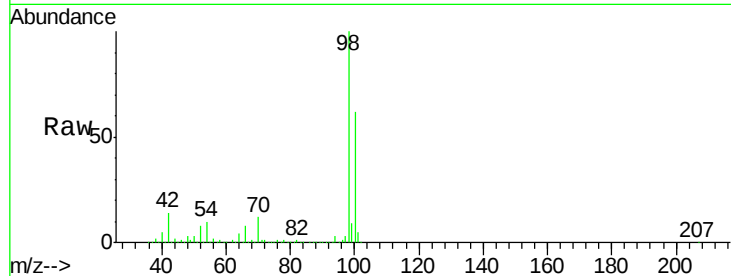

#63

4-Bromofluorobenzene

Concen: 55.71 ug/l

RT: 12.52 min Scan# 3399

Delta R.T. 0.00 min

Lab File: VN027332.D

Acq: 21 Sep 2015 14:41




Tgt Ion: 95 Resp: 539780


Ion Ratio Lower Upper

95 100

174 62.2 0.0 137.0

176 60.7 0.0 130.8


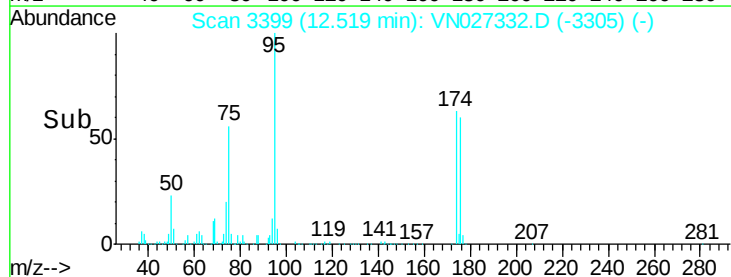
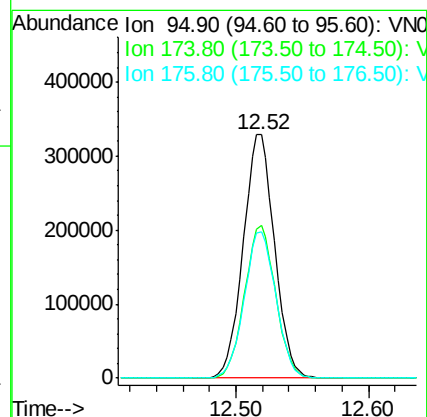
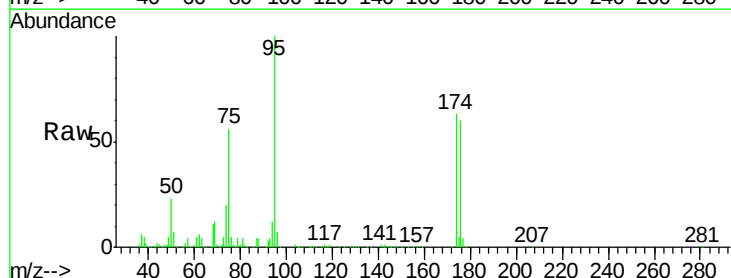


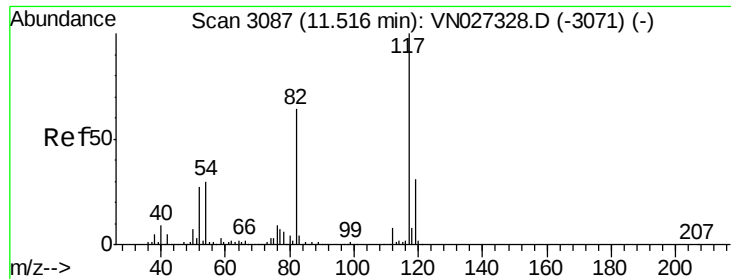

#64
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.52 min Scan# 3087
Delta R.T. 0.00 min
Lab File: VN027332.D
Acq: 21 Sep 2015 14:41

Instrument :
MSVOA_N
ClientSampleId :
VN0921WBL01

Tot Ion:117 Resp: 1008190
Ion Ratio Lower Upper
117 100
82 64.8 49.6 74.4
119 31.1 24.6 36.8

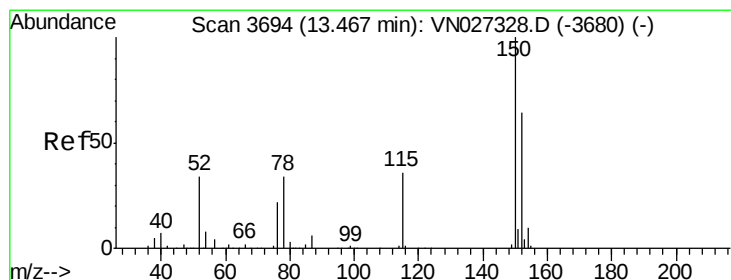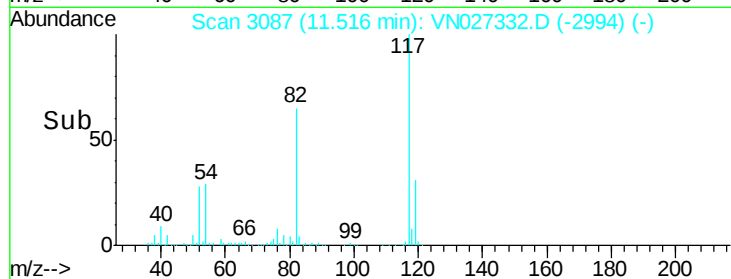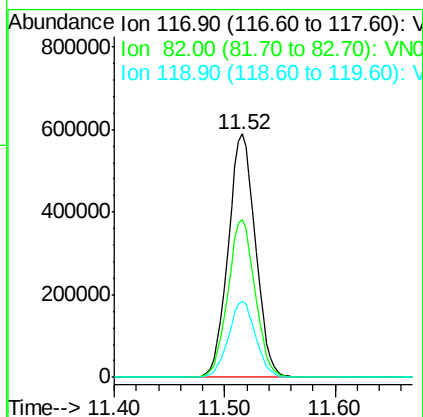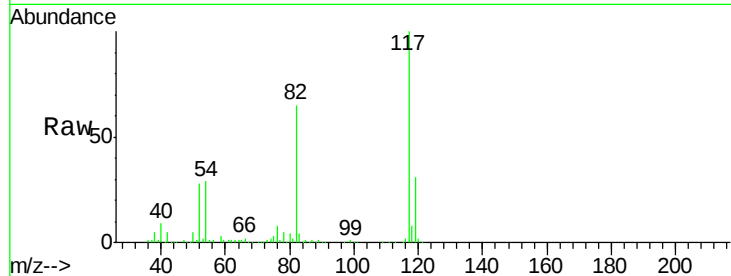

#73
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.47 min Scan# 3695
Delta R.T. 0.00 min
Lab File: VN027332.D
Acq: 21 Sep 2015 14:41

Tgt Ion:152 Resp: 363106
Ion Ratio Lower Upper
152 100
115 68.5 30.8 92.3
150 159.6 0.0 345.0

