


Data Path : W:\HPCHEM1\MSVOA N\DATA\VN092115\
 Data File : VN027324.D
 Acq On : 21 Sep 2015 9:24
 Operator : MD\FY
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_N\METHODS\82N092115W.M
 Title : SW846 8260
 Last Update : Mon Sep 21 13:12:32 2015

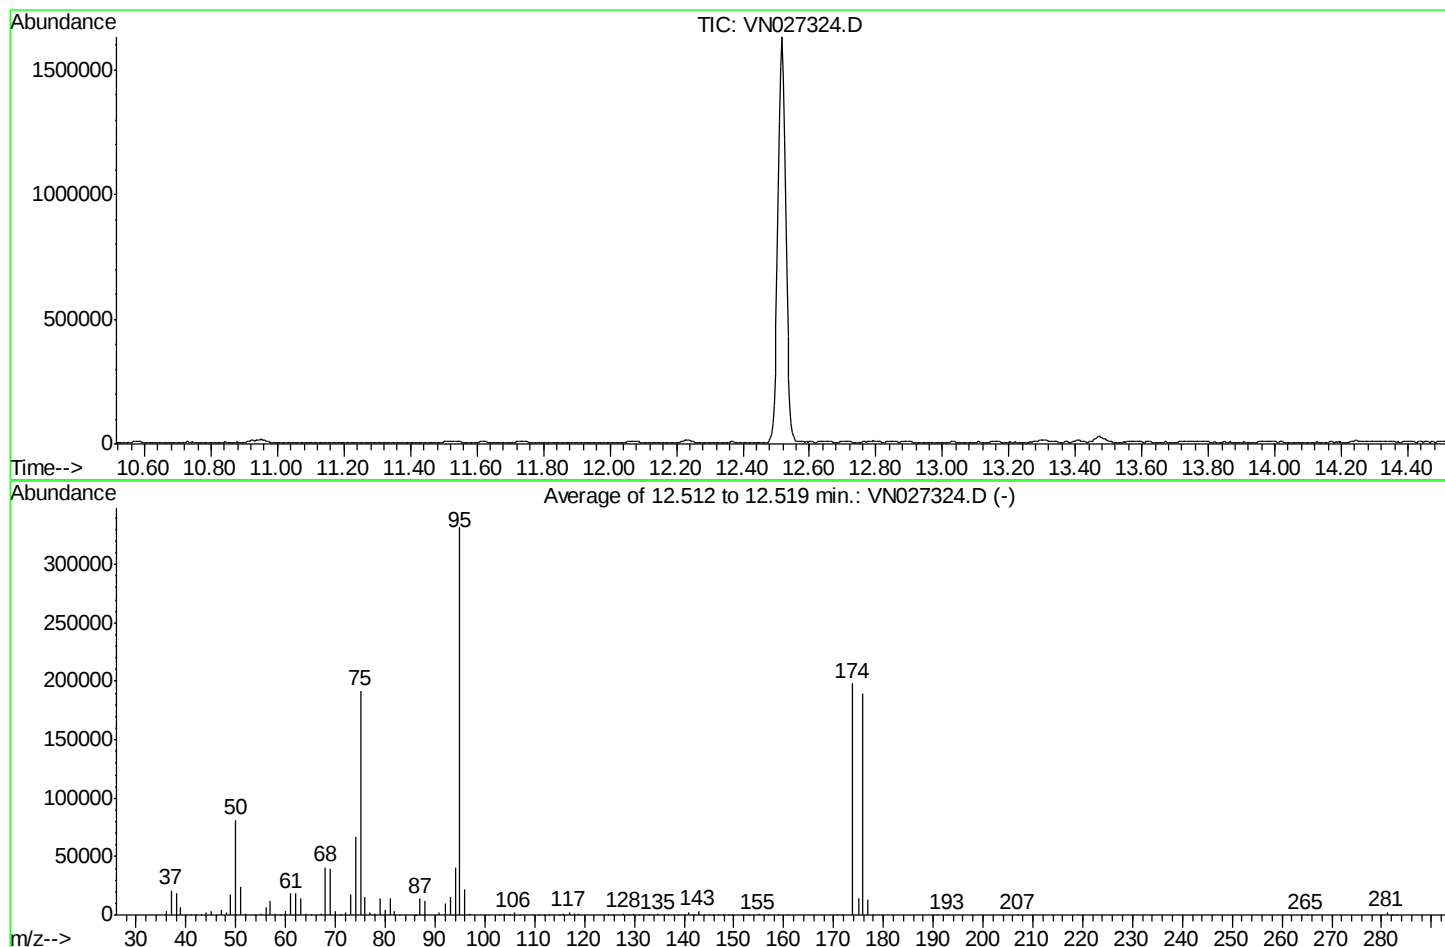

AutoFind: Scans 3397, 3398, 3399; Background Corrected with Scan 3382

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.5	81256	PASS
75	95	30	60	57.9	192170	PASS
95	95	100	100	100.0	331818	PASS
96	95	5	9	6.5	21493	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	59.7	198037	PASS
175	174	5	9	7.4	14671	PASS
176	174	95	101	95.6	189376	PASS
177	176	5	9	6.8	12828	PASS