


Data Path : W:\HPCHEM1\MSVOA N\DATA\VN092115\
Data File : VN027343.D
Acq On : 21 Sep 2015 21:26
Operator : MD\FY
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_N\METHODS\82N092115W.M
Title : SW846 8260
Last Update : Mon Sep 21 13:12:32 2015

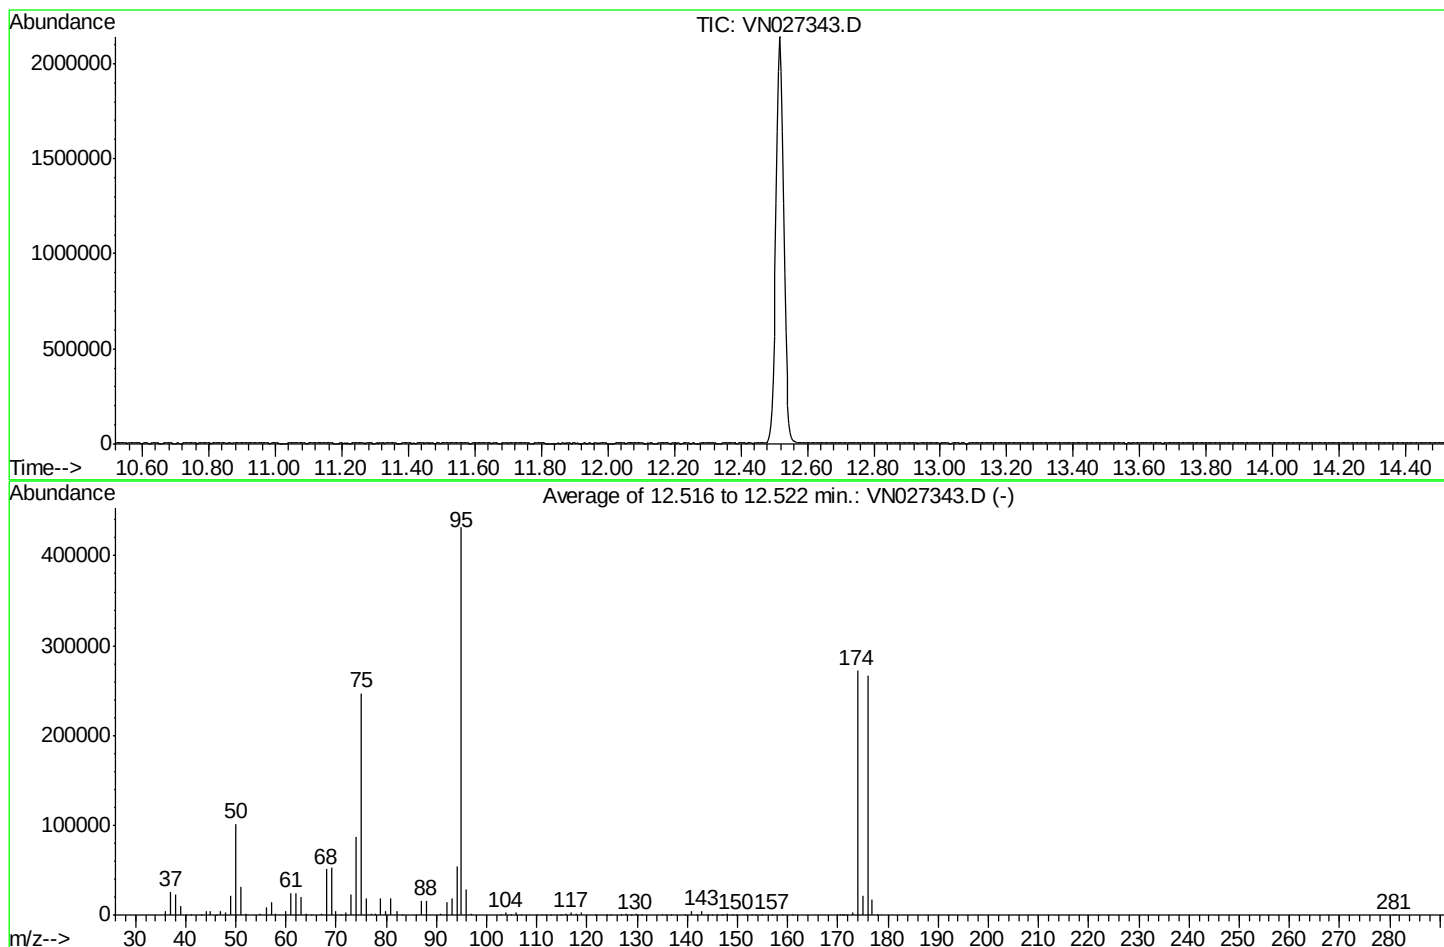

AutoFind: Scans 3398, 3399, 3400; Background Corrected with Scan 3383

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.5	101669	PASS
75	95	30	60	57.2	246890	PASS
95	95	100	100	100.0	431765	PASS
96	95	5	9	6.5	28272	PASS
173	174	0.00	2	1.3	3559	PASS
174	95	50	100	63.0	271829	PASS
175	174	5	9	7.7	20834	PASS
176	174	95	101	98.0	266261	PASS
177	176	5	9	6.2	16527	PASS