


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN092218\
Data File : VN051364.D
Acq On : 21 Sep 2018 12:49
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N092018W.M
Title : SW846 8260
Last Update : Fri Sep 21 04:23:57 2018

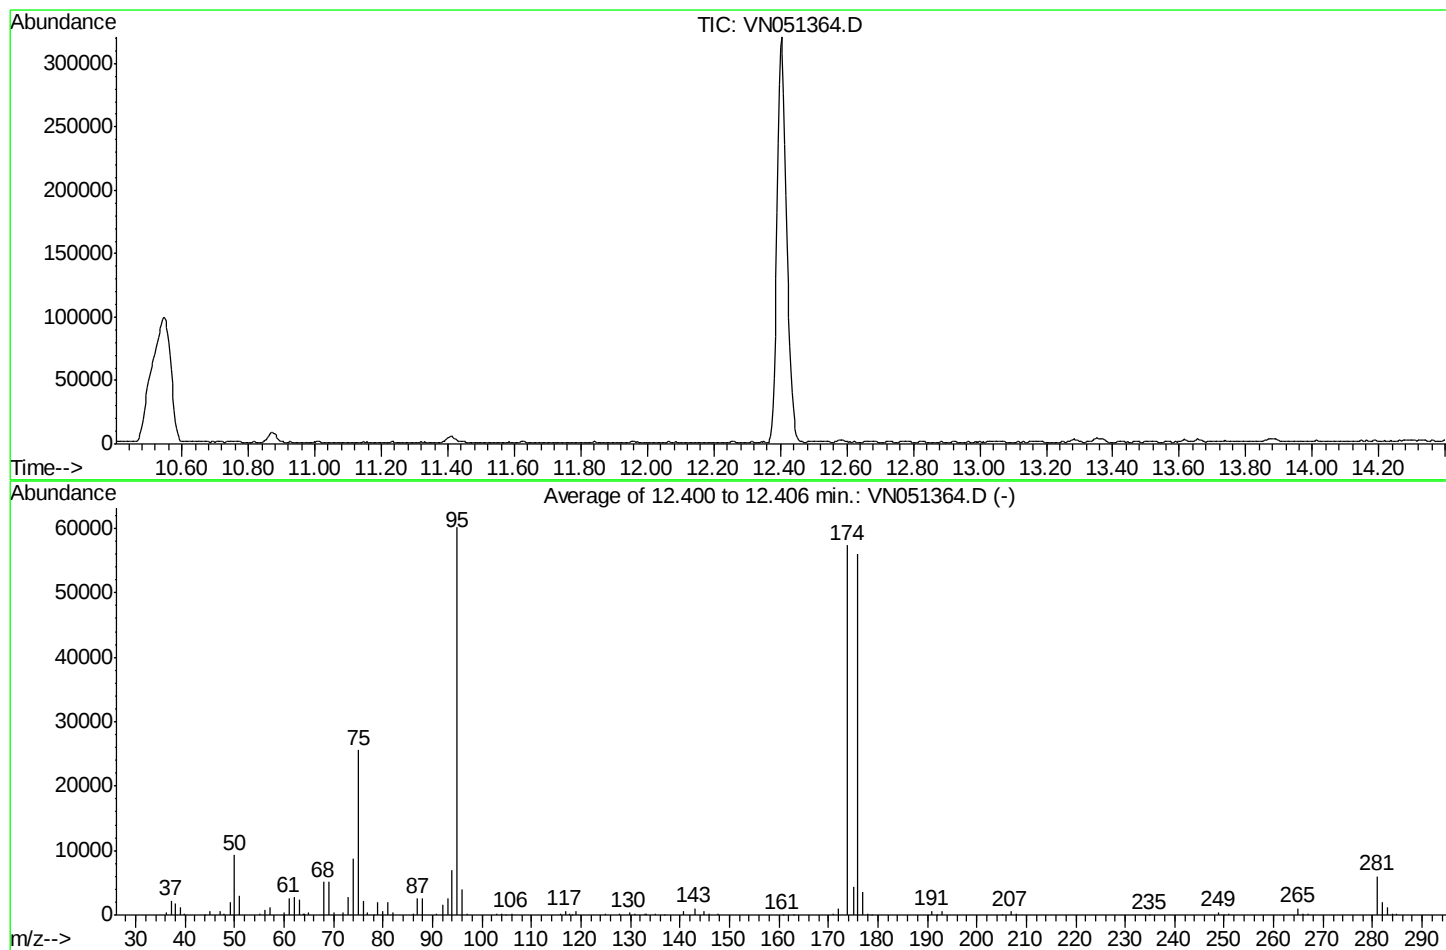

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.4	9291	PASS
75	95	30	60	42.6	25621	PASS
95	95	100	100	100.0	60157	PASS
96	95	5	9	6.8	4074	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	95.4	57360	PASS
175	174	5	9	7.7	4399	PASS
176	174	95	101	97.6	55973	PASS
177	176	5	9	6.3	3519	PASS