

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN092718\
 Data File : VN051540.D
 Acq On : 26 Sep 2018 17:27
 Operator : MD\SY
 Sample : VN0927WBL01
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0927WBL01

Quant Time: Sep 27 08:12:47 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N092318W.M
 Quant Title : SW846 8260
 QLast Update : Mon Sep 24 06:41:32 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.67	168	698480	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.59	114	1086778	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.41	117	905479	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.35	152	325927	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.03	65	481159	54.99	ug/l	0.00
Spiked Amount	50.000		Recovery	=	109.98%	
35) Dibromofluoromethane	7.59	113	425072	48.91	ug/l	0.00
Spiked Amount	50.000		Recovery	=	97.82%	
50) Toluene-d8	10.09	98	1518948	46.42	ug/l	0.00
Spiked Amount	50.000		Recovery	=	92.84%	
62) 4-Bromofluorobenzene	12.40	95	415012	39.20	ug/l	0.00
Spiked Amount	50.000		Recovery	=	78.40%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN092718\
Data File : VN051540.D
Acq On : 26 Sep 2018 17:27
Operator : MD\SY
Sample : VN0927WBL01
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0927WBL01

Quant Time: Sep 27 08:12:47 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N092318W.M
Quant Title : SW846 8260
QLast Update : Mon Sep 24 06:41:32 2018
Response via : Initial Calibration

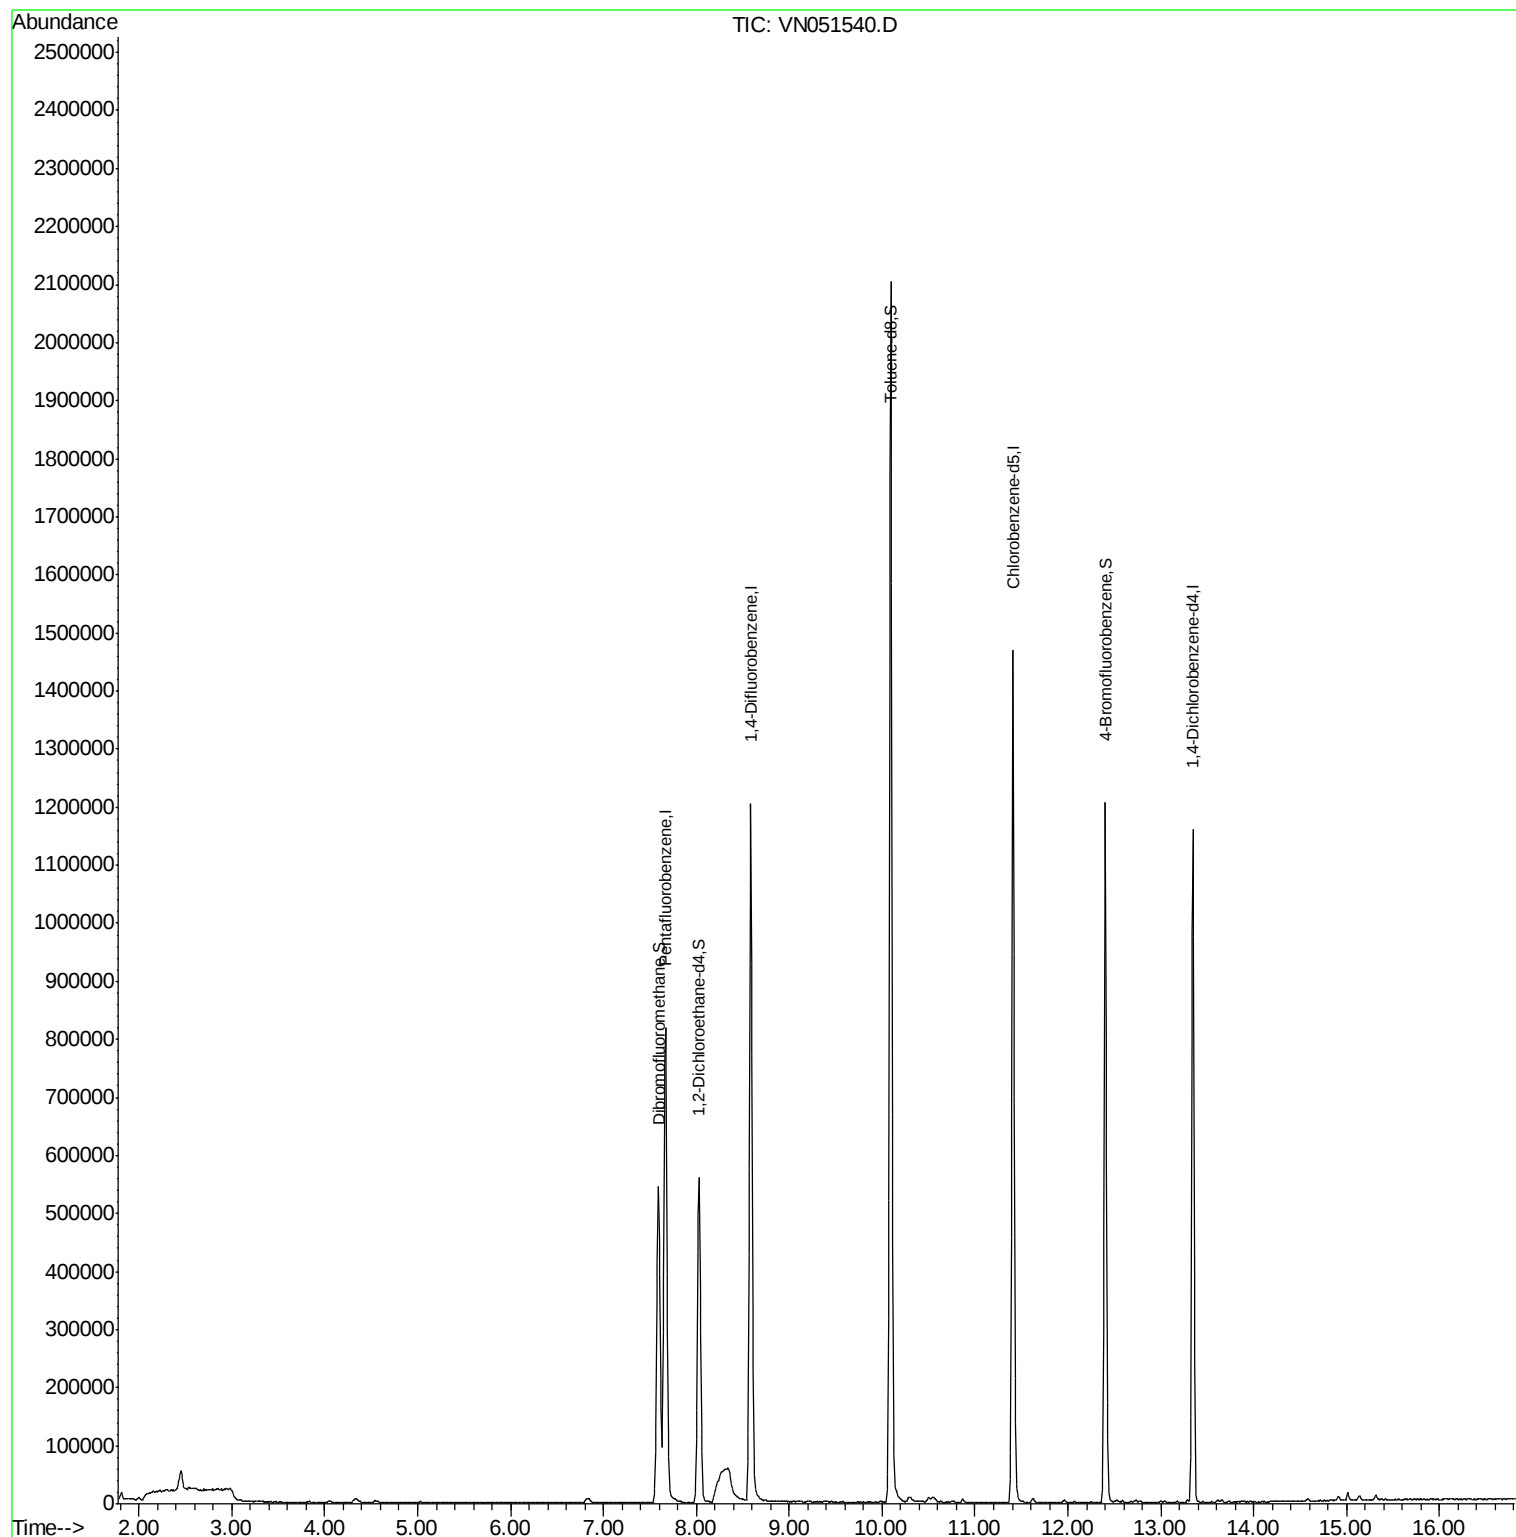

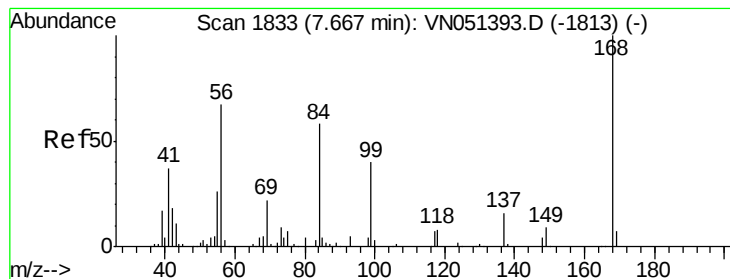

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.67 min Scan# 1833

Delta R.T. -0.00 min

Lab File: VN051540.D

Acq: 26 Sep 2018 17:27

Instrument :

MSVOA_N

ClientSampleId :


VN0927WBL01

Tot Ion:168 Resp: 698480

Ion Ratio Lower Upper

168 100

99 51.5 40.2 60.2

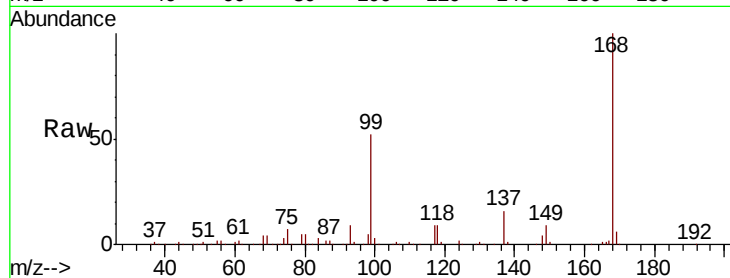

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VN

7.67



300000

200000

100000

0

Time-->

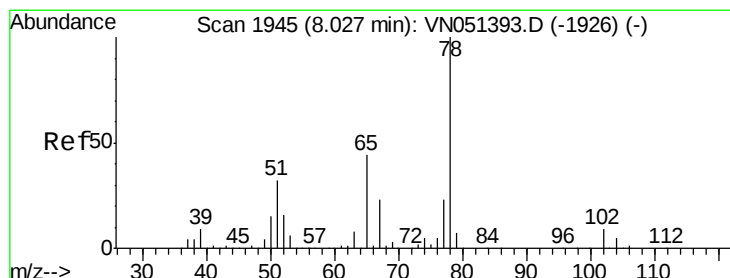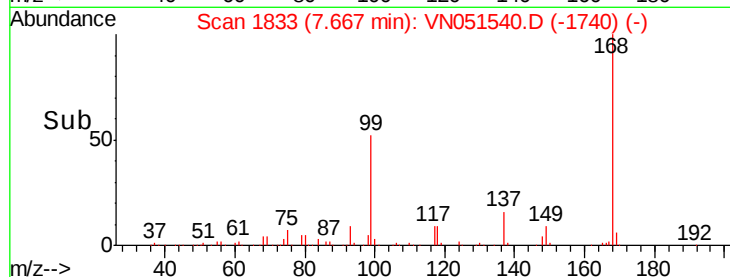

#33

1,2-Dichloroethane-d4

Concen: 54.991 ug/l

RT: 8.03 min Scan# 1946

Delta R.T. 0.00 min

Lab File: VN051540.D


Acq: 26 Sep 2018 17:27

Tgt Ion: 65 Resp: 481159

Ion Ratio Lower Upper

65 100

67 53.8 0.0 107.8

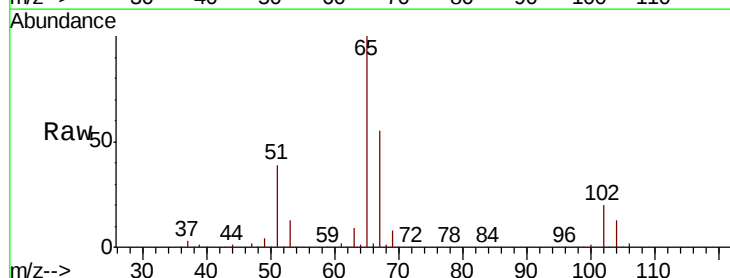

Abundance Ion 64.90 (64.60 to 65.60): VNO

Ion 66.90 (66.60 to 67.60): VNO

8.03

200000


150000


100000

50000

0

Time-->

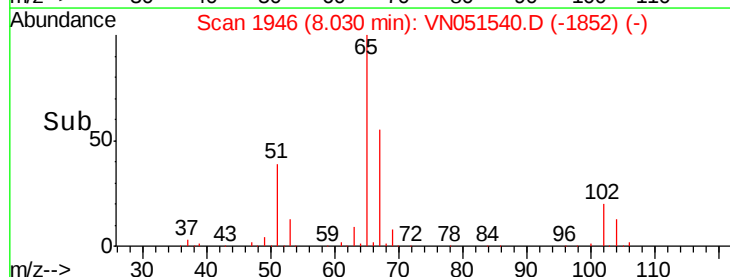

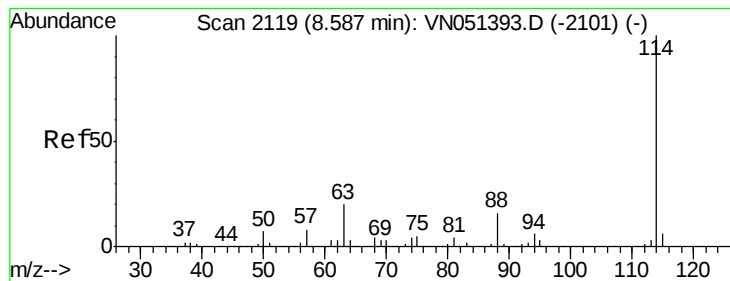

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.59 min Scan# 2119

Delta R.T. -0.00 min

Lab File: VN051540.D

Acq: 26 Sep 2018 17:27

Instrument :

MSVOA_N

ClientSampleId :

VN0927WBL01


Tot Ion:114 Resp: 1086778

Ion Ratio Lower Upper

114 100

63 20.7 0.0 40.2




88 15.7 0.0 31.4

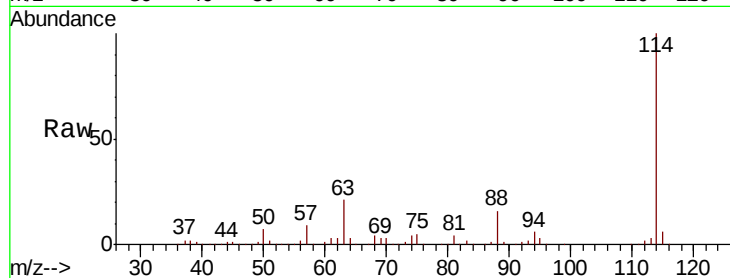

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VN0

Ion 87.90 (87.60 to 88.60): VN0

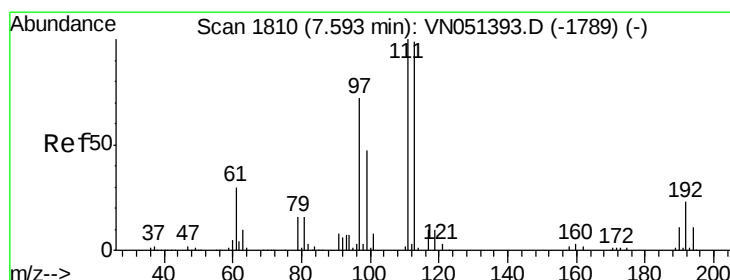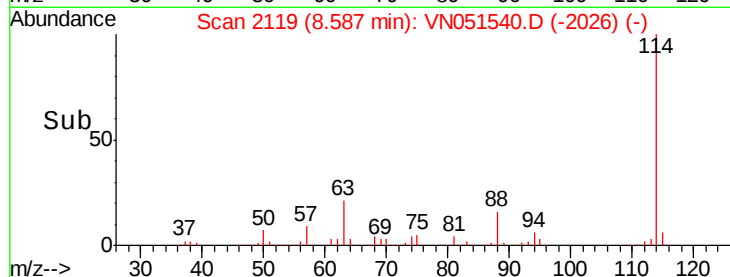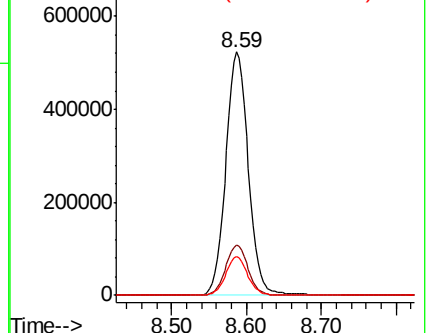

#35

Dibromofluoromethane

Concen: 48.912 ug/l

RT: 7.59 min Scan# 1810

Delta R.T. -0.00 min

Lab File: VN051540.D

Acq: 26 Sep 2018 17:27


Tgt Ion:113 Resp: 425072

Ion Ratio Lower Upper

113 100

111 100.6 82.6 123.8



192 21.7 18.0 27.0

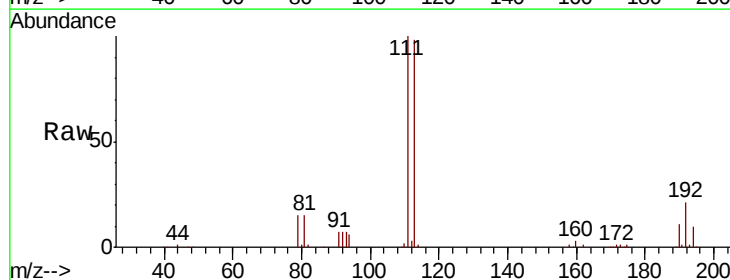


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V



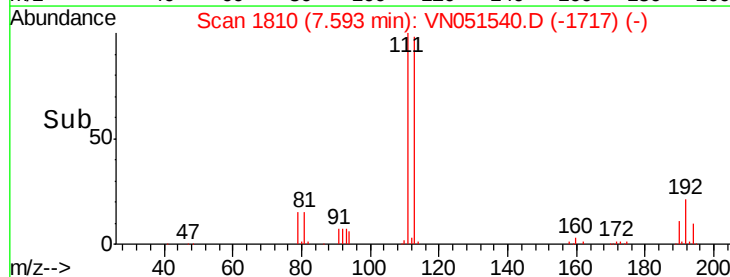
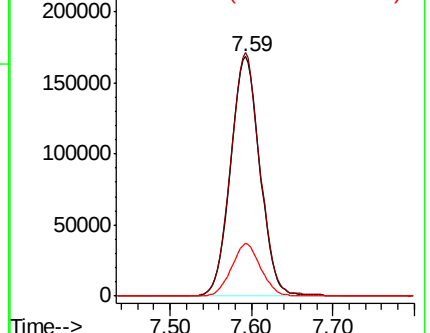


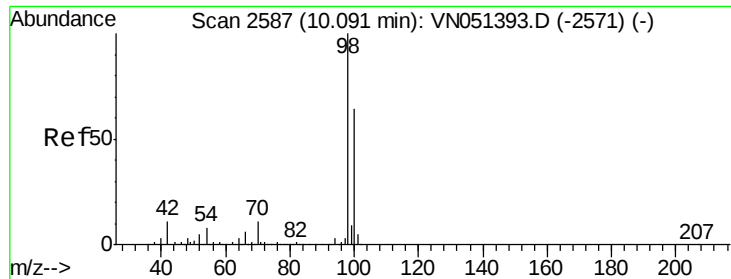

#50
Toluene-d8
Concen: 46.415 ug/l
RT: 10.09 min Scan# 2587
Delta R.T. -0.00 min
Lab File: VN051540.D
Acq: 26 Sep 2018 17:27




Instrument :
MSVOA_N
ClientSampleId :
VN0927WBL01


Tot Ion: 98 Resp: 1518948
Ion Ratio Lower Upper
98 100
100 63.1 50.6 75.8

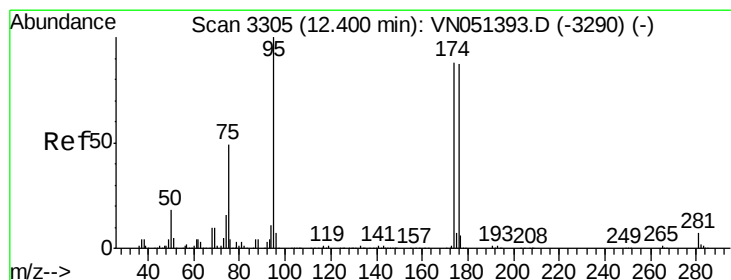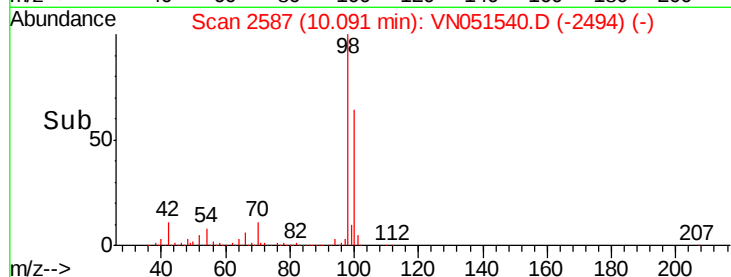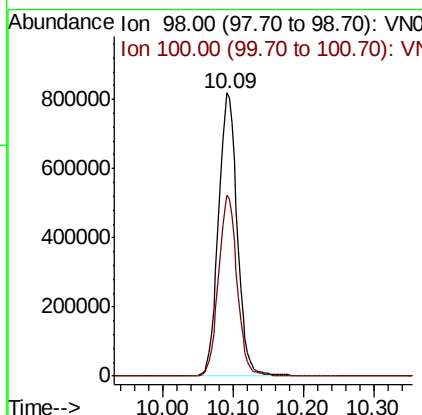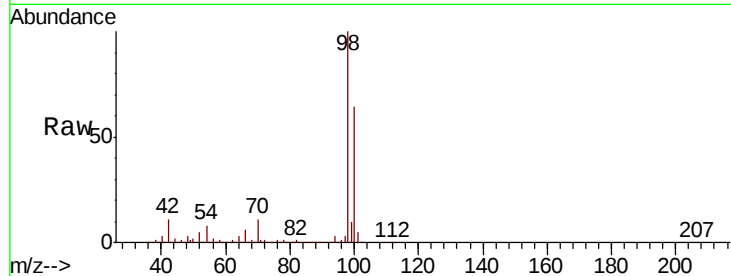

#62
4-Bromofluorobenzene
Concen: 39.202 ug/l
RT: 12.40 min Scan# 3306
Delta R.T. 0.00 min
Lab File: VN051540.D
Acq: 26 Sep 2018 17:27

Tgt Ion: 95 Resp: 415012
Ion Ratio Lower Upper
95 100
174 89.2 0.0 181.6
176 85.9 0.0 176.4


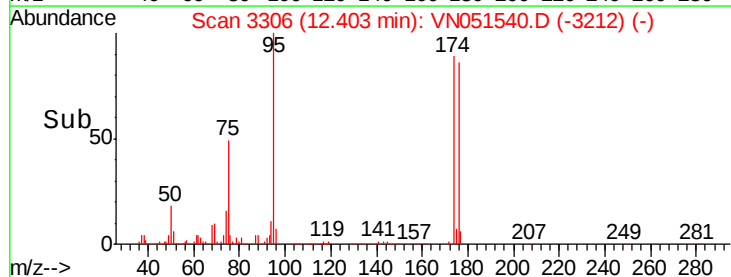
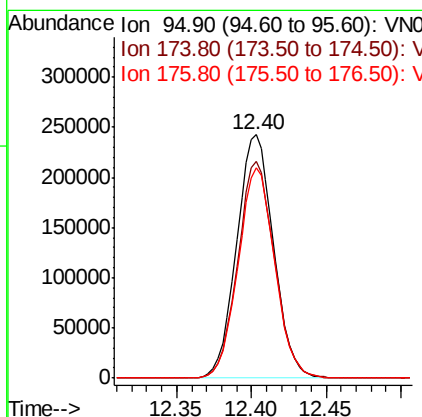
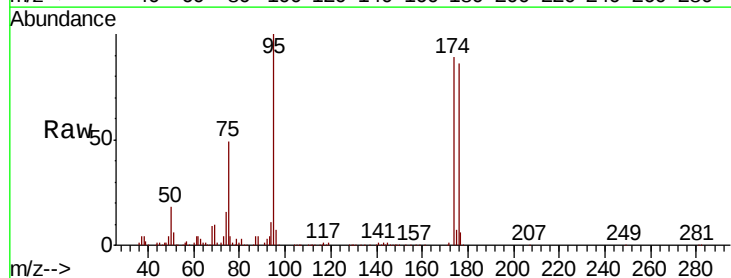


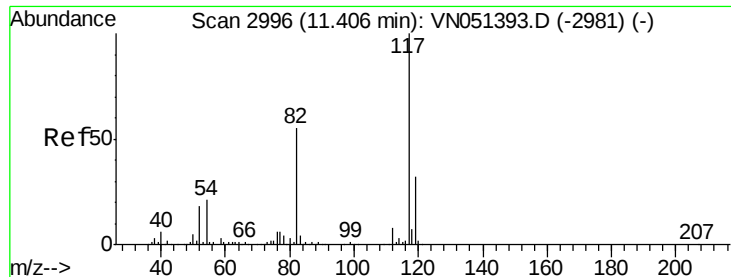

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.41 min Scan# 2997
Delta R.T. 0.00 min
Lab File: VN051540.D
Acq: 26 Sep 2018 17:27

Instrument :
MSVOA_N
ClientSampleId :
VN0927WBL01

Tot Ion:117 Resp: 905479
Ion Ratio Lower Upper
117 100
82 53.9 44.2 66.2
119 32.4 25.9 38.9

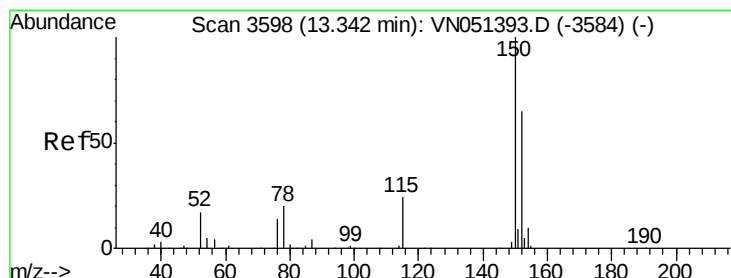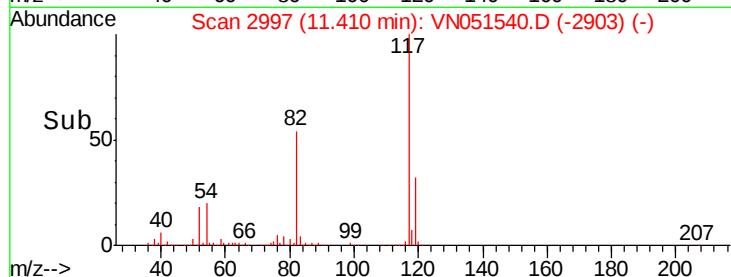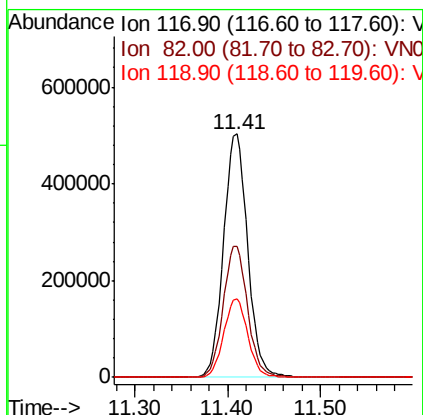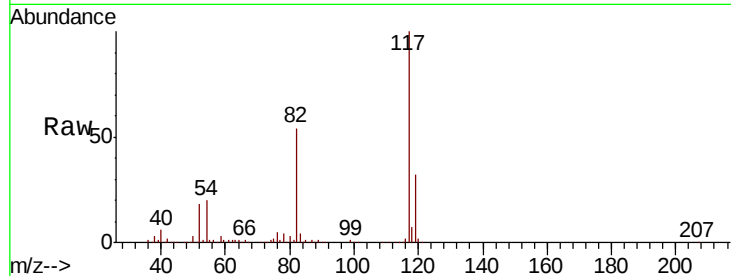

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.35 min Scan# 3599
Delta R.T. 0.00 min
Lab File: VN051540.D
Acq: 26 Sep 2018 17:27

Tgt Ion:152 Resp: 325927
Ion Ratio Lower Upper
152 100
115 57.5 28.3 84.9
150 157.3 0.0 353.6

