


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN092718\
Data File : VN051582.D
Acq On : 27 Sep 2018 14:22
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N092318W.M
Title : SW846 8260
Last Update : Mon Sep 24 06:41:32 2018

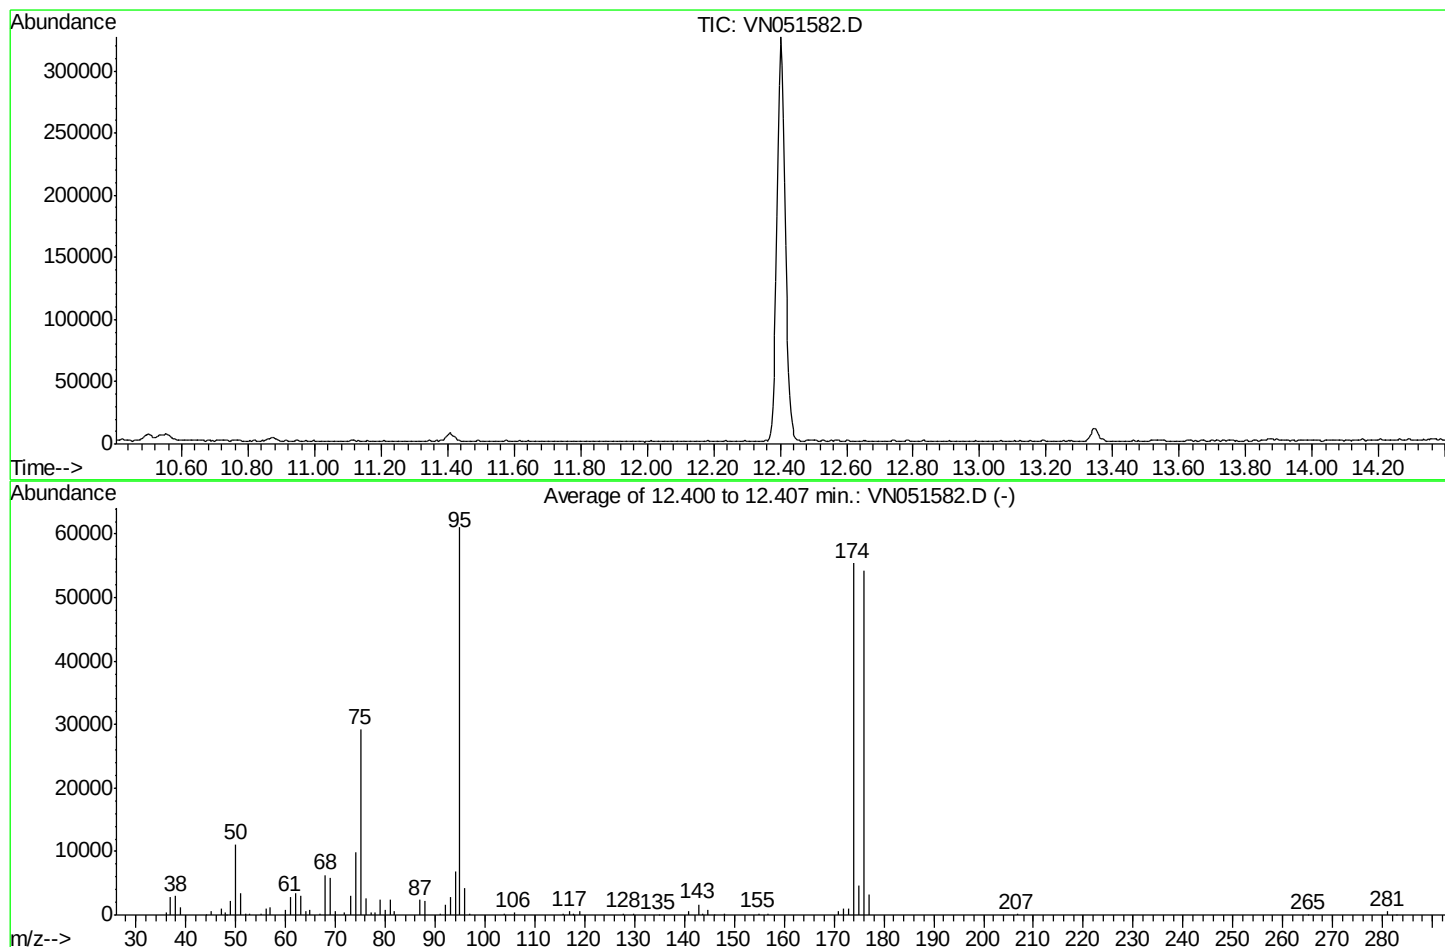

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	11065	PASS
75	95	30	60	47.8	29176	PASS
95	95	100	100	100.0	61066	PASS
96	95	5	9	6.9	4196	PASS
173	174	0.00	2	1.9	1031	PASS
174	95	50	100	90.7	55410	PASS
175	174	5	9	8.4	4653	PASS
176	174	95	101	97.9	54245	PASS
177	176	5	9	6.1	3333	PASS