
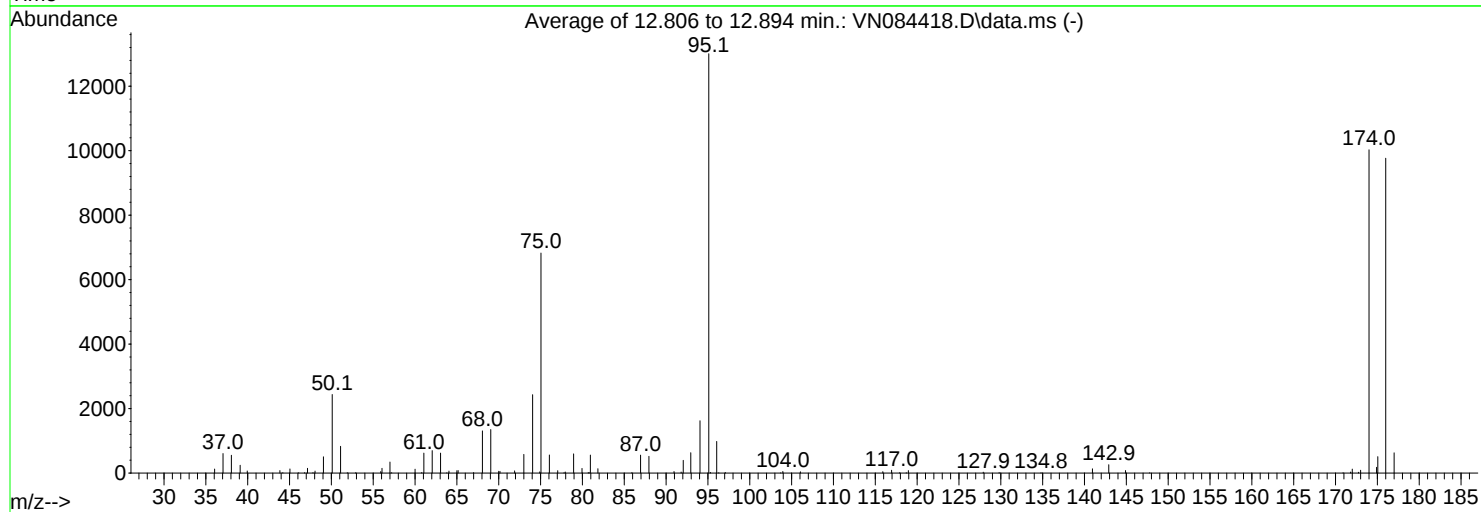


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN101824\
Data File : VN084418.D
Acq On : 18 Oct 2024 08:52
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N100824W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Wed Oct 09 02:22:28 2024

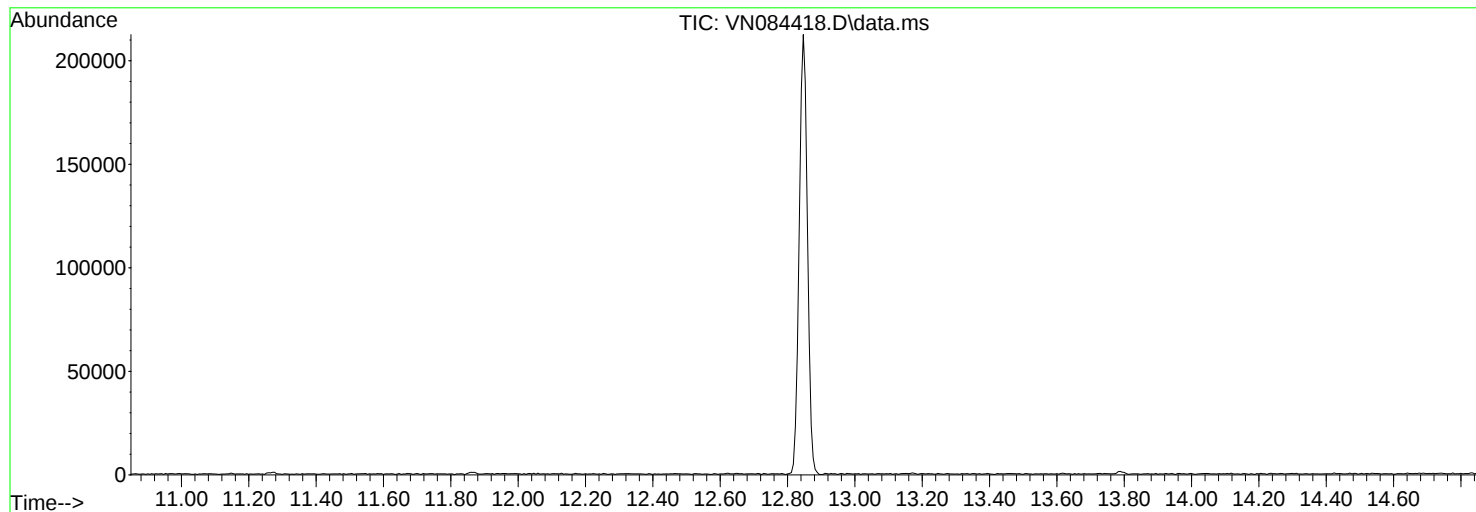

AutoFind: Averaged scan 1845 to 1860; Bkg corrected with scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	2437	PASS
75	95	30	60	52.5	6825	PASS
95	95	100	100	100.0	13007	PASS
96	95	5	9	7.5	981	PASS
173	174	0.00	2	0.9	88	PASS
174	95	50	100	77.1	10028	PASS
175	174	5	9	5.1	509	PASS
176	174	95	101	97.4	9766	PASS
177	176	5	9	6.4	629	PASS